

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020323\
 Data File : PL080745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2023 19:56
 Operator : AR\AJ
 Sample : 01413-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-5-020223

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/06/2023
 Supervised By : Ankita Jodhani 02/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:06:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.687	17508452	18133370	8.163	8.256
28)	SA Decachlor...	8.788	7.835	18783125	20762011	10.729	8.714
Target Compounds							
12)	B 4,4'-DDE	5.985	5.145	1160884	1328743	0.521m	0.563m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020323\
Data File : PL080745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2023 19:56
Operator : AR\AJ
Sample : 01413-01
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-5-020223


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/06/2023
Supervised By : Ankita Jodhani 02/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:06:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

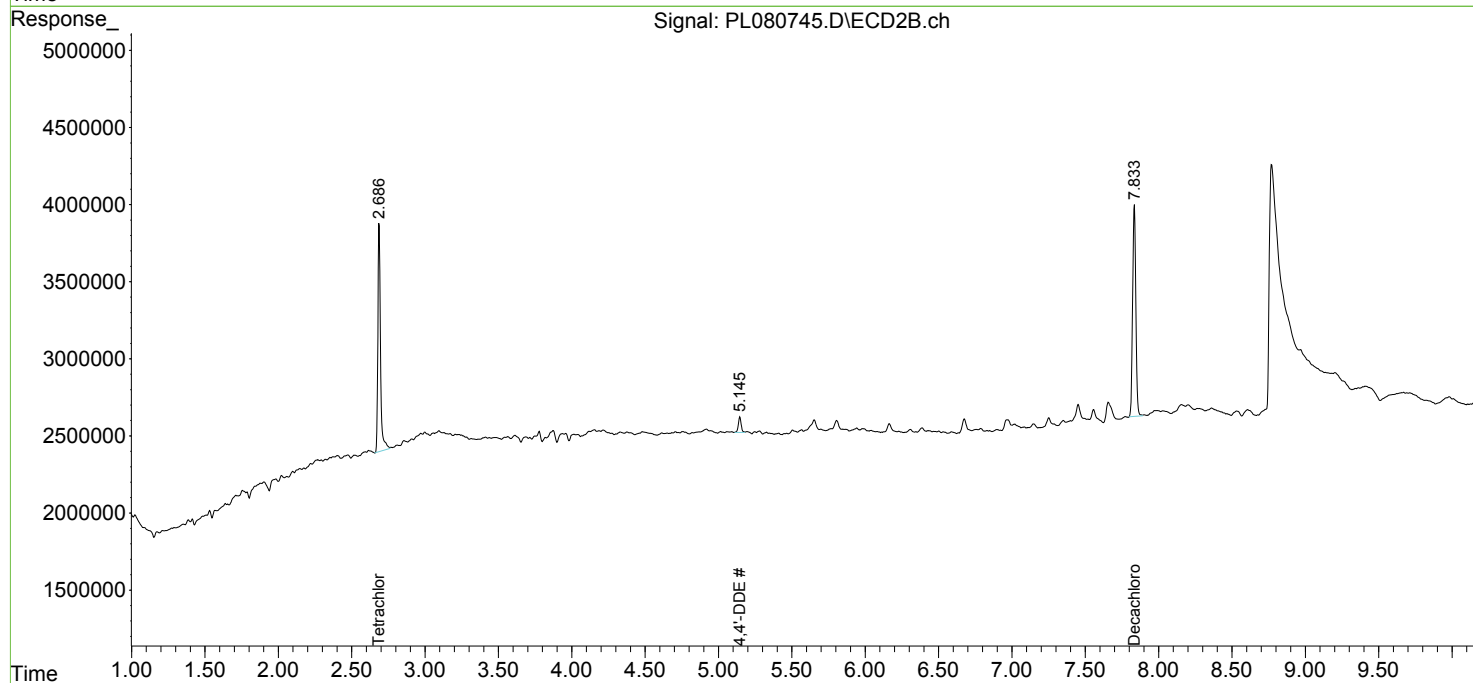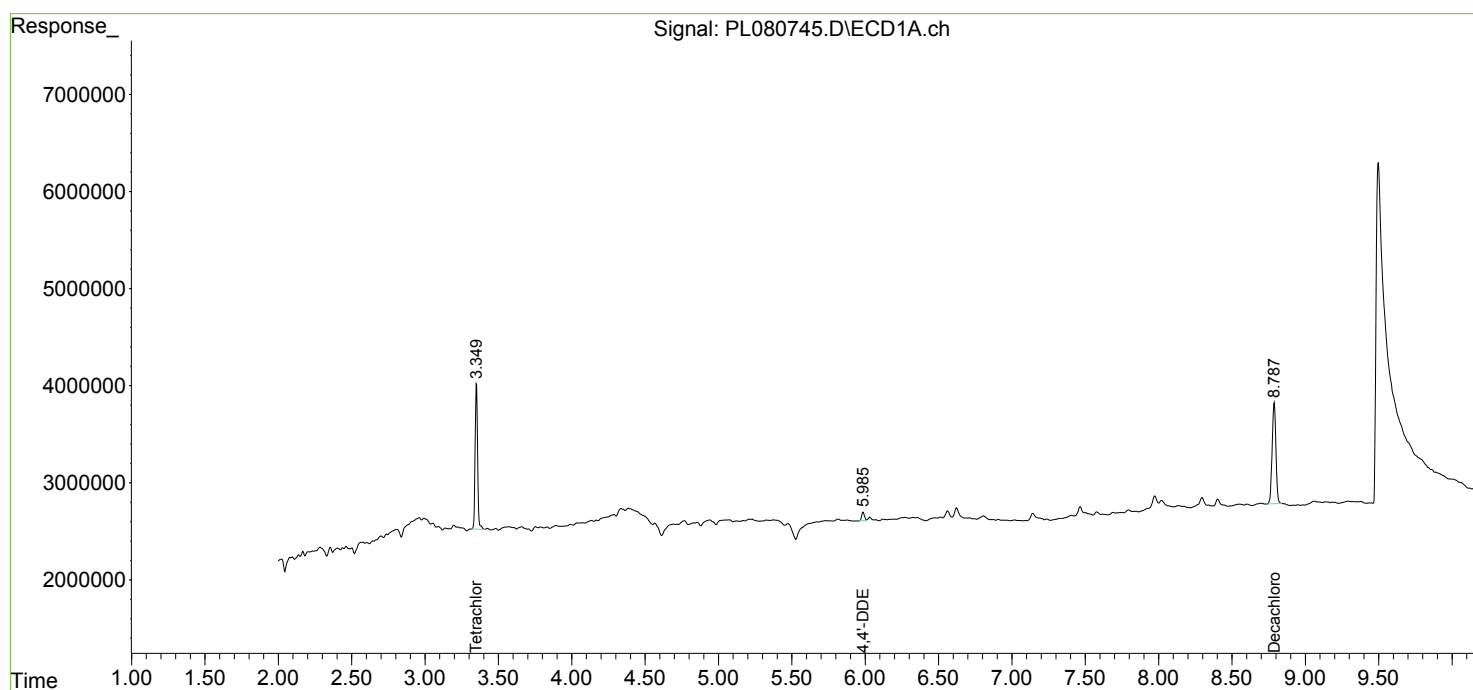

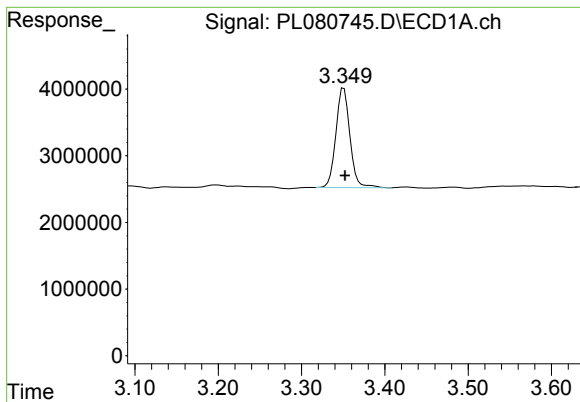


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: -0.001 min
Response: 17508452
Conc: 8.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-5-020223


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/06/2023
Supervised By :Ankita Jodhani 02/06/2023

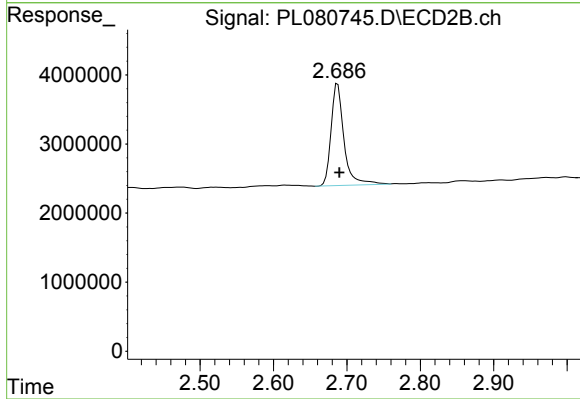


#1 Tetrachloro-m-xylene

R.T.: 2.687 min
Delta R.T.: -0.002 min
Response: 18133370
Conc: 8.26 ng/ml

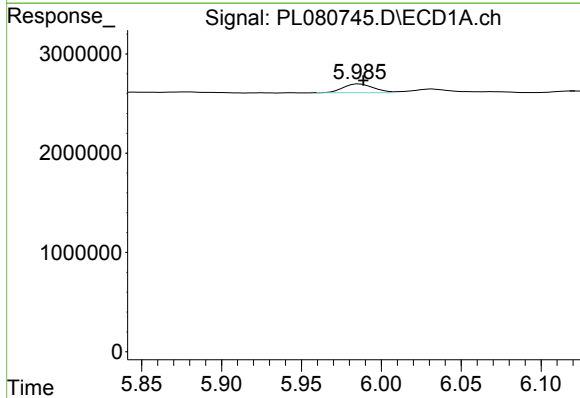


#12 4,4'-DDE

R.T.: 5.985 min
Delta R.T.: -0.004 min
Response: 1160884
Conc: 0.52 ng/ml m

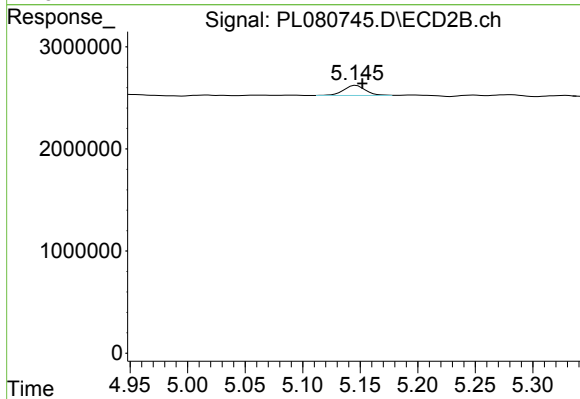

#12 4,4'-DDE

R.T.: 5.145 min
Delta R.T.: -0.007 min
Response: 1328743
Conc: 0.56 ng/ml m

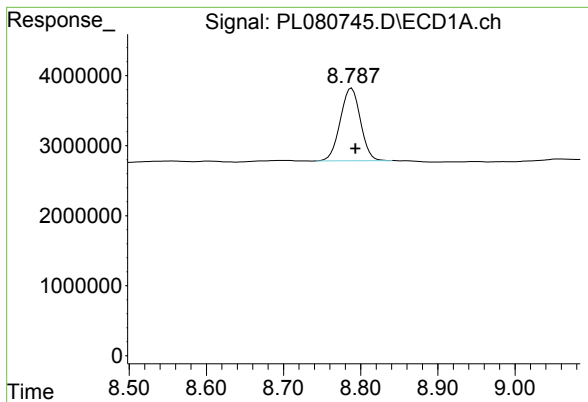

#28 Decachlorobiphenyl

R.T.: 8.788 min
Delta R.T.: -0.005 min
Response: 18783125
Conc: 10.73 ng/ml

Instrument :

ECD_L

ClientSampleId :


TR-5-020223

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 02/06/2023

Supervised By :Ankita Jodhani 02/06/2023

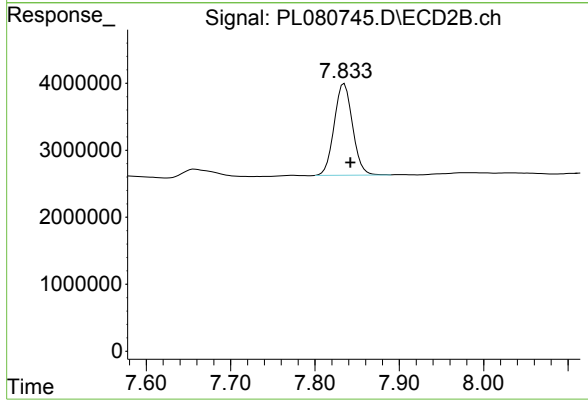

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.007 min
Response: 20762011
Conc: 8.71 ng/ml