

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020325\
 Data File : PL094017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2025 21:22
 Operator : AR\AJ
 Sample : Q1241-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JPP-5.4-013025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/04/2025
 Supervised By :Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:52:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.537	2.773	60746247	74590470	22.559m	22.851m
28) SA Decachlor...	9.055	7.910	51322457	91734968	24.534	26.180

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020325\
Data File : PL094017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2025 21:22
Operator : AR\AJ
Sample : Q1241-16
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
JPP-5.4-013025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/04/2025
Supervised By : Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:52:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

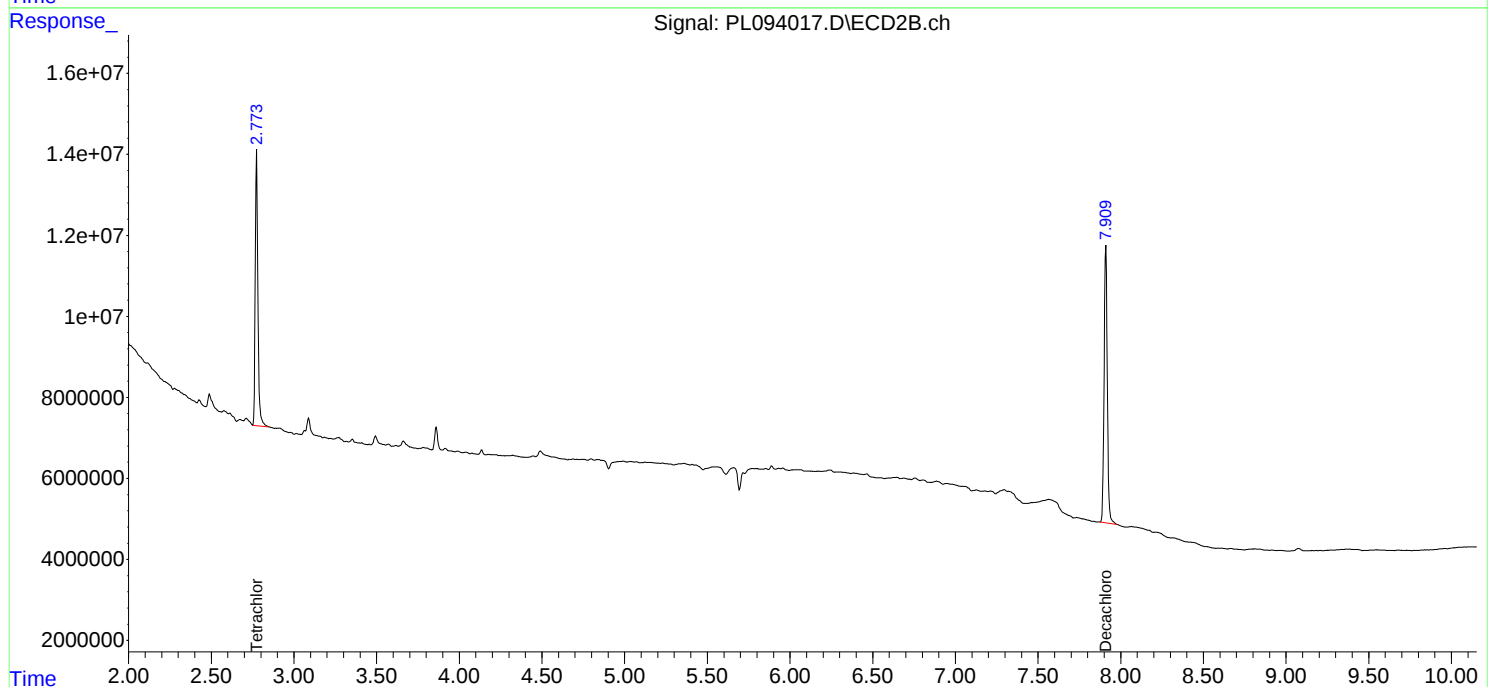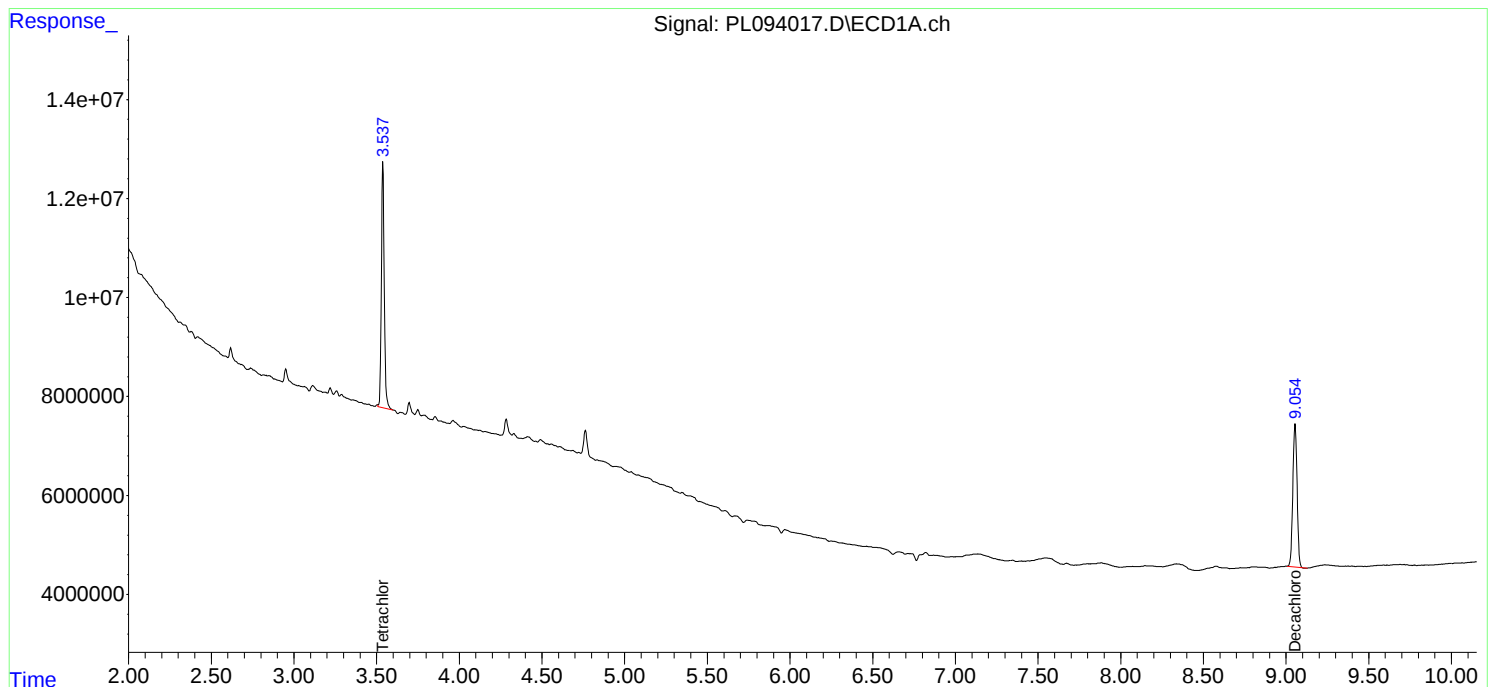

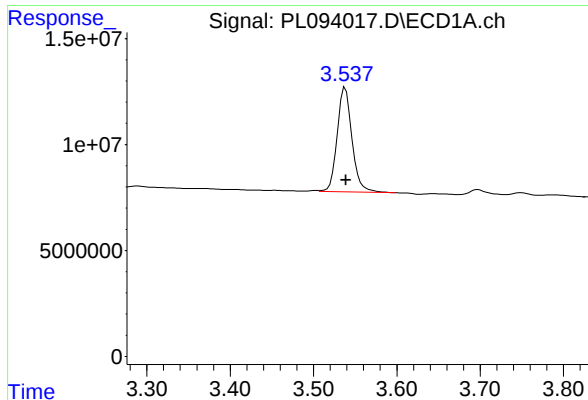


#1 Tetrachloro-m-xylene

R.T.: 3.537 min
Delta R.T.: -0.002 min
Response: 60746247
Conc: 22.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
JPP-5.4-013025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/04/2025
Supervised By :Ankita Jodhani 02/04/2025

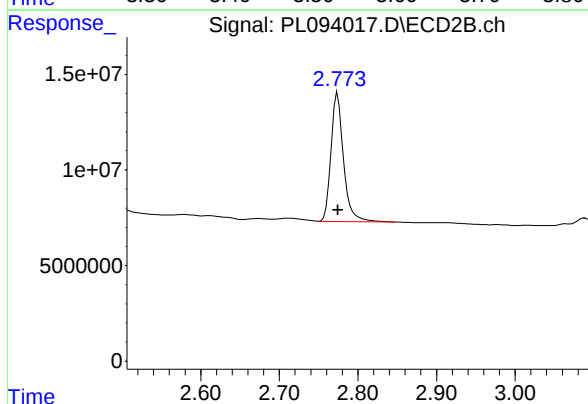


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: -0.002 min
Response: 74590470
Conc: 22.85 ng/ml

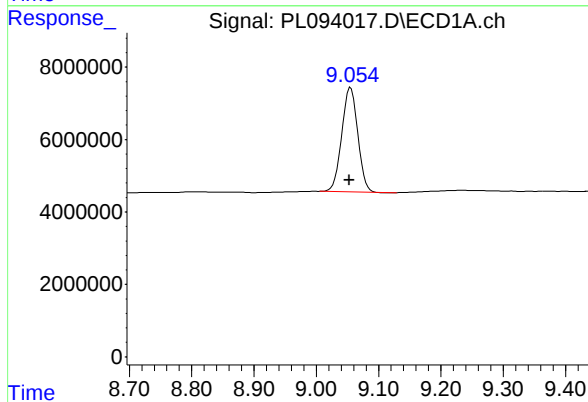

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.002 min
Response: 51322457
Conc: 24.53 ng/ml

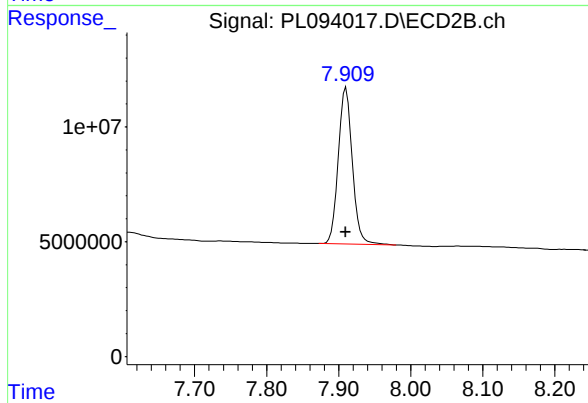

#28 Decachlorobiphenyl

R.T.: 7.910 min
Delta R.T.: 0.000 min
Response: 91734968
Conc: 26.18 ng/ml