

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020325\
 Data File : PL094028.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2025 00:27
 Operator : AR\AJ
 Sample : Q1262-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CONCRETE-PAD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/04/2025
 Supervised By :Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 05:11:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.773	64306210	81683877	23.881	25.025
28) SA Decachlor...	9.055	7.909	81877756	68227508	39.140m	19.471m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020325\
Data File : PL094028.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 00:27
Operator : AR\AJ
Sample : Q1262-03
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CONCRETE-PAD


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/04/2025
Supervised By : Ankita Jodhani 02/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 05:11:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

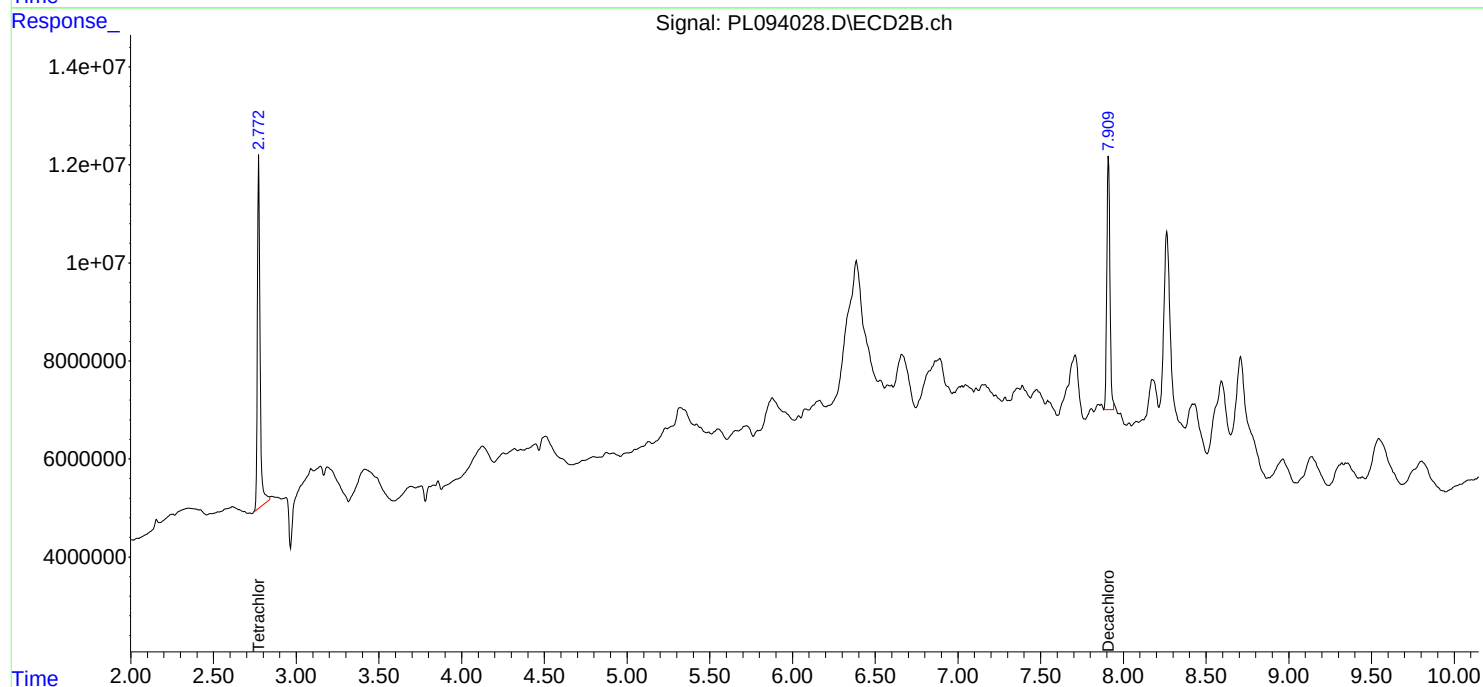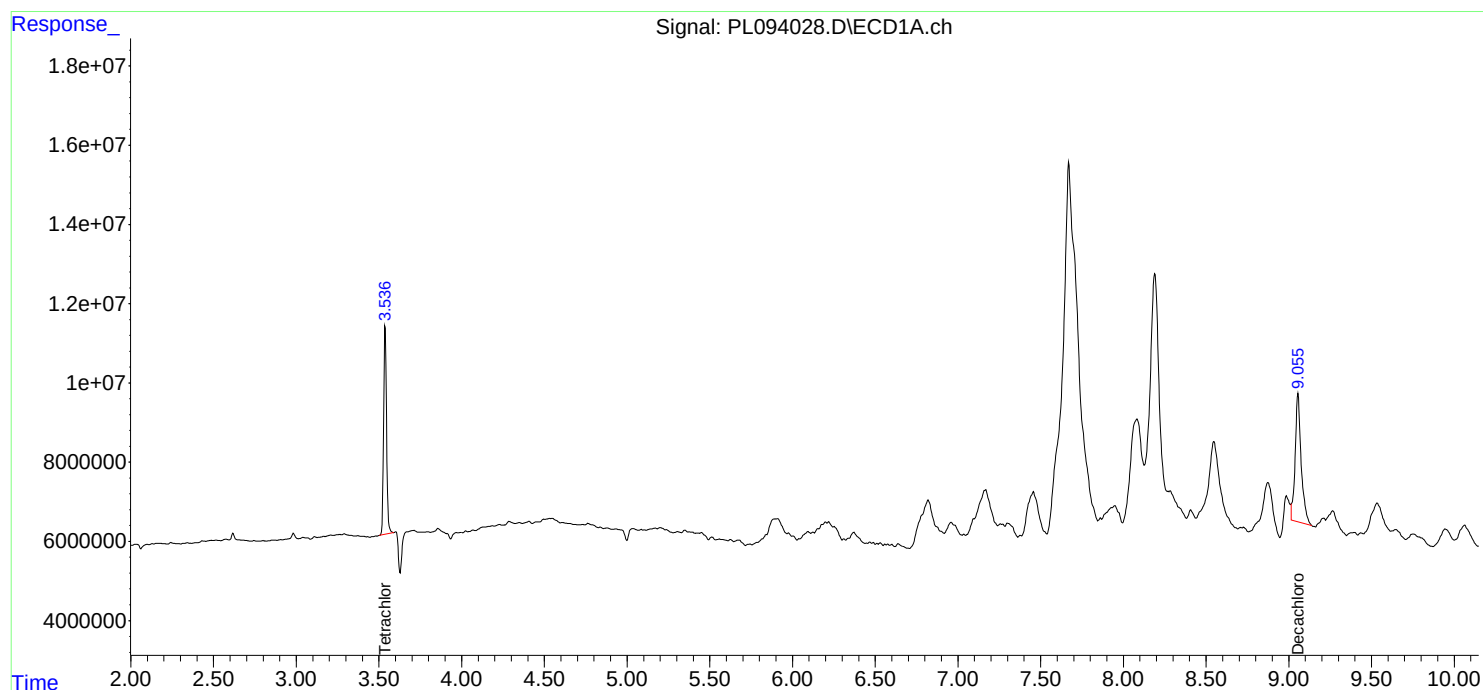

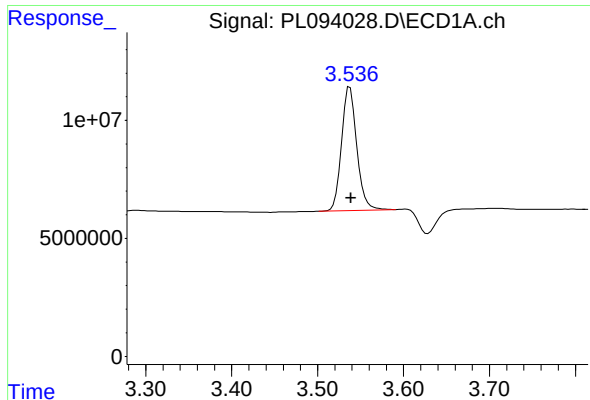


#1 Tetrachloro-m-xylene

R.T.: 3.538 min
Delta R.T.: -0.001 min
Response: 64306210
Conc: 23.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
CONCRETE-PAD


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/04/2025
Supervised By :Ankita Jodhani 02/04/2025

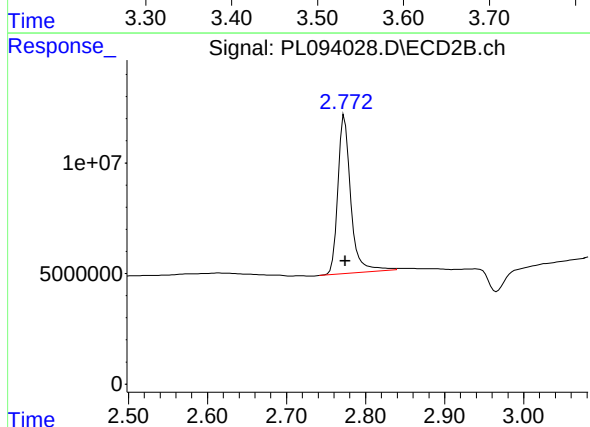


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 81683877
Conc: 25.02 ng/ml

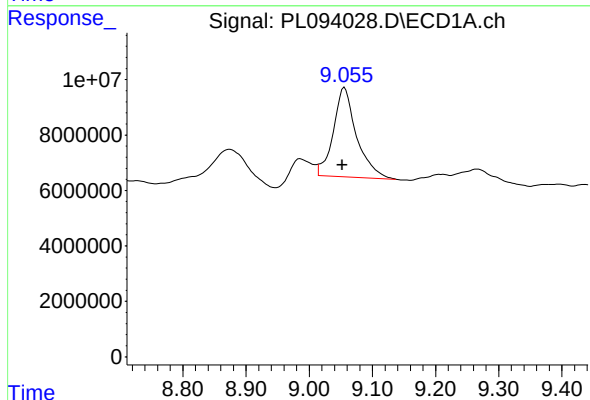

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.002 min
Response: 81877756
Conc: 39.14 ng/ml m

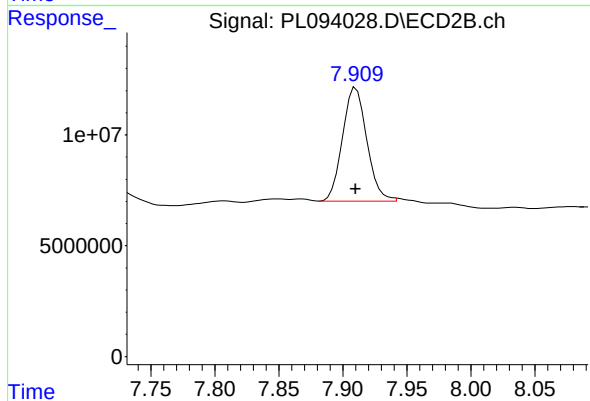

#28 Decachlorobiphenyl

R.T.: 7.909 min
Delta R.T.: -0.001 min
Response: 68227508
Conc: 19.47 ng/ml m