

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020419\
 Data File : PL044404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2019 14:55
 Operator : AJ\SJ
 Sample : K1284-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-004-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 00:06:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 28 01:20:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.366	3.985	138.7E6	46303995	22.889	21.228
28)	SA Decachlor...	8.050	9.044	130.8E6	39246464	18.854	17.692
Target Compounds							
6)	B beta-BHC	4.284f	0.000	9508024	0	2.743	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020419\
Data File : PL044404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2019 14:55
Operator : AJ\SJ
Sample : K1284-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-004-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 00:06:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Mon Jan 28 01:20:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

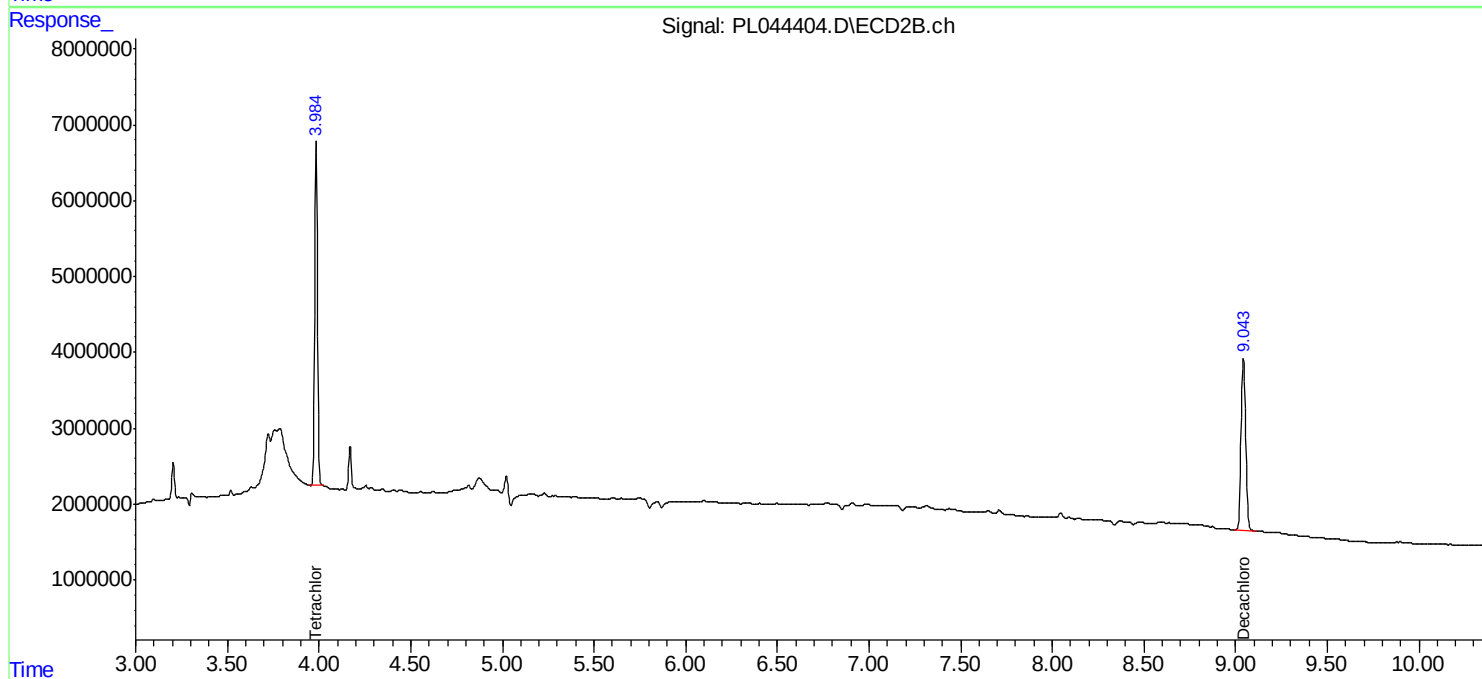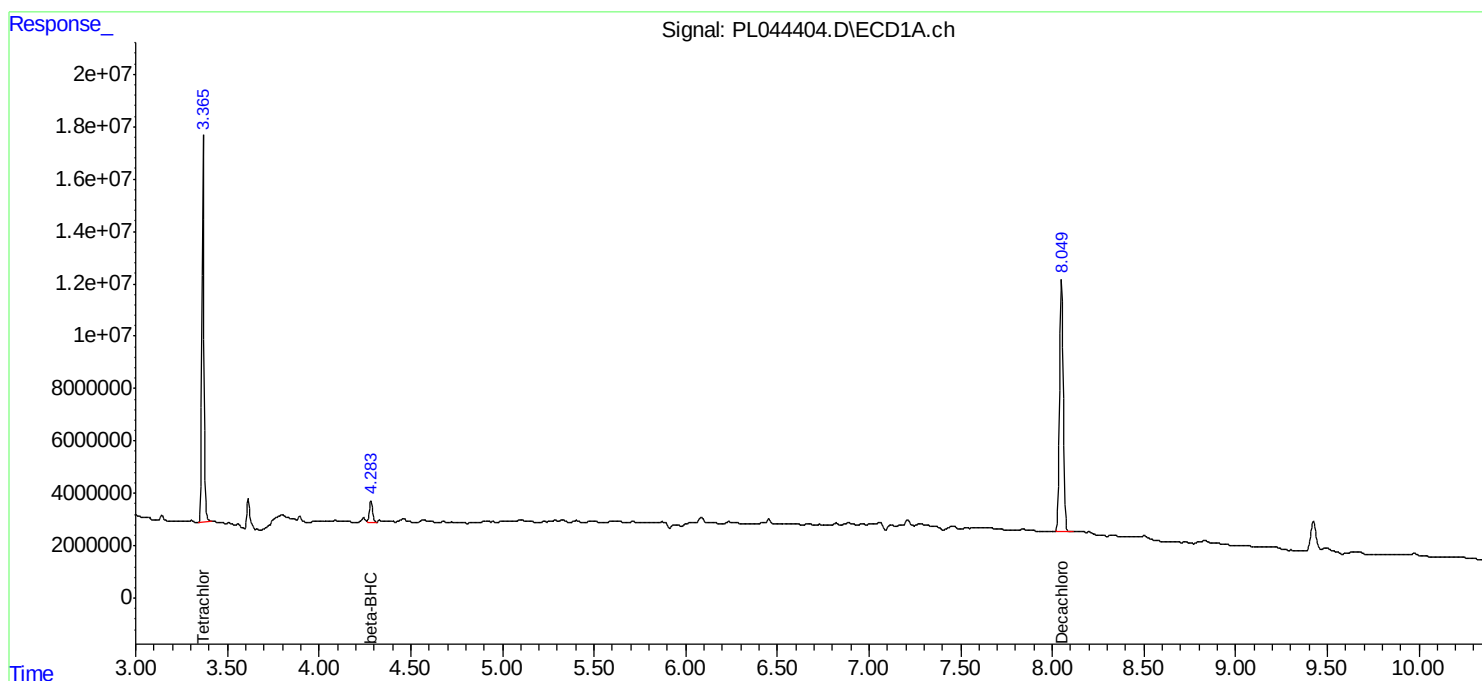


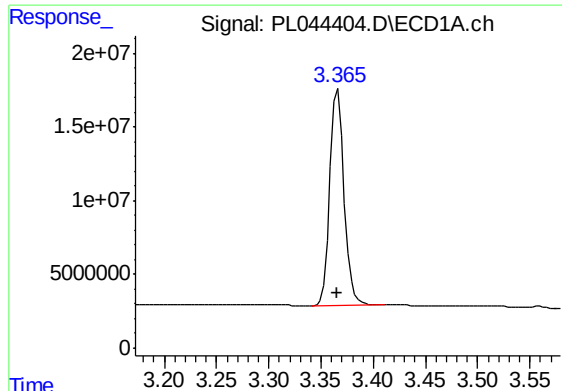

#1 Tetrachloro-m-xylene


R.T.: 3.366 min
Delta R.T.: 0.001 min
Response: 138713912
Conc: 22.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-004-ABCD

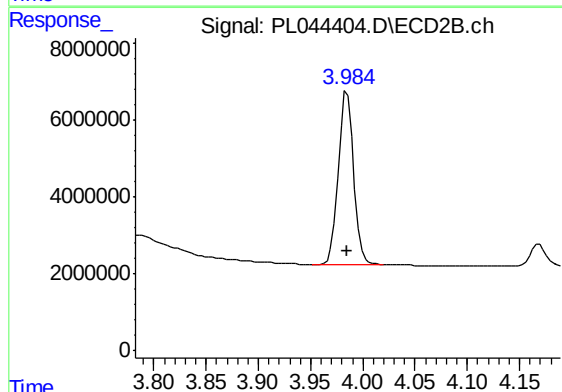


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 46303995
Conc: 21.23 ng/ml

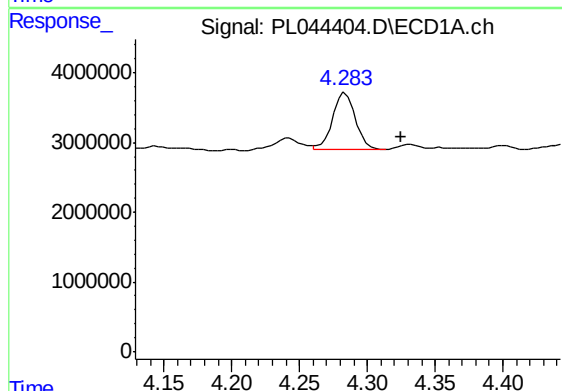


#6 beta-BHC

R.T.: 4.284 min
Delta R.T.: -0.041 min
Response: 9508024
Conc: 2.74 ng/ml

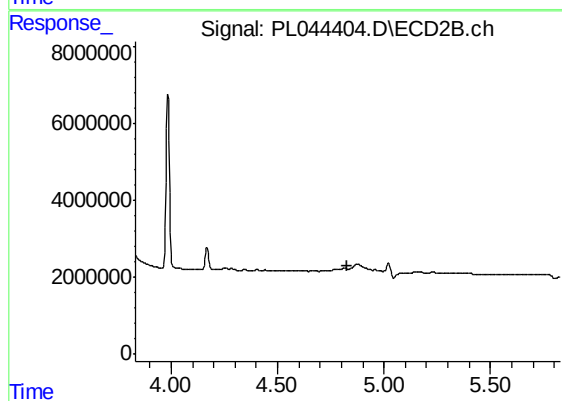

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.830 min
Response: 0
Conc: N.D.

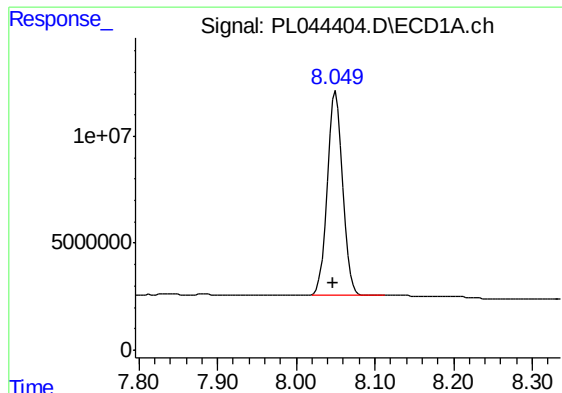

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.002 min
Response: 130753384
Conc: 18.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-004-ABCD

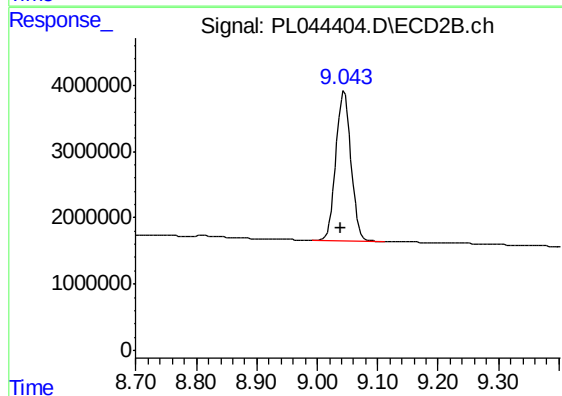

#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.005 min
Response: 39246464
Conc: 17.69 ng/ml