

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020420\
 Data File : PL056319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2020 16:59
 Operator : AJ\MA
 Sample : L1383-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 03:19:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.016	157.0E6	49675646	14.992	16.988
28)	SA Decachlor...	8.252	9.095	151.4E6	31870524	14.379	14.090
Target Compounds							
3)	MA gamma-BHC...	4.229	4.675	25830816	11427436	1.578	2.787 #
9)	A Endosulfan I	5.577f	0.000	99252674	0	6.840	N.D. #
10)	B gamma-Chl...	0.000	6.117	0	13065802	N.D.	4.109 #
13)	MA Dieldrin	5.799	0.000	37403628	0	2.432	N.D. #
14)	MA Endrin	6.047	0.000	11607153	0	0.826	N.D. #
15)	B Endosulfa...	6.330	0.000	15102438	0	1.155	N.D. #
16)	A 4,4'-DDD	6.179	6.848	10786360	8903056	1.003	3.773 #
19)	B Endosulfa...	6.727f	0.000	16134851	0	1.327	N.D. #
21)	B Endrin ke...	7.217f	0.000	9583047	0	0.732	N.D. #
23)	Chlordane-1	4.379	0.000	11282141	0	29.804	N.D. #
25)	Chlordane-3	0.000	6.117	0	13065802	N.D.	34.765 #
27)	Chlordane-5	6.330	0.000	15102438	0	36.406	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020420\
Data File : PL056319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2020 16:59
Operator : AJ\MA
Sample : L1383-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 03:19:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

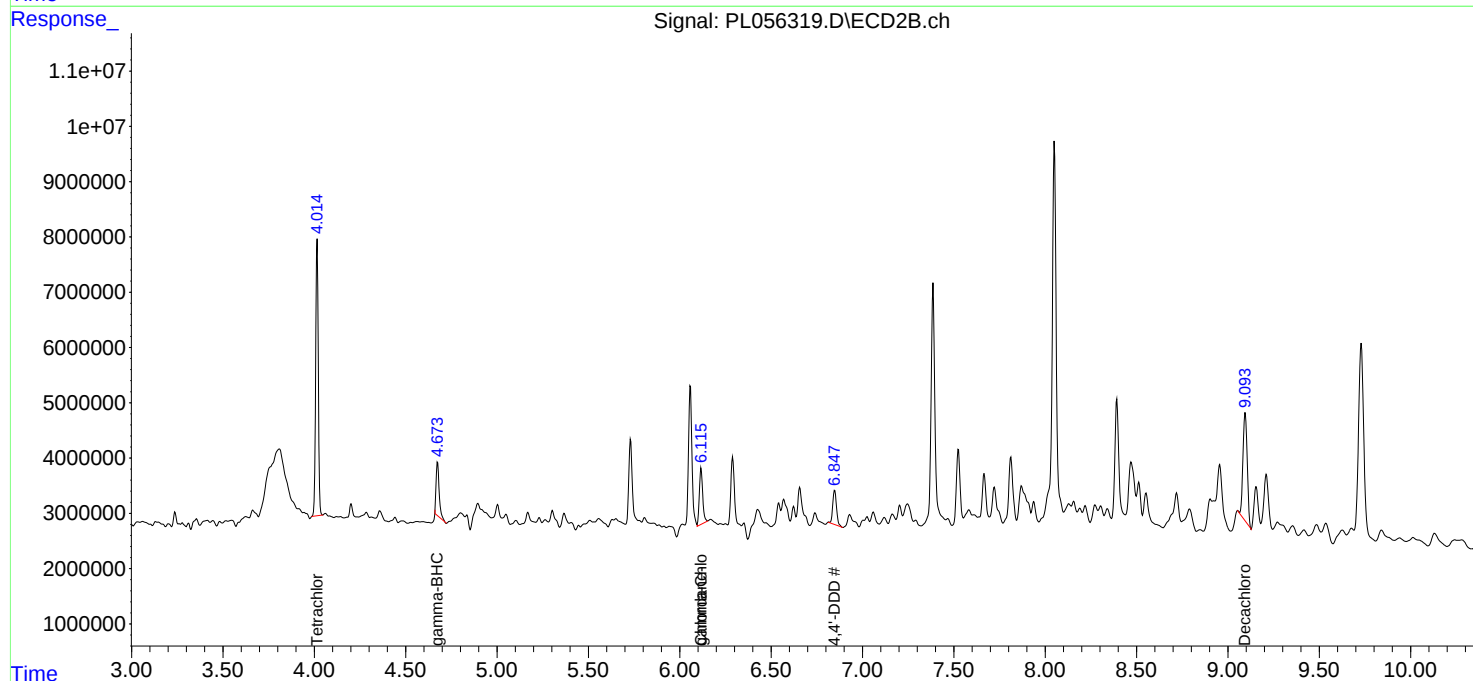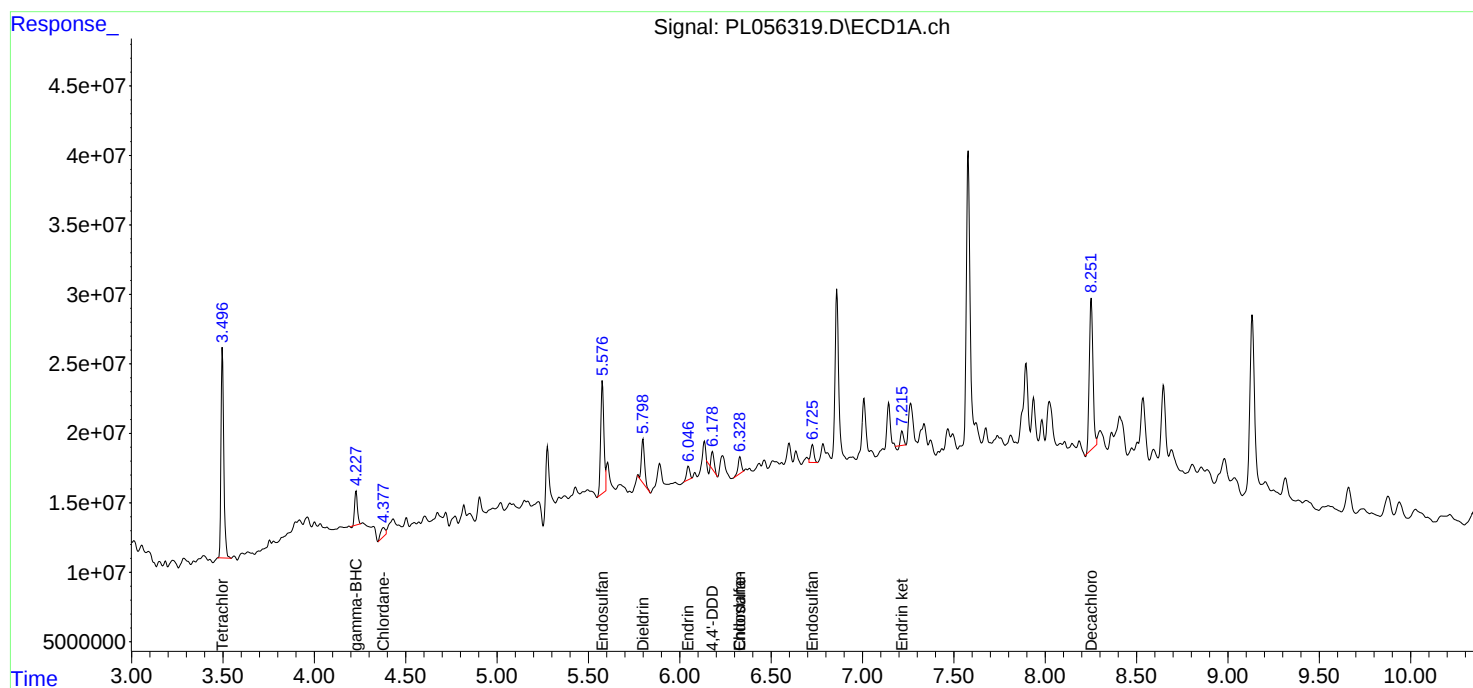


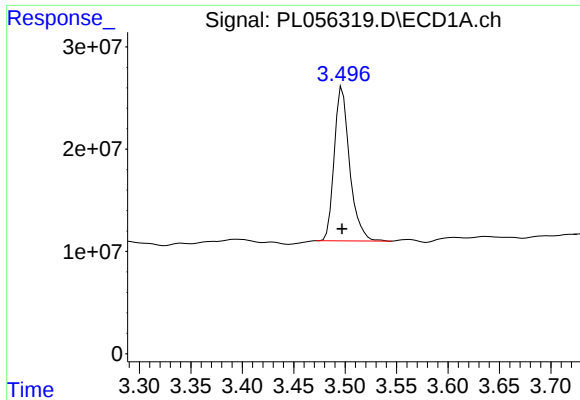

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 157014960
Conc: 14.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

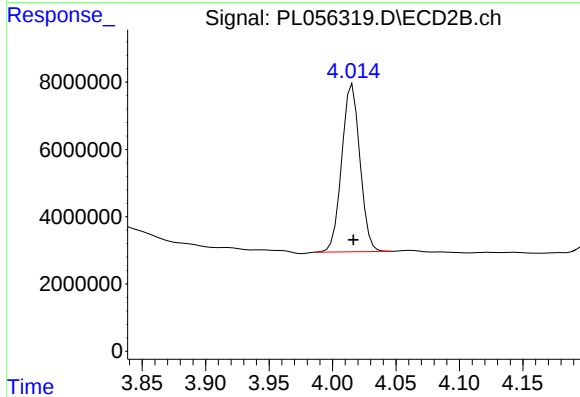


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 49675646
Conc: 16.99 ng/ml

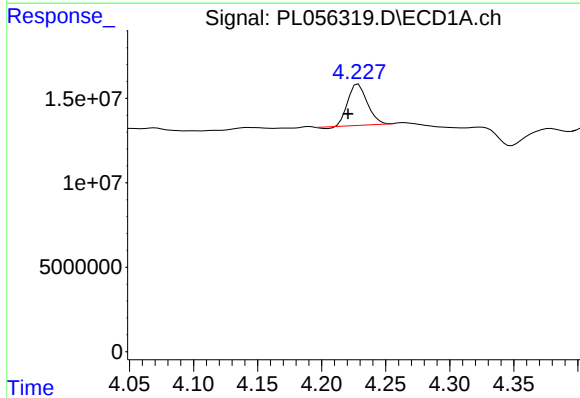


#3 gamma-BHC (Lindane)

R.T.: 4.229 min
Delta R.T.: 0.008 min
Response: 25830816
Conc: 1.58 ng/ml

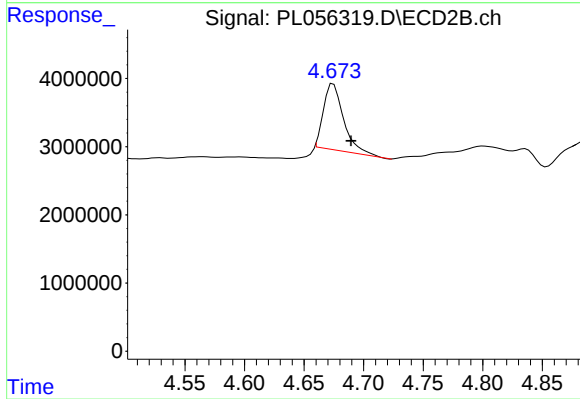

#3 gamma-BHC (Lindane)


R.T.: 4.675 min
Delta R.T.: -0.015 min
Response: 11427436
Conc: 2.79 ng/ml

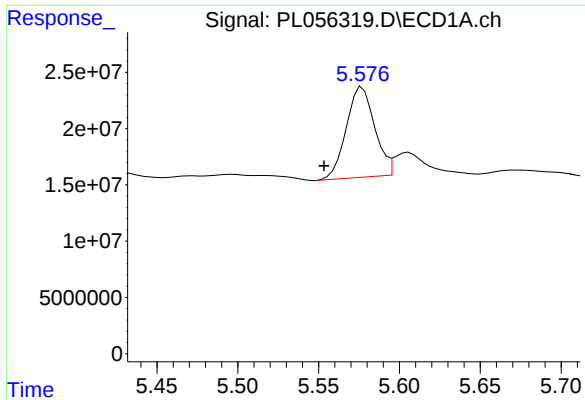

#9 Endosulfan I


R.T.: 5.577 min
Delta R.T.: 0.024 min
Response: 99252674
Conc: 6.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

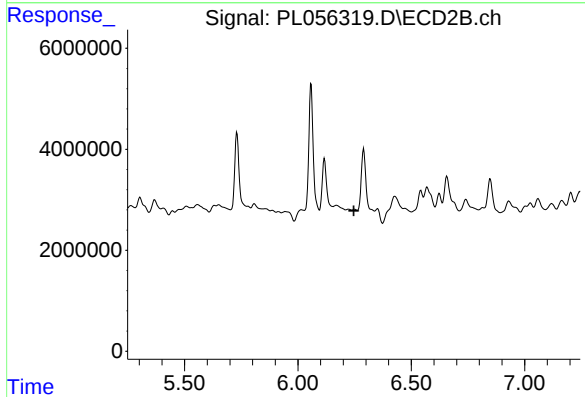


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

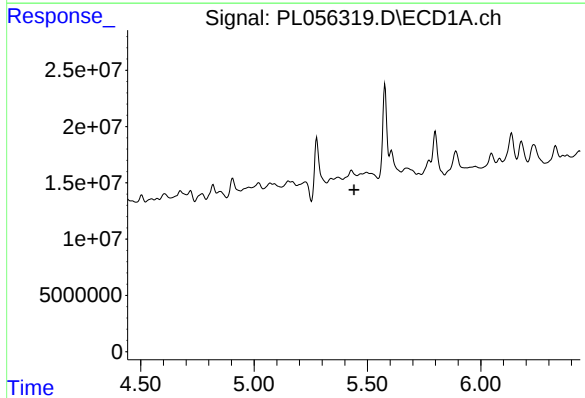


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.441 min
Response: 0
Conc: N.D.

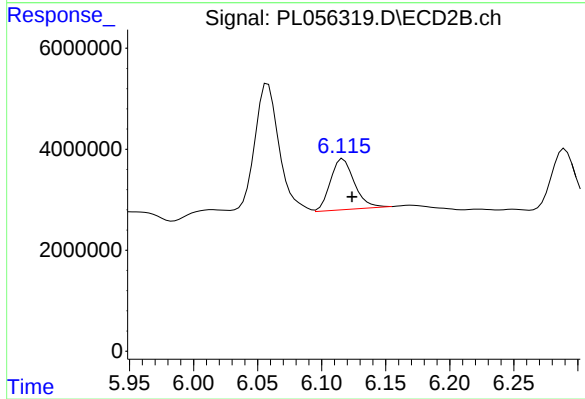

#10 gamma-Chlordane


R.T.: 6.117 min
Delta R.T.: -0.007 min
Response: 13065802
Conc: 4.11 ng/ml

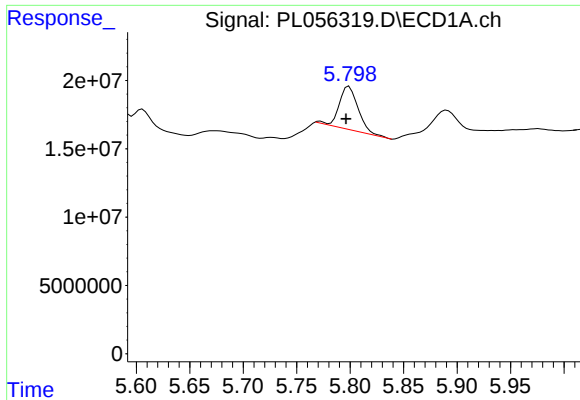

#13 Dieldrin


R.T.: 5.799 min
Delta R.T.: 0.003 min
Response: 37403628
Conc: 2.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

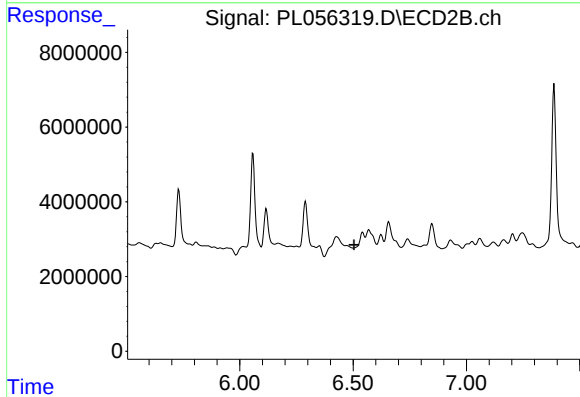


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.504 min
Response: 0
Conc: N.D.

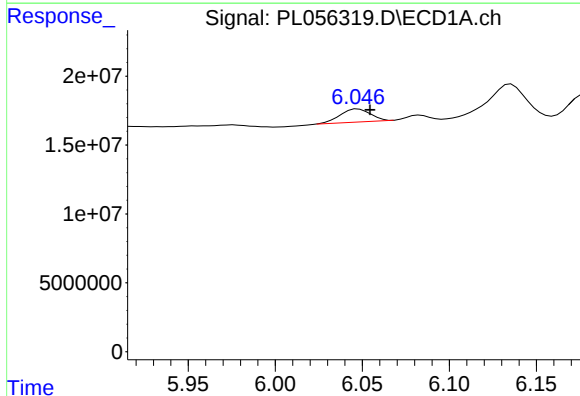


#14 Endrin

R.T.: 6.047 min
Delta R.T.: -0.007 min
Response: 11607153
Conc: 0.83 ng/ml

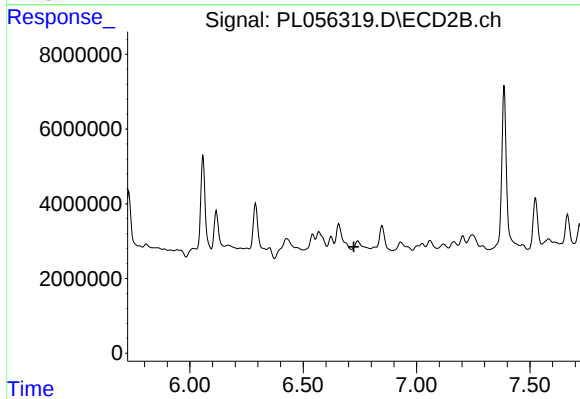

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.723 min
Response: 0
Conc: N.D.

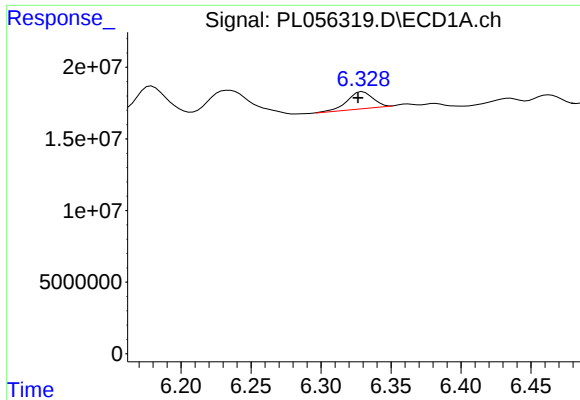

#15 Endosulfan II


R.T.: 6.330 min
Delta R.T.: 0.003 min
Response: 15102438
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

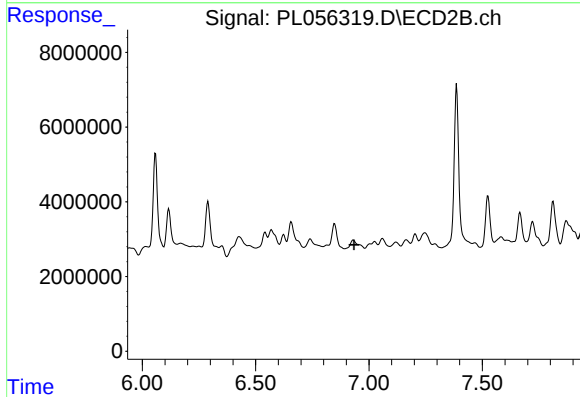


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.934 min
Response: 0
Conc: N.D.

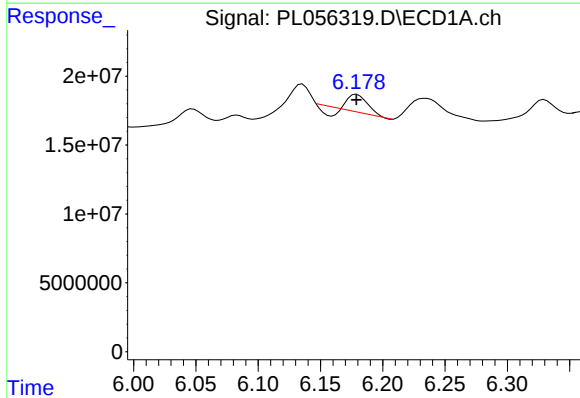


#16 4,4'-DDD

R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 10786360
Conc: 1.00 ng/ml

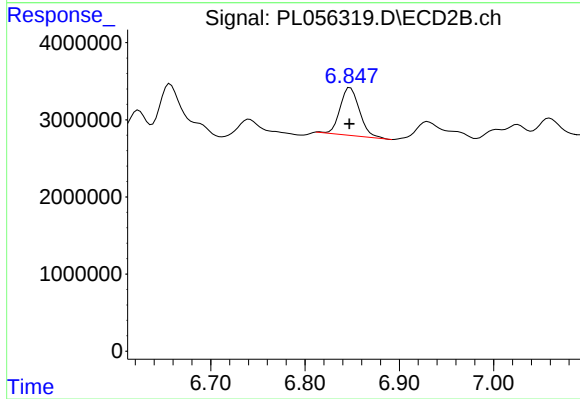

#16 4,4'-DDD


R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 8903056
Conc: 3.77 ng/ml

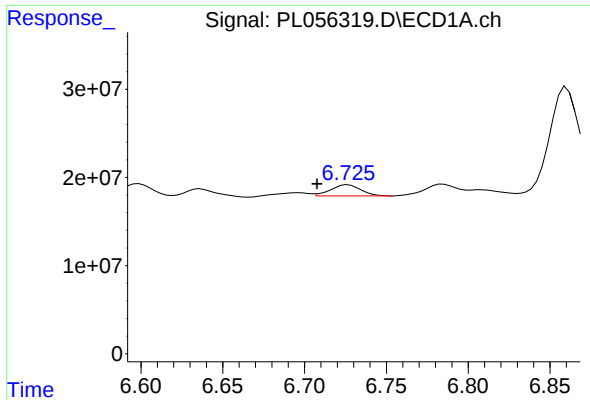

#19 Endosulfan Sulfate


R.T.: 6.727 min
Delta R.T.: 0.019 min
Response: 16134851
Conc: 1.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

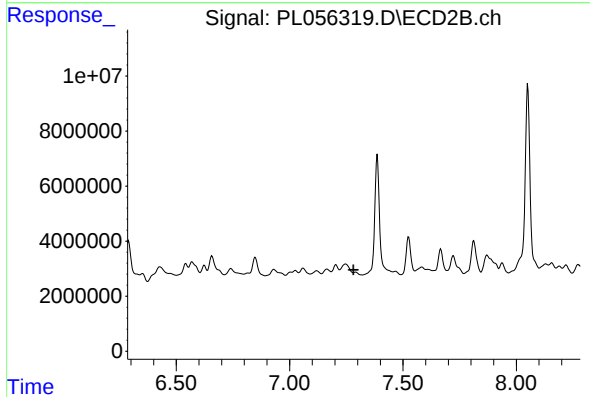


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.282 min
Response: 0
Conc: N.D.

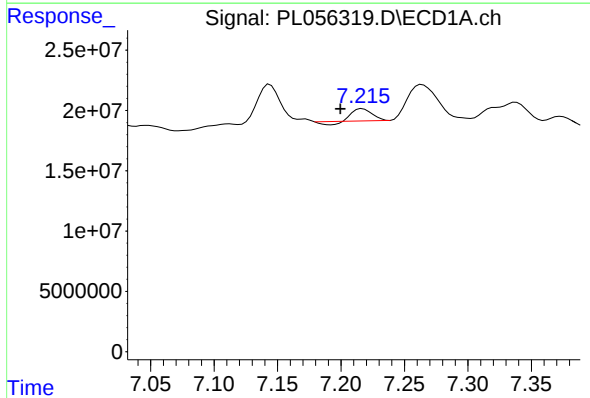


#21 Endrin ketone

R.T.: 7.217 min
Delta R.T.: 0.017 min
Response: 9583047
Conc: 0.73 ng/ml

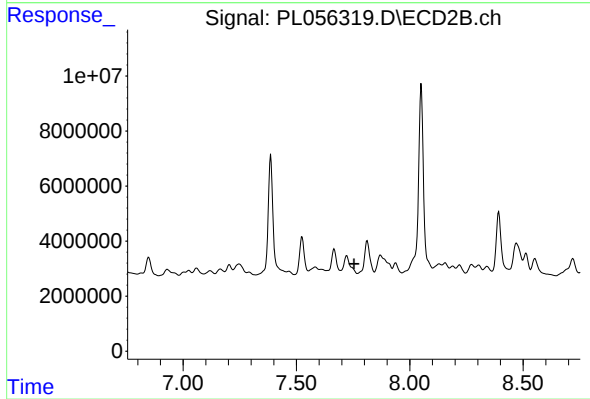

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.755 min
Response: 0
Conc: N.D.

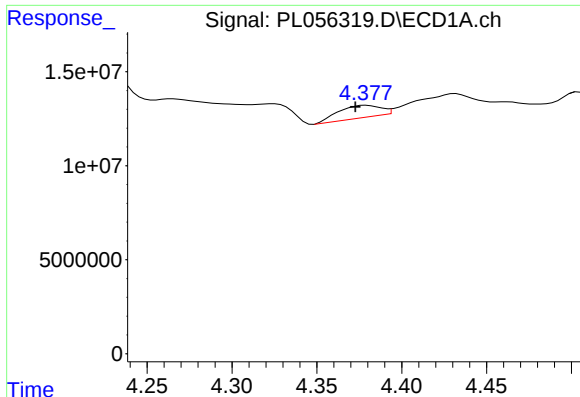

#23 Chlordane-1


R.T.: 4.379 min
Delta R.T.: 0.006 min
Response: 11282141
Conc: 29.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

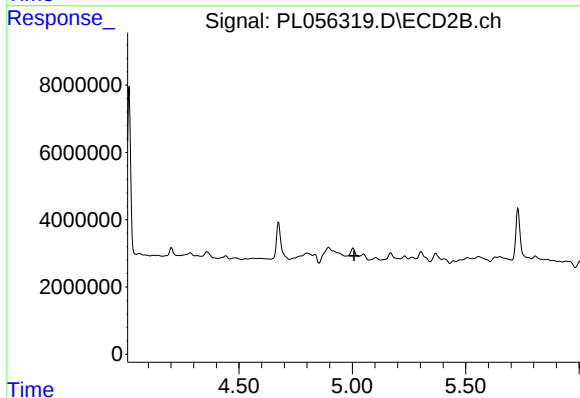


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

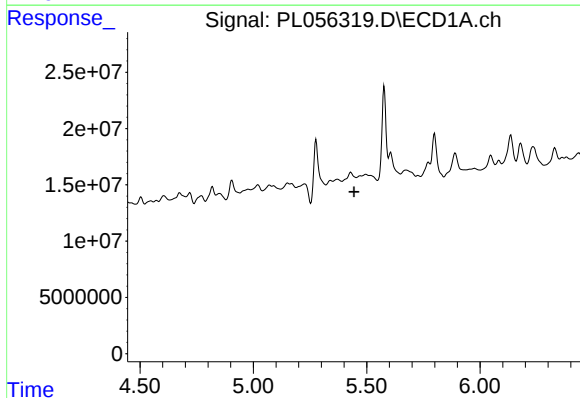


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.445 min
Response: 0
Conc: N.D.

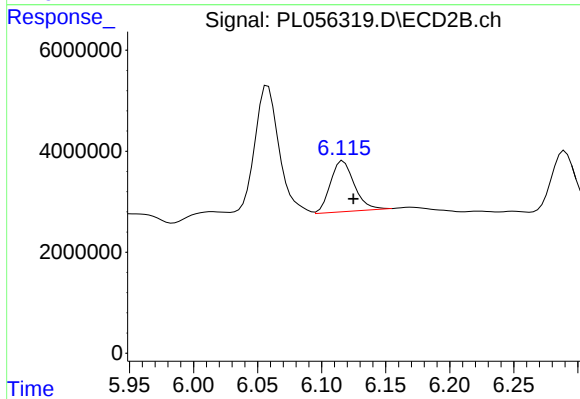

#25 Chlordane-3


R.T.: 6.117 min
Delta R.T.: -0.008 min
Response: 13065802
Conc: 34.76 ng/ml

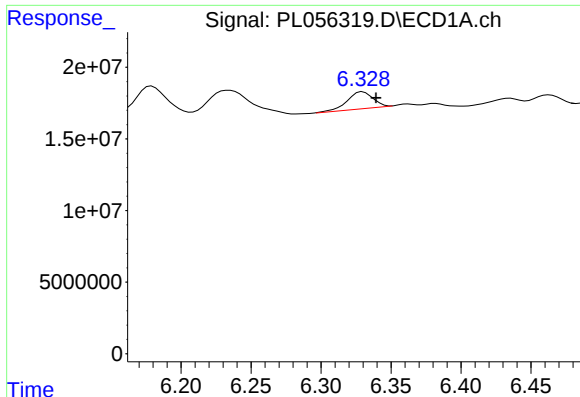

#27 Chlordane-5


R.T.: 6.330 min
Delta R.T.: -0.010 min
Response: 15102438
Conc: 36.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-A

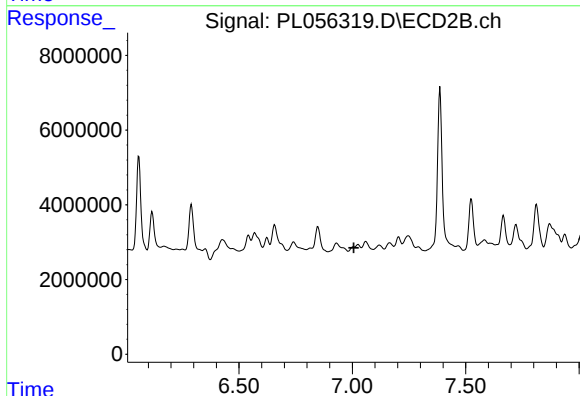


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

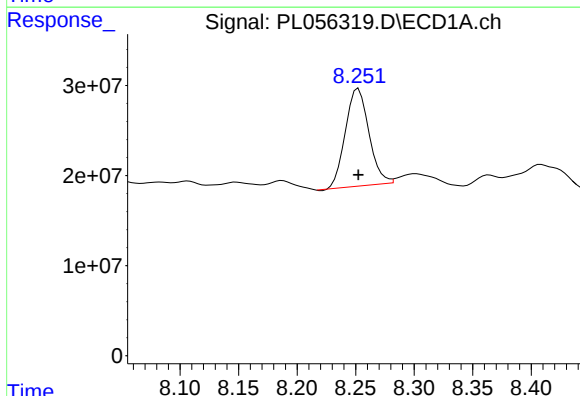

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 151381723
Conc: 14.38 ng/ml

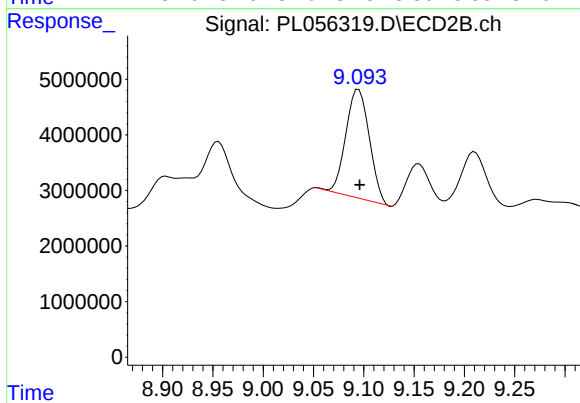

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.001 min
Response: 31870524
Conc: 14.09 ng/ml