

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 13:03
 Operator : AR\AJ
 Sample : PB142491BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:29:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.491	10263999	34371650	18.487	21.163
28)	SA Decachlor...	10.319	11.386	15920115	29649088	17.919	18.376
Target Compounds							
2)	A alpha-BHC	5.280	0.000	139119	0	0.180	N.D. #
5)	MB Aldrin	0.000	7.517f	0	57548	N.D.	0.026 #
7)	B delta-BHC	0.000	7.017f	0	1183644	N.D.	0.481 #
9)	A Endosulfan I	0.000	8.358	0	109553	N.D.	0.061 #
10)	B gamma-Chl...	0.000	8.226	0	228066	N.D.	0.113 #
15)	B Endosulfa...	0.000	9.148f	0	906844	N.D.	0.529 #
17)	MA 4,4'-DDT	0.000	9.337f	0	30697	N.D.	0.019 #
20)	A Methoxychlor	0.000	9.853	0	470766	N.D.	0.568 #
22)	Mirex	0.000	10.485f	0	34141	N.D.	0.027 #
25)	Chlordane-3	0.000	8.226	0	228066	N.D.	0.821 #
27)	Chlordane-5	0.000	9.175f	0	47218	N.D.	0.774 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 13:03
Operator : AR\AJ
Sample : PB142491BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:29:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

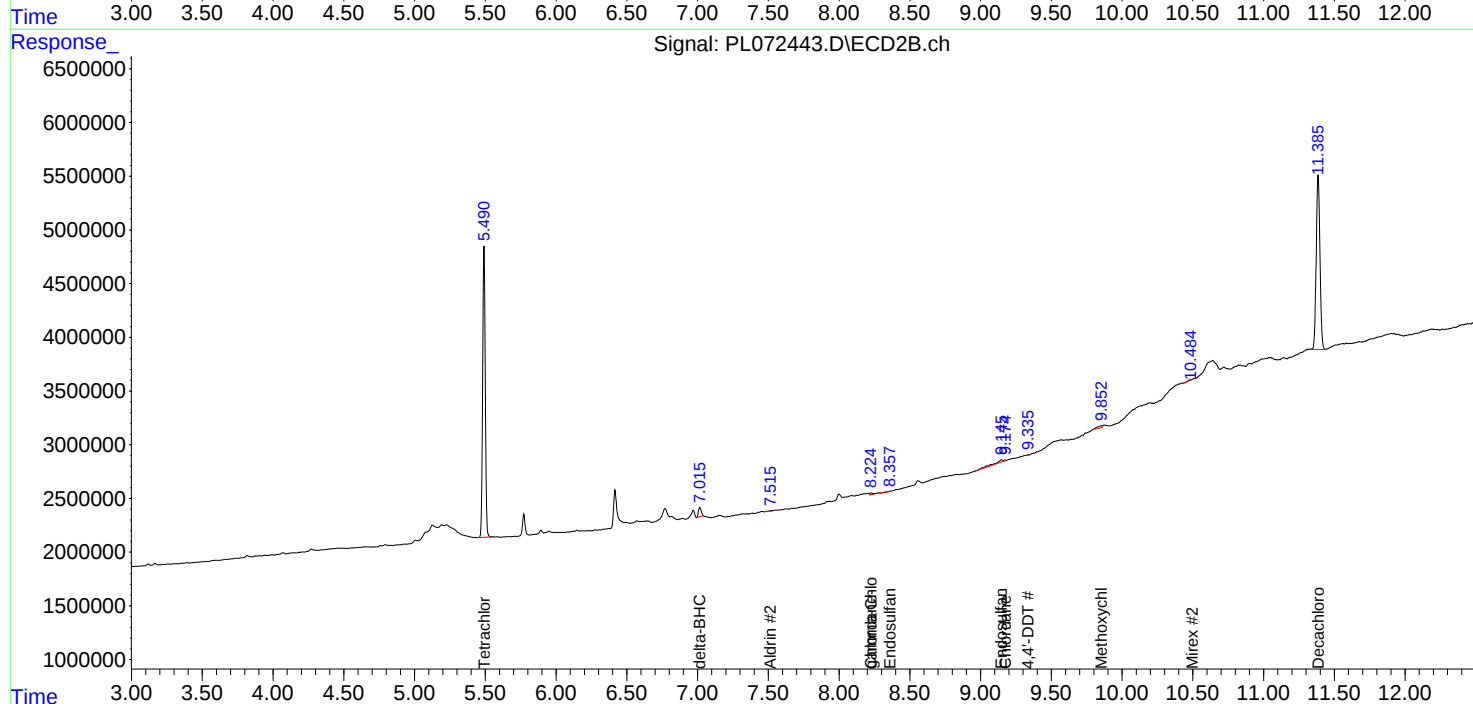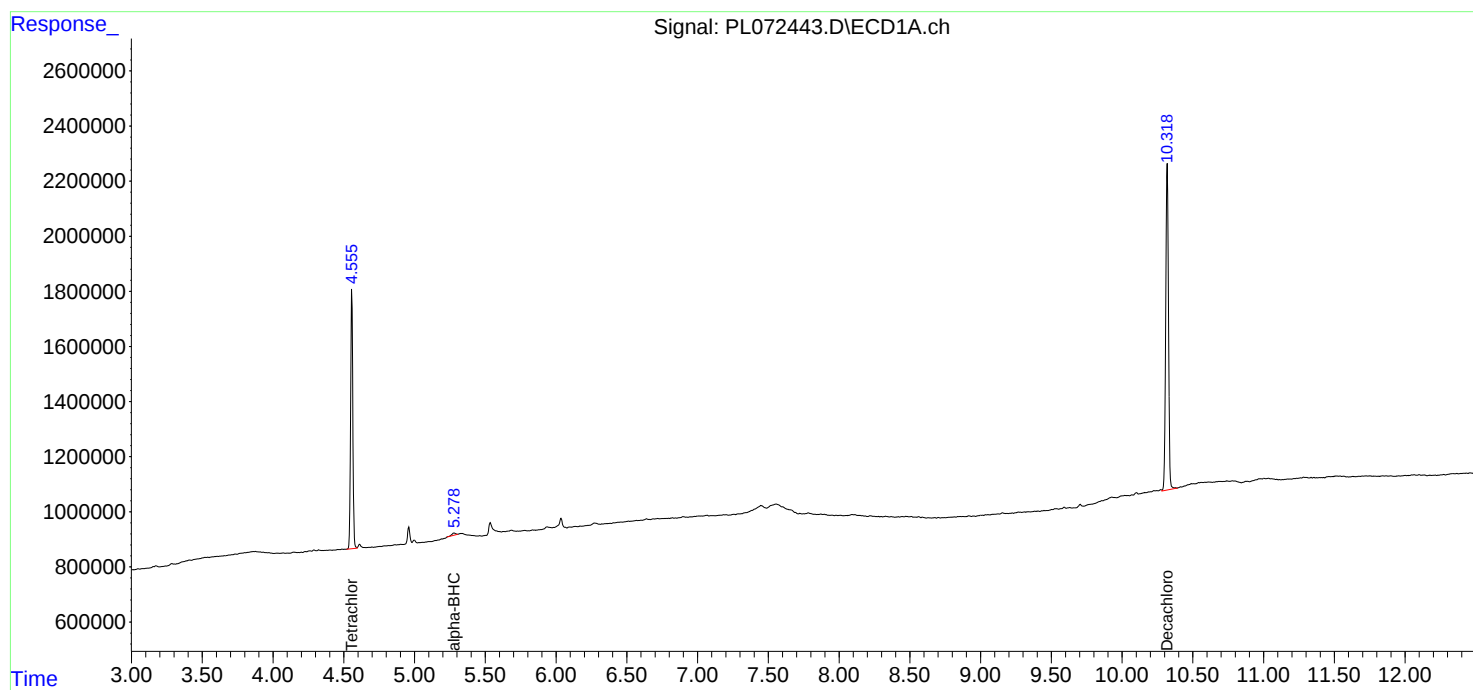


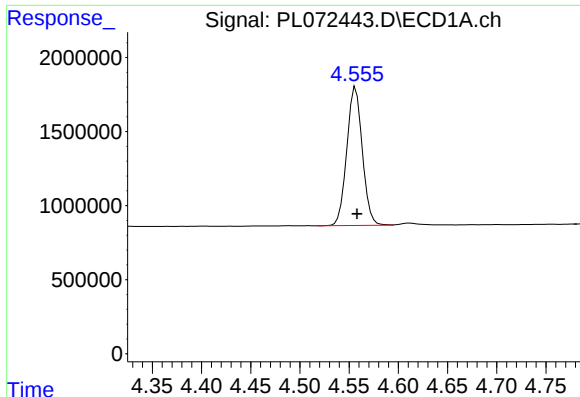

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: -0.001 min
Response: 10263999
Conc: 18.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

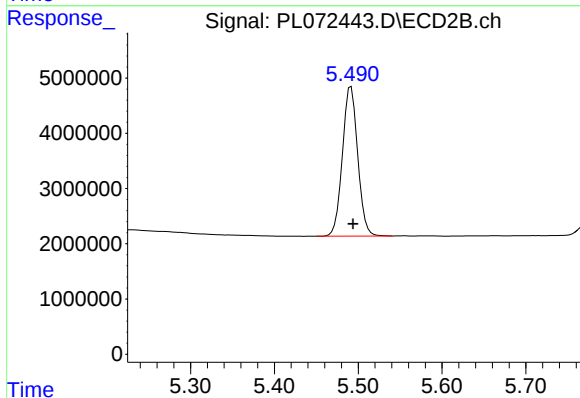


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 34371650
Conc: 21.16 ng/ml

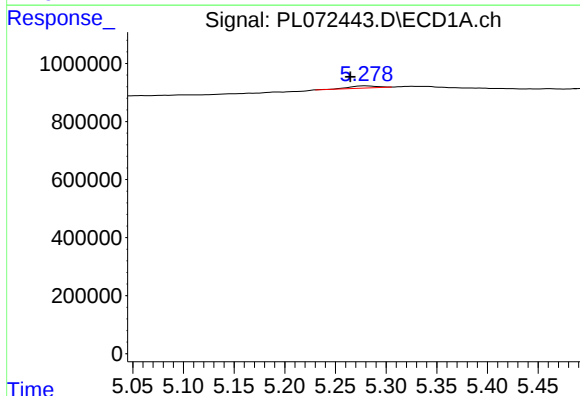


#2 alpha-BHC

R.T.: 5.280 min
Delta R.T.: 0.015 min
Response: 139119
Conc: 0.18 ng/ml

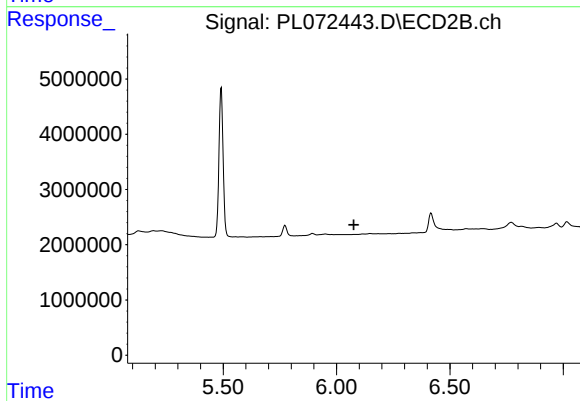

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

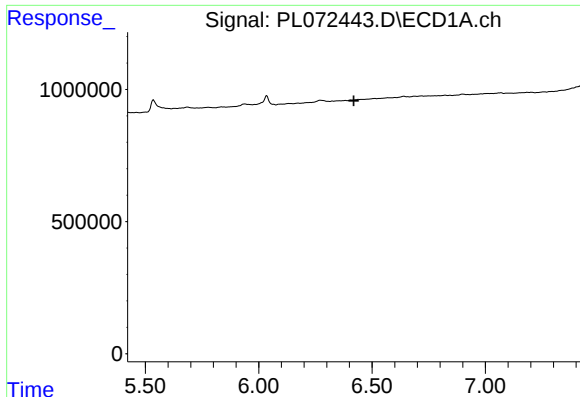

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

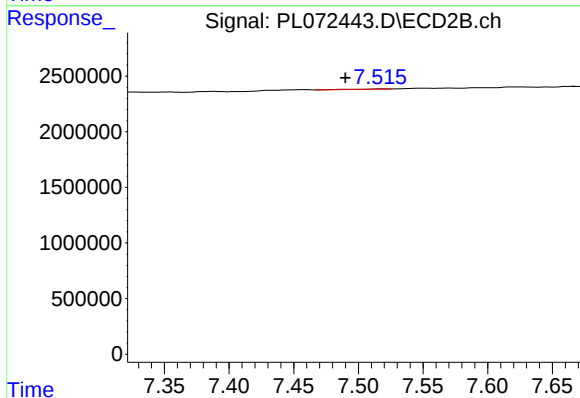


#5 Aldrin

R.T.: 7.517 min
Delta R.T.: 0.027 min
Response: 57548
Conc: 0.03 ng/ml

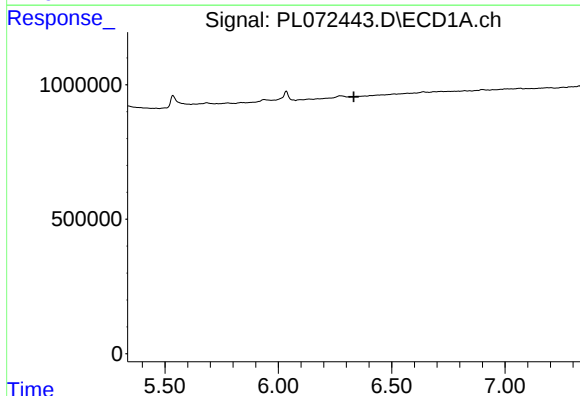


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

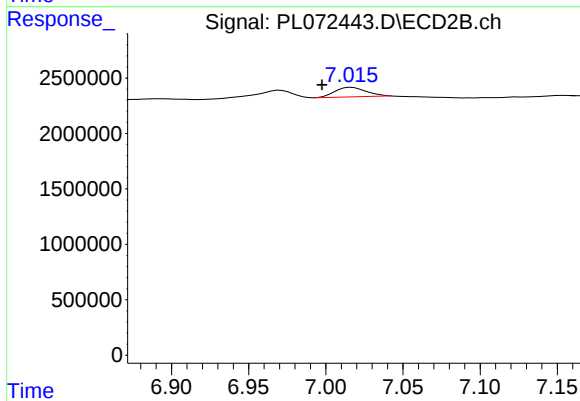

#7 delta-BHC


R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 1183644
Conc: 0.48 ng/ml

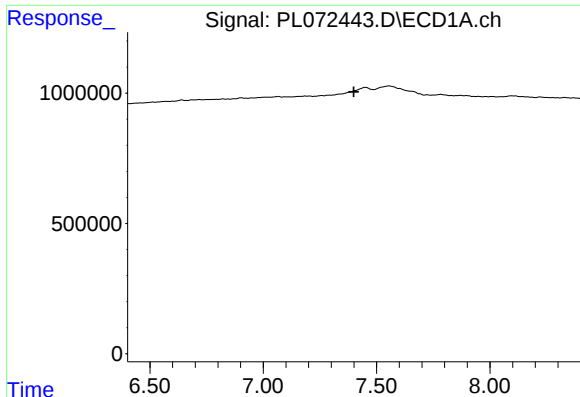

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

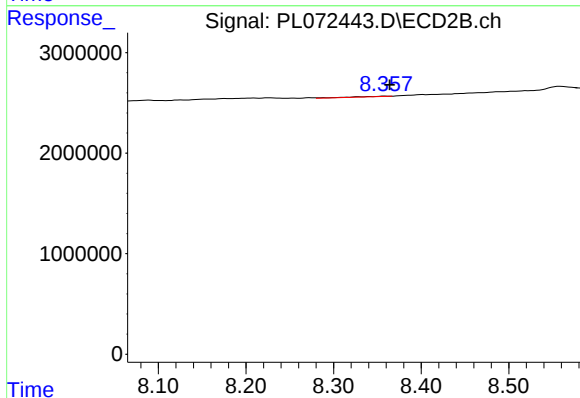


#9 Endosulfan I

R.T.: 8.358 min
Delta R.T.: -0.006 min
Response: 109553
Conc: 0.06 ng/ml

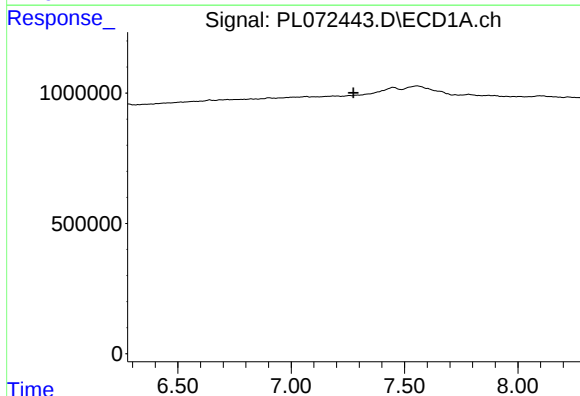


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

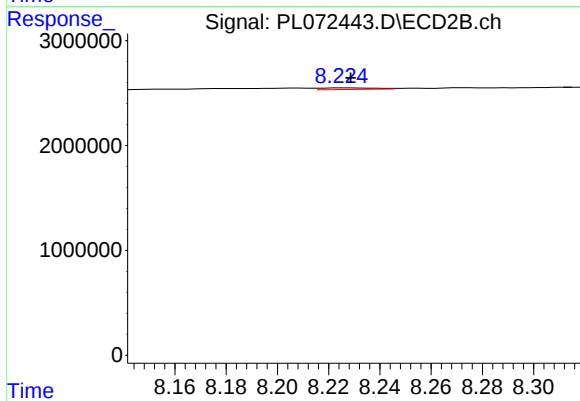

#10 gamma-Chlordane


R.T.: 8.226 min
Delta R.T.: -0.002 min
Response: 228066
Conc: 0.11 ng/ml

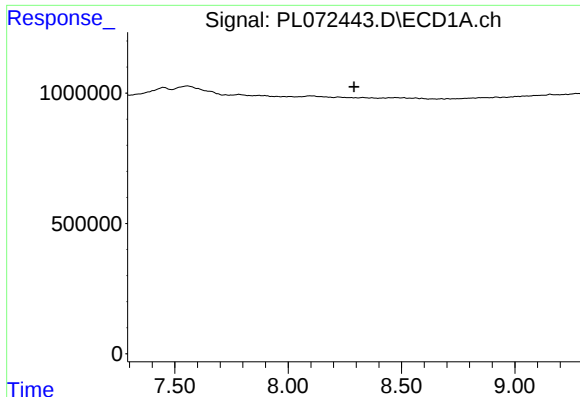

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

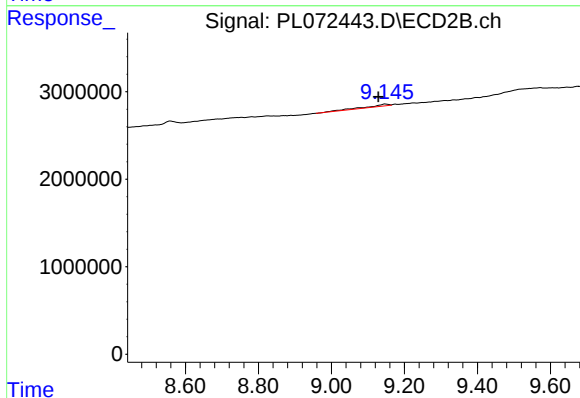


#15 Endosulfan II

R.T.: 9.148 min
Delta R.T.: 0.019 min
Response: 906844
Conc: 0.53 ng/ml

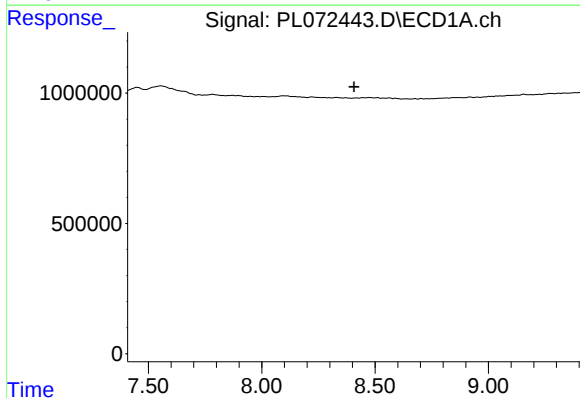


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

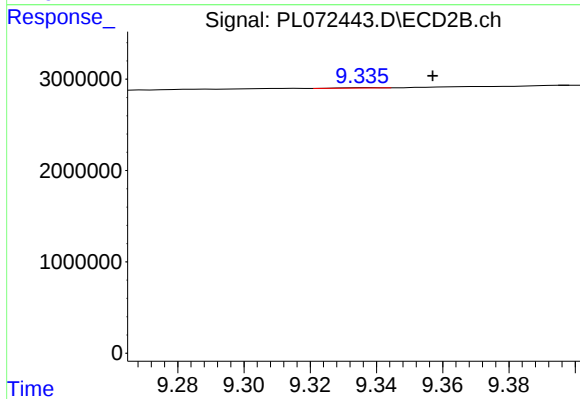

#17 4,4'-DDT


R.T.: 9.337 min
Delta R.T.: -0.020 min
Response: 30697
Conc: 0.02 ng/ml

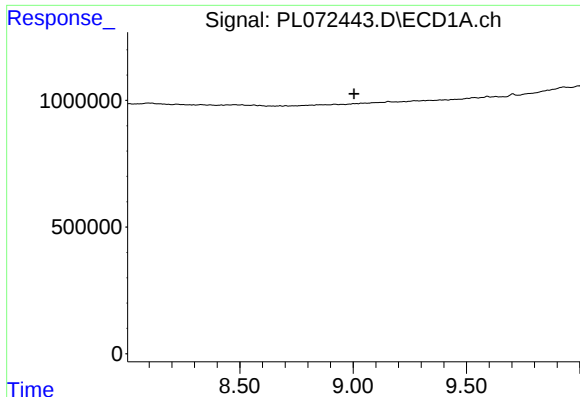

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

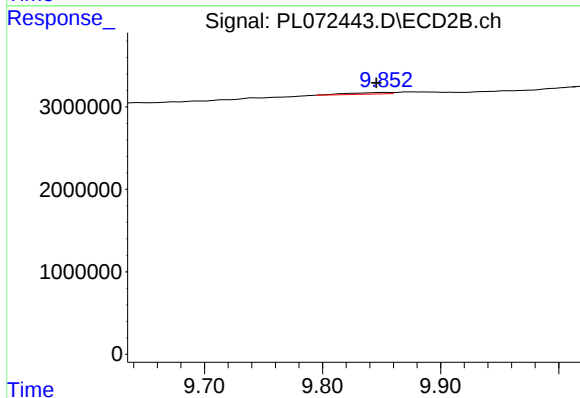


#20 Methoxychlor

R.T.: 9.853 min
Delta R.T.: 0.008 min
Response: 470766
Conc: 0.57 ng/ml

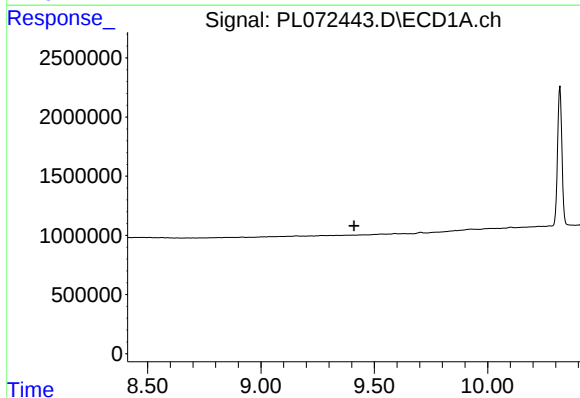


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.410 min
Response: 0
Conc: N.D.

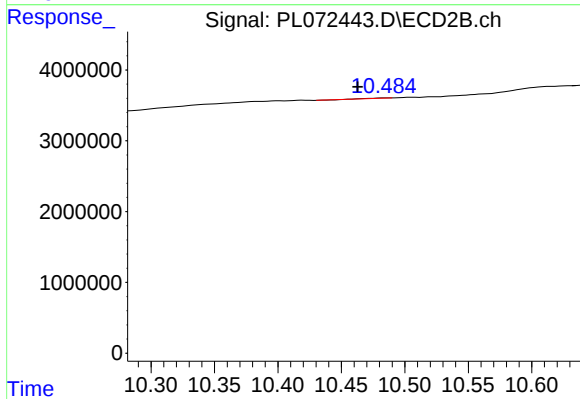

#22 Mirex


R.T.: 10.485 min
Delta R.T.: 0.022 min
Response: 34141
Conc: 0.03 ng/ml

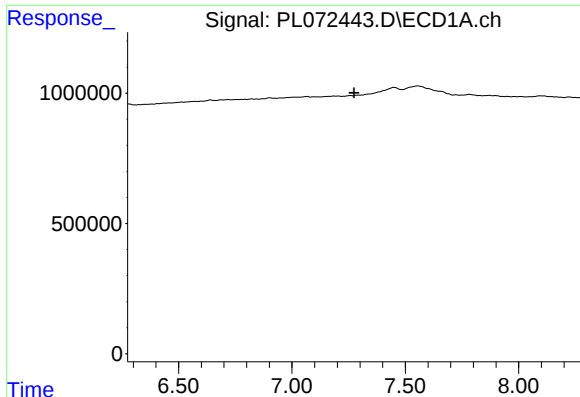

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

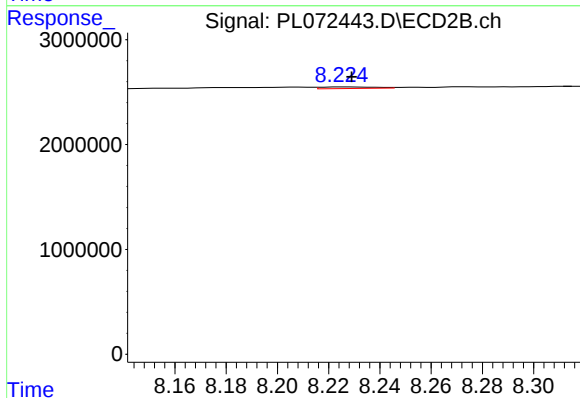


#25 Chlordane-3

R.T.: 8.226 min
Delta R.T.: -0.003 min
Response: 228066
Conc: 0.82 ng/ml

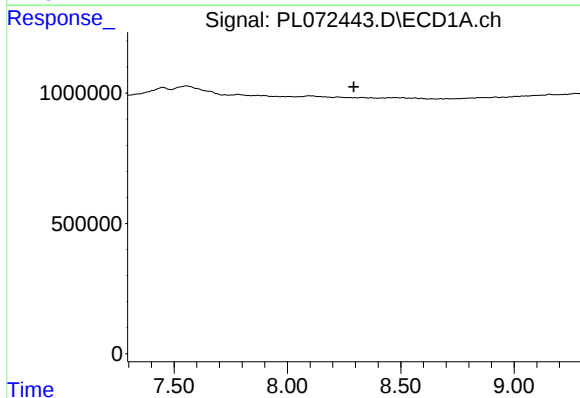


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

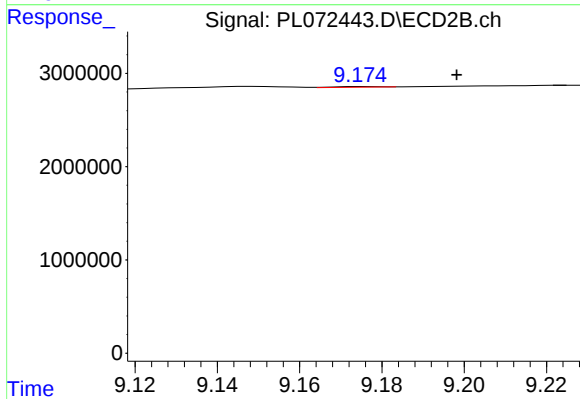

#27 Chlordane-5


R.T.: 9.175 min
Delta R.T.: -0.023 min
Response: 47218
Conc: 0.77 ng/ml

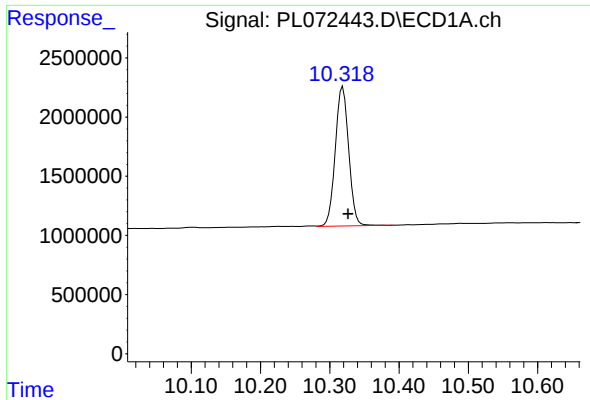

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.008 min
Response: 15920115
Conc: 17.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

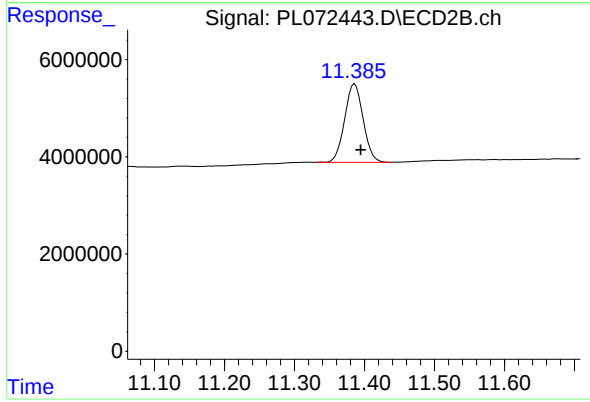

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: -0.009 min
Response: 29649088
Conc: 18.38 ng/ml