

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 13:20
 Operator : AR\AJ
 Sample : PB142420TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:29:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.491	9594274	31790423	17.281	19.574
28)	SA Decachlor...	10.317	11.385	14963034	27578588	16.842	17.092
Target Compounds							
2)	A alpha-BHC	5.280f	0.000	226323	0	0.293	N.D. #
7)	B delta-BHC	0.000	7.015f	0	1346237	N.D.	0.547 #
9)	A Endosulfan I	0.000	8.345f	0	68114	N.D.	0.038 #
10)	B gamma-Chl...	0.000	8.232	0	199782	N.D.	0.099 #
15)	B Endosulfa...	0.000	9.147f	0	966322	N.D.	0.563 #
17)	MA 4,4'-DDT	0.000	9.339f	0	36790	N.D.	0.023 #
23)	Chlordane-1	0.000	6.892f	0	89617	N.D.	1.373 #
25)	Chlordane-3	0.000	8.232	0	199782	N.D.	0.719 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072444.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 13:20
Operator : AR\AJ
Sample : PB142420TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:29:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

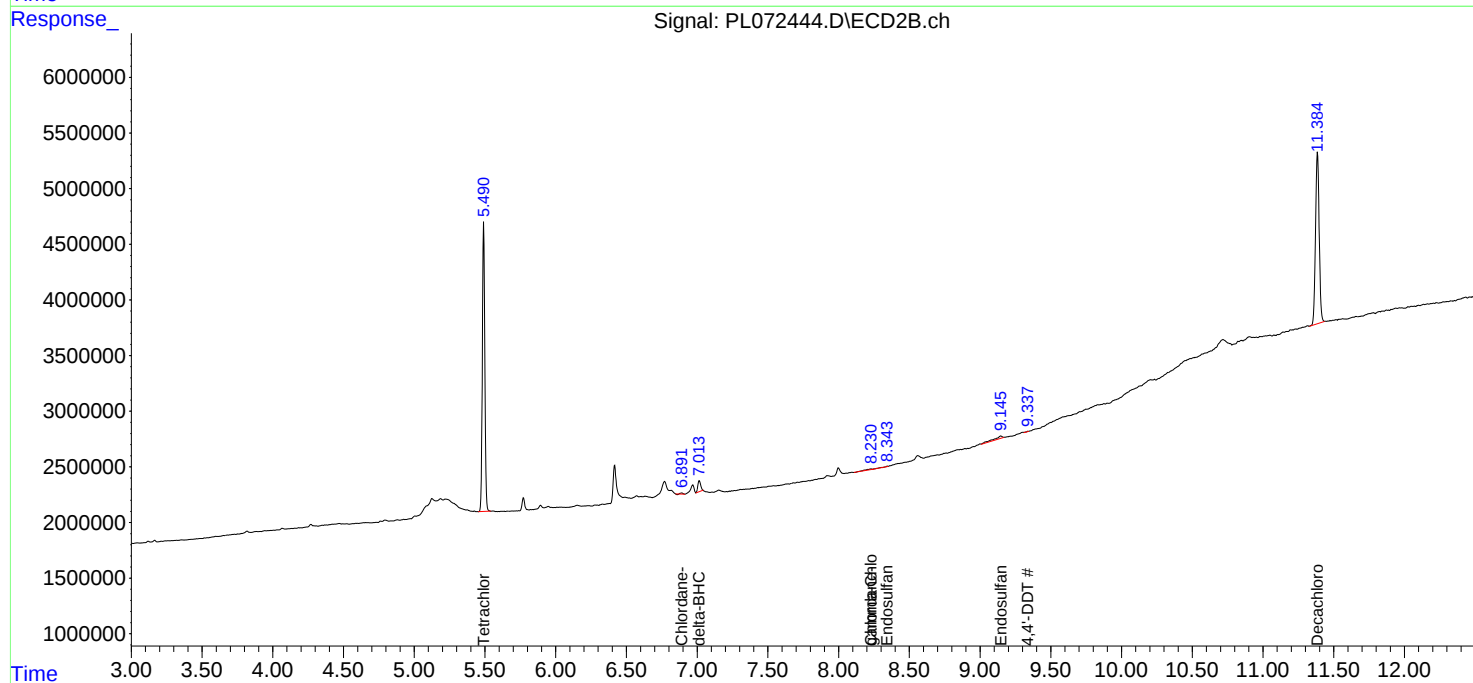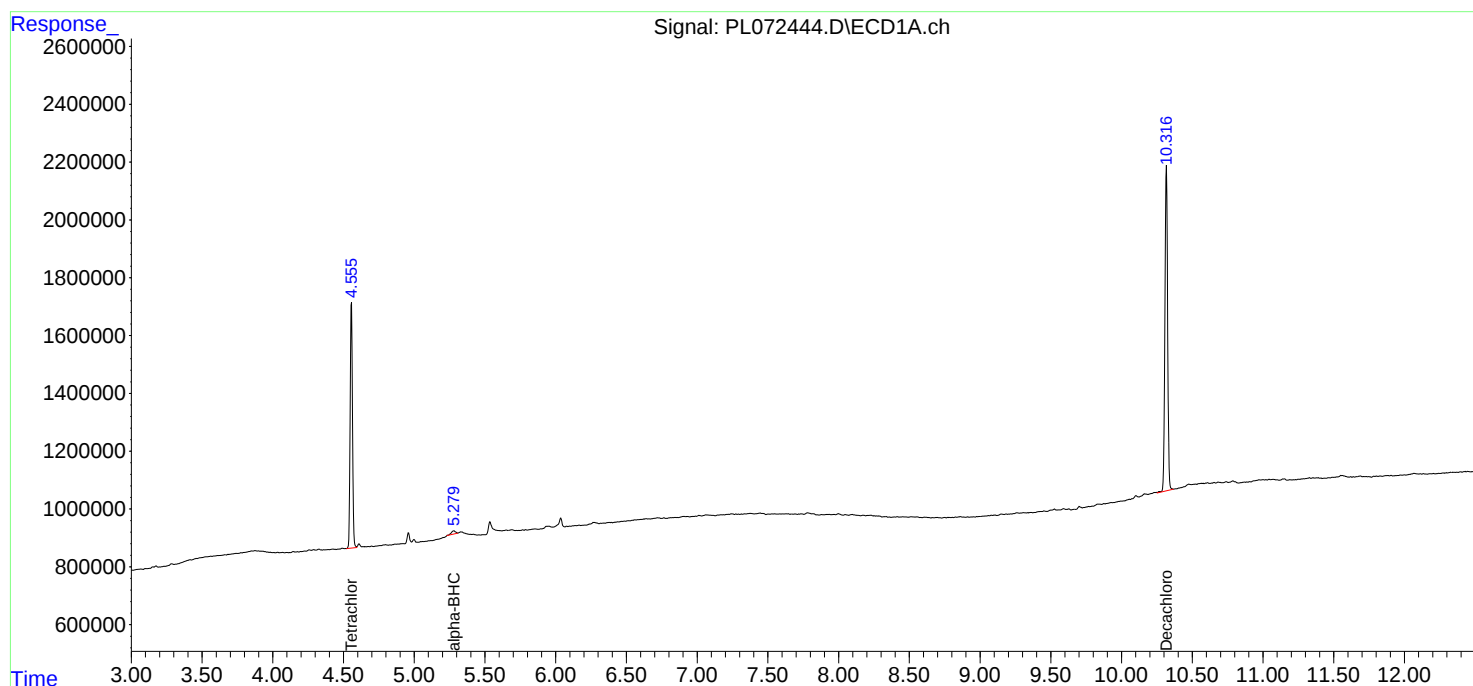


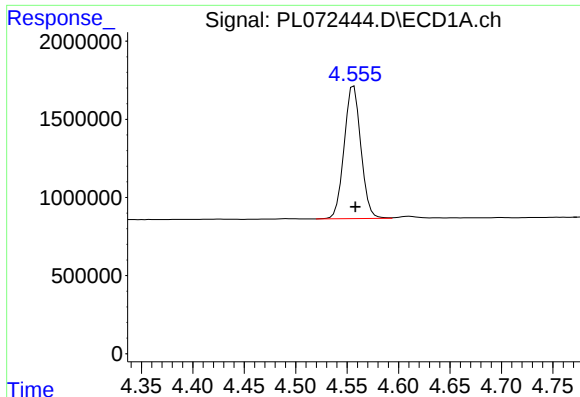

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 9594274
Conc: 17.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

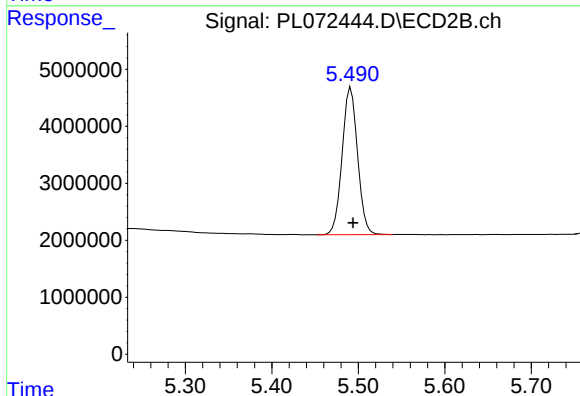


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 31790423
Conc: 19.57 ng/ml

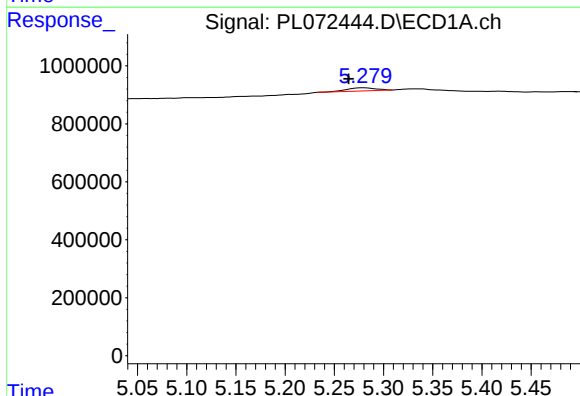


#2 alpha-BHC

R.T.: 5.280 min
Delta R.T.: 0.016 min
Response: 226323
Conc: 0.29 ng/ml

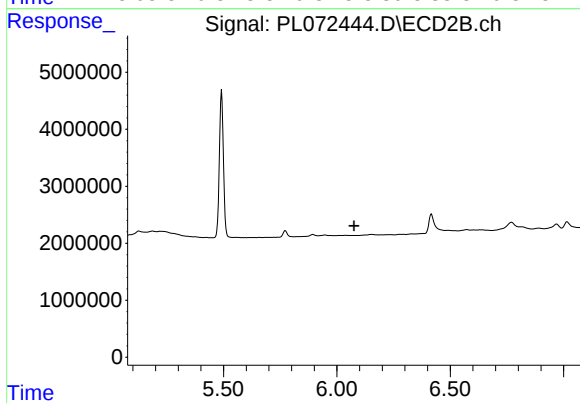

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

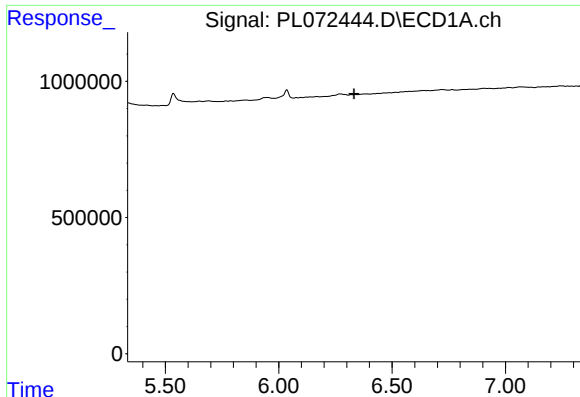

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

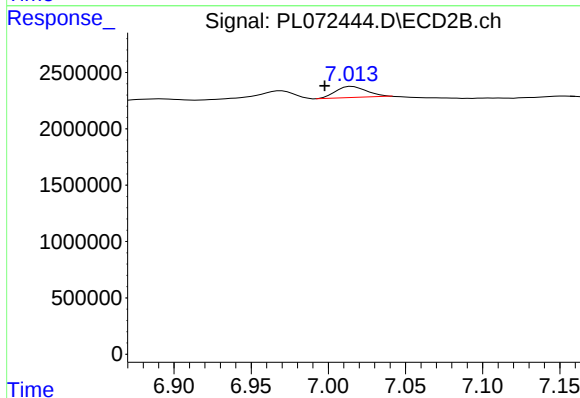


#7 delta-BHC

R.T.: 7.015 min
Delta R.T.: 0.018 min
Response: 1346237
Conc: 0.55 ng/ml

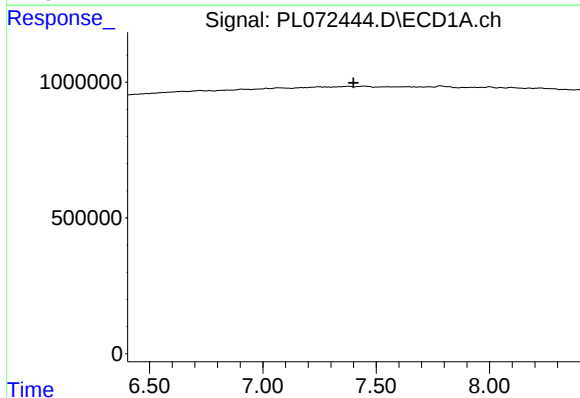


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

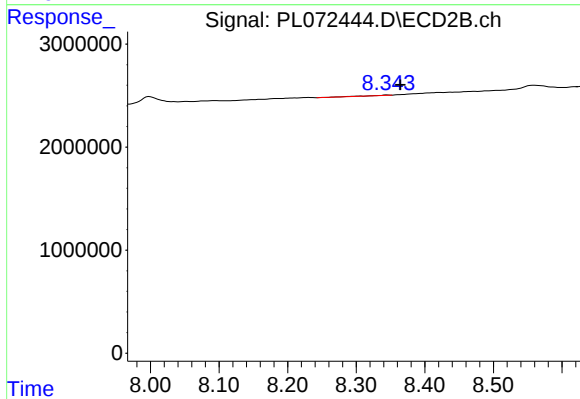

#9 Endosulfan I


R.T.: 8.345 min
Delta R.T.: -0.019 min
Response: 68114
Conc: 0.04 ng/ml

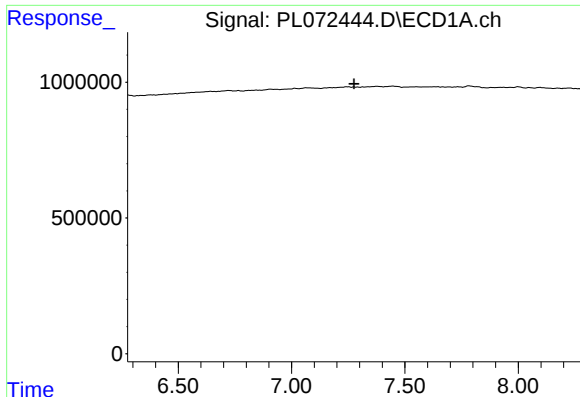

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

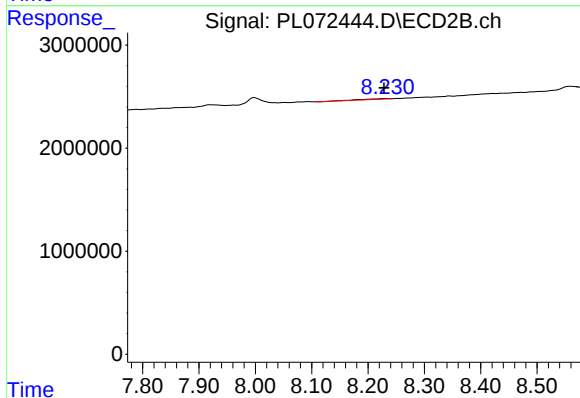


#10 gamma-Chlordane

R.T.: 8.232 min
Delta R.T.: 0.003 min
Response: 199782
Conc: 0.10 ng/ml

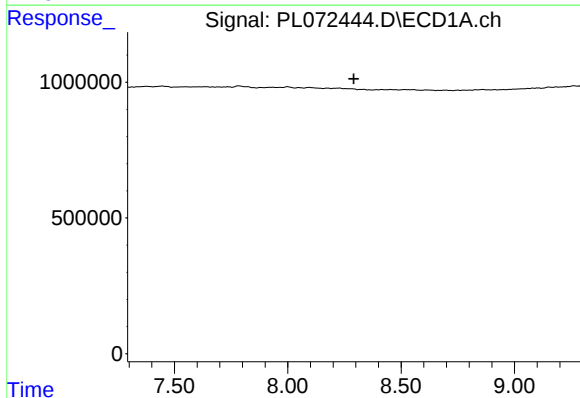


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

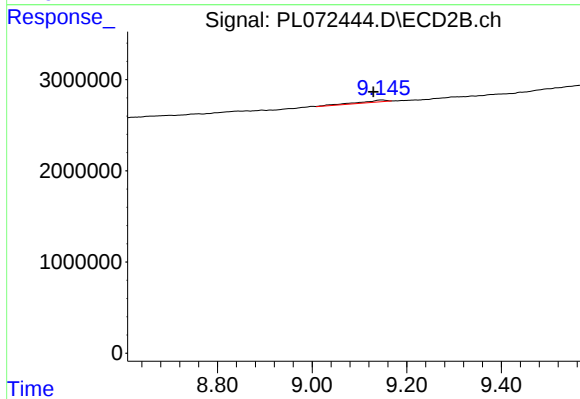

#15 Endosulfan II


R.T.: 9.147 min
Delta R.T.: 0.018 min
Response: 966322
Conc: 0.56 ng/ml

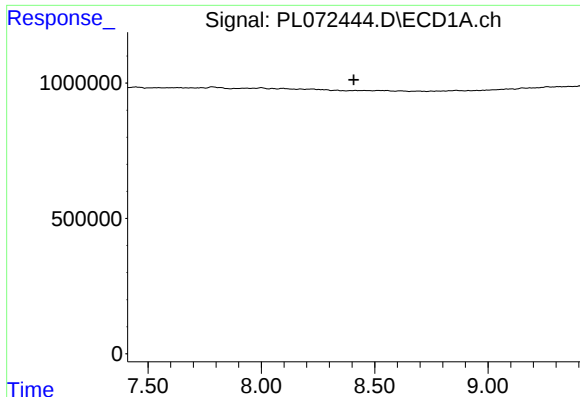

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

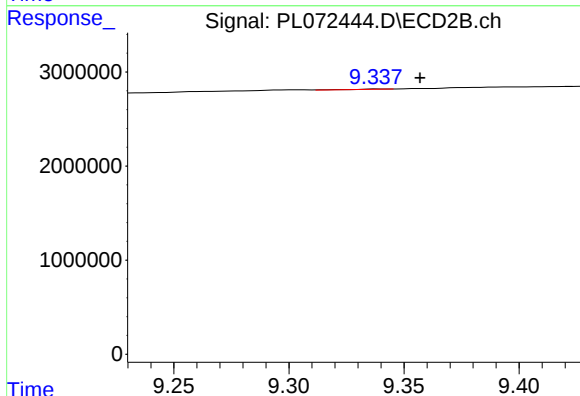


#17 4,4'-DDT

R.T.: 9.339 min
Delta R.T.: -0.018 min
Response: 36790
Conc: 0.02 ng/ml

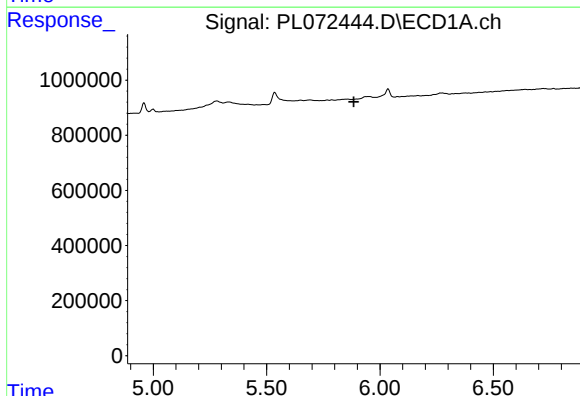


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.884 min
Response: 0
Conc: N.D.

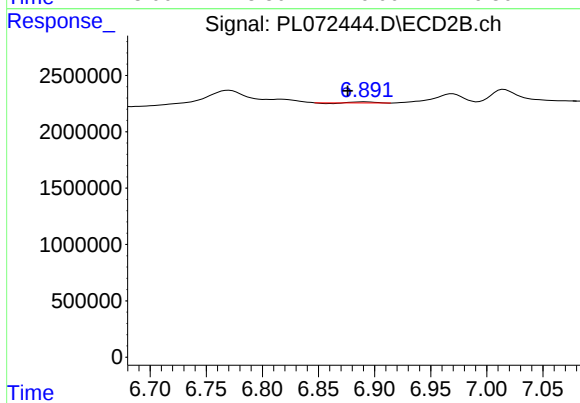

#23 Chlordane-1


R.T.: 6.892 min
Delta R.T.: 0.016 min
Response: 89617
Conc: 1.37 ng/ml

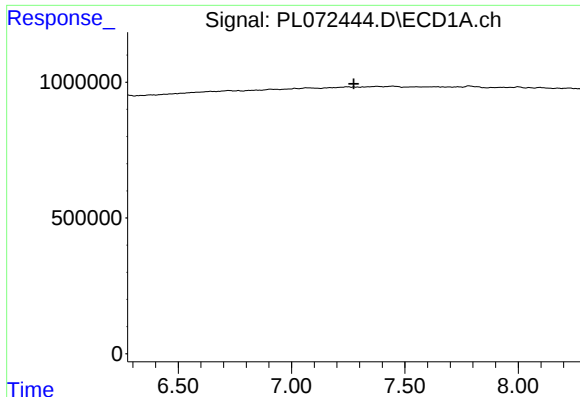

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

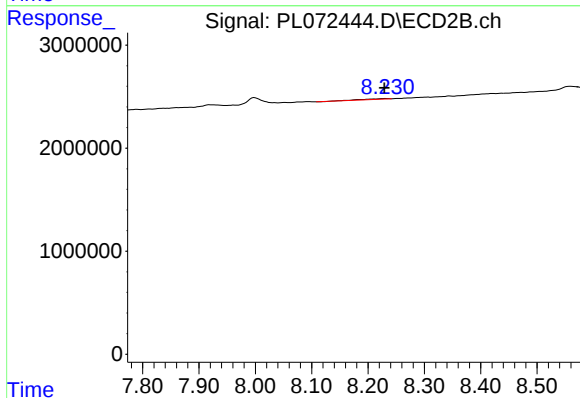


#25 Chlordane-3

R.T.: 8.232 min
Delta R.T.: 0.003 min
Response: 199782
Conc: 0.72 ng/ml

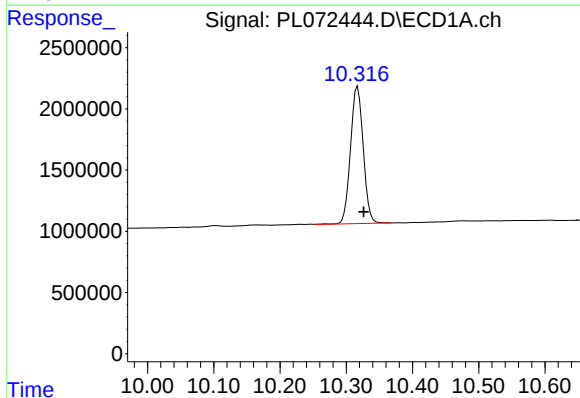

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.009 min
Response: 14963034
Conc: 16.84 ng/ml

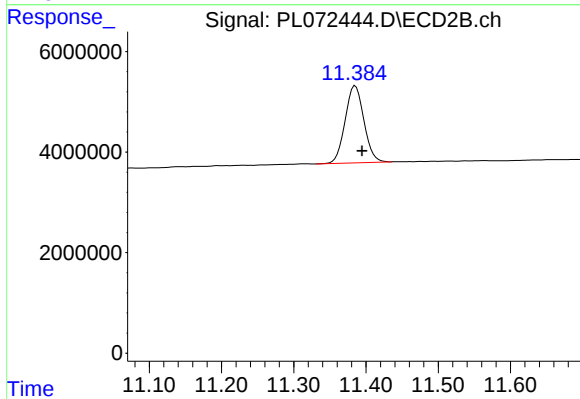

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.009 min
Response: 27578588
Conc: 17.09 ng/ml