

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 14:47
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:31:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.492	10230210	34386556	18.427	21.172
28)	SA Decachlor...	10.318	11.387	15959846	29630030	17.964	18.364
Target Compounds							
7)	B delta-BHC	0.000	7.018f	0	322358	N.D.	0.131 #
9)	A Endosulfan I	0.000	8.356	0	371629	N.D.	0.205 #
10)	B gamma-Chl...	0.000	8.231	0	441826	N.D.	0.219 #
12)	B 4,4'-DDE	0.000	8.509	0	17764	N.D.	0.009 #
13)	MA Dieldrin	0.000	8.649	0	38424	N.D.	0.020 #
15)	B Endosulfa...	0.000	9.145f	0	685147	N.D.	0.400 #
16)	A 4,4'-DDD	0.000	9.063f	0	467472	N.D.	0.327 #
20)	A Methoxychlor	0.000	9.856	0	59714	N.D.	0.072 #
25)	Chlordane-3	0.000	8.231	0	441826	N.D.	1.590 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 14:47
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:31:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

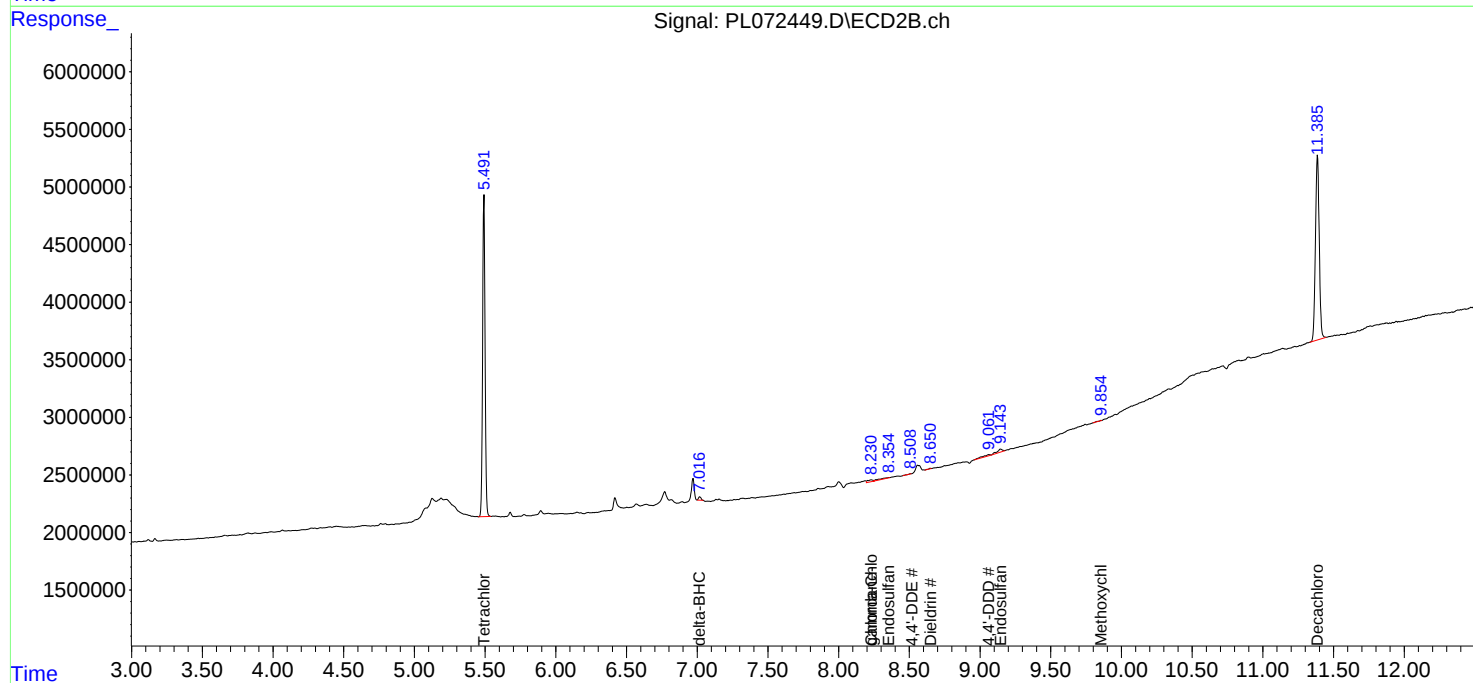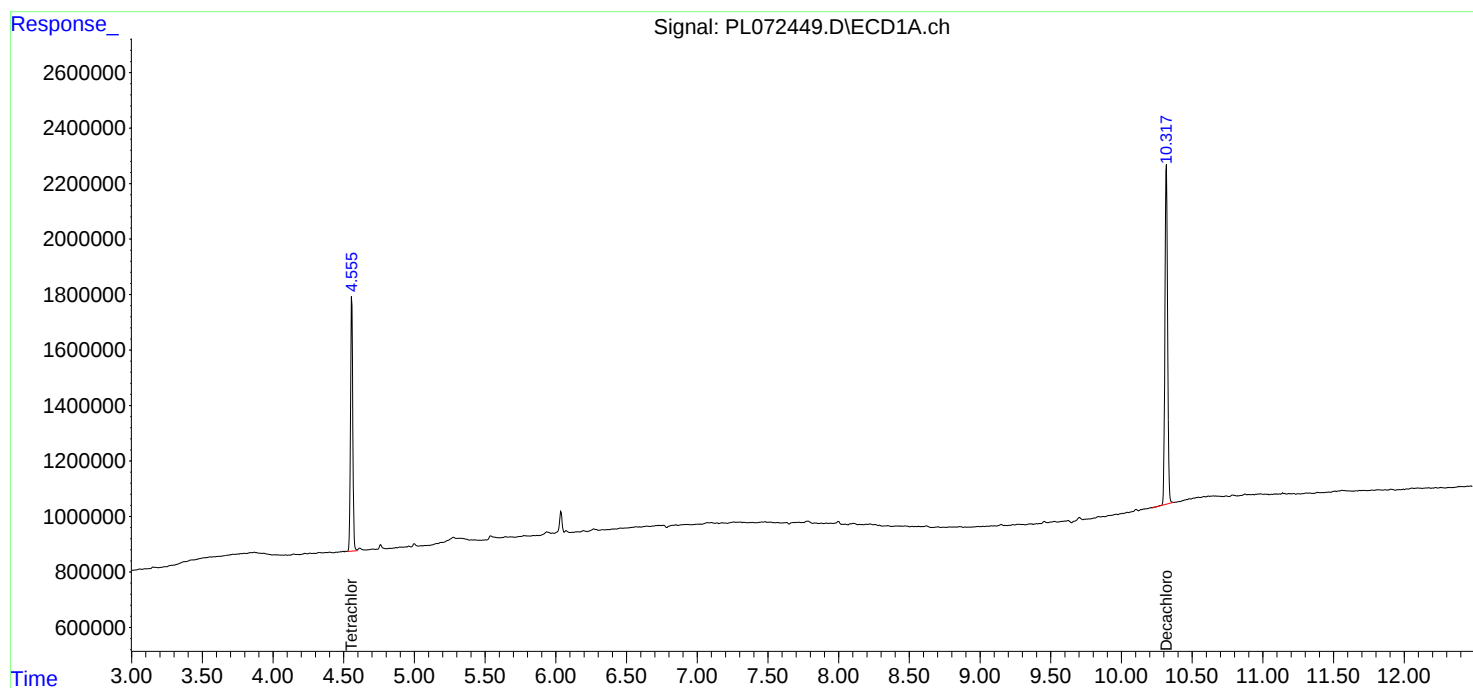


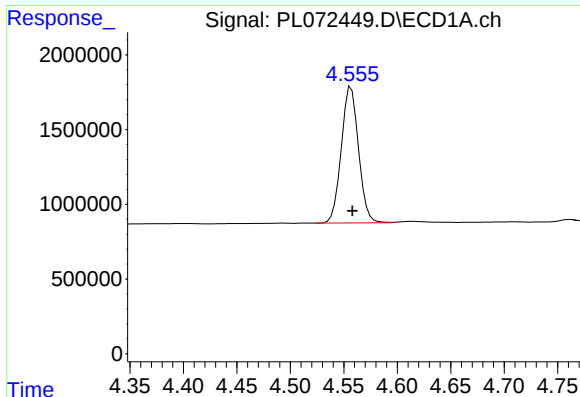

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: -0.001 min
Response: 10230210
Conc: 18.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

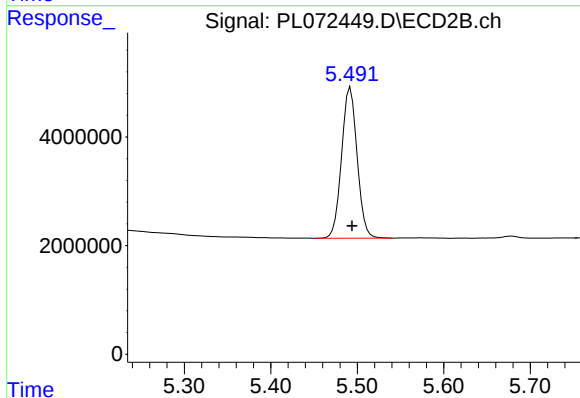


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 34386556
Conc: 21.17 ng/ml

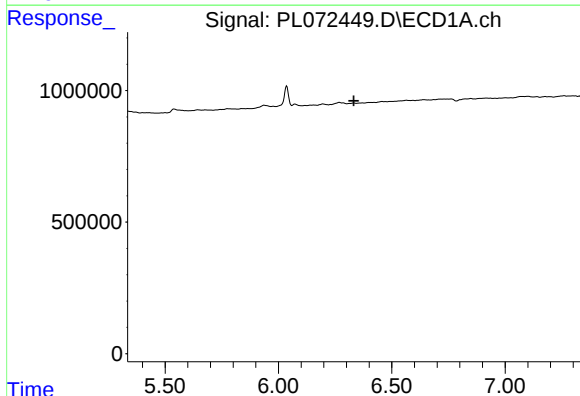


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

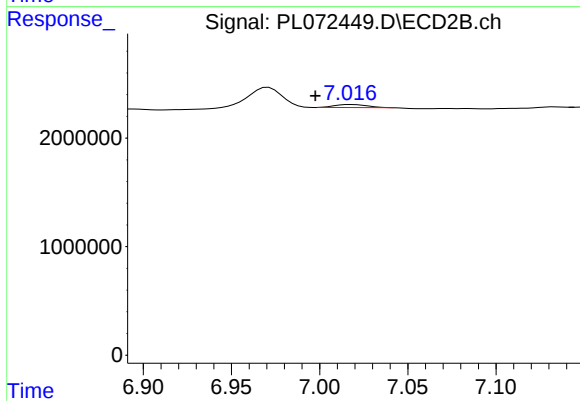

#7 delta-BHC


R.T.: 7.018 min
Delta R.T.: 0.020 min
Response: 322358
Conc: 0.13 ng/ml

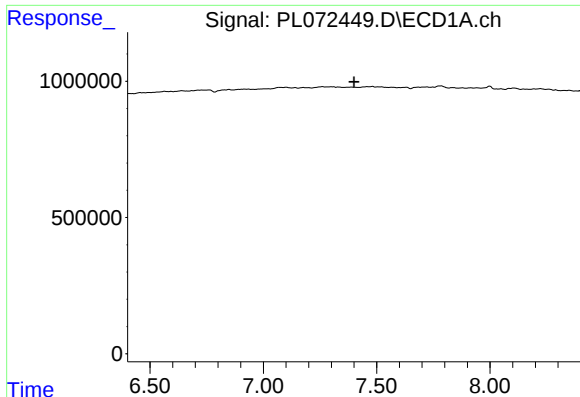

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

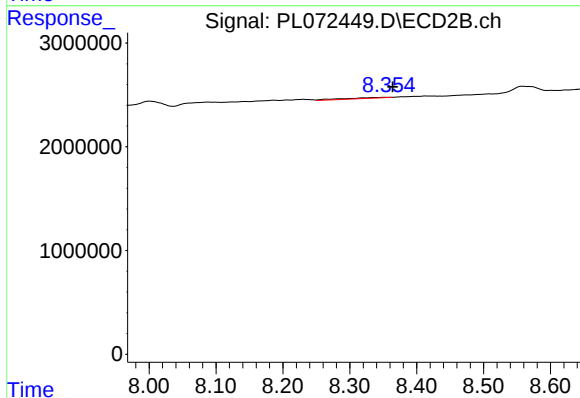


#9 Endosulfan I

R.T.: 8.356 min
Delta R.T.: -0.008 min
Response: 371629
Conc: 0.21 ng/ml

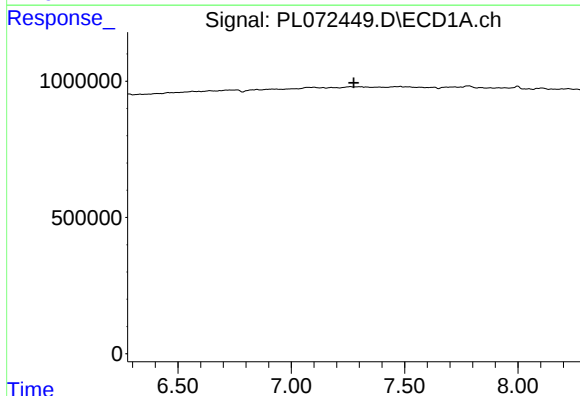


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

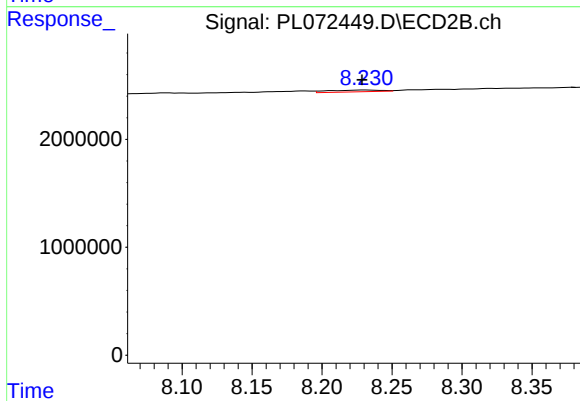

#10 gamma-Chlordane


R.T.: 8.231 min
Delta R.T.: 0.002 min
Response: 441826
Conc: 0.22 ng/ml

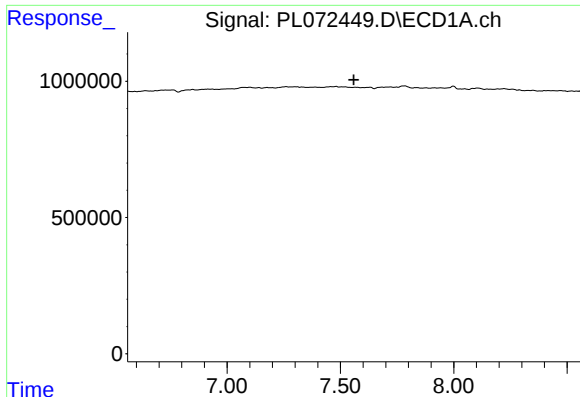

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

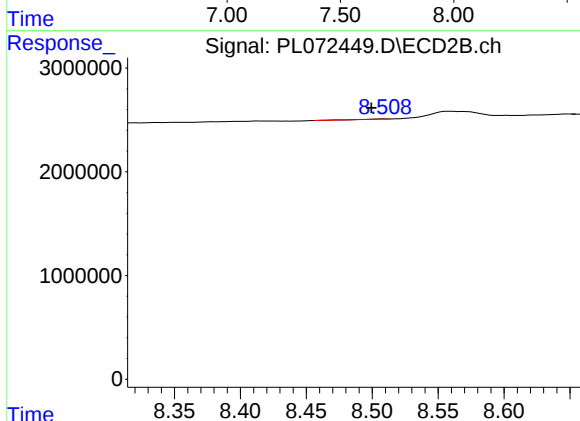


#12 4,4'-DDE

R.T.: 8.509 min
Delta R.T.: 0.010 min
Response: 17764
Conc: 0.01 ng/ml

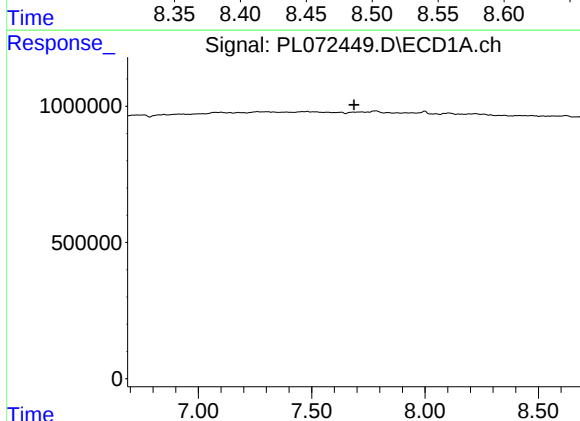


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

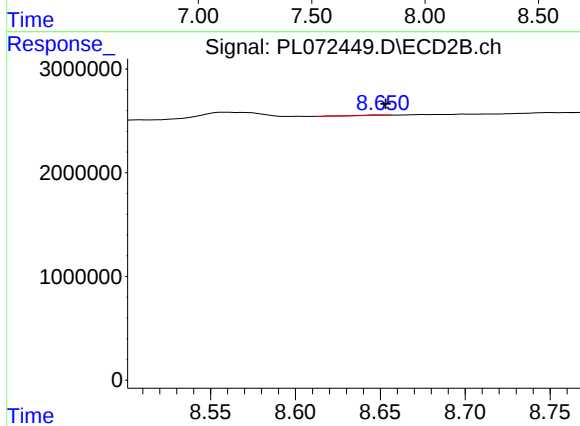

#13 Dieldrin


R.T.: 8.649 min
Delta R.T.: -0.004 min
Response: 38424
Conc: 0.02 ng/ml

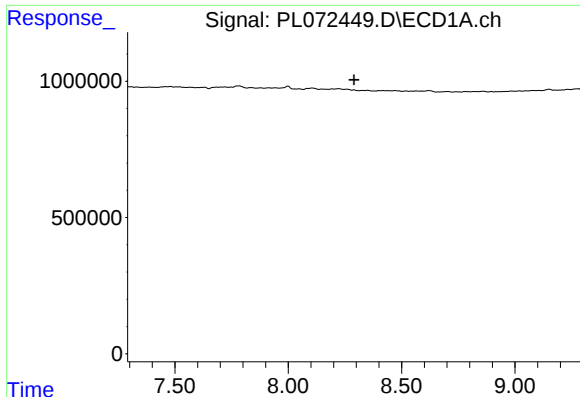

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

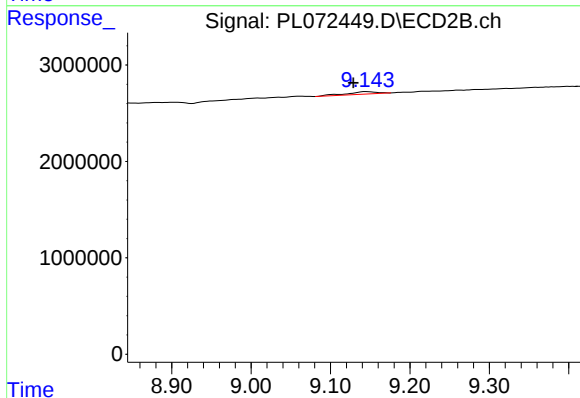


#15 Endosulfan II

R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 685147
Conc: 0.40 ng/ml

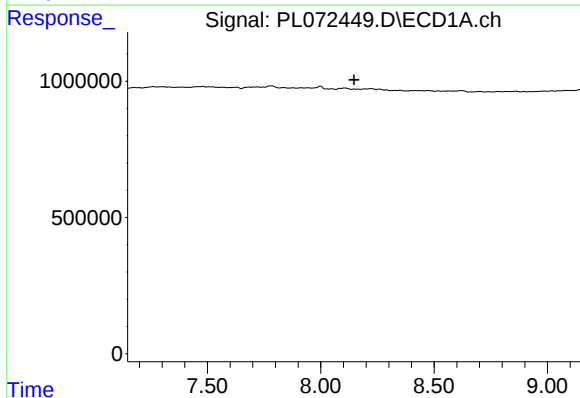


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

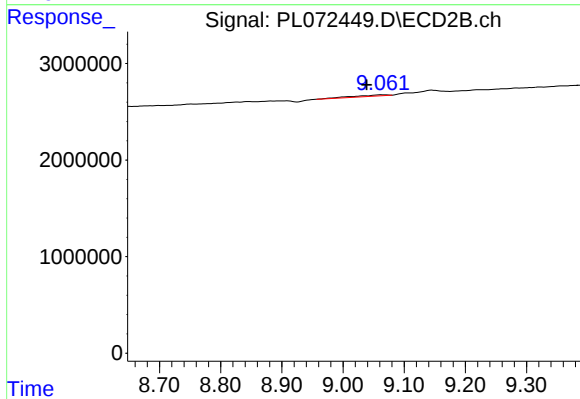

#16 4,4'-DDD

R.T.: 9.063 min
Delta R.T.: 0.024 min
Response: 467472
Conc: 0.33 ng/ml

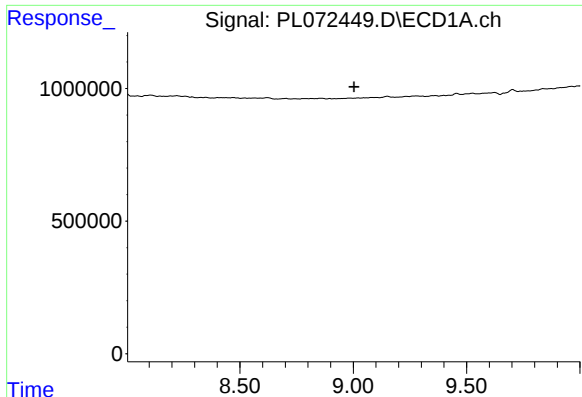

#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

#20 Methoxychlor


R.T.: 9.856 min
Delta R.T.: 0.011 min
Response: 59714
Conc: 0.07 ng/ml

#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

#25 Chlordane-3


R.T.: 8.231 min
Delta R.T.: 0.002 min
Response: 441826
Conc: 1.59 ng/ml

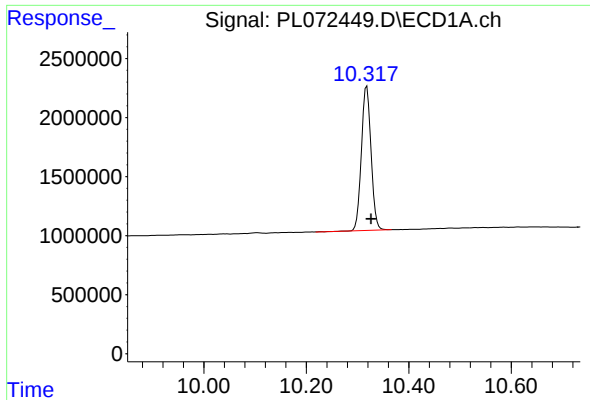

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.009 min
Response: 15959846
Conc: 17.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

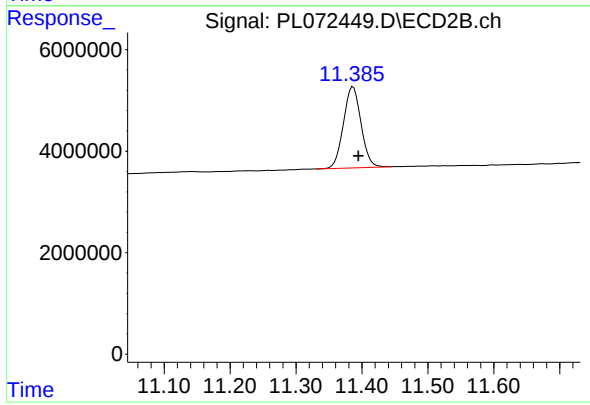

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: -0.008 min
Response: 29630030
Conc: 18.36 ng/ml