

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 17:11
 Operator : AR\AJ
 Sample : PB142501BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:32:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.491	9516111	32631727	17.140	20.092
28)	SA Decachlor...	10.323	11.389	15061542	28378451	16.953	17.588
Target Compounds							
6)	B beta-BHC	0.000	6.736	0	559016	N.D.	0.565 #
7)	B delta-BHC	0.000	7.017f	0	3668514	N.D.	1.491 #
9)	A Endosulfan I	0.000	8.387f	0	177242	N.D.	0.098 #
10)	B gamma-Chl...	0.000	8.218	0	144417	N.D.	0.071 #
15)	B Endosulfa...	0.000	9.146f	0	972959	N.D.	0.567 #
16)	A 4,4'-DDD	0.000	9.034	0	195090	N.D.	0.136 #
18)	B Endrin al...	0.000	9.271	0	136806	N.D.	0.110 #
25)	Chlordane-3	0.000	8.218	0	144417	N.D.	0.520 #
27)	Chlordane-5	0.000	9.210	0	163798	N.D.	2.684 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 17:11
Operator : AR\AJ
Sample : PB142501BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:32:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

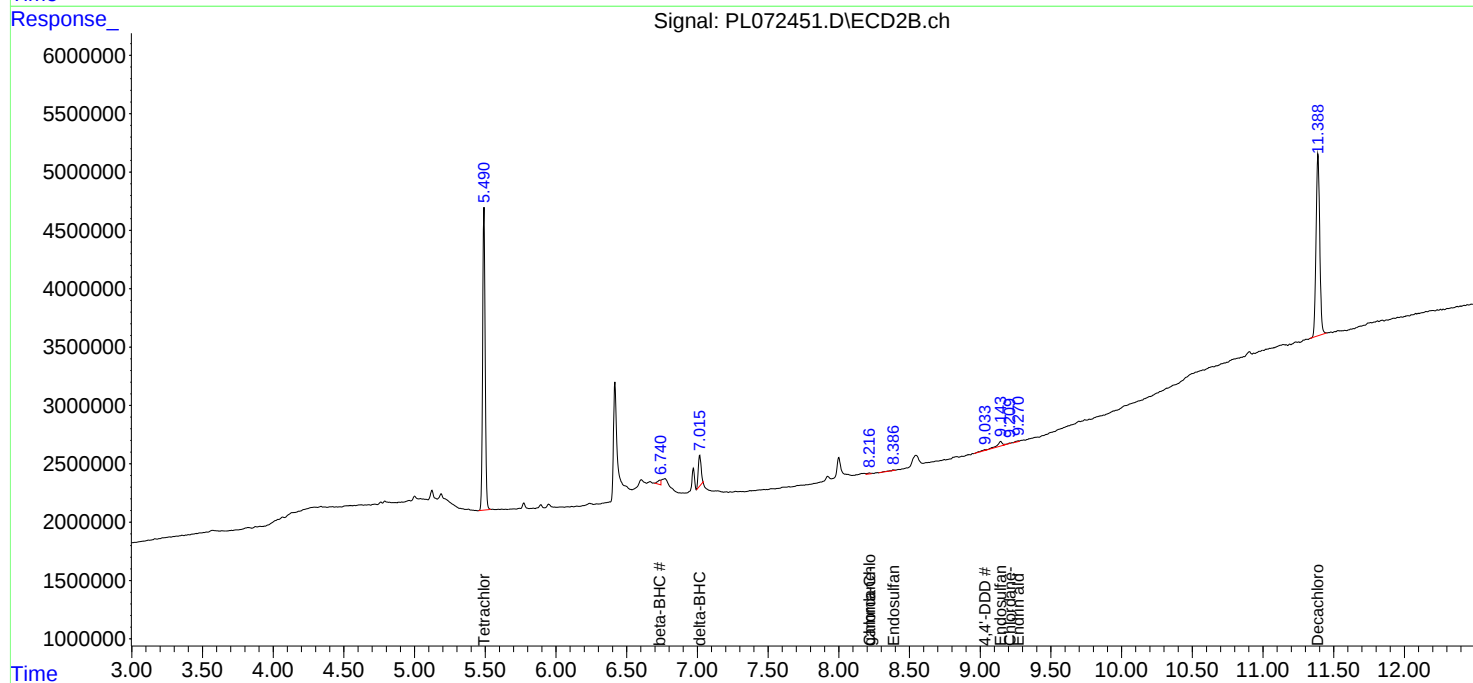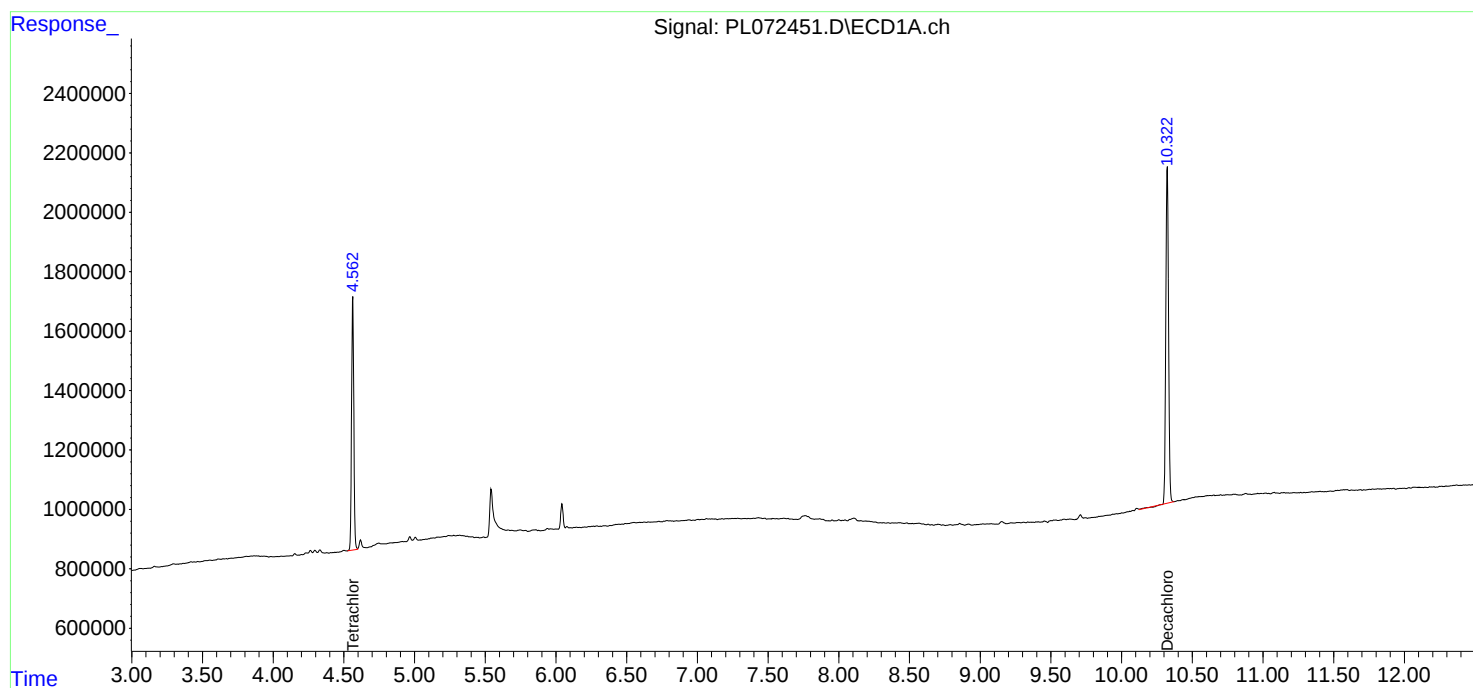


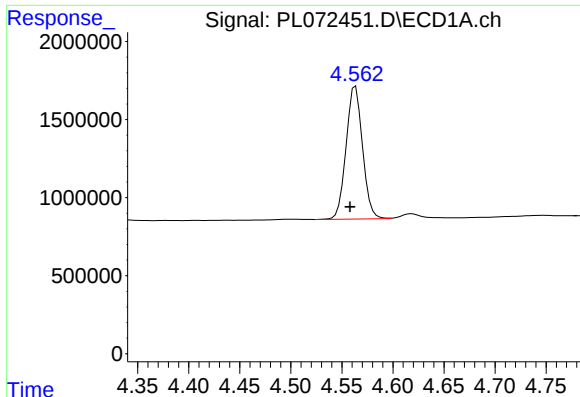

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.005 min
Response: 9516111
Conc: 17.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

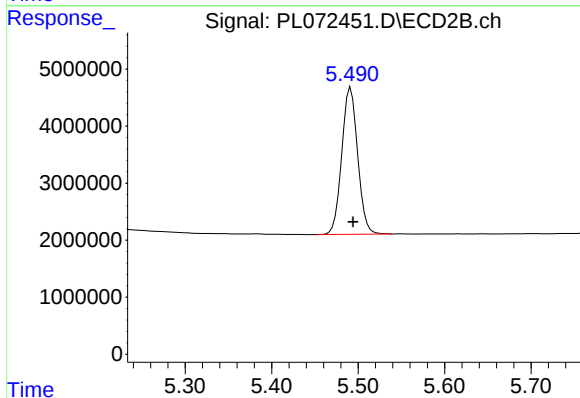


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 32631727
Conc: 20.09 ng/ml

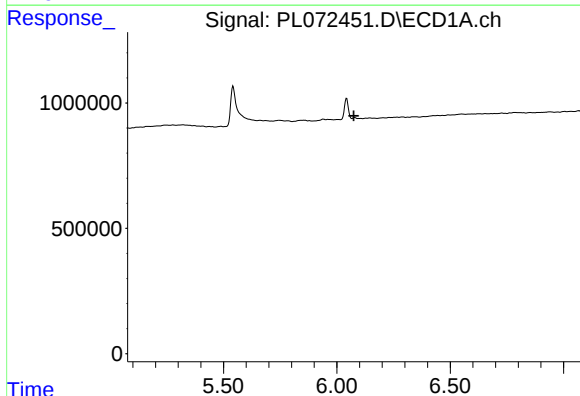


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.074 min
Response: 0
Conc: N.D.

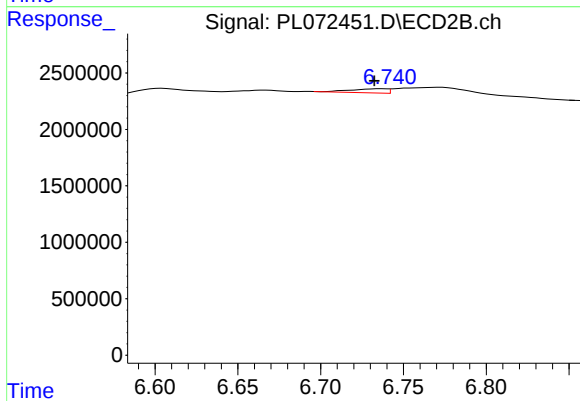

#6 beta-BHC


R.T.: 6.736 min
Delta R.T.: 0.004 min
Response: 559016
Conc: 0.56 ng/ml

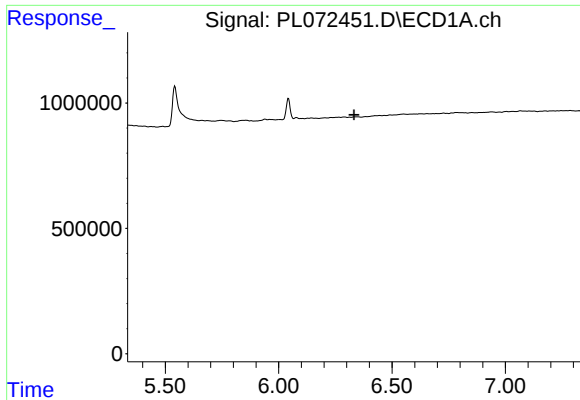

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

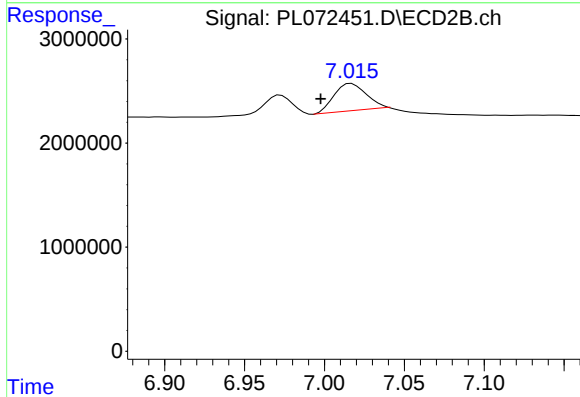


#7 delta-BHC

R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 3668514
Conc: 1.49 ng/ml

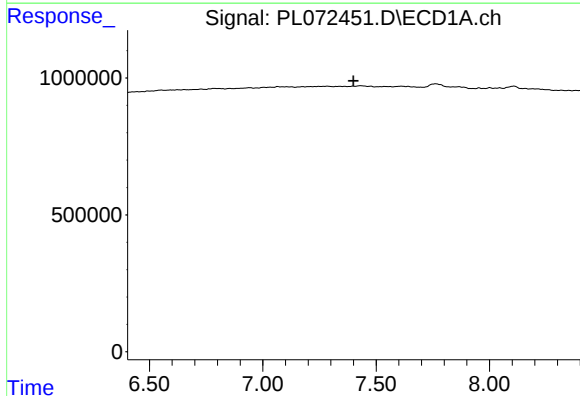


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

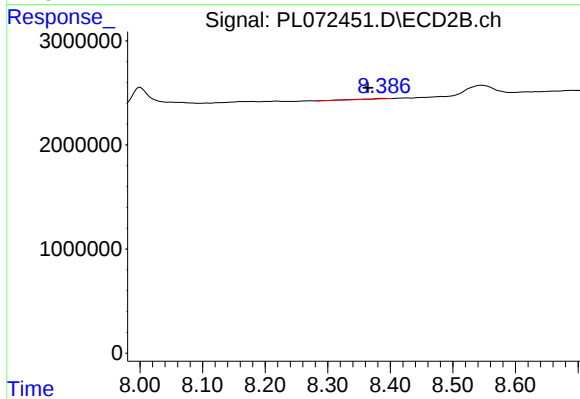

#9 Endosulfan I


R.T.: 8.387 min
Delta R.T.: 0.023 min
Response: 177242
Conc: 0.10 ng/ml

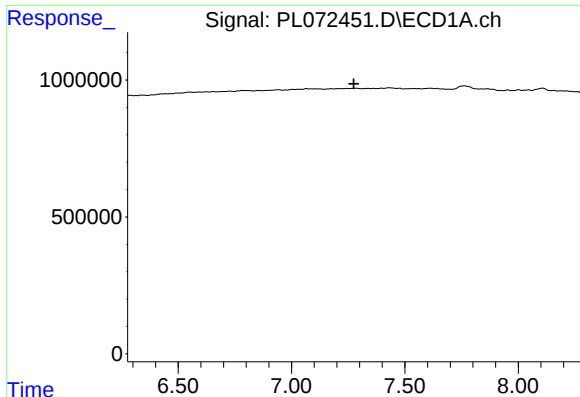

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

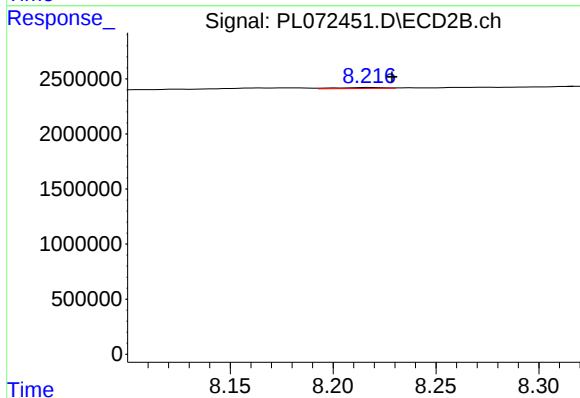


#10 gamma-Chlordane

R.T.: 8.218 min
Delta R.T.: -0.011 min
Response: 144417
Conc: 0.07 ng/ml

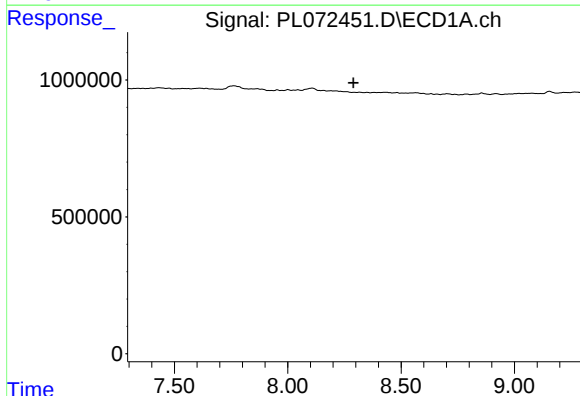


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

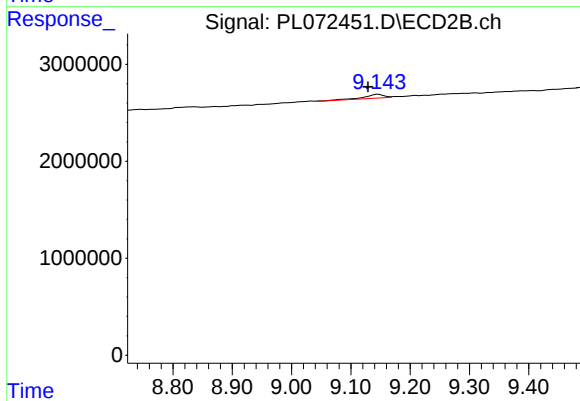

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.016 min
Response: 972959
Conc: 0.57 ng/ml

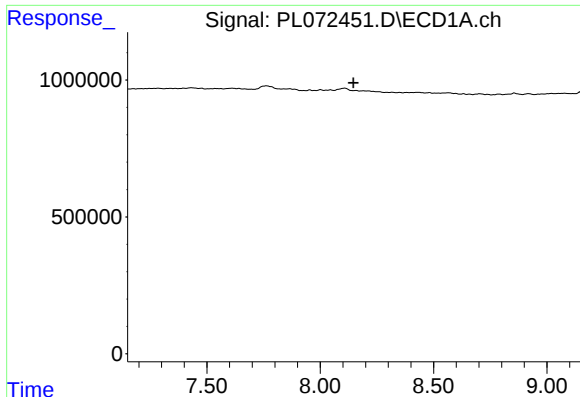

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

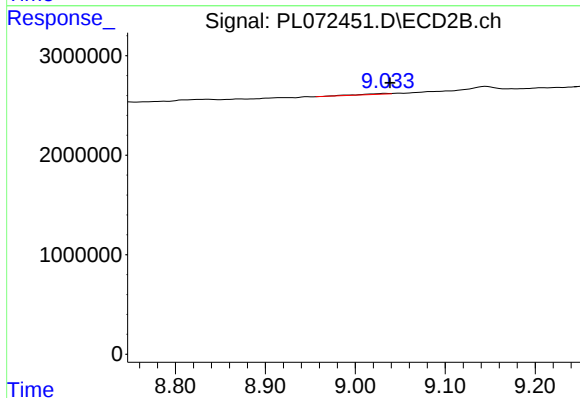


#16 4,4'-DDD

R.T.: 9.034 min
Delta R.T.: -0.004 min
Response: 195090
Conc: 0.14 ng/ml

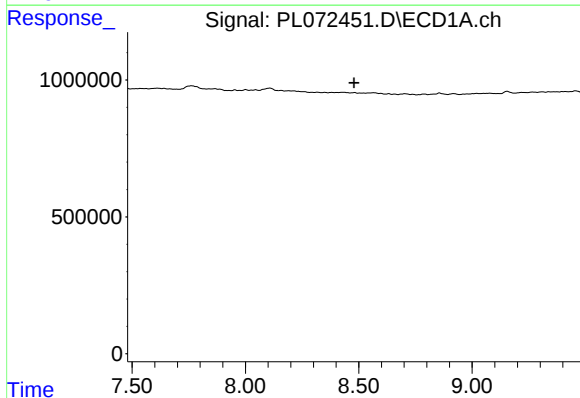


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

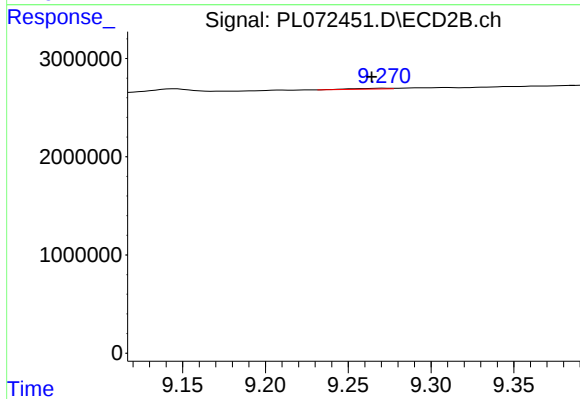

#18 Endrin aldehyde


R.T.: 9.271 min
Delta R.T.: 0.007 min
Response: 136806
Conc: 0.11 ng/ml

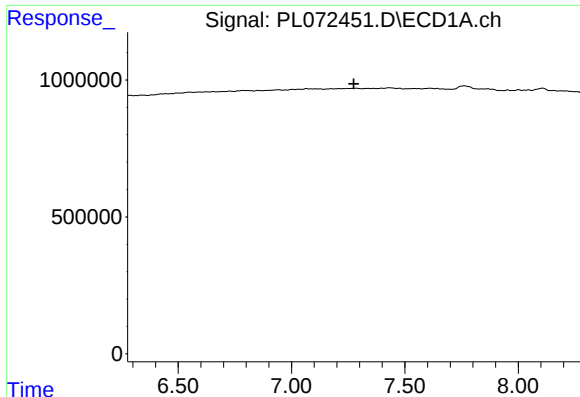

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

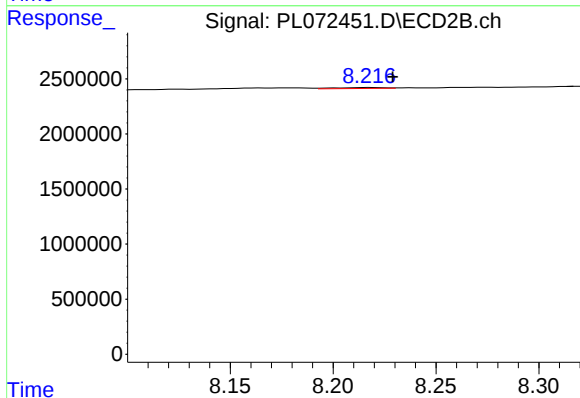


#25 Chlordane-3

R.T.: 8.218 min
Delta R.T.: -0.011 min
Response: 144417
Conc: 0.52 ng/ml

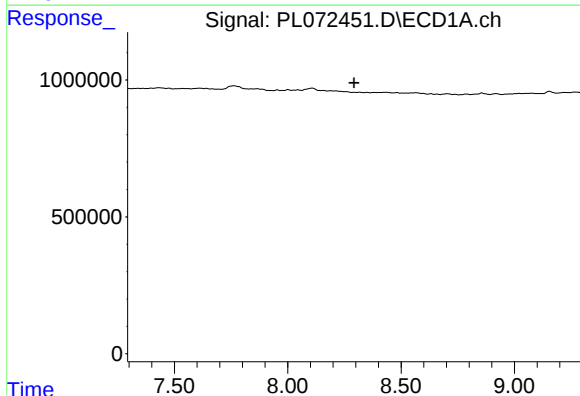


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

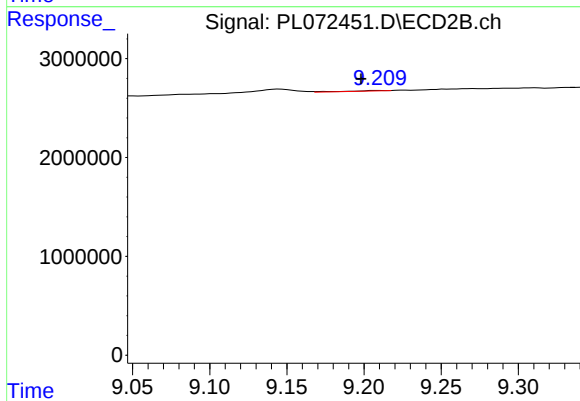

#27 Chlordane-5


R.T.: 9.210 min
Delta R.T.: 0.011 min
Response: 163798
Conc: 2.68 ng/ml

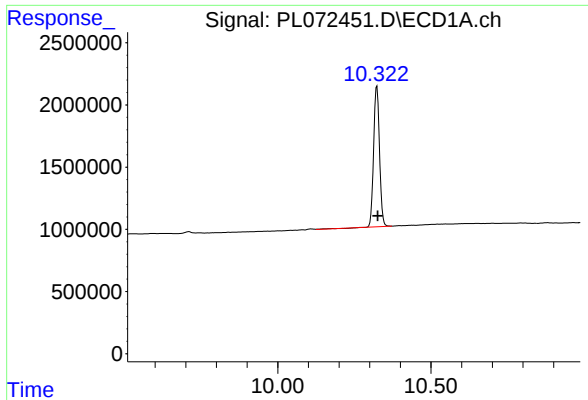

#28 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.003 min
Response: 15061542
Conc: 16.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

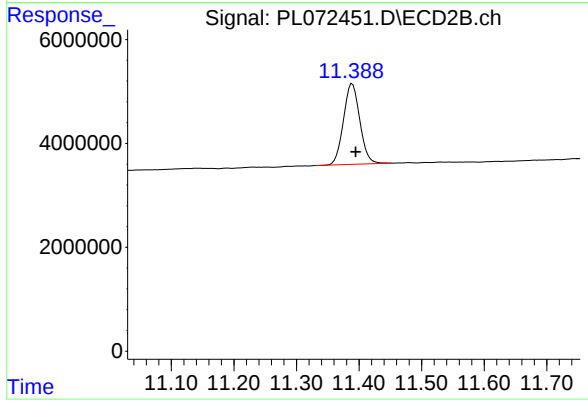

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: -0.005 min
Response: 28378451
Conc: 17.59 ng/ml