

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 19:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:34:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.491	10388404	34565910	18.712	21.283
28)	SA Decachlor...	10.317	11.385	16327626	30938848	18.378	19.175
Target Compounds							
2)	A alpha-BHC	5.279	0.000	137500	0	0.178	N.D. #
7)	B delta-BHC	0.000	7.016f	0	700696	N.D.	0.285 #
9)	A Endosulfan I	0.000	8.392f	0	133006	N.D.	0.073 #
10)	B gamma-Chl...	0.000	8.225	0	656756	N.D.	0.325 #
11)	B alpha-Chl...	0.000	8.308	0	133671	N.D.	0.067 #
15)	B Endosulfa...	0.000	9.146f	0	432278	N.D.	0.252 #
16)	A 4,4'-DDD	0.000	9.041	0	171525	N.D.	0.120 #
17)	MA 4,4'-DDT	0.000	9.358	0	51830	N.D.	0.033 #
19)	B Endosulfa...	0.000	9.513	0	107050	N.D.	0.069 #
20)	A Methoxychlor	0.000	9.830f	0	34665	N.D.	0.042 #
25)	Chlordane-3	0.000	8.225	0	656756	N.D.	2.364 #
26)	Chlordane-4	0.000	8.308	0	133671	N.D.	0.403 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 19:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:34:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

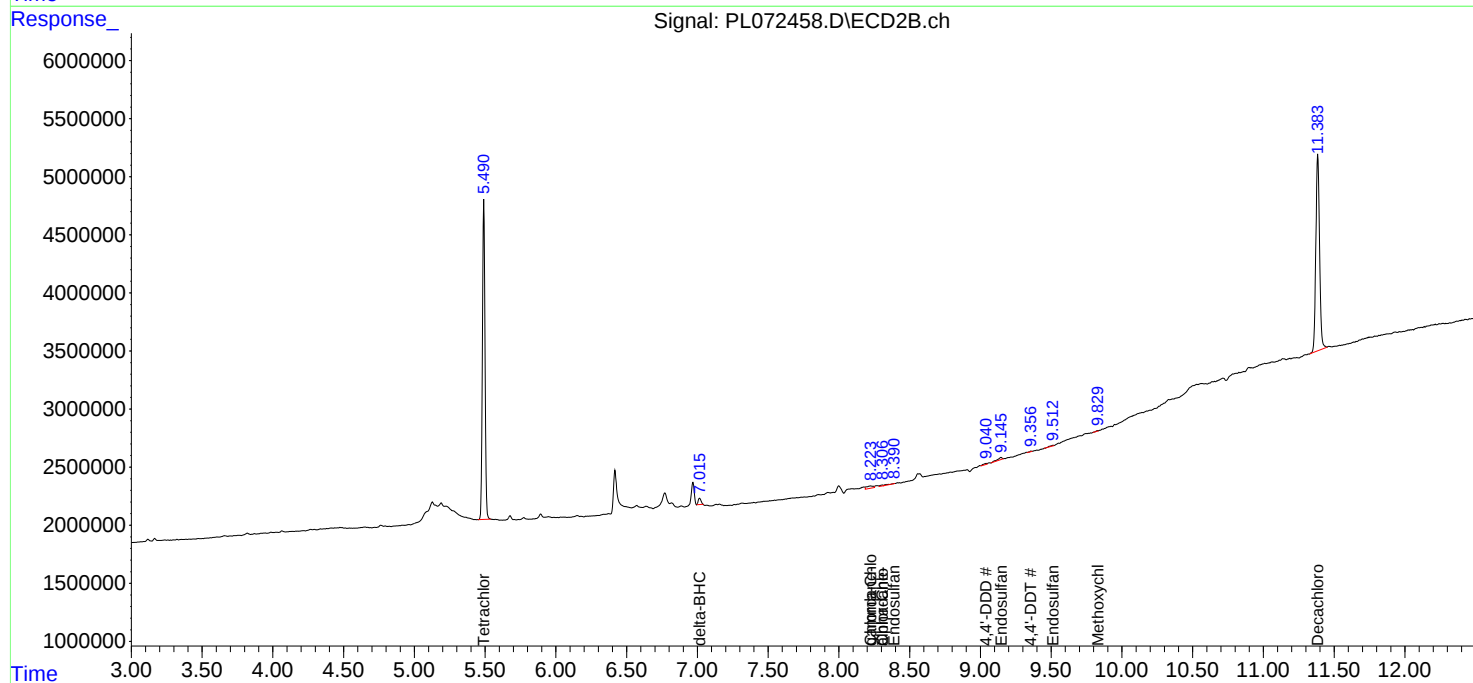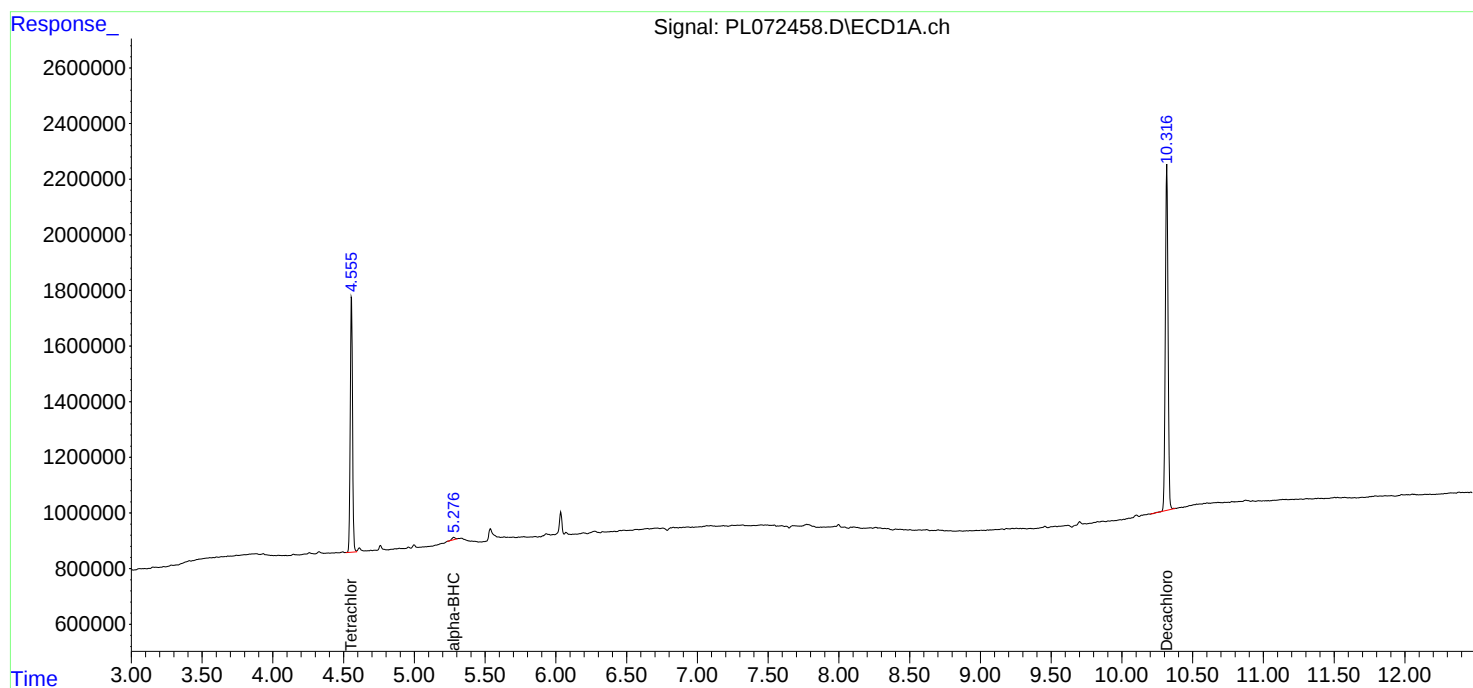


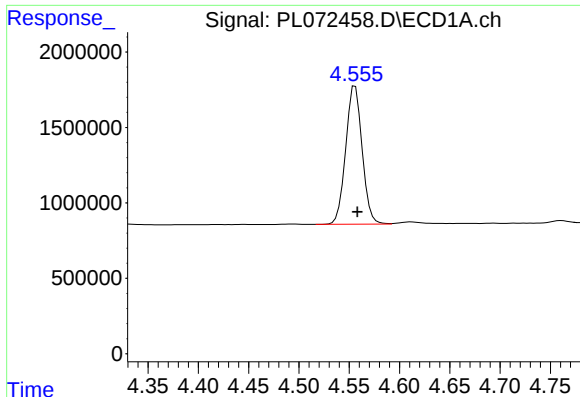

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 10388404
Conc: 18.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

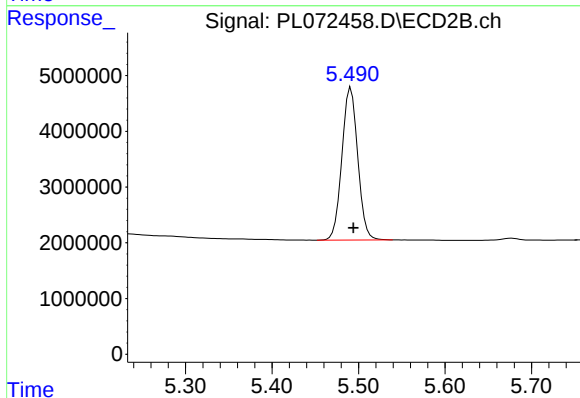


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 34565910
Conc: 21.28 ng/ml

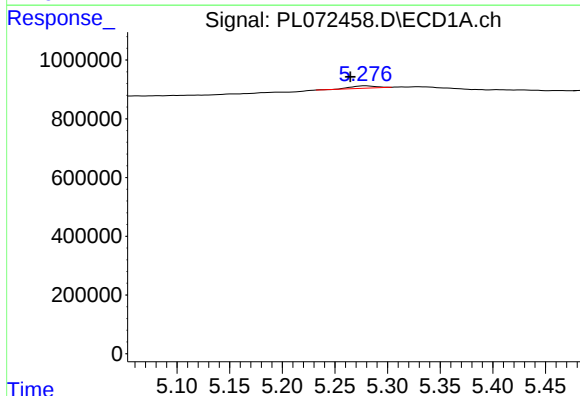


#2 alpha-BHC

R.T.: 5.279 min
Delta R.T.: 0.014 min
Response: 137500
Conc: 0.18 ng/ml

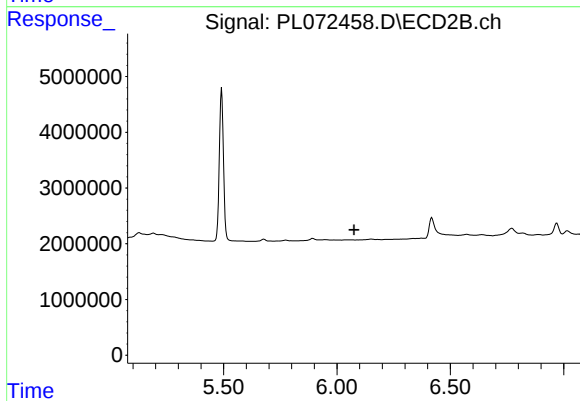

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

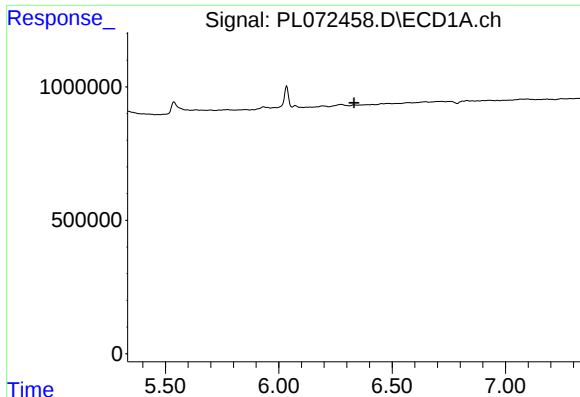

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

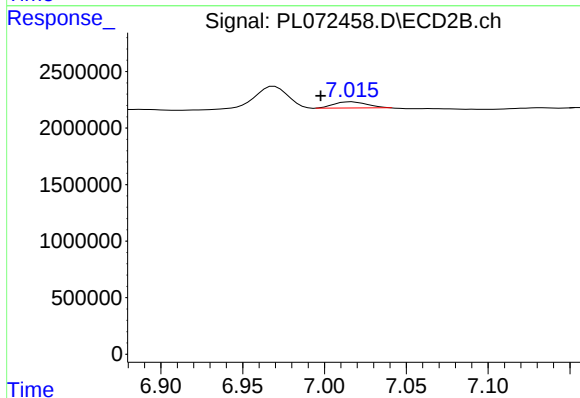


#7 delta-BHC

R.T.: 7.016 min
Delta R.T.: 0.019 min
Response: 700696
Conc: 0.28 ng/ml

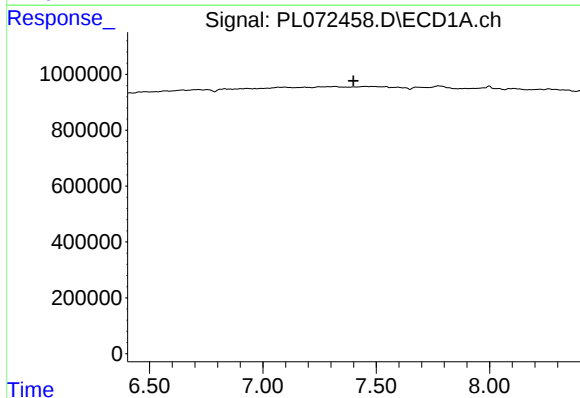


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

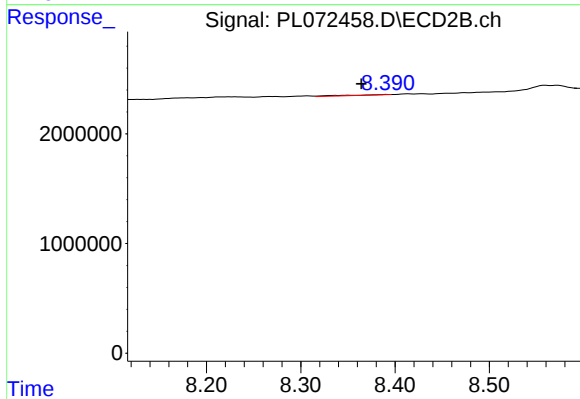

#9 Endosulfan I


R.T.: 8.392 min
Delta R.T.: 0.028 min
Response: 133006
Conc: 0.07 ng/ml

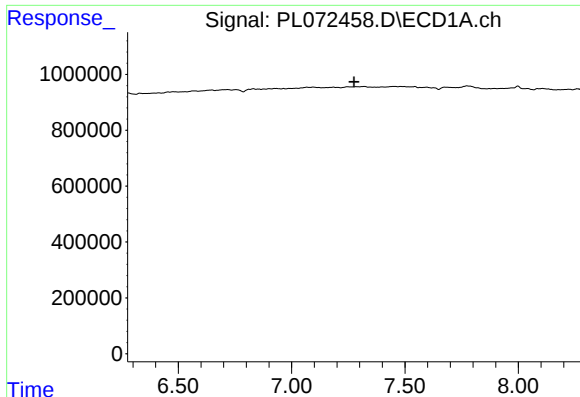

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

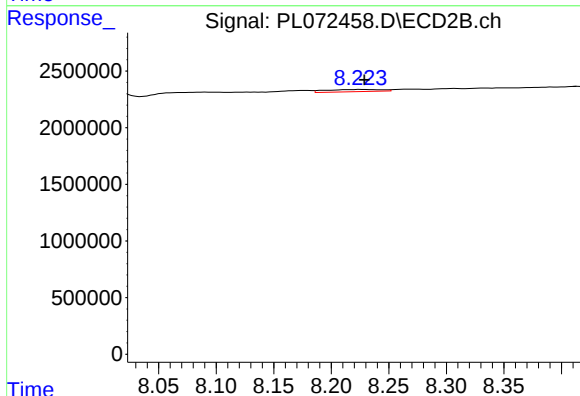


#10 gamma-Chlordane

R.T.: 8.225 min
Delta R.T.: -0.004 min
Response: 656756
Conc: 0.32 ng/ml

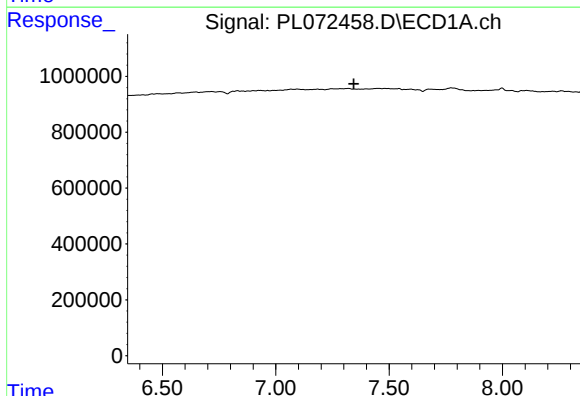


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

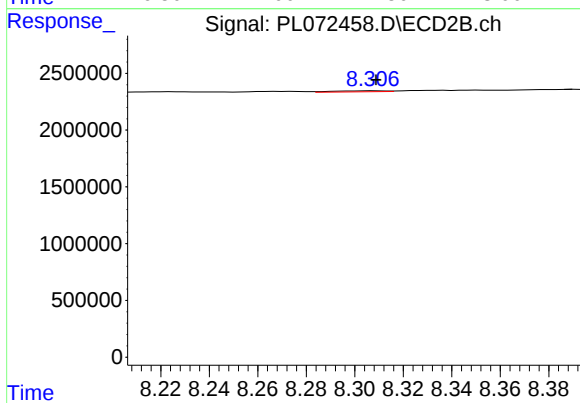

#11 alpha-Chlordane


R.T.: 8.308 min
Delta R.T.: 0.000 min
Response: 133671
Conc: 0.07 ng/ml

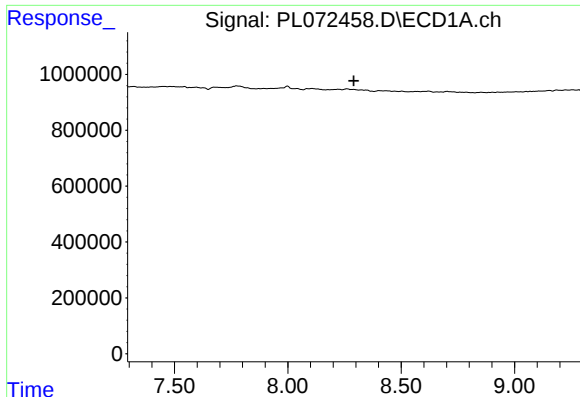

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

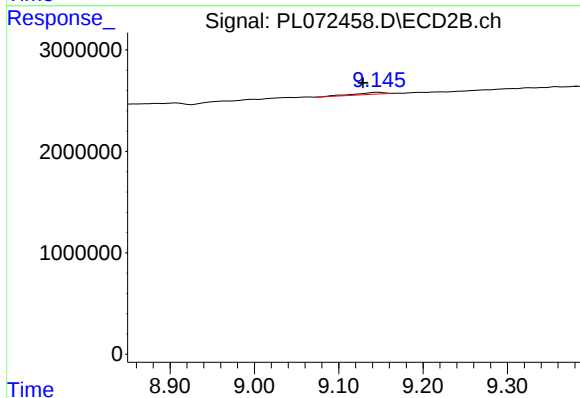


#15 Endosulfan II

R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 432278
Conc: 0.25 ng/ml

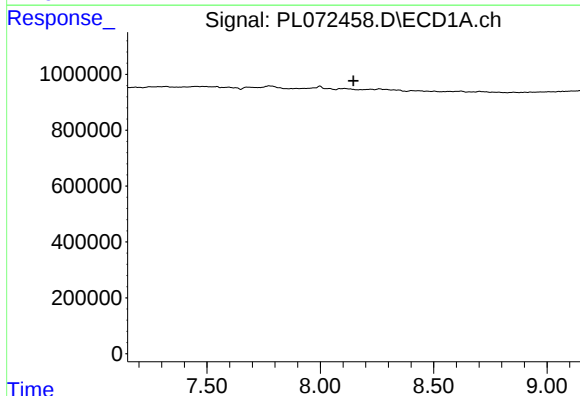


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

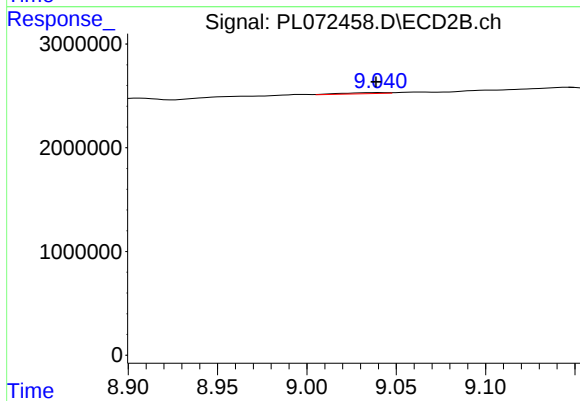

#16 4,4'-DDD


R.T.: 9.041 min
Delta R.T.: 0.003 min
Response: 171525
Conc: 0.12 ng/ml

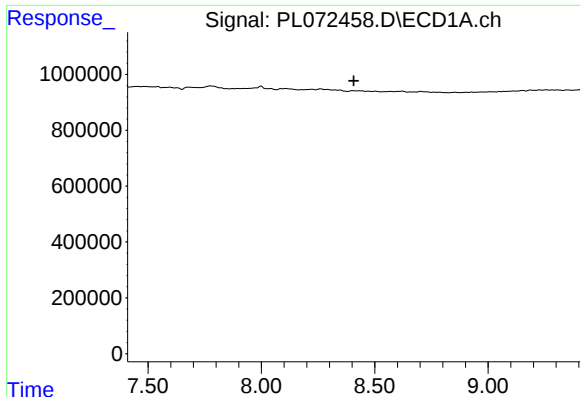

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

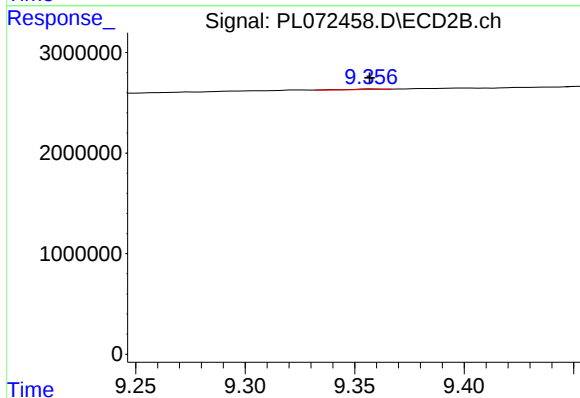


#17 4,4'-DDT

R.T.: 9.358 min
Delta R.T.: 0.000 min
Response: 51830
Conc: 0.03 ng/ml

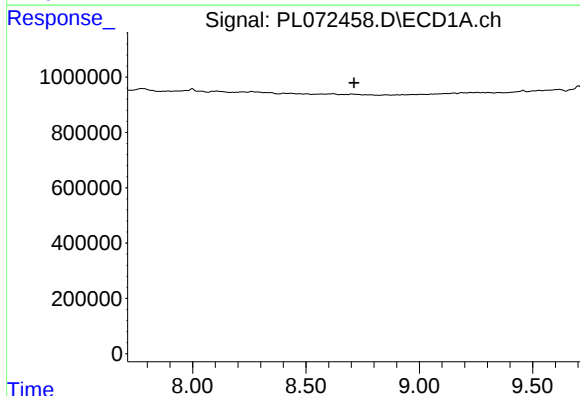


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.712 min
Response: 0
Conc: N.D.

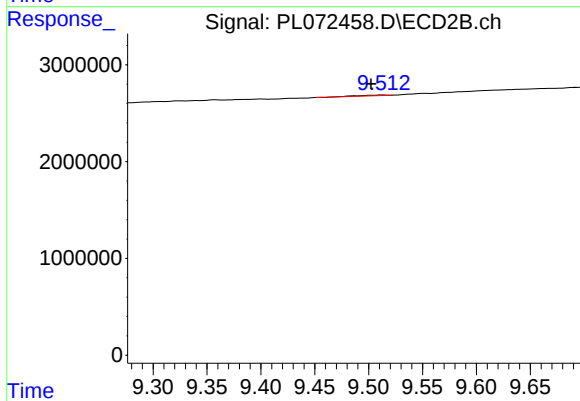

#19 Endosulfan Sulfate


R.T.: 9.513 min
Delta R.T.: 0.011 min
Response: 107050
Conc: 0.07 ng/ml

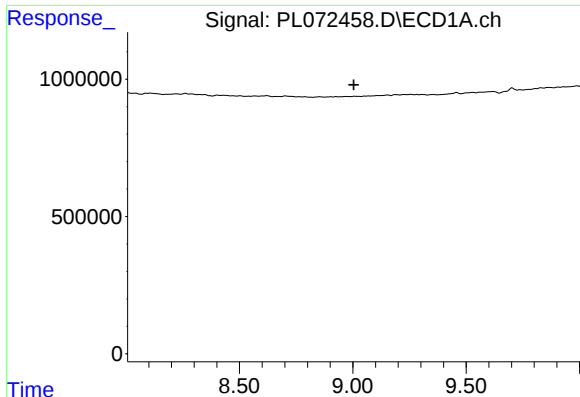

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

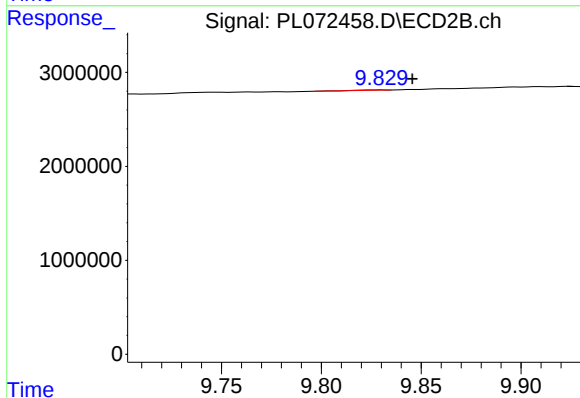


#20 Methoxychlor

R.T.: 9.830 min
Delta R.T.: -0.016 min
Response: 34665
Conc: 0.04 ng/ml

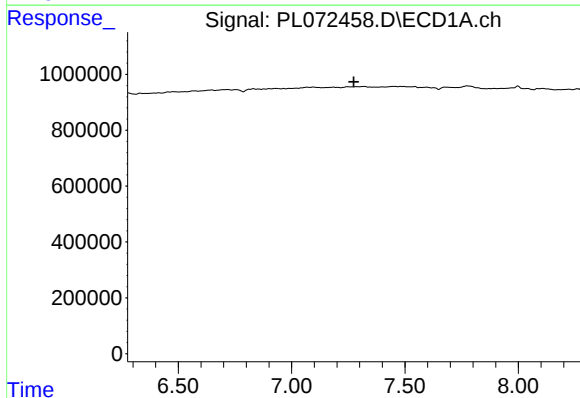


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

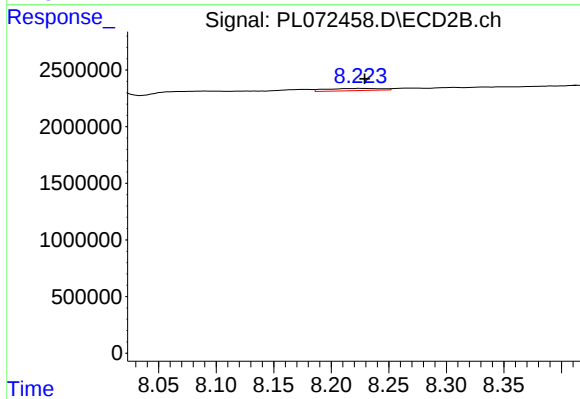

#25 Chlordane-3


R.T.: 8.225 min
Delta R.T.: -0.004 min
Response: 656756
Conc: 2.36 ng/ml

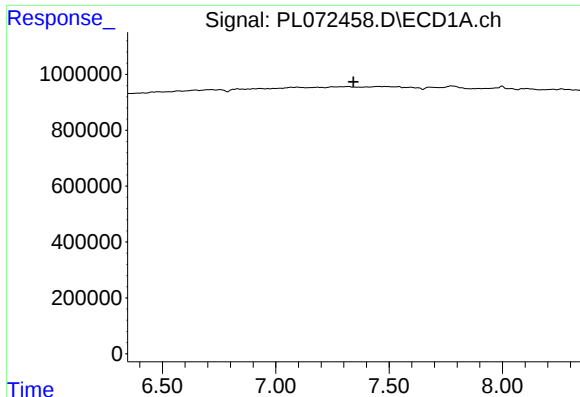

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

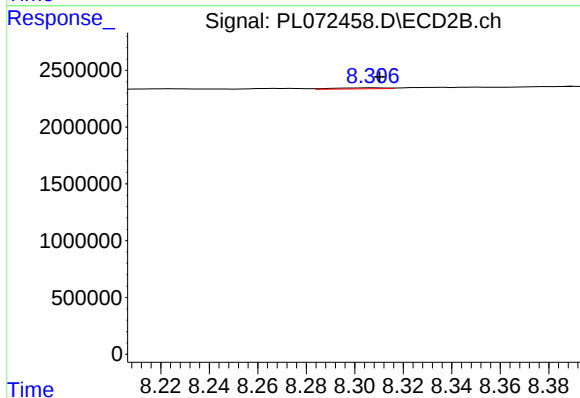


#26 Chlordane-4

R.T.: 8.308 min
Delta R.T.: -0.002 min
Response: 133671
Conc: 0.40 ng/ml

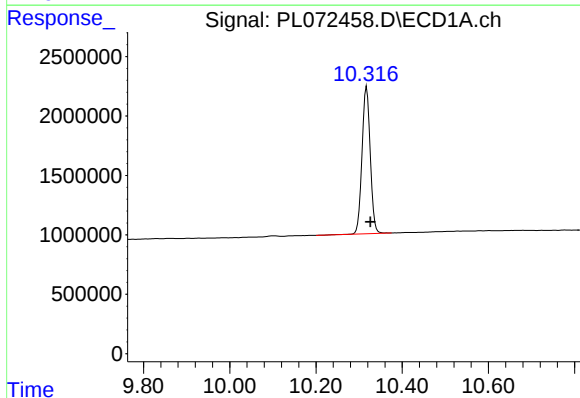

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.009 min
Response: 16327626
Conc: 18.38 ng/ml

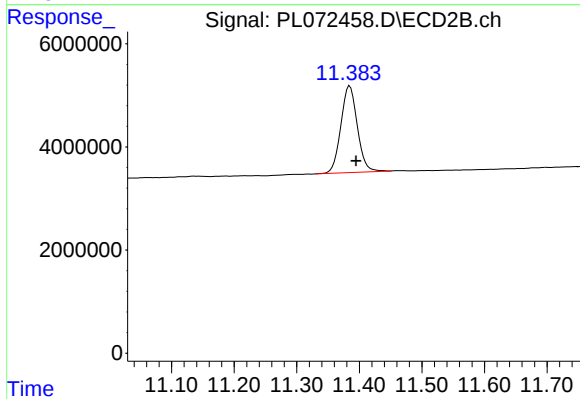

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: -0.010 min
Response: 30938848
Conc: 19.17 ng/ml