

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 10:18
 Operator : AR\AJ
 Sample : N1370-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:27:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.563	5.492	6816181	13053786	12.277	8.037m#
28)	SA Decachlor...	10.320	11.384	13889753	13048793	15.634m	8.087m#
Target Compounds							
12)	B 4,4'-DDE	7.561	8.505	1434640	6226374	1.987m	3.292m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 10:18
Operator : AR\AJ
Sample : N1370-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:27:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

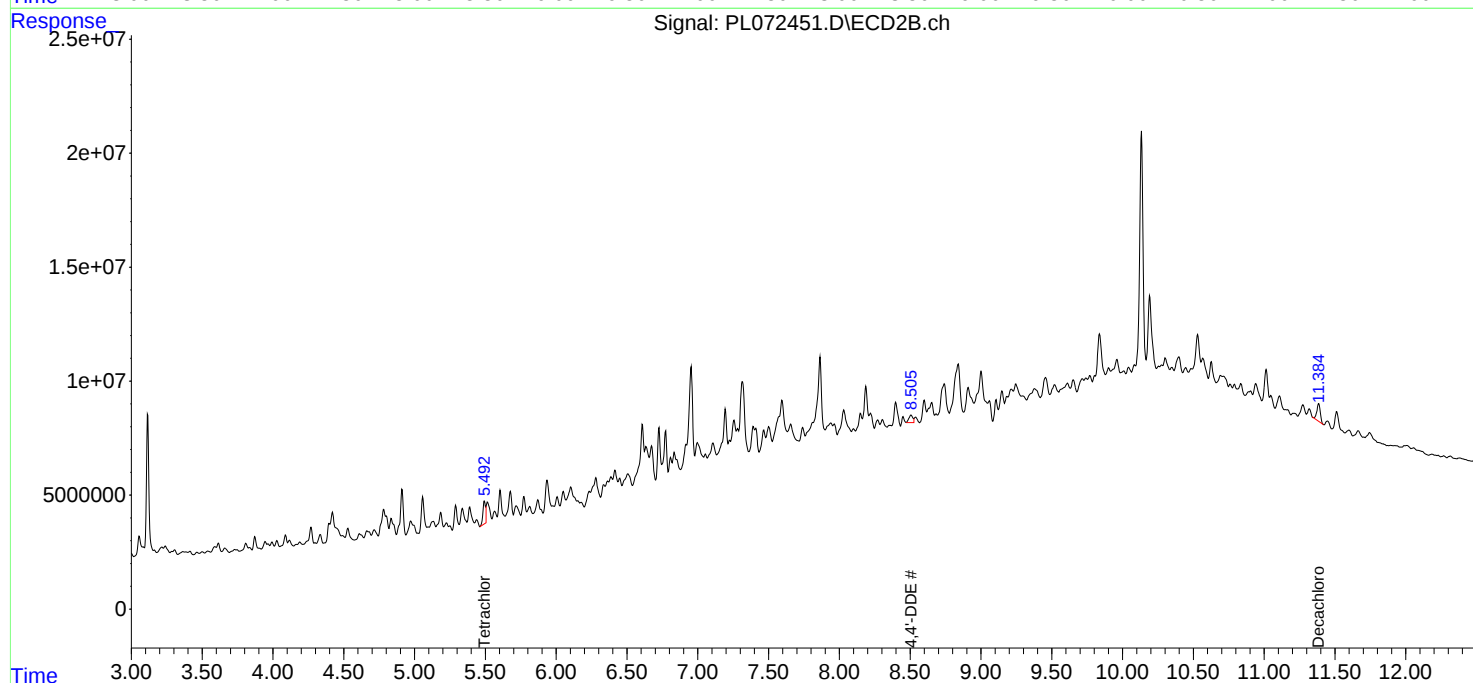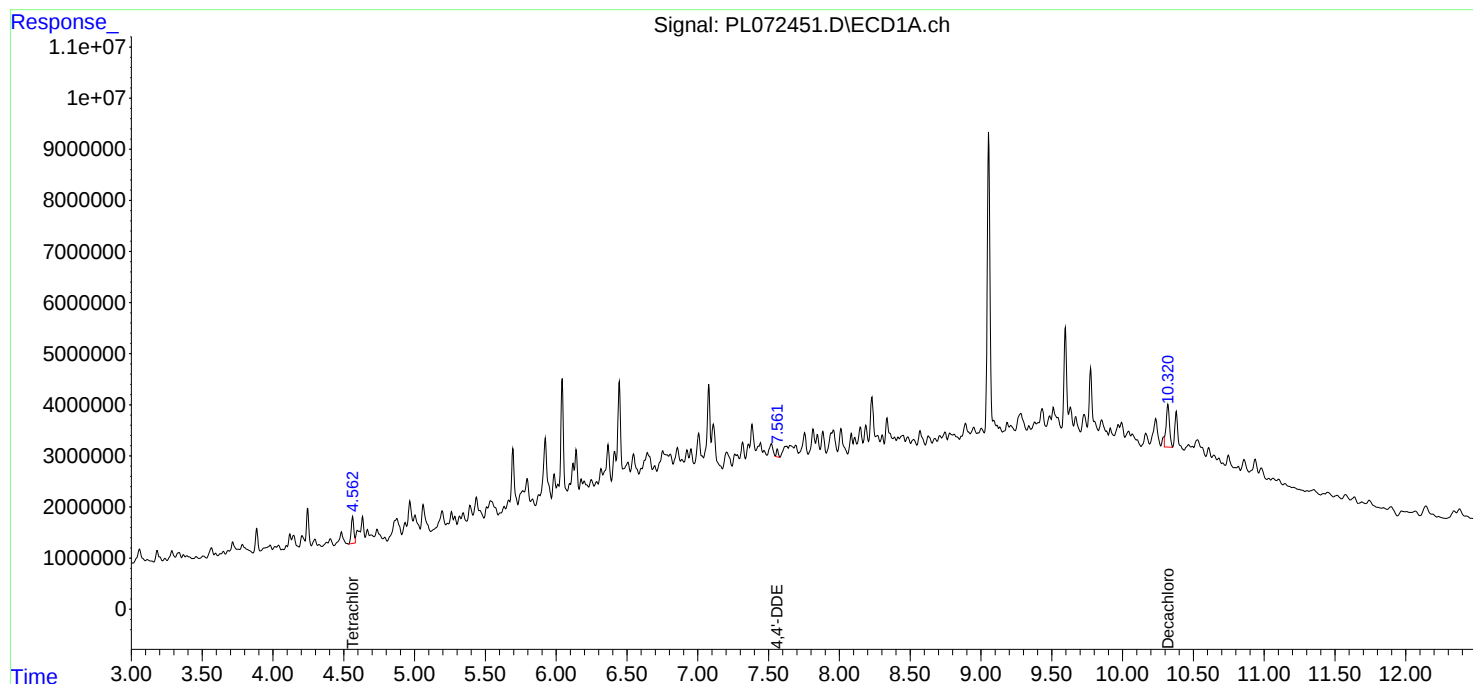


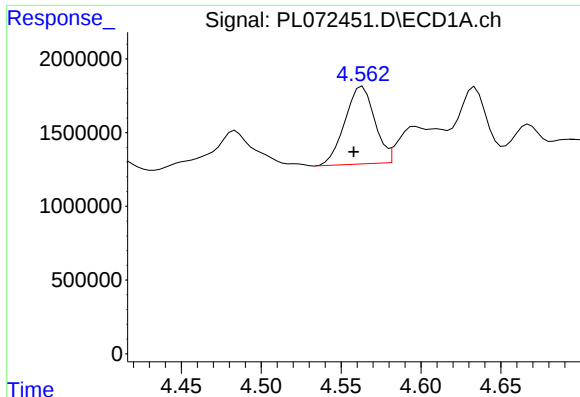

#1 Tetrachloro-m-xylene


R.T.: 4.563 min
Delta R.T.: 0.005 min
Response: 6816181
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

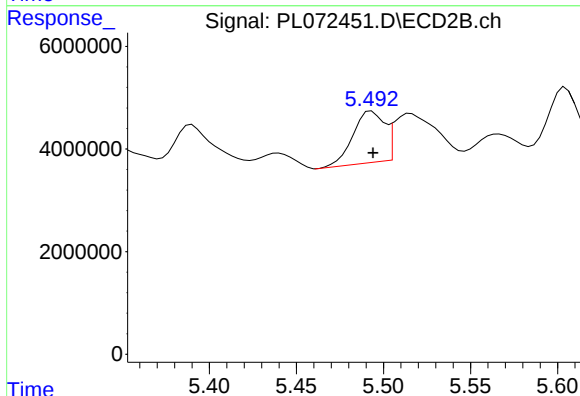


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 13053786
Conc: 8.04 ng/ml m

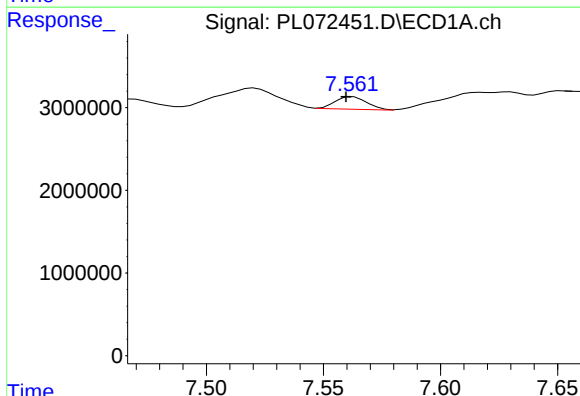


#12 4,4'-DDE

R.T.: 7.561 min
Delta R.T.: 0.001 min
Response: 1434640
Conc: 1.99 ng/ml m

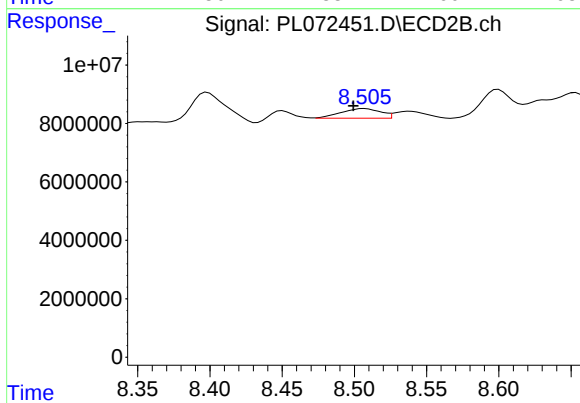

#12 4,4'-DDE


R.T.: 8.505 min
Delta R.T.: 0.006 min
Response: 6226374
Conc: 3.29 ng/ml m

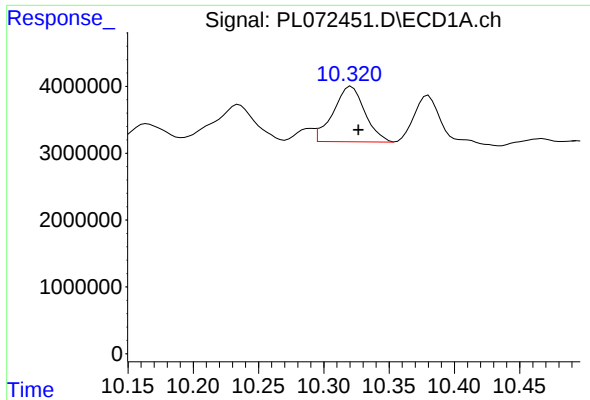

#28 Decachlorobiphenyl

R.T.: 10.320 min
Delta R.T.: -0.007 min
Response: 13889753
Conc: 15.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-DECANT

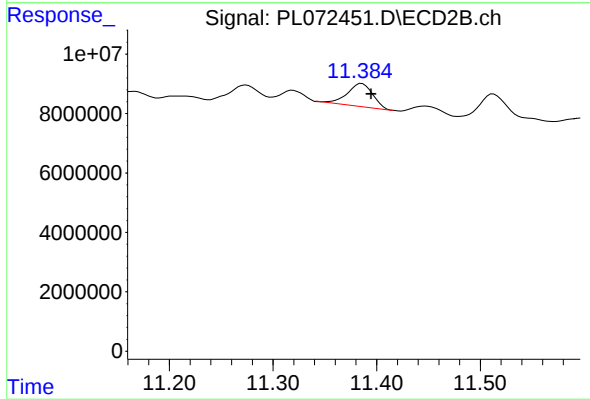

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.010 min
Response: 13048793
Conc: 8.09 ng/ml m