

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 11:16
 Operator : AR\AJ
 Sample : N1375-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MONTHLY-OUTFALL-002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:28:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.562	5.492	9397011	18616556	16.926	11.463m#
2) SA Decachlor...	10.319	11.384	15528135	15869231	17.478m	9.835m#
Target Compounds						
5) MB Aldrin	6.411	7.501	9090890	11308424	11.513	5.114m#
13) MA Dieldrin	7.691	8.651	1375658	5815607	1.816m	2.960m#
20) A Methoxychlor	9.001	9.837	2258996	49049279	5.354m	59.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 11:16
Operator : AR\AJ
Sample : N1375-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:28:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

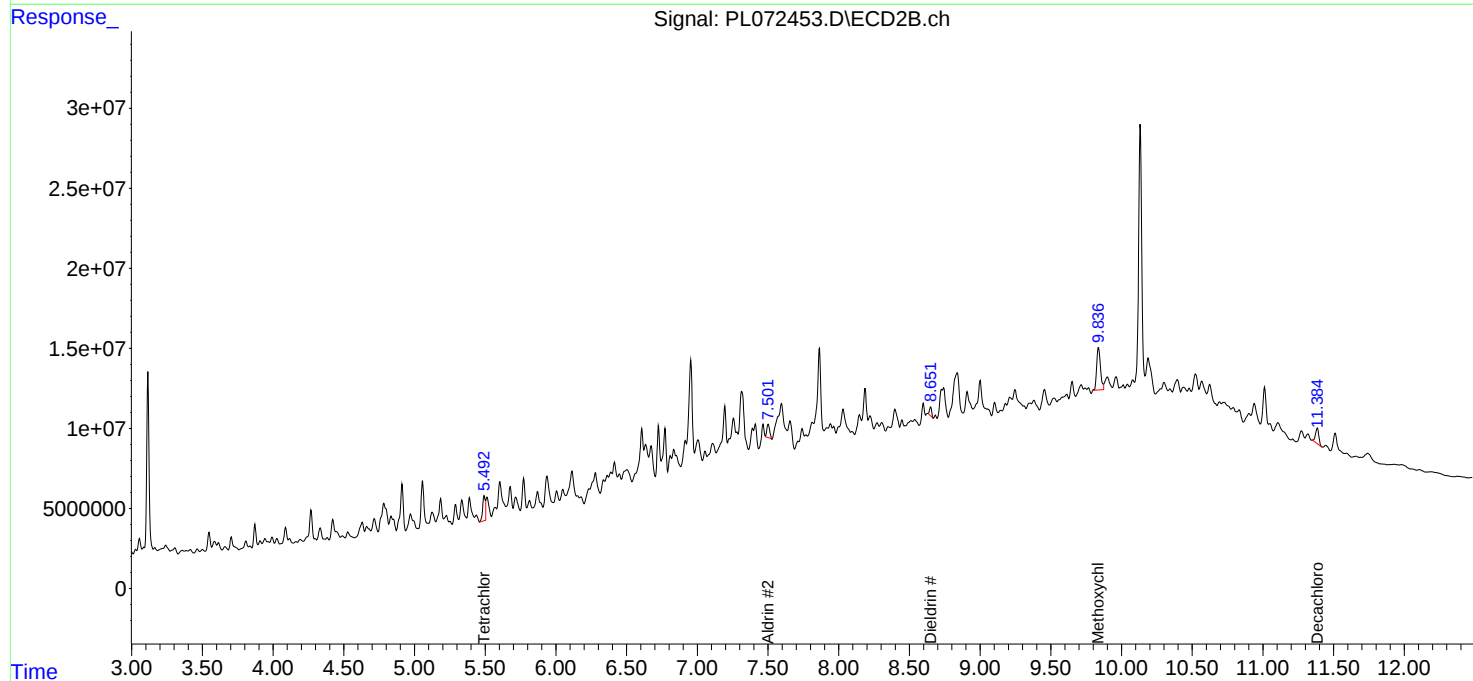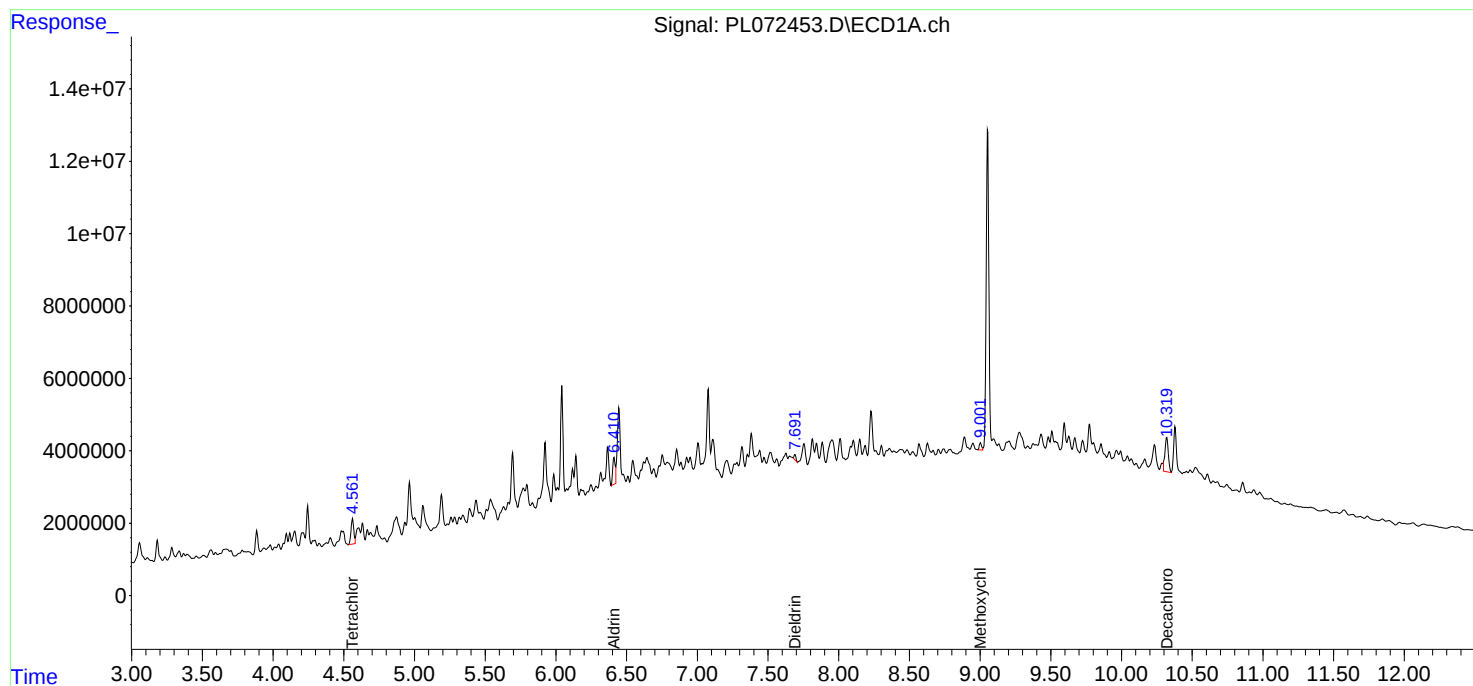


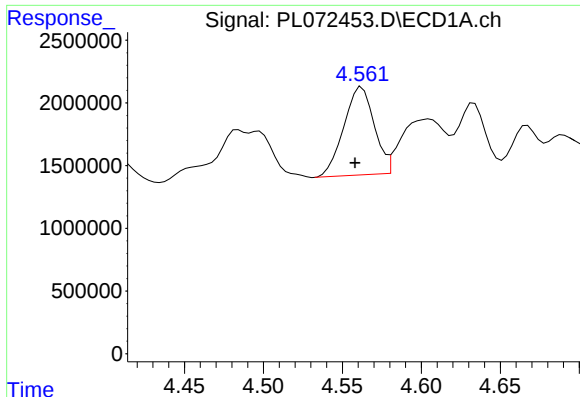

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: 0.004 min
Response: 9397011
Conc: 16.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002

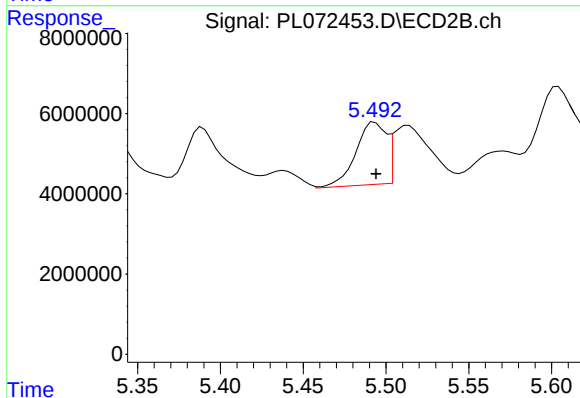


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 18616556
Conc: 11.46 ng/ml m

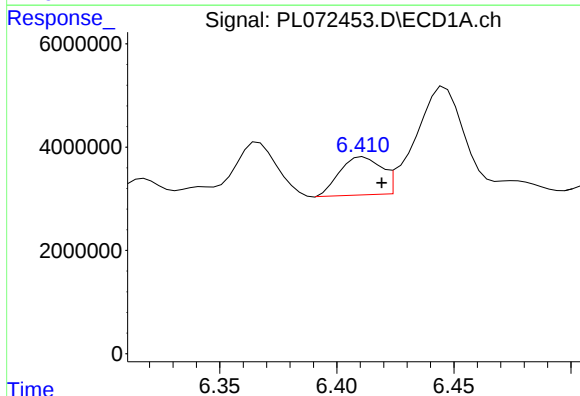


#5 Aldrin

R.T.: 6.411 min
Delta R.T.: -0.008 min
Response: 9090890
Conc: 11.51 ng/ml

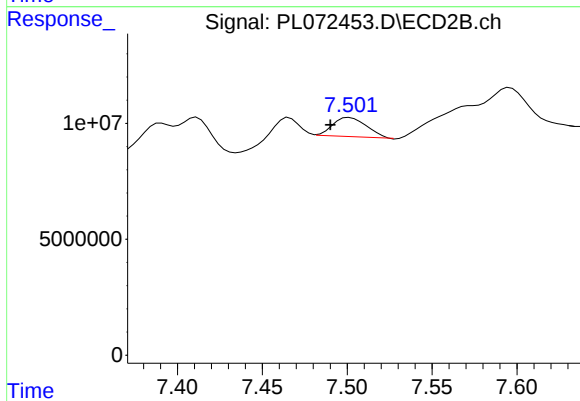

#5 Aldrin


R.T.: 7.501 min
Delta R.T.: 0.011 min
Response: 11308424
Conc: 5.11 ng/ml m

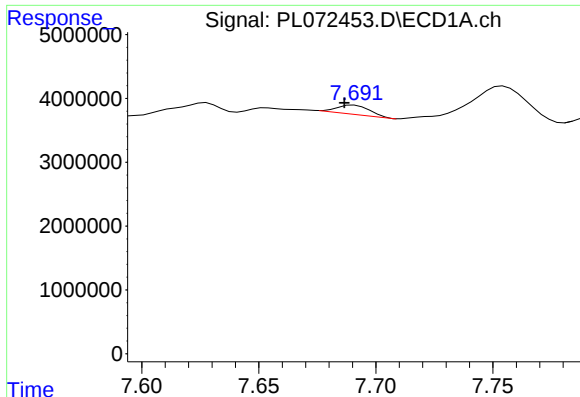

#13 Dieldrin


R.T.: 7.691 min
Delta R.T.: 0.004 min
Response: 1375658
Conc: 1.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002

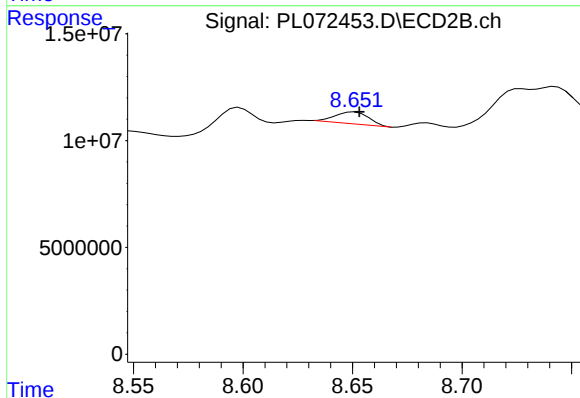


#13 Dieldrin

R.T.: 8.651 min
Delta R.T.: -0.003 min
Response: 5815607
Conc: 2.96 ng/ml m

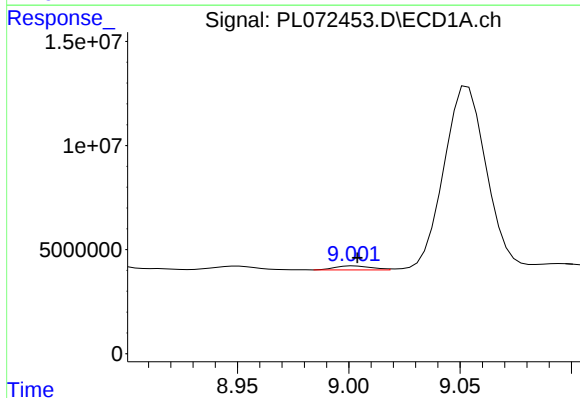


#20 Methoxychlor

R.T.: 9.001 min
Delta R.T.: -0.003 min
Response: 2258996
Conc: 5.35 ng/ml m

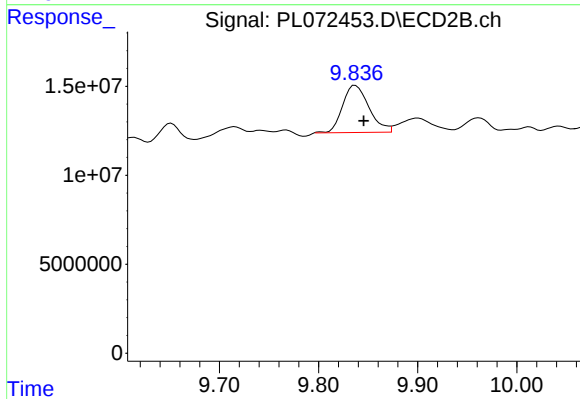

#20 Methoxychlor


R.T.: 9.837 min
Delta R.T.: -0.009 min
Response: 49049279
Conc: 59.21 ng/ml

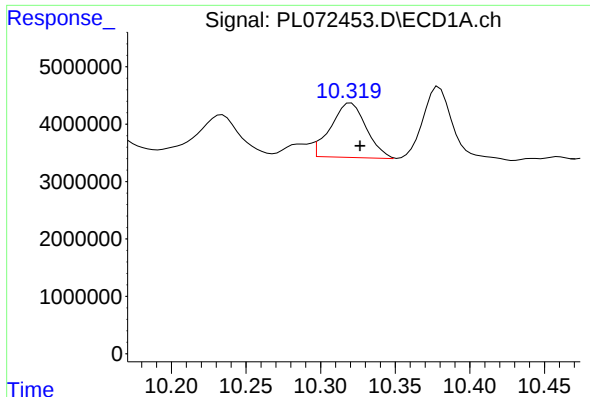

#28 Decachlorobiphenyl

R.T.: 10.319 min
Delta R.T.: -0.007 min
Response: 15528135
Conc: 17.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
MONTHLY-OUTFALL-002

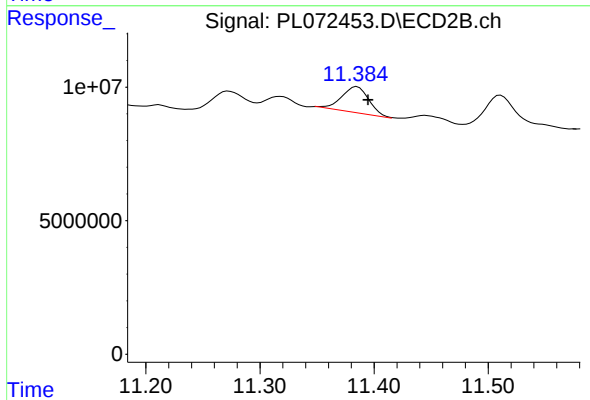

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.011 min
Response: 15869231
Conc: 9.84 ng/ml m