

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 11:42
 Operator : AR\AJ
 Sample : N1372-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENTRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:28:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.561	5.492	6913085	13291023	12.452	8.184m#
28)	SA Decachlor...	10.318	11.384	11913303	12230638	13.409m	7.580m#
Target Compounds							
12)	B 4,4'-DDE	7.558	8.504	1634516	3846450	2.264m	2.034m
13)	MA Dieldrin	7.690	8.650	406143	6586907	0.536m	3.353m#
20)	A Methoxychlor	9.002	9.837	847600	34658736	2.009m	41.841 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 11:42
Operator : AR\AJ
Sample : N1372-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:28:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

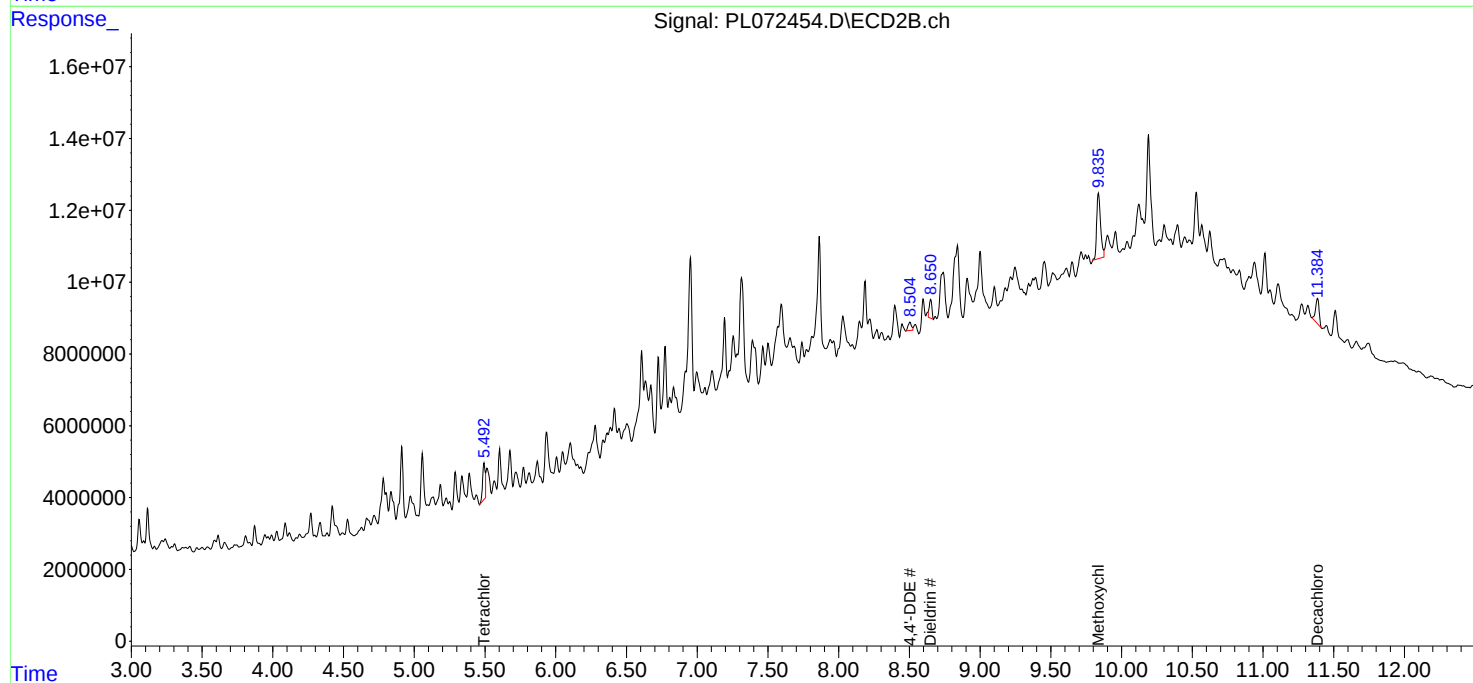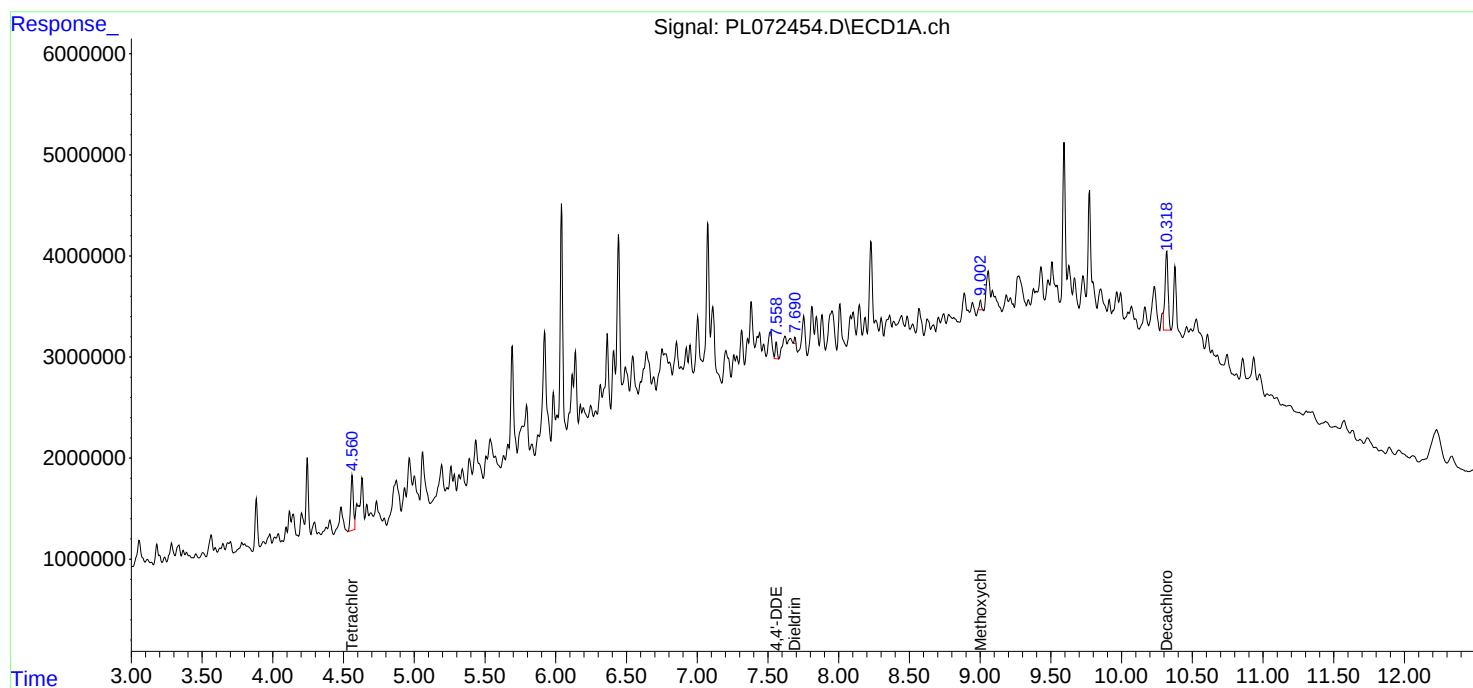


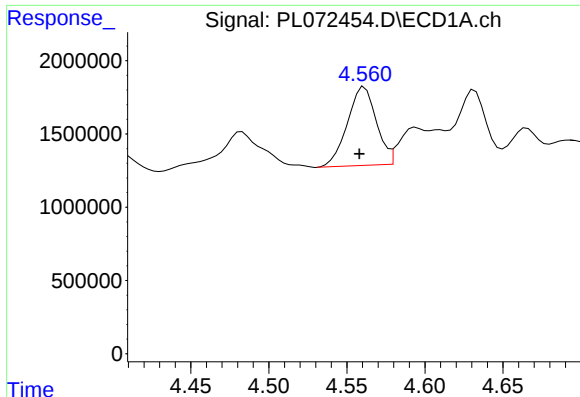

#1 Tetrachloro-m-xylene


R.T.: 4.561 min
Delta R.T.: 0.003 min
Response: 6913085
Conc: 12.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE

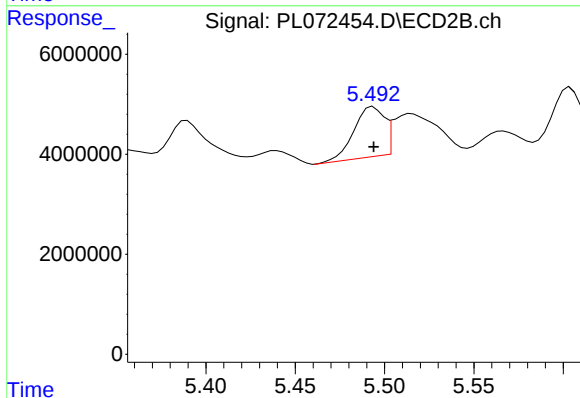


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 13291023
Conc: 8.18 ng/ml m

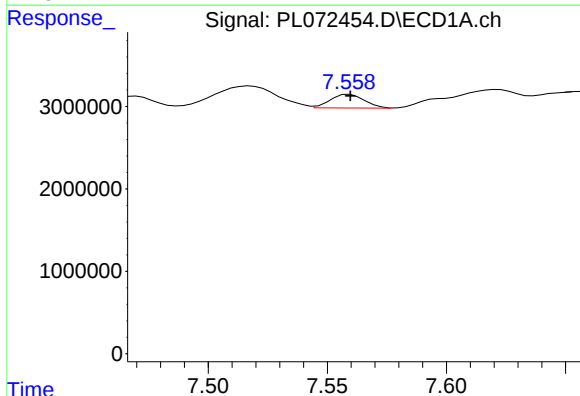


#12 4,4'-DDE

R.T.: 7.558 min
Delta R.T.: -0.002 min
Response: 1634516
Conc: 2.26 ng/ml m

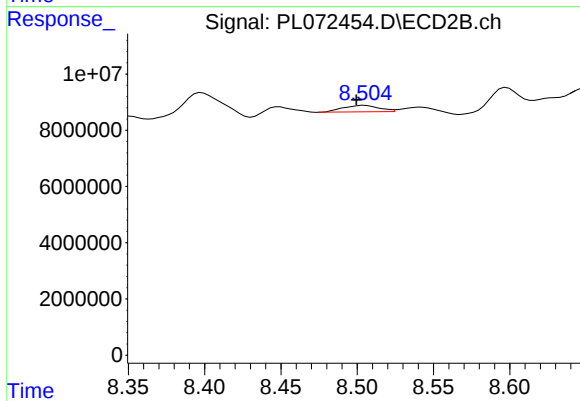

#12 4,4'-DDE


R.T.: 8.504 min
Delta R.T.: 0.004 min
Response: 3846450
Conc: 2.03 ng/ml m

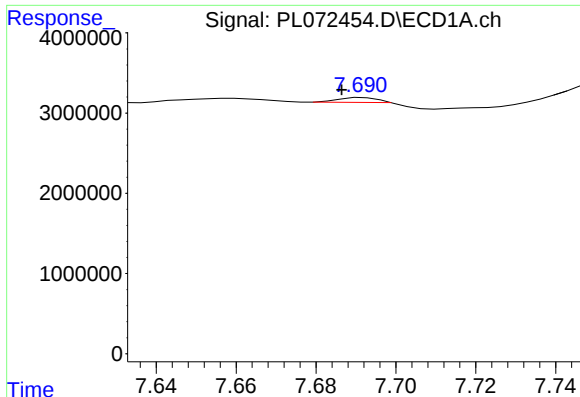

#13 Dieldrin


R.T.: 7.690 min
Delta R.T.: 0.004 min
Response: 406143
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE

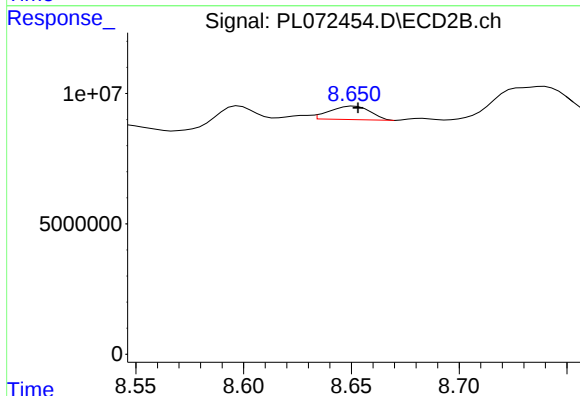


#13 Dieldrin

R.T.: 8.650 min
Delta R.T.: -0.003 min
Response: 6586907
Conc: 3.35 ng/ml m

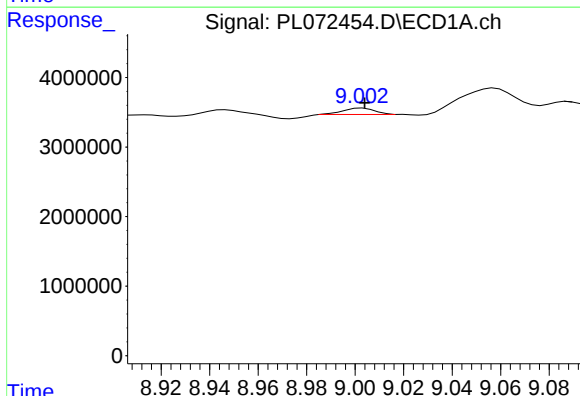


#20 Methoxychlor

R.T.: 9.002 min
Delta R.T.: -0.002 min
Response: 847600
Conc: 2.01 ng/ml m

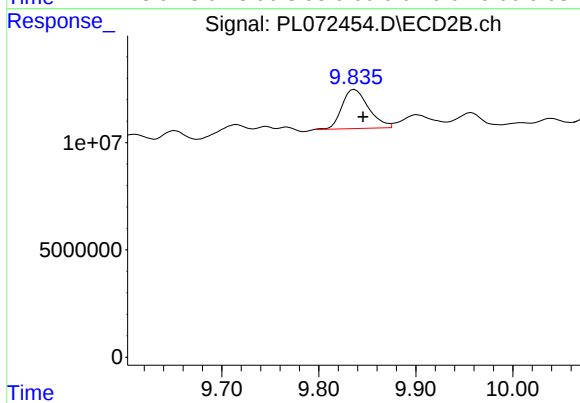

#20 Methoxychlor


R.T.: 9.837 min
Delta R.T.: -0.009 min
Response: 34658736
Conc: 41.84 ng/ml

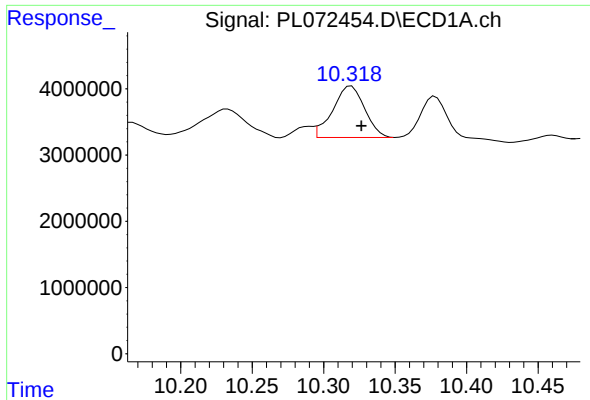

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: -0.008 min
Response: 11913303
Conc: 13.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE

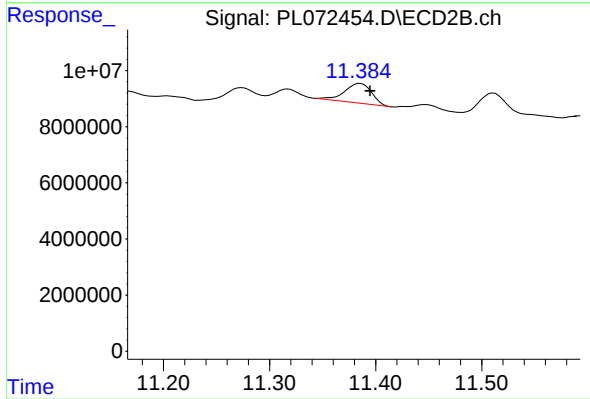

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.011 min
Response: 12230638
Conc: 7.58 ng/ml m