

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
 Data File : PL072470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2022 18:20
 Operator : AR\AJ
 Sample : N1400-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS1-WC-L-MH-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:33:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.490	8070071	24697306	14.536m	15.207m
28)	SA Decachlor...	10.317	11.384	8896016	17743739	10.013m	10.997
Target Compounds							
6)	B beta-BHC	6.072	6.727	301810	832096	0.913	0.840



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020422\
Data File : PL072470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2022 18:20
Operator : AR\AJ
Sample : N1400-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
KTS1-WC-L-MH-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:33:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

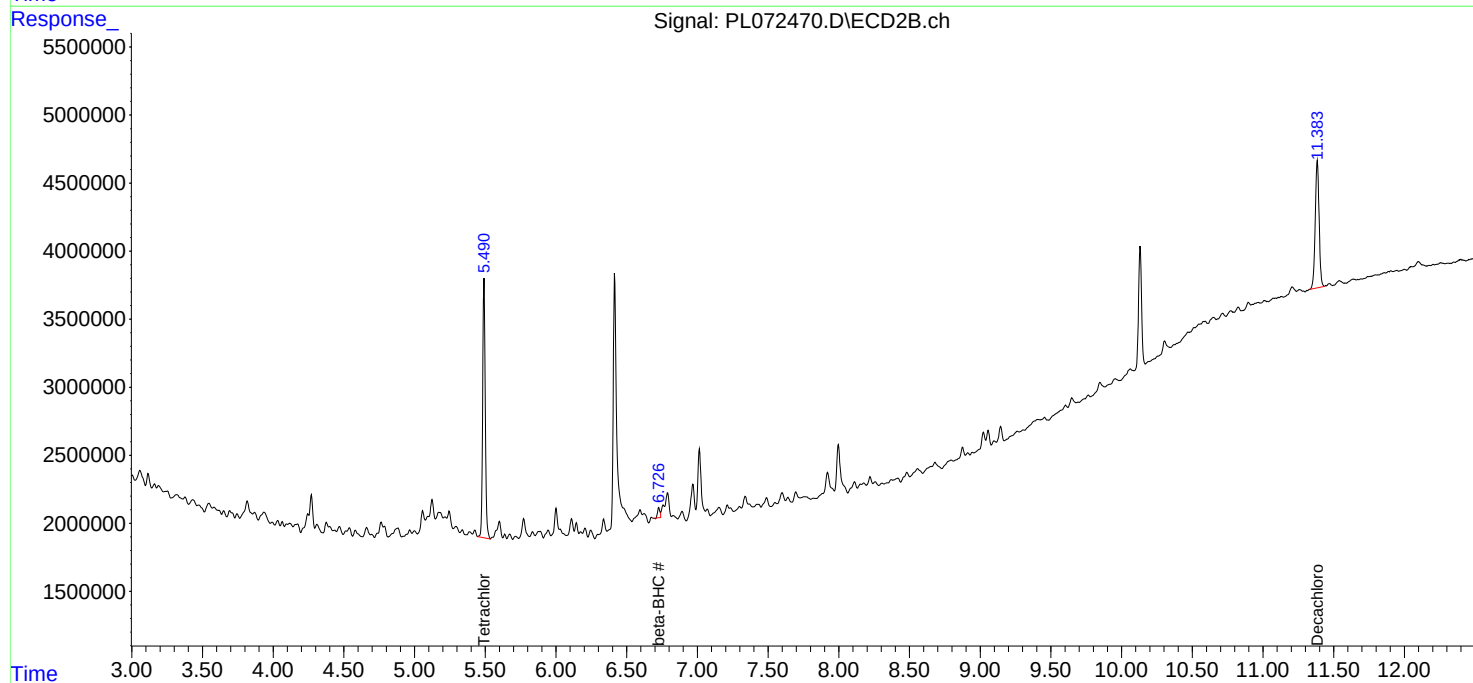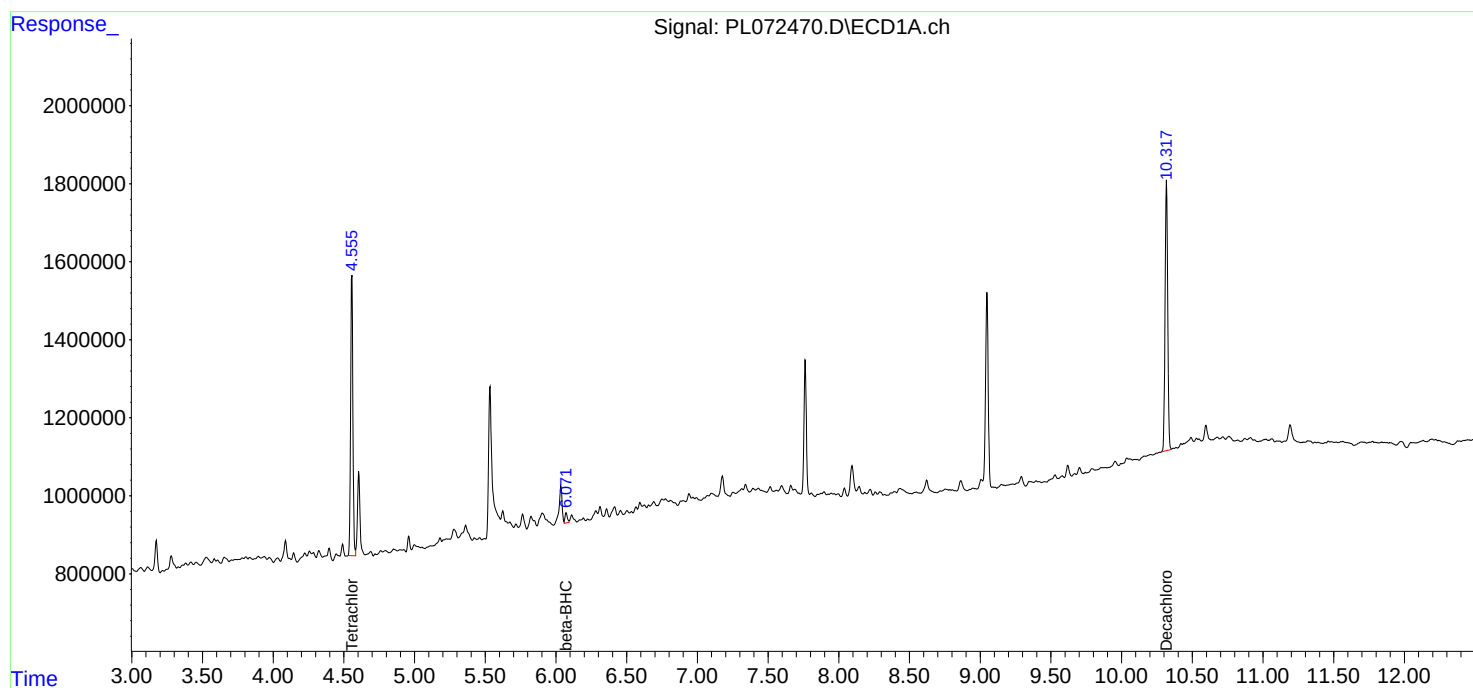


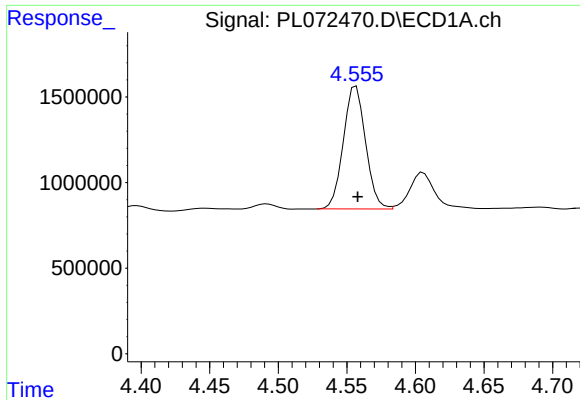

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 8070071
Conc: 14.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS1-WC-L-MH-02

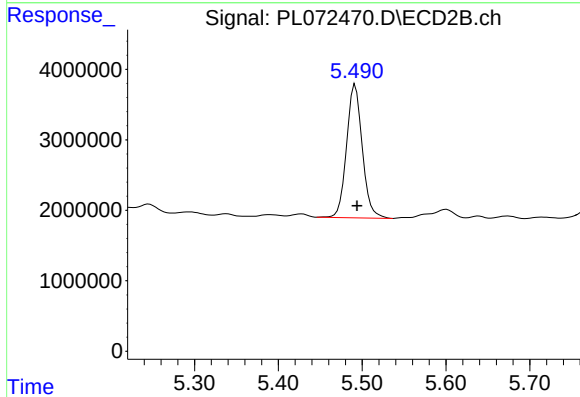


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.004 min
Response: 24697306
Conc: 15.21 ng/ml m

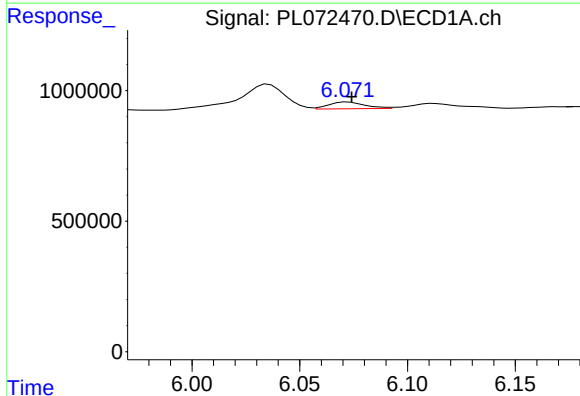


#6 beta-BHC

R.T.: 6.072 min
Delta R.T.: -0.002 min
Response: 301810
Conc: 0.91 ng/ml

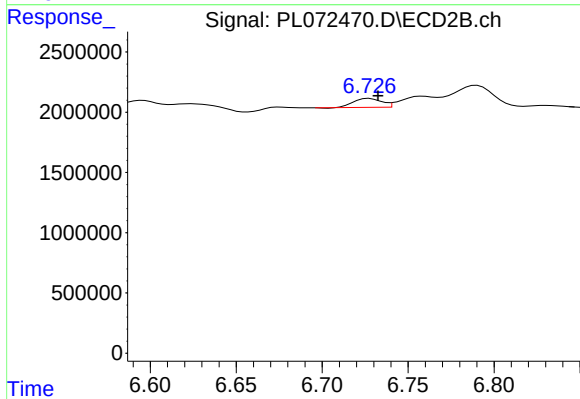

#6 beta-BHC


R.T.: 6.727 min
Delta R.T.: -0.005 min
Response: 832096
Conc: 0.84 ng/ml

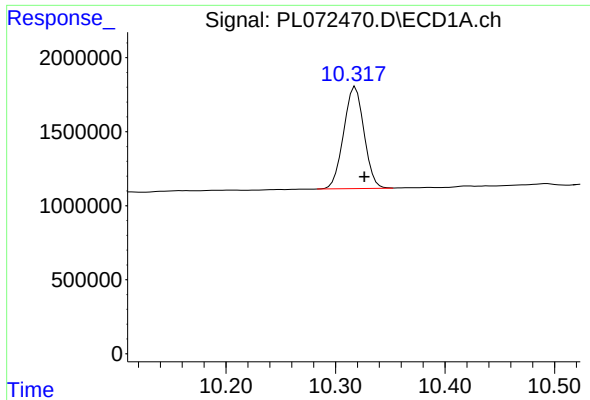

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.010 min
Response: 8896016
Conc: 10.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS1-WC-L-MH-02

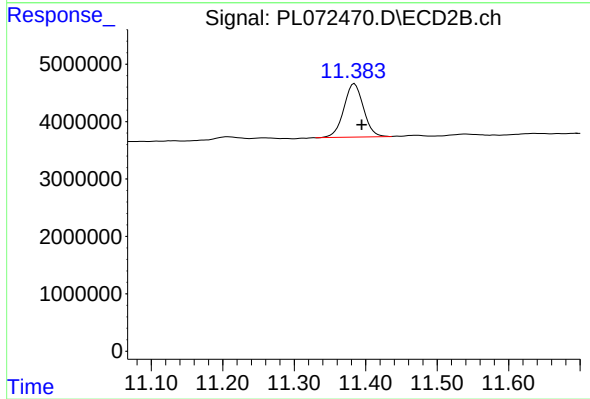

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.010 min
Response: 17743739
Conc: 11.00 ng/ml