

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020425\
 Data File : PL094043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2025 12:42
 Operator : AR\AJ
 Sample : PB166527BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB166527BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/05/2025
 Supervised By : Ankita Jodhani 02/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:38:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.775	62167298	71837452	23.087	22.008
28) SA Decachlor...	9.066	7.913	48857880	76646147	23.356m	21.873m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020425\
Data File : PL094043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2025 12:42
Operator : AR\AJ
Sample : PB166527BL
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB166527BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/05/2025
Supervised By : Ankita Jodhani 02/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:38:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

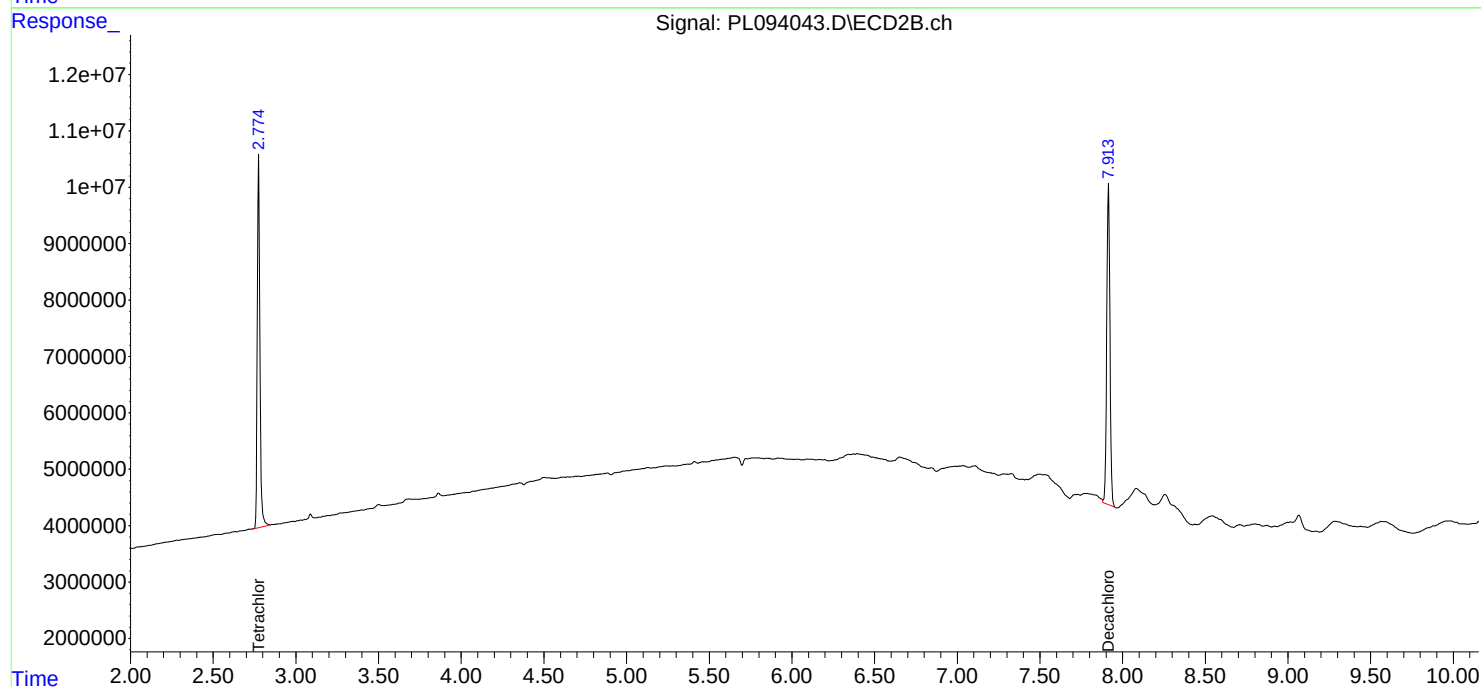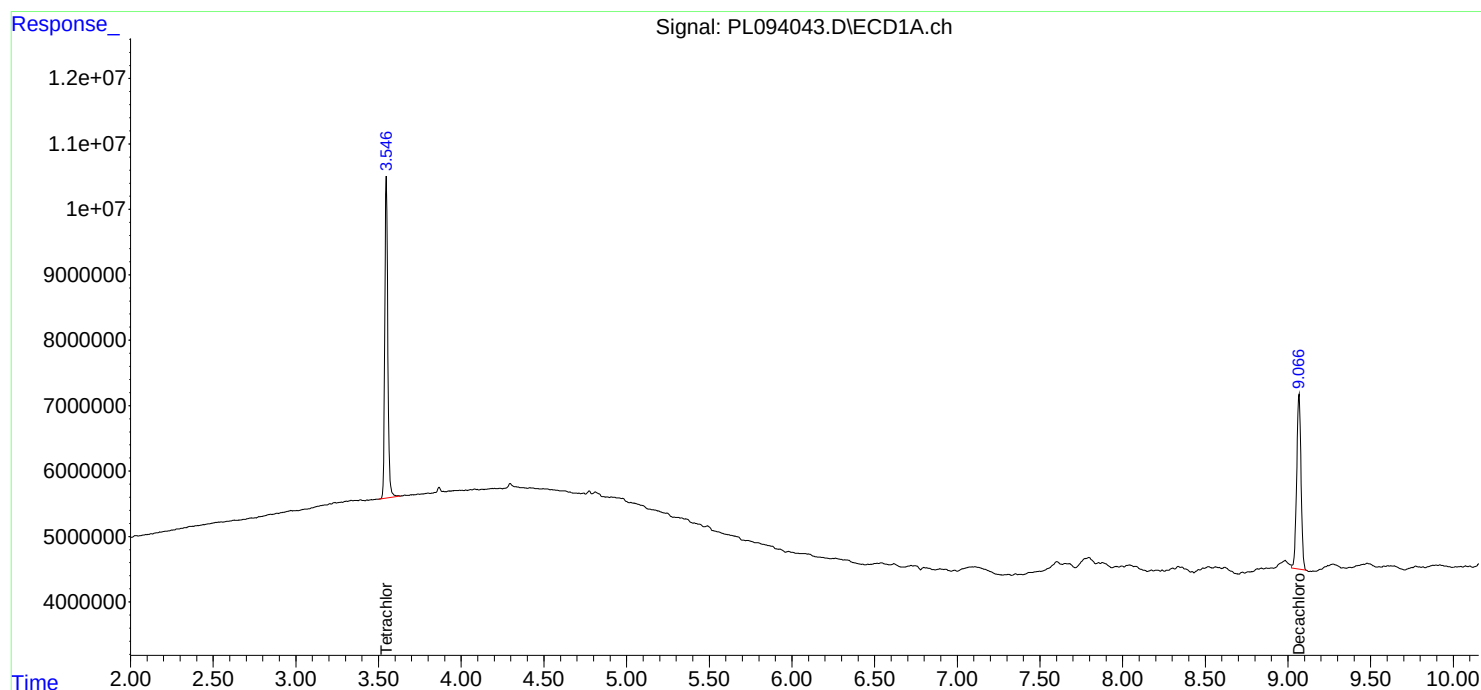

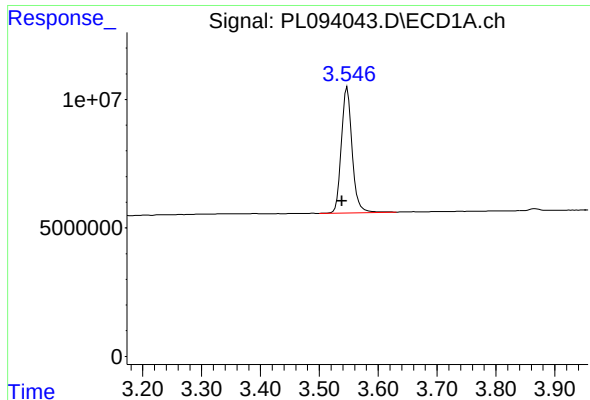


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.008 min
Response: 62167298
Conc: 23.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB166527BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/05/2025
Supervised By :Ankita Jodhani 02/05/2025

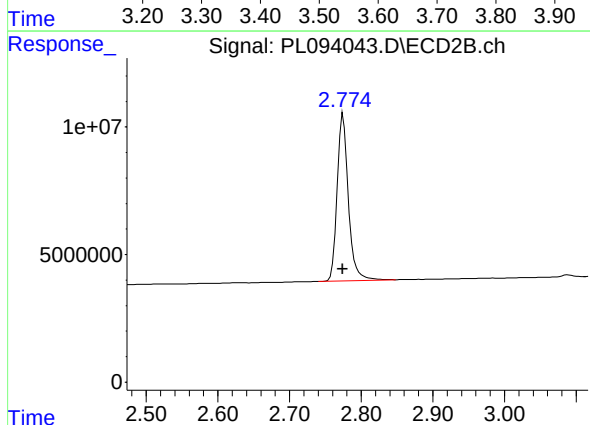


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 71837452
Conc: 22.01 ng/ml

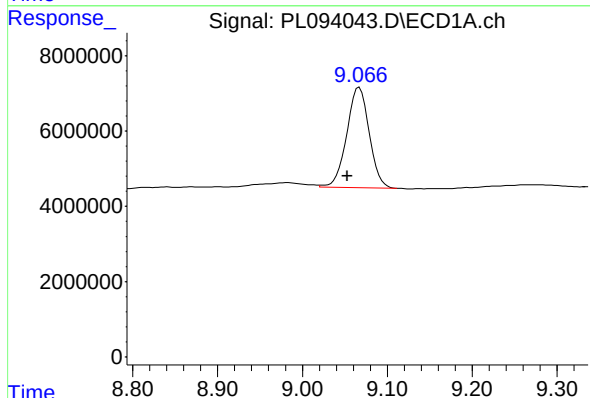

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.013 min
Response: 48857880
Conc: 23.36 ng/ml m

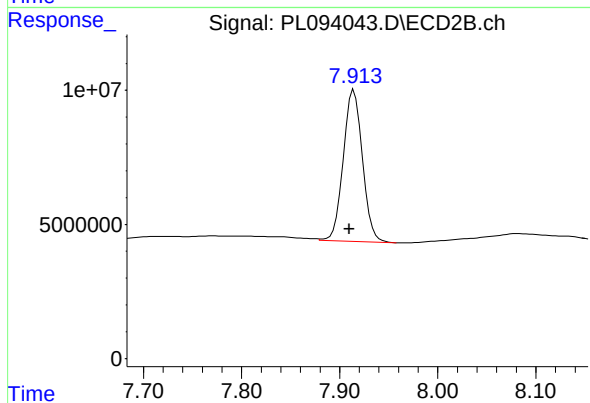

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.003 min
Response: 76646147
Conc: 21.87 ng/ml m