

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020520\
 Data File : PL056336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2020 13:56
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:48:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
10) B	gamma-Chl...	5.462f	0.000	4677350	0	0.298	N.D. #
14) MA	Endrin	6.066	0.000	31181233	0	2.219	N.D. #
17) MA	4,4'-DDT	6.392f	0.000	51703285	0	4.731	N.D. #
23)	Chlordane-1	4.377	0.000	2435824	0	6.435	N.D. #
25)	Chlordane-3	5.462f	0.000	4677350	0	3.705	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020520\
Data File : PL056336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2020 13:56
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:48:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

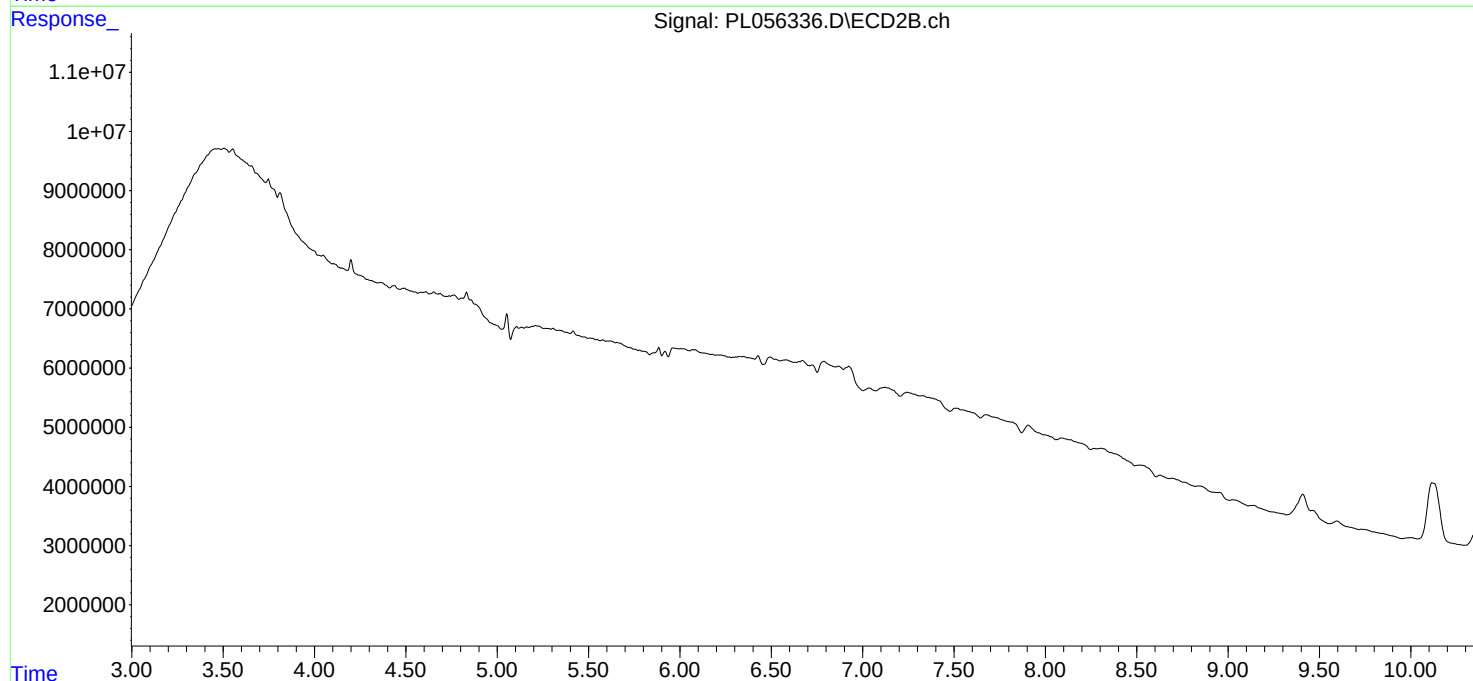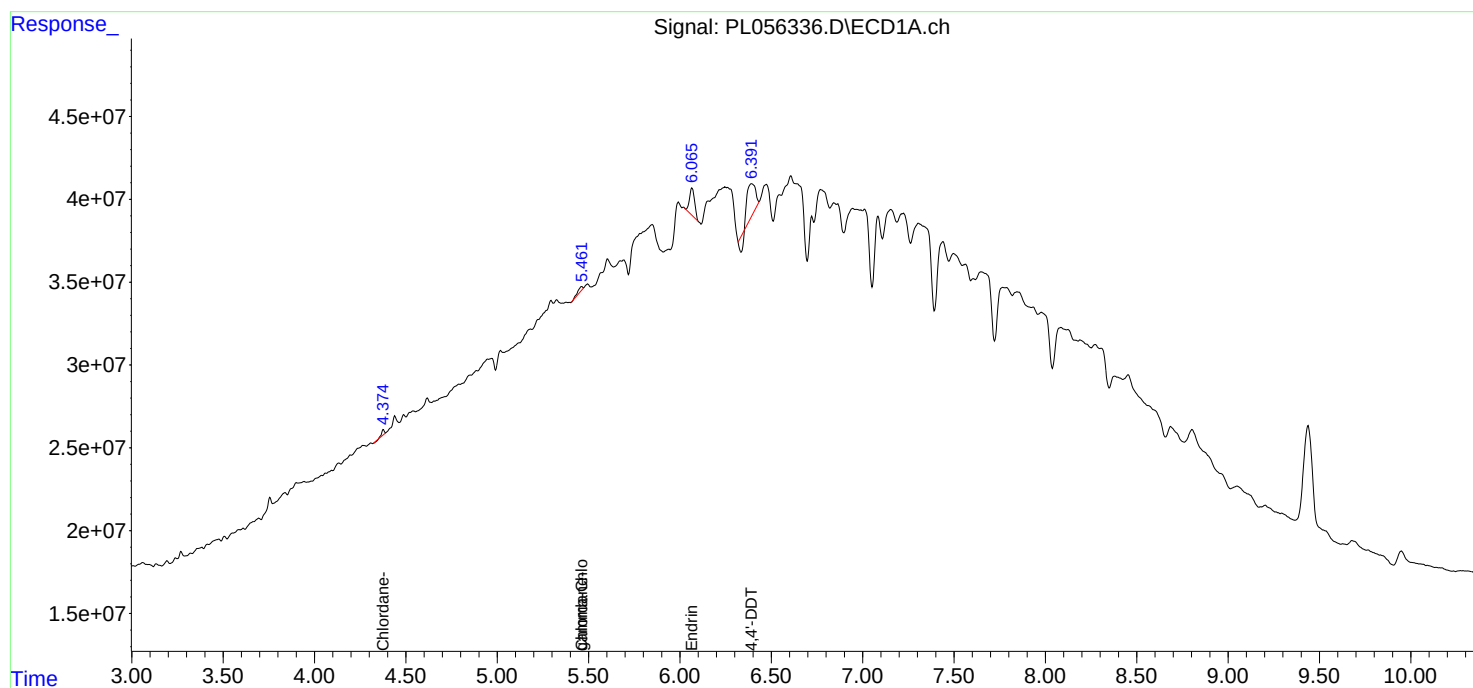


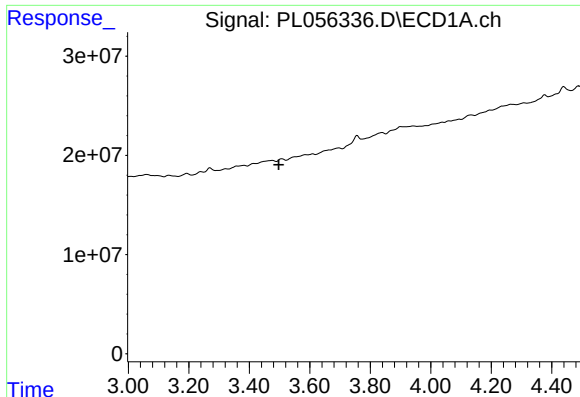

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

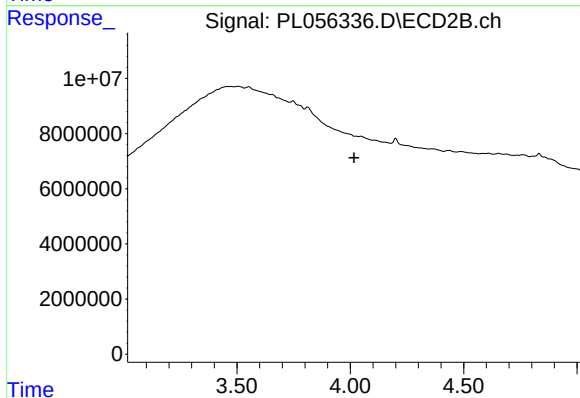


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.016 min
Response: 0
Conc: N.D.

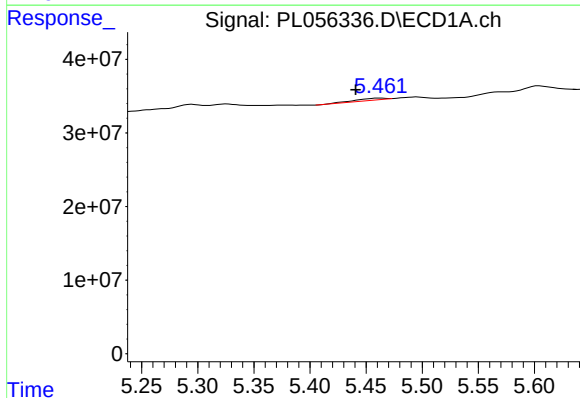


#10 gamma-Chlordane

R.T.: 5.462 min
Delta R.T.: 0.022 min
Response: 4677350
Conc: 0.30 ng/ml

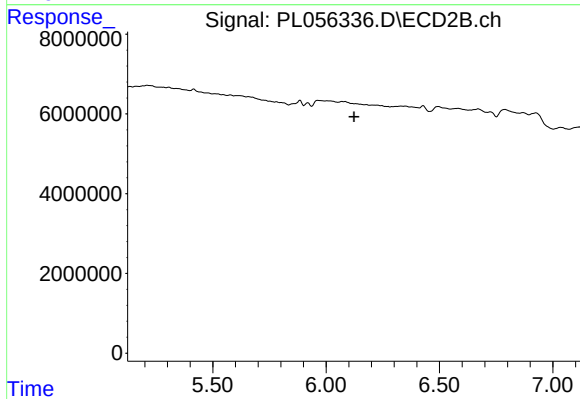

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.124 min
Response: 0
Conc: N.D.

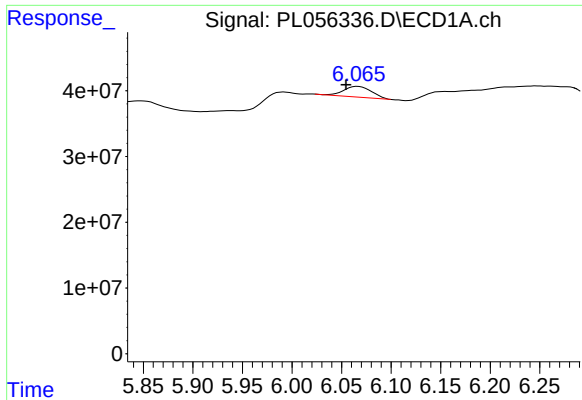

#14 Endrin


R.T.: 6.066 min
Delta R.T.: 0.011 min
Response: 31181233
Conc: 2.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

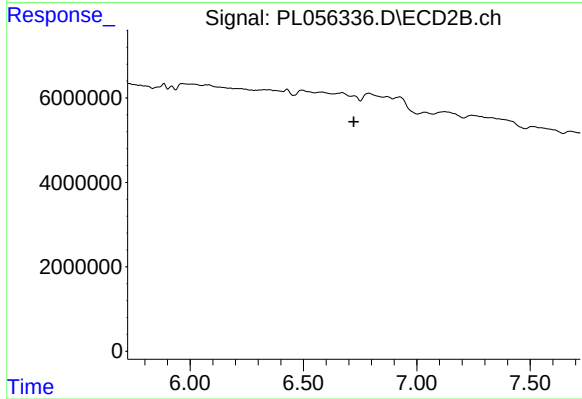


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.723 min
Response: 0
Conc: N.D.

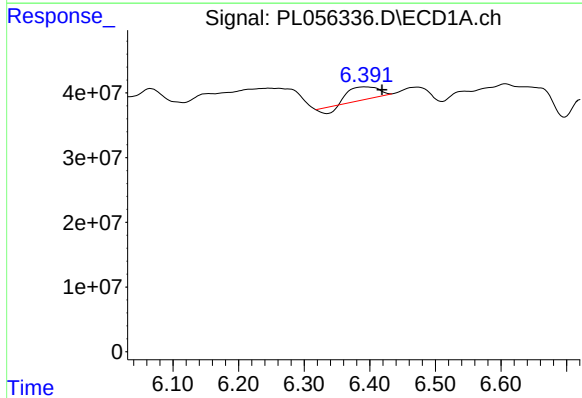


#17 4,4'-DDT

R.T.: 6.392 min
Delta R.T.: -0.026 min
Response: 51703285
Conc: 4.73 ng/ml

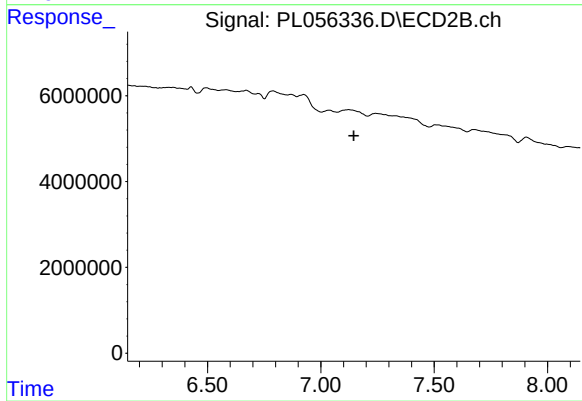

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

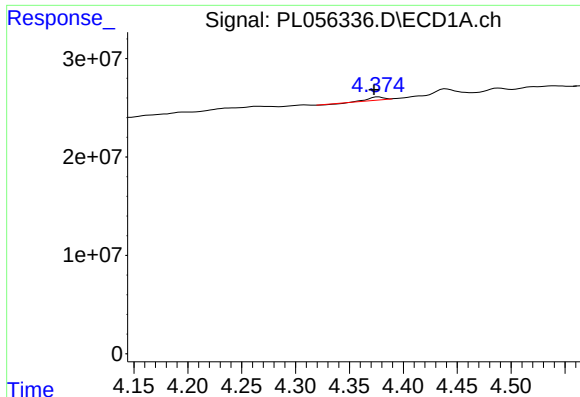

#23 Chlordane-1


R.T.: 4.377 min
Delta R.T.: 0.004 min
Response: 2435824
Conc: 6.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

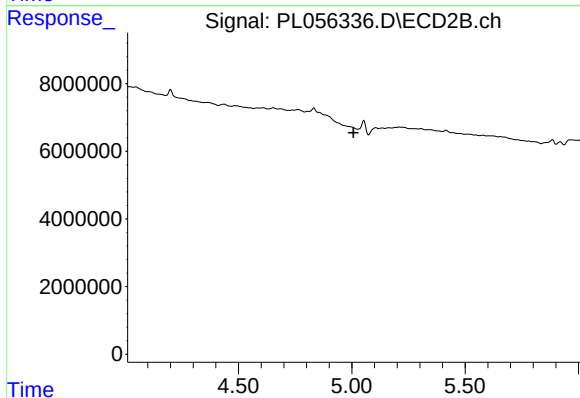


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

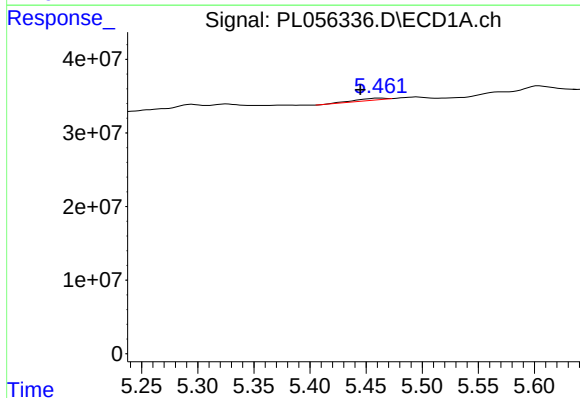


#25 Chlordane-3

R.T.: 5.462 min
Delta R.T.: 0.018 min
Response: 4677350
Conc: 3.70 ng/ml

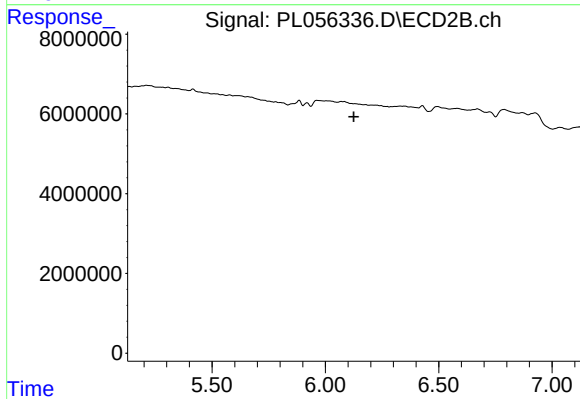

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

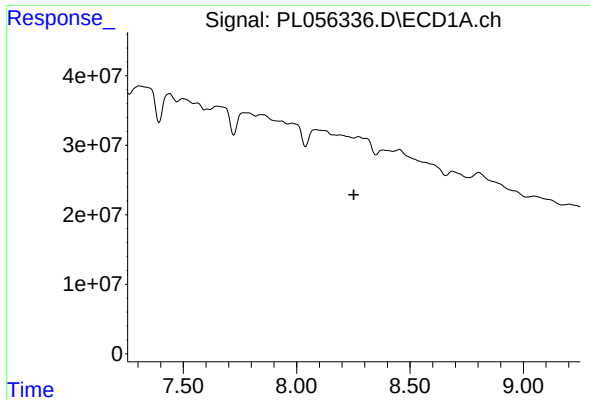

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.252 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

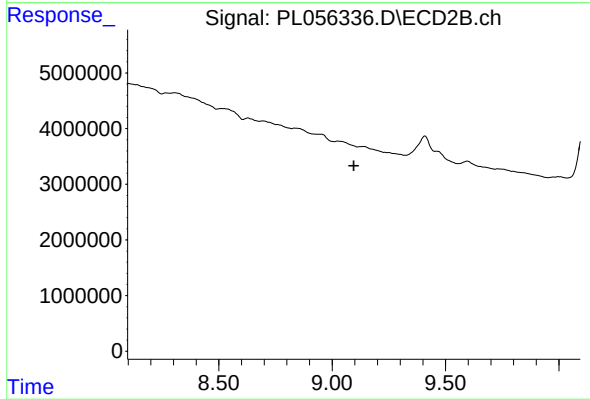

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.096 min
Response: 0
Conc: N.D.