

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020520\
 Data File : PL056340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2020 15:58
 Operator : AJ\MA
 Sample : PB126587BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:49:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.015	235.8E6	70851559	22.514	24.230
28)	SA Decachlor...	8.260	9.095	253.4E6	56589478	24.069	25.018
Target Compounds							
4)	MA Heptachlor	4.513	0.000	79422322	0	4.947	N.D. #
7)	B delta-BHC	4.675	5.054f	11761714	23838812	0.734	7.433 #
11)	B alpha-Chl...	5.493	0.000	53068307	0	3.450	N.D. #
12)	B 4,4'-DDE	5.690f	0.000	4261539	0	0.294	N.D. #
15)	B Endosulfa...	6.344f	6.947	8794670	9355705	0.672	3.475 #
21)	B Endrin ke...	0.000	7.750	0	7258034	N.D.	2.722 #
23)	Chlordane-1	4.356f	0.000	16796268	0	44.371	N.D. #
26)	Chlordane-4	5.493	0.000	53068307	0	49.045	N.D. #
27)	Chlordane-5	6.344	0.000	8794670	0	21.201	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020520\
Data File : PL056340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2020 15:58
Operator : AJ\MA
Sample : PB126587BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:49:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

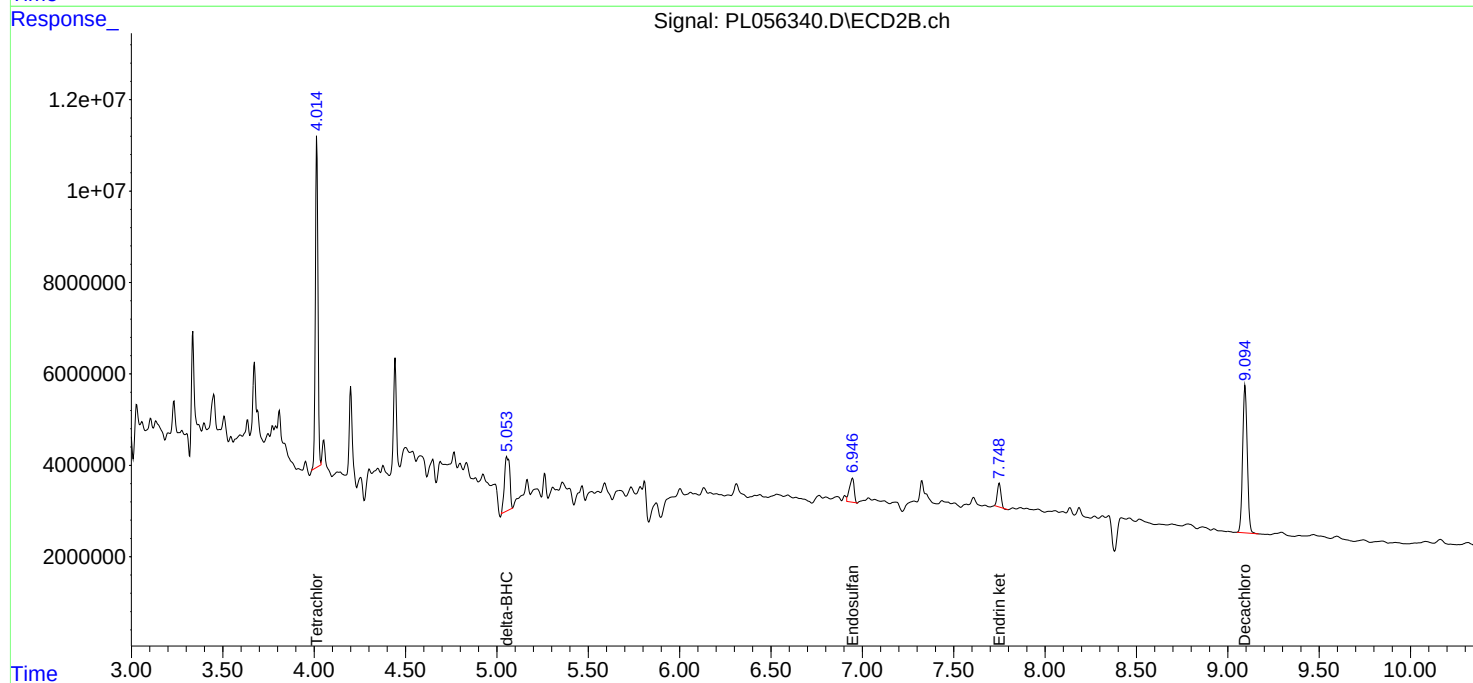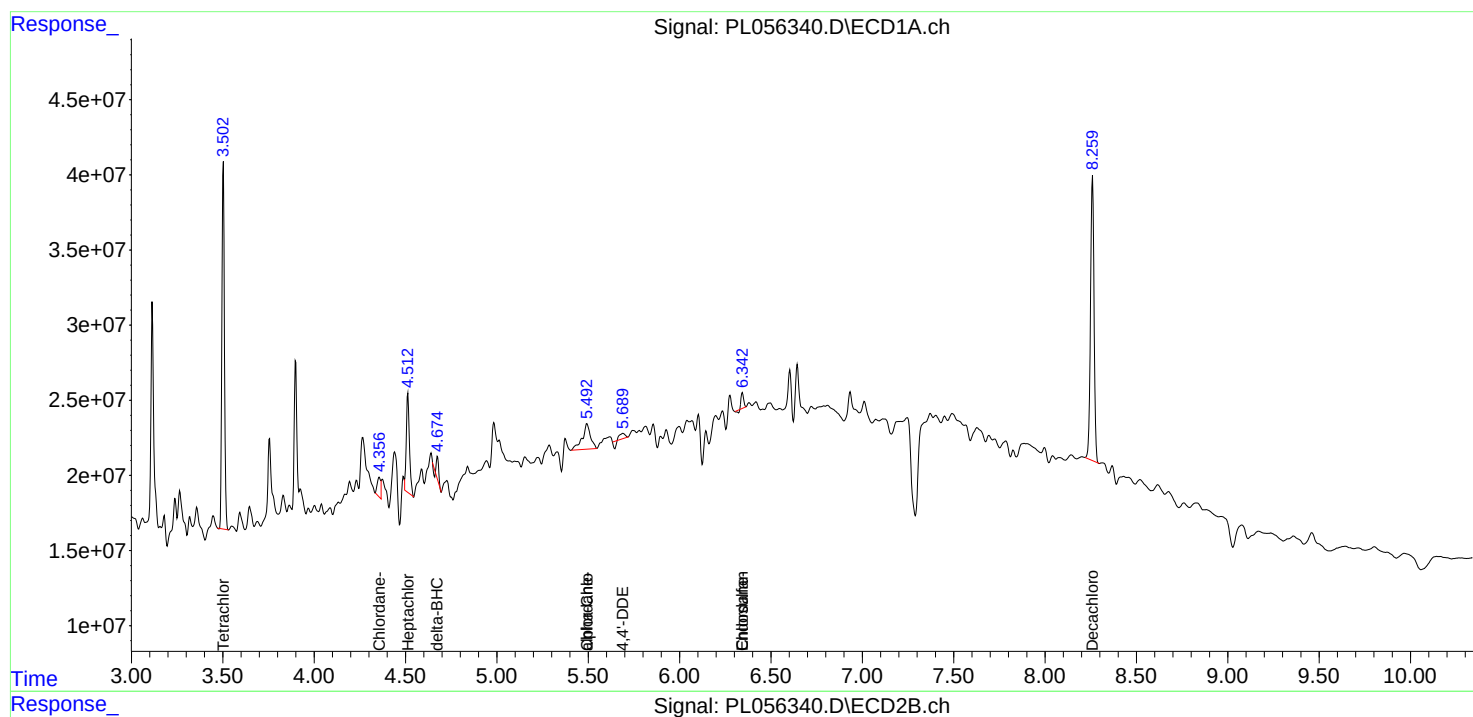


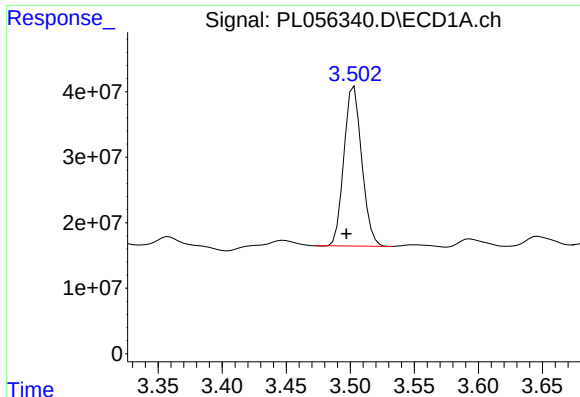

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.006 min
Response: 235785114
Conc: 22.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

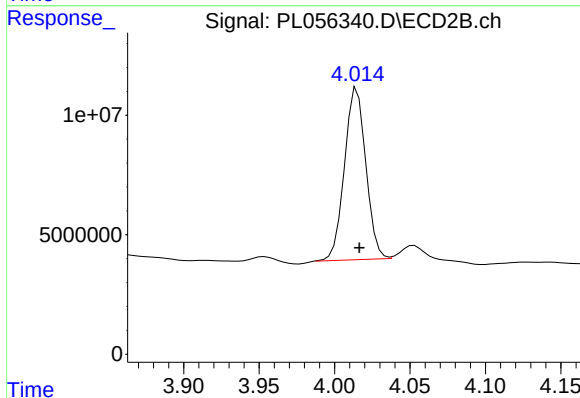


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.001 min
Response: 70851559
Conc: 24.23 ng/ml

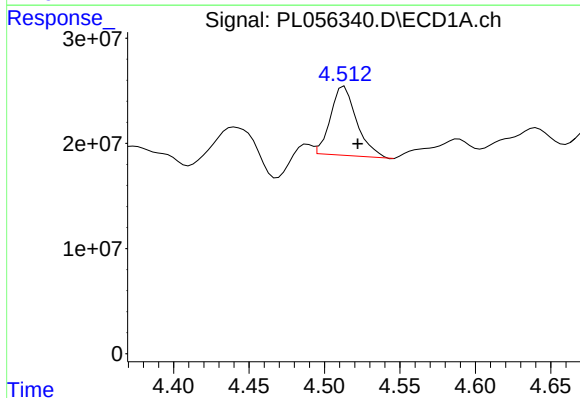


#4 Heptachlor

R.T.: 4.513 min
Delta R.T.: -0.009 min
Response: 79422322
Conc: 4.95 ng/ml

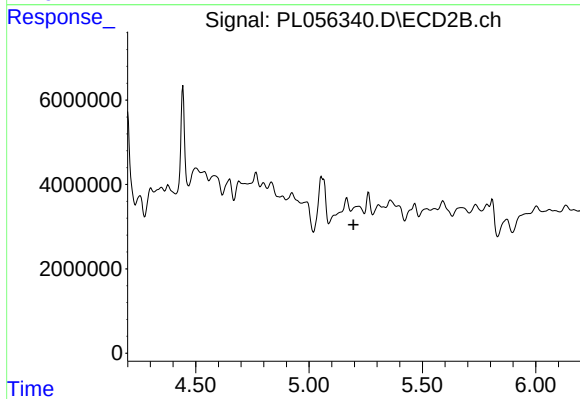

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

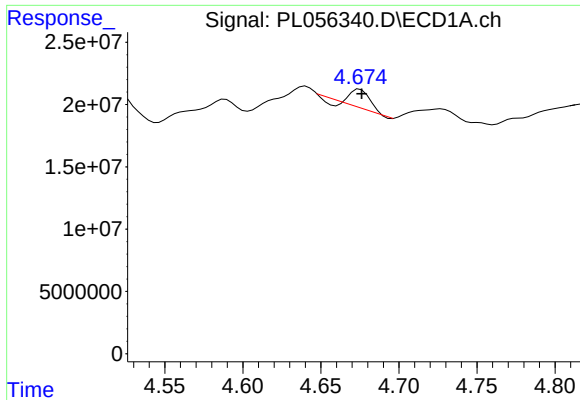

#7 delta-BHC


R.T.: 4.675 min
Delta R.T.: 0.000 min
Response: 11761714
Conc: 0.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

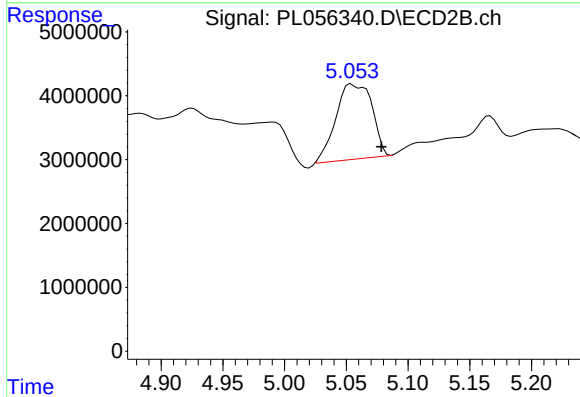


#7 delta-BHC

R.T.: 5.054 min
Delta R.T.: -0.024 min
Response: 23838812
Conc: 7.43 ng/ml

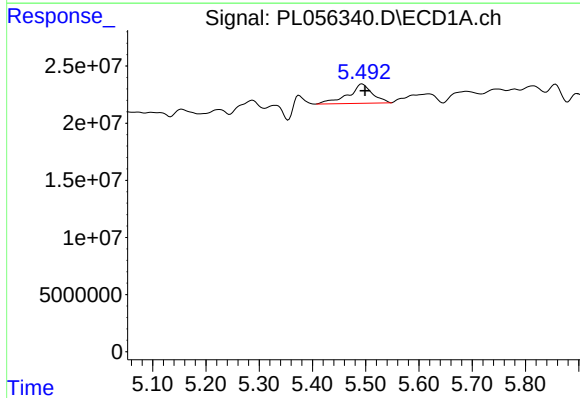


#11 alpha-Chlordane

R.T.: 5.493 min
Delta R.T.: -0.006 min
Response: 53068307
Conc: 3.45 ng/ml

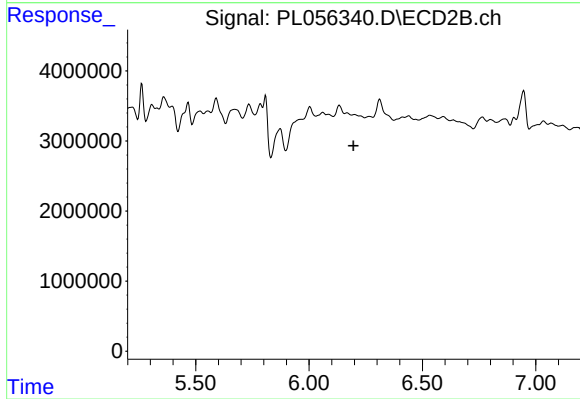

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

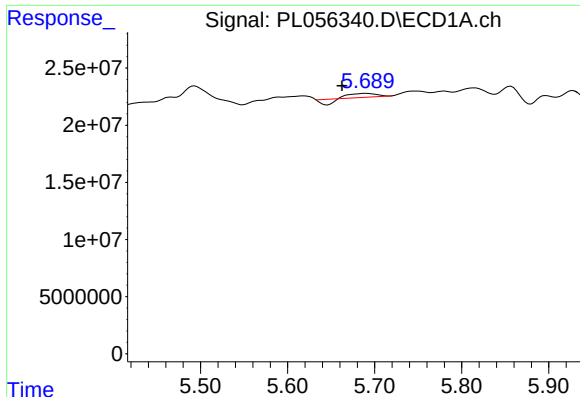

#12 4,4'-DDE


R.T.: 5.690 min
Delta R.T.: 0.028 min
Response: 4261539
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

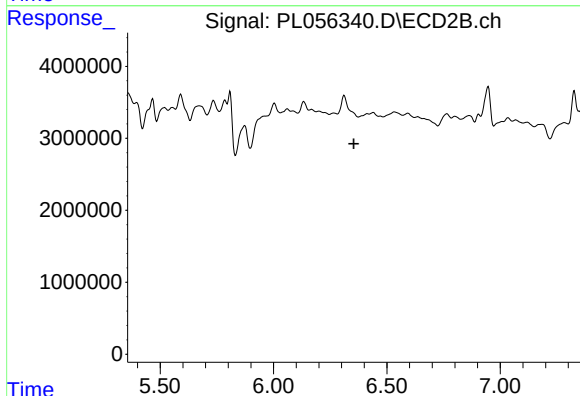


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

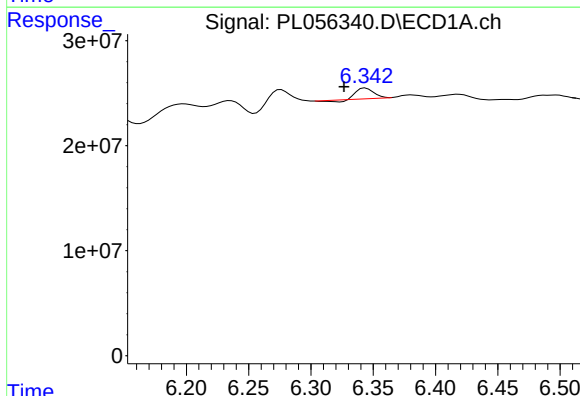


#15 Endosulfan II

R.T.: 6.344 min
Delta R.T.: 0.017 min
Response: 8794670
Conc: 0.67 ng/ml

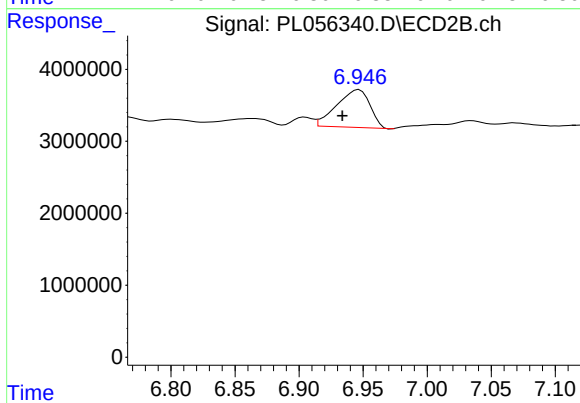

#15 Endosulfan II


R.T.: 6.947 min
Delta R.T.: 0.013 min
Response: 9355705
Conc: 3.48 ng/ml

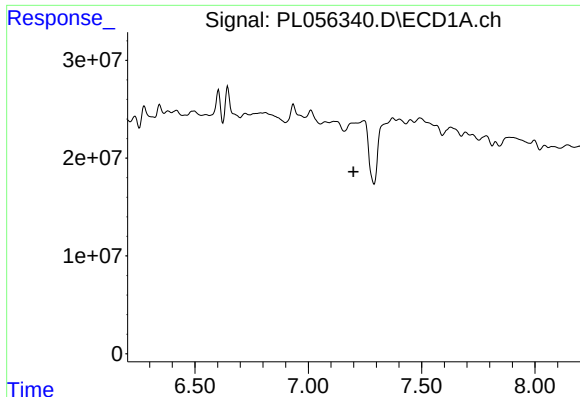

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

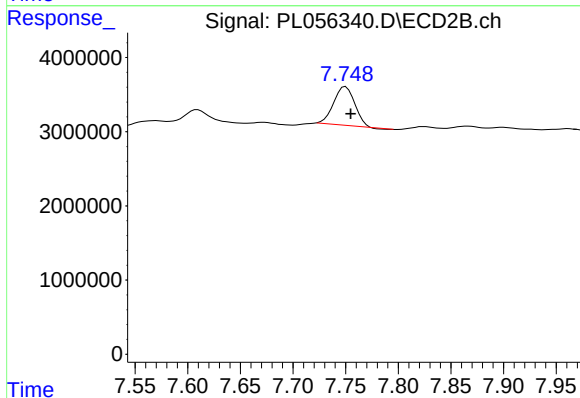


#21 Endrin ketone

R.T.: 7.750 min
Delta R.T.: -0.005 min
Response: 7258034
Conc: 2.72 ng/ml

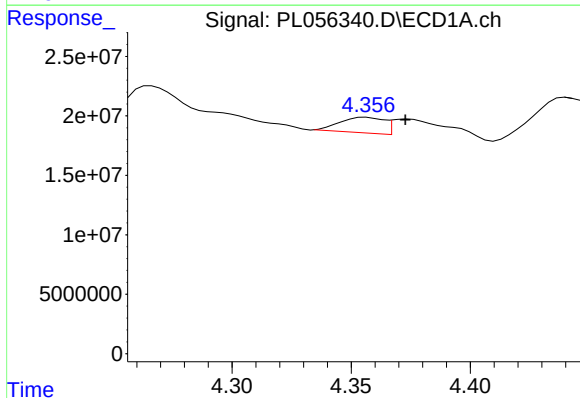


#23 Chlordane-1

R.T.: 4.356 min
Delta R.T.: -0.016 min
Response: 16796268
Conc: 44.37 ng/ml

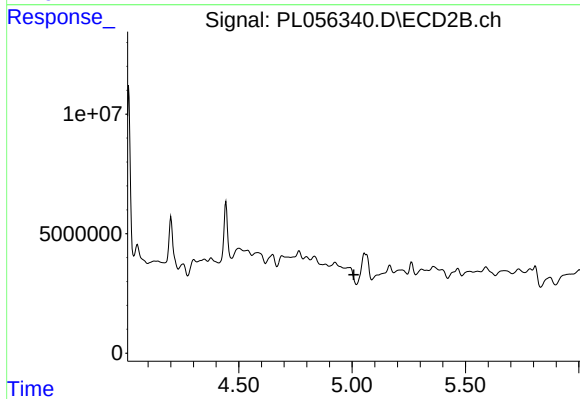

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

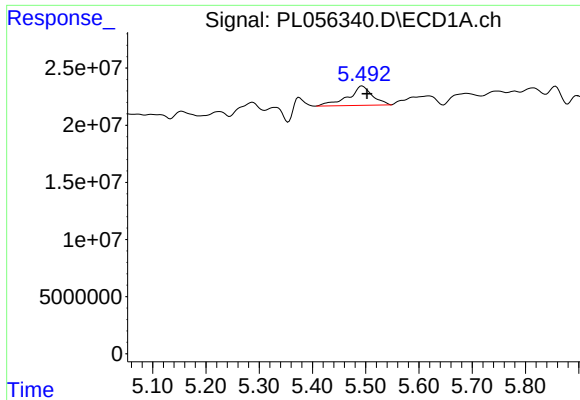

#26 Chlordane-4


R.T.: 5.493 min
Delta R.T.: -0.009 min
Response: 53068307
Conc: 49.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

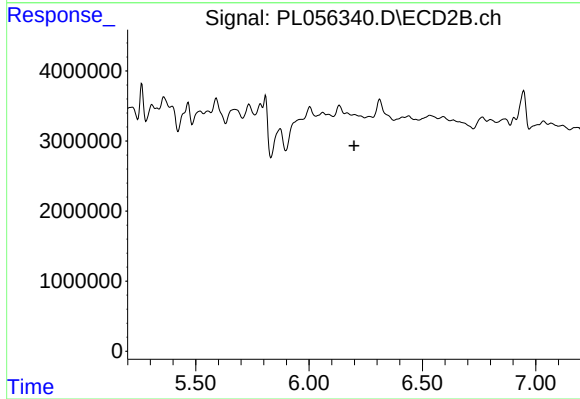


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

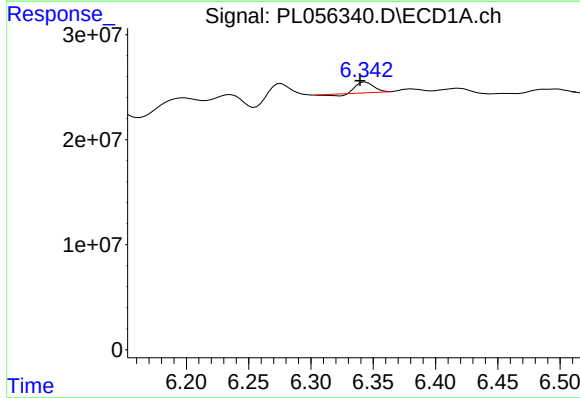


#27 Chlordane-5

R.T.: 6.344 min
Delta R.T.: 0.004 min
Response: 8794670
Conc: 21.20 ng/ml

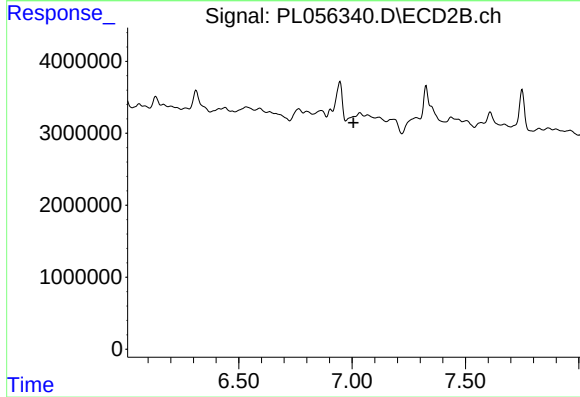

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

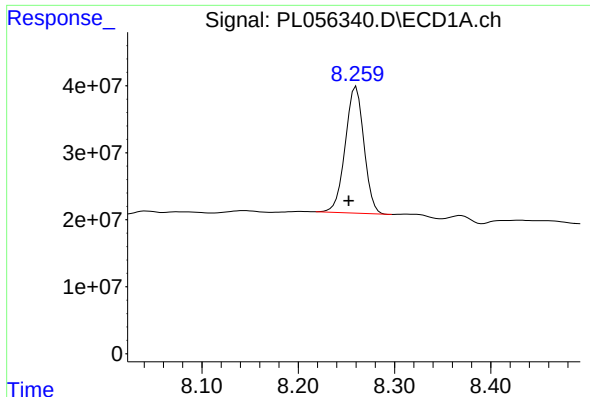

#28 Decachlorobiphenyl

R.T.: 8.260 min
Delta R.T.: 0.008 min
Response: 253399455
Conc: 24.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

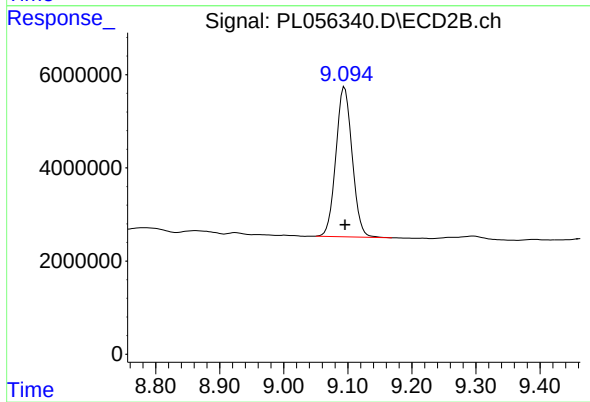

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 56589478
Conc: 25.02 ng/ml