

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020520\
 Data File : PL056351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2020 18:33
 Operator : AJ\MA
 Sample : L1388-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TOTE-COMP

Manual Integrations
 APPROVED

mohammad
 2/6/2020 12:36:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 00:52:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.499	4.013	884.4E6	45701875	84.446	15.629m#
28)	SA Decachlor...	8.252	9.090	109.5E6	23388351	10.404	10.340

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020520\
Data File : PL056351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2020 18:33
Operator : AJ\MA
Sample : L1388-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

mohammad
2/6/2020 12:36:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 00:52:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

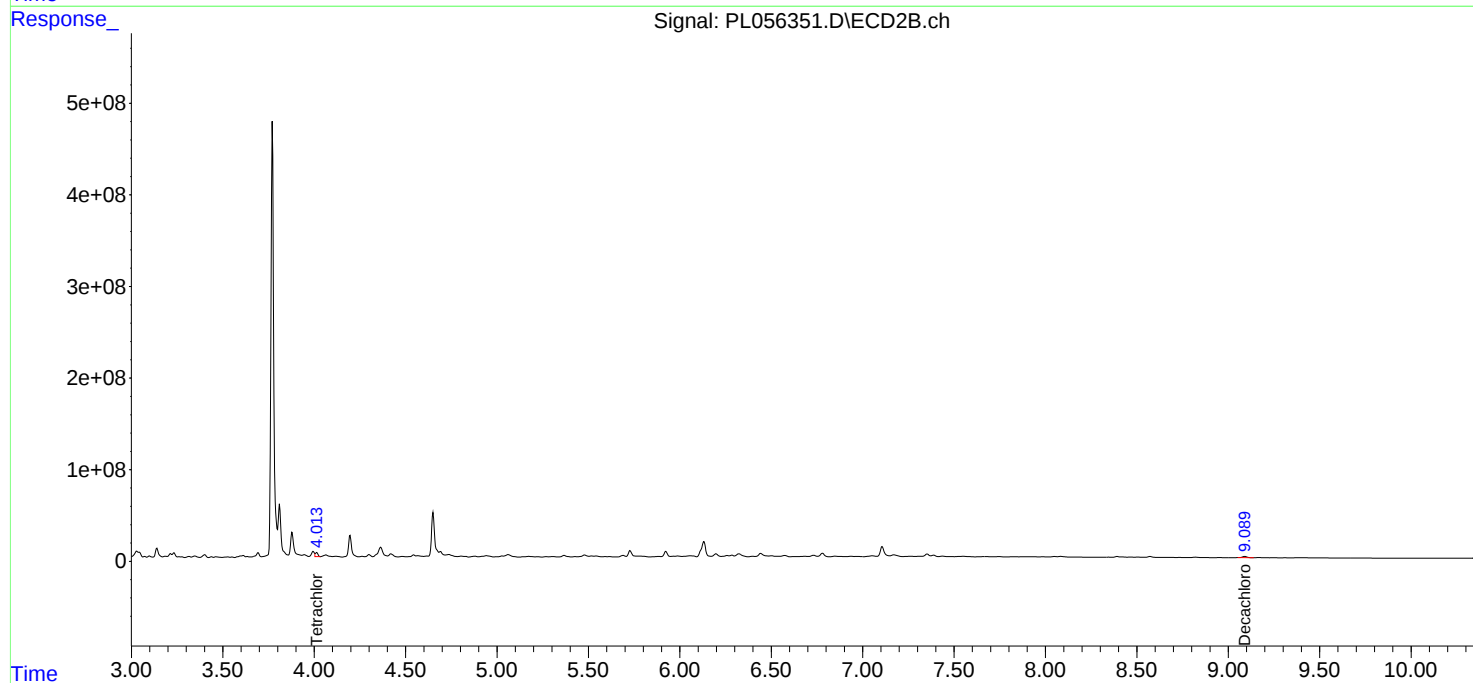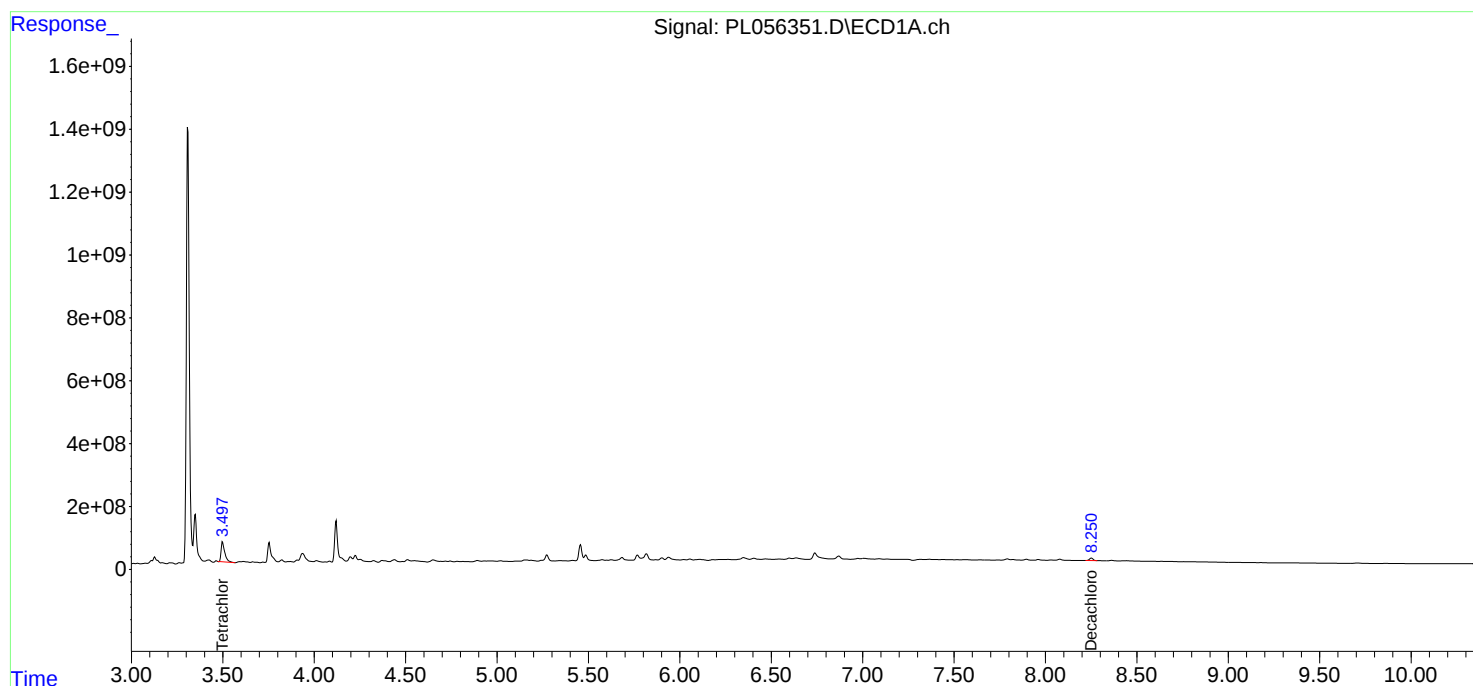

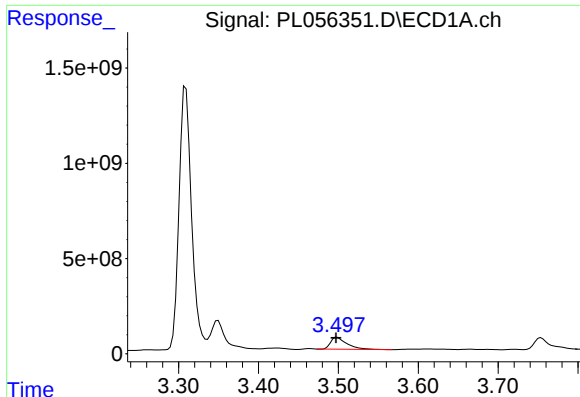


#1 Tetrachloro-m-xylene

R.T.: 3.499 min
Delta R.T.: 0.002 min
Response: 884407030
Conc: 84.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

mohammad
2/6/2020 12:36:13 PM

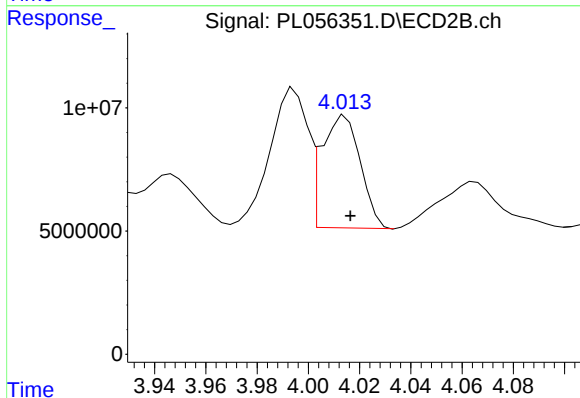


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.003 min
Response: 45701875
Conc: 15.63 ng/ml m

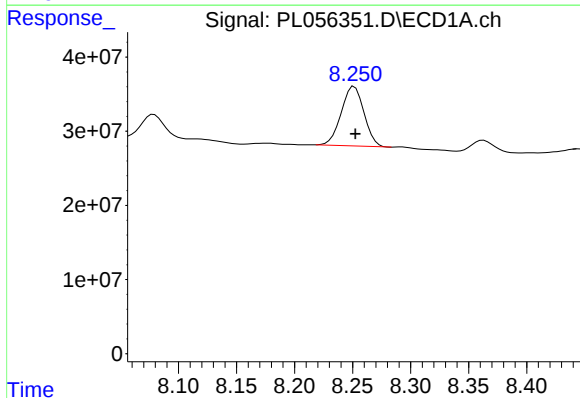

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 109531348
Conc: 10.40 ng/ml

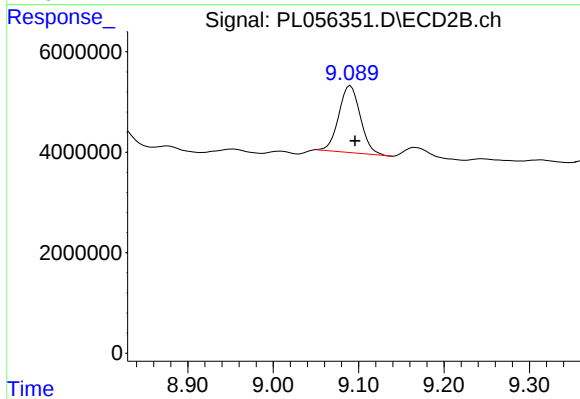

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: -0.006 min
Response: 23388351
Conc: 10.34 ng/ml