

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
 Data File : PL064643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2021 08:55
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:41:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4) MA	Heptachlor	0.000	5.303	0	9272598	N.D. 2.661 #
6) B	beta-BHC	0.000	4.984	0	4649297	N.D. 2.747 #
10) B	gamma-Chl...	0.000	6.224f	0	444968	N.D. 0.153 #
15) B	Endosulfa...	0.000	7.068	0	897799	N.D. 0.364 #
16) A	4,4'-DDD	0.000	6.951f	0	69914	N.D. 0.030 #
23)	Chlordane-1	4.307	0.000	4167221	0	37.910 N.D. #
25)	Chlordane-3	0.000	6.224f	0	444968	N.D. 1.241 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
Data File : PL064643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2021 08:55
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:41:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

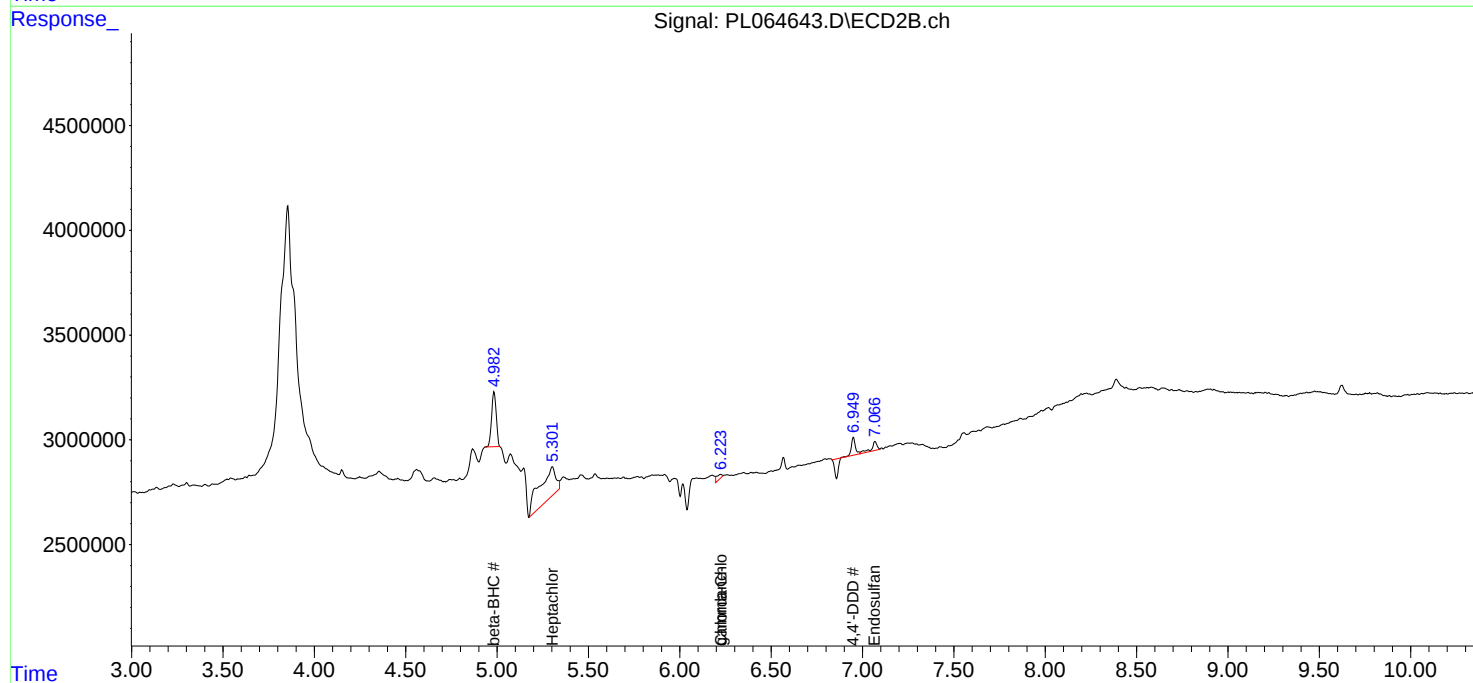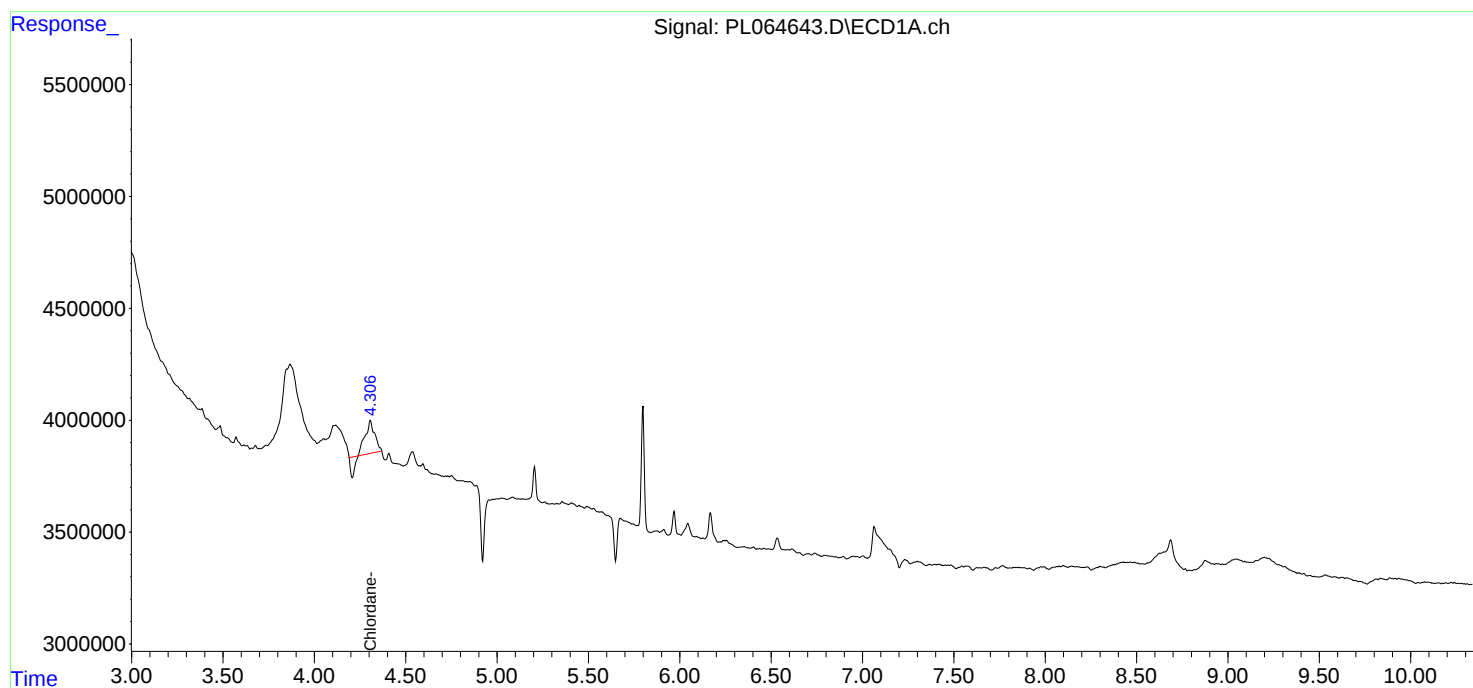


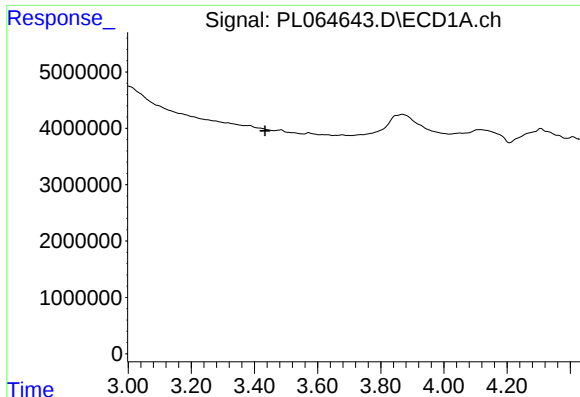

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.433 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

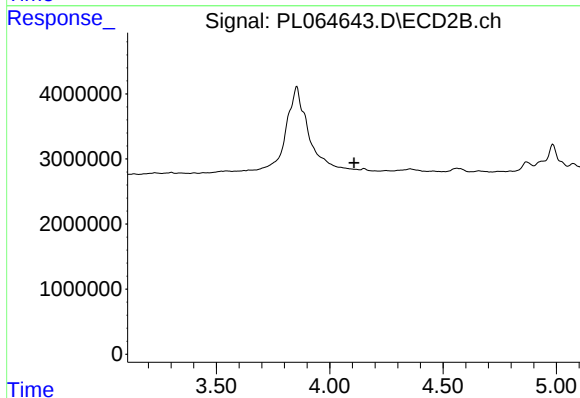


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

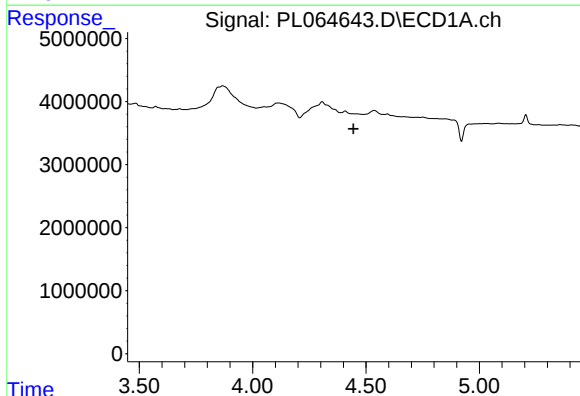


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

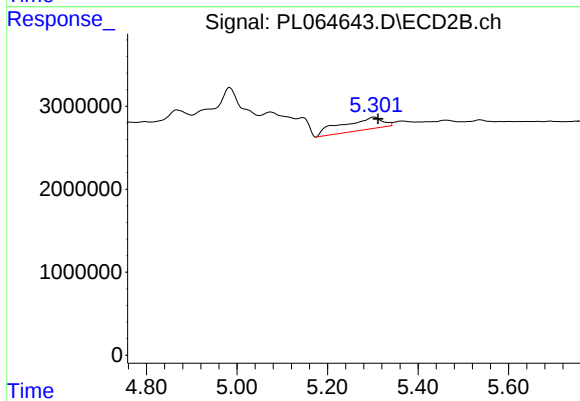

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: -0.009 min
Response: 9272598
Conc: 2.66 ng/ml

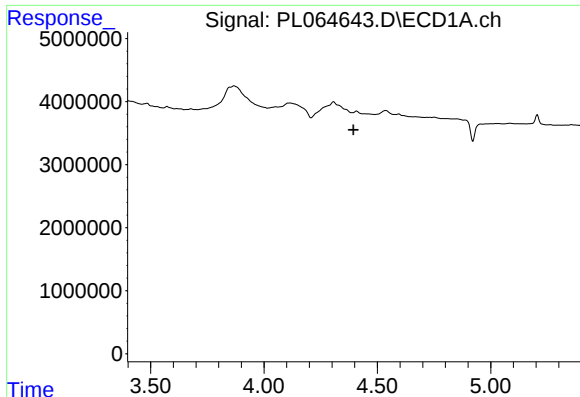

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

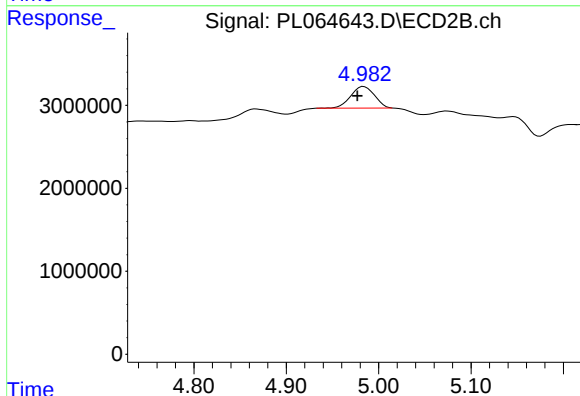


#6 beta-BHC

R.T.: 4.984 min
Delta R.T.: 0.007 min
Response: 4649297
Conc: 2.75 ng/ml

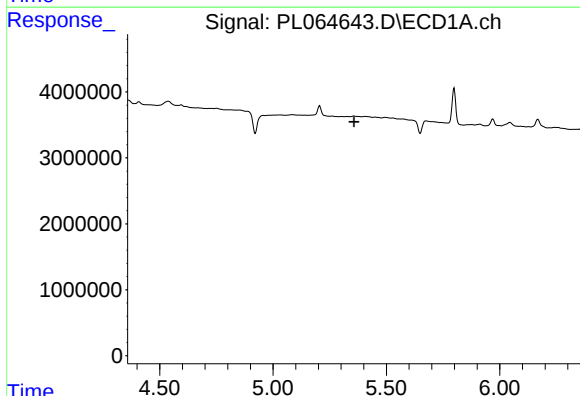


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

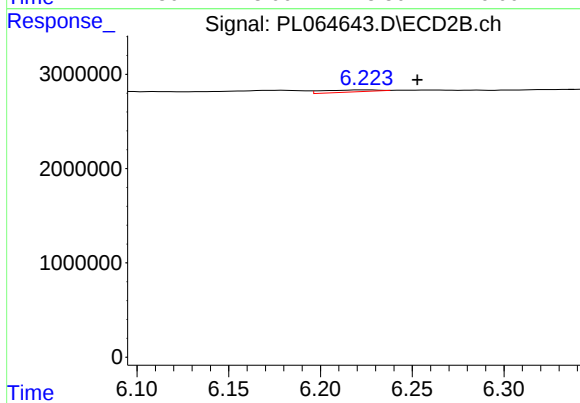

#10 gamma-Chlordane


R.T.: 6.224 min
Delta R.T.: -0.029 min
Response: 444968
Conc: 0.15 ng/ml

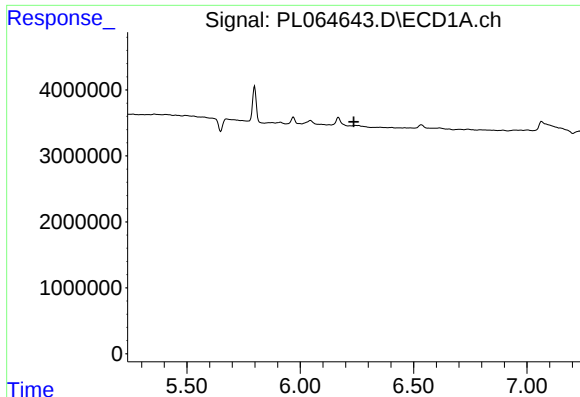

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

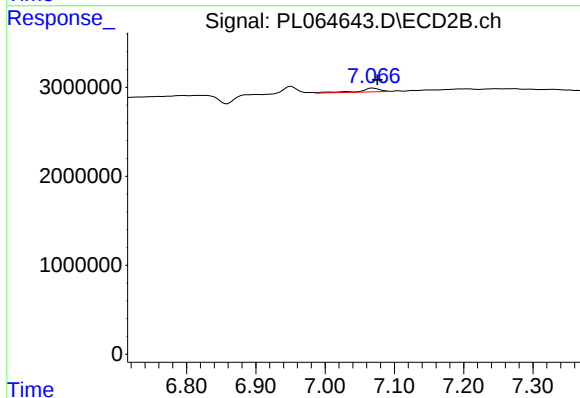


#15 Endosulfan II

R.T.: 7.068 min
Delta R.T.: -0.007 min
Response: 897799
Conc: 0.36 ng/ml

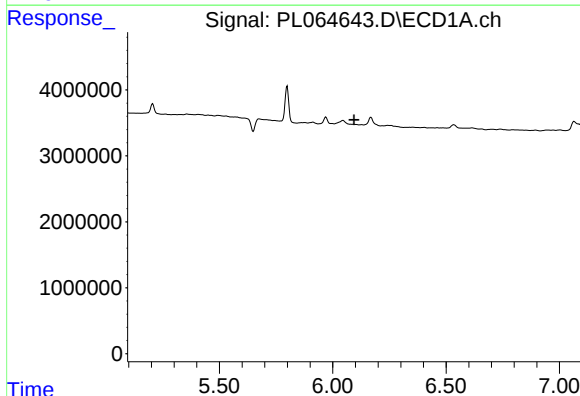


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

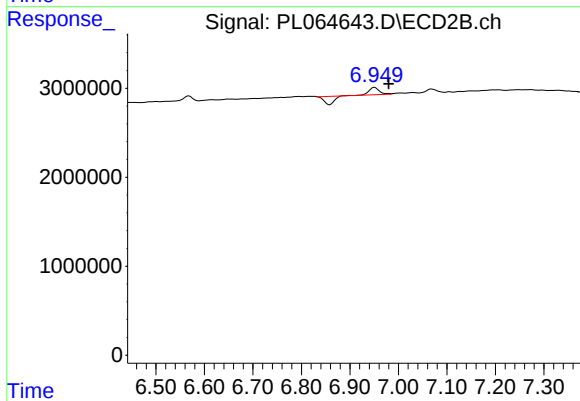

#16 4,4'-DDD


R.T.: 6.951 min
Delta R.T.: -0.029 min
Response: 69914
Conc: 0.03 ng/ml

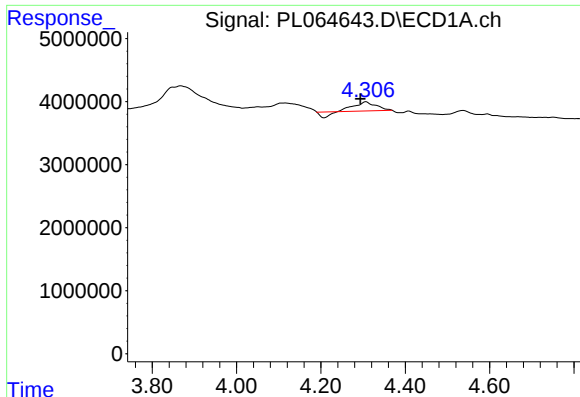

#23 Chlordane-1


R.T.: 4.307 min
Delta R.T.: 0.014 min
Response: 4167221
Conc: 37.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

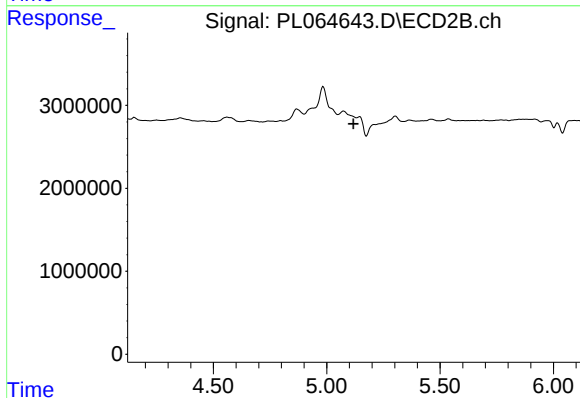


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

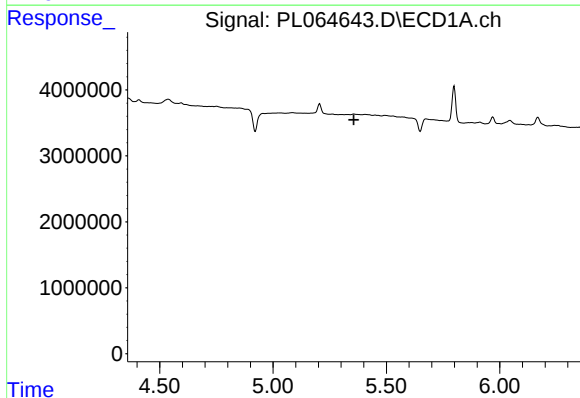


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

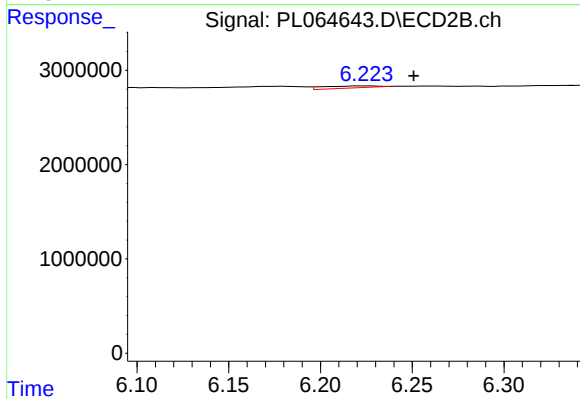

#25 Chlordane-3


R.T.: 6.224 min
Delta R.T.: -0.027 min
Response: 444968
Conc: 1.24 ng/ml

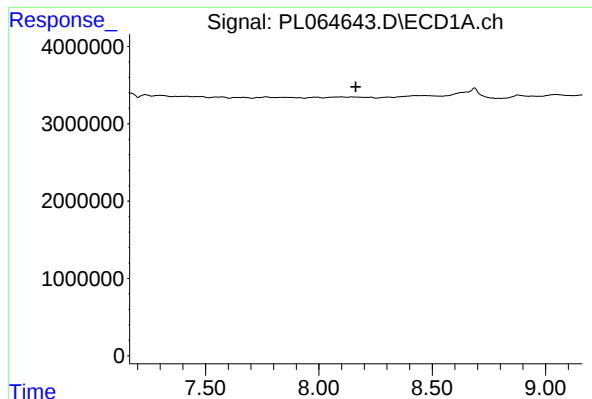

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

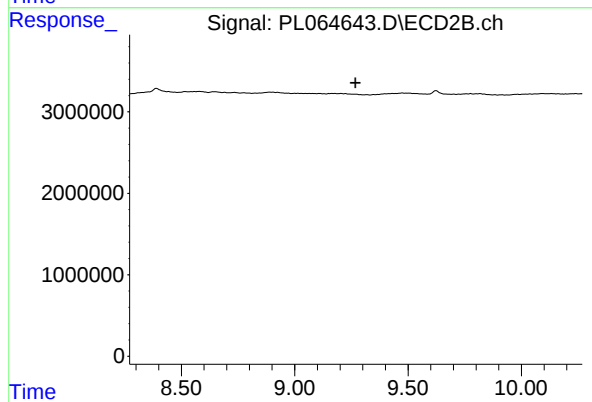

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.268 min
Response: 0
Conc: N.D.