

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
 Data File : PL064656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Feb 2021 17:17
 Operator : AR\AJ
 Sample : M1317-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 R-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 06 02:46:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.109	44494340	20259203	14.616	8.505 #
28)	SA Decachlor...	8.165	9.273	29592504	25292318	9.390	12.353 #
Target Compounds							
5)	MB Aldrin	4.668f	5.597f	-11080728	3063.5E6	N.D.	1026.377
9)	A Endosulfan I	5.446f	0.000	86702565	0	22.960	N.D. #
11)	B alpha-Chl...	5.427	0.000	44786796	0	10.922	N.D. #
16)	A 4,4'-DDD	0.000	6.986	0	2998182	N.D.	1.302 #
17)	MA 4,4'-DDT	0.000	7.255f	0	4130026	N.D.	2.011 #
20)	A Methoxychlor	6.863f	0.000	3670483	0	2.032	N.D. #
21)	B Endrin ke...	0.000	7.911	0	2153959	N.D.	0.886 #
24)	Chlordane-2	0.000	5.597	0	3063.5E6	N.D.	29536.533 #
26)	Chlordane-4	5.427	0.000	44786796	0	150.571	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020521\
Data File : PL064656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Feb 2021 17:17
Operator : AR\AJ
Sample : M1317-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
R-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 06 02:46:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

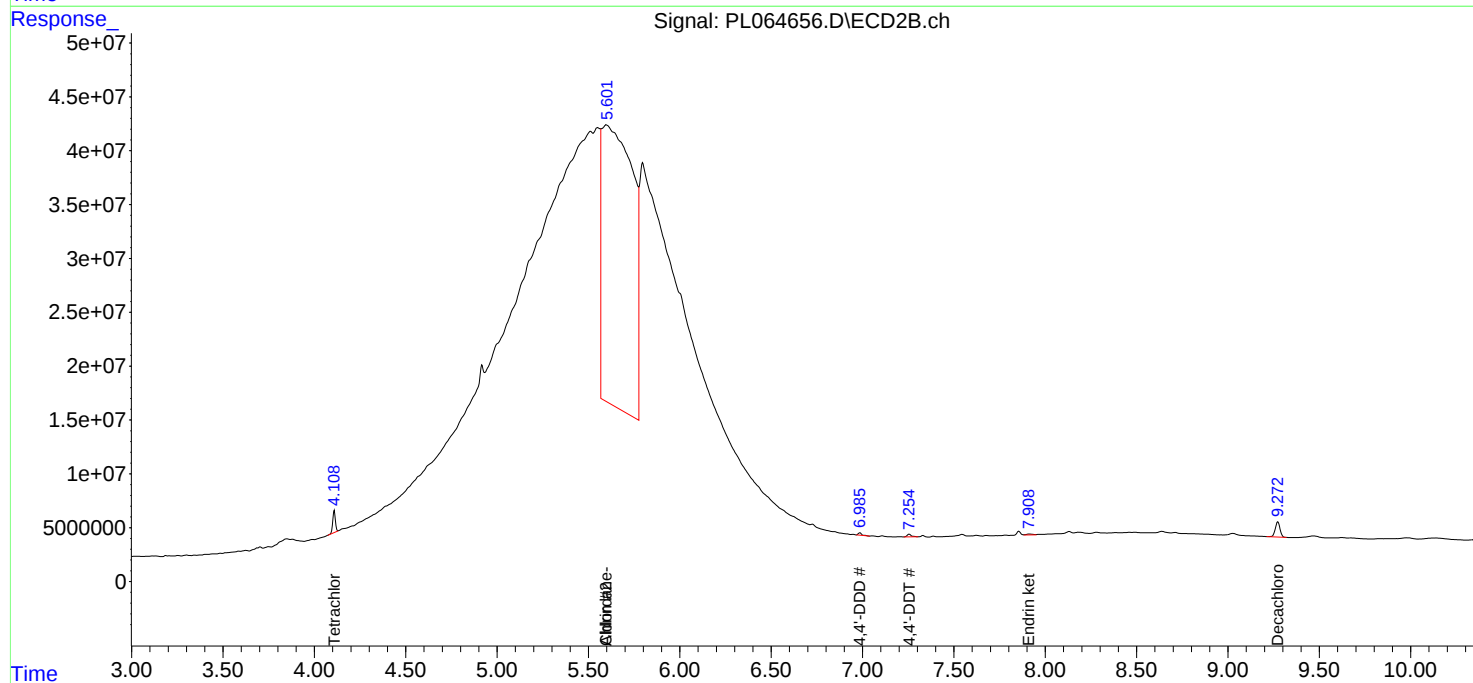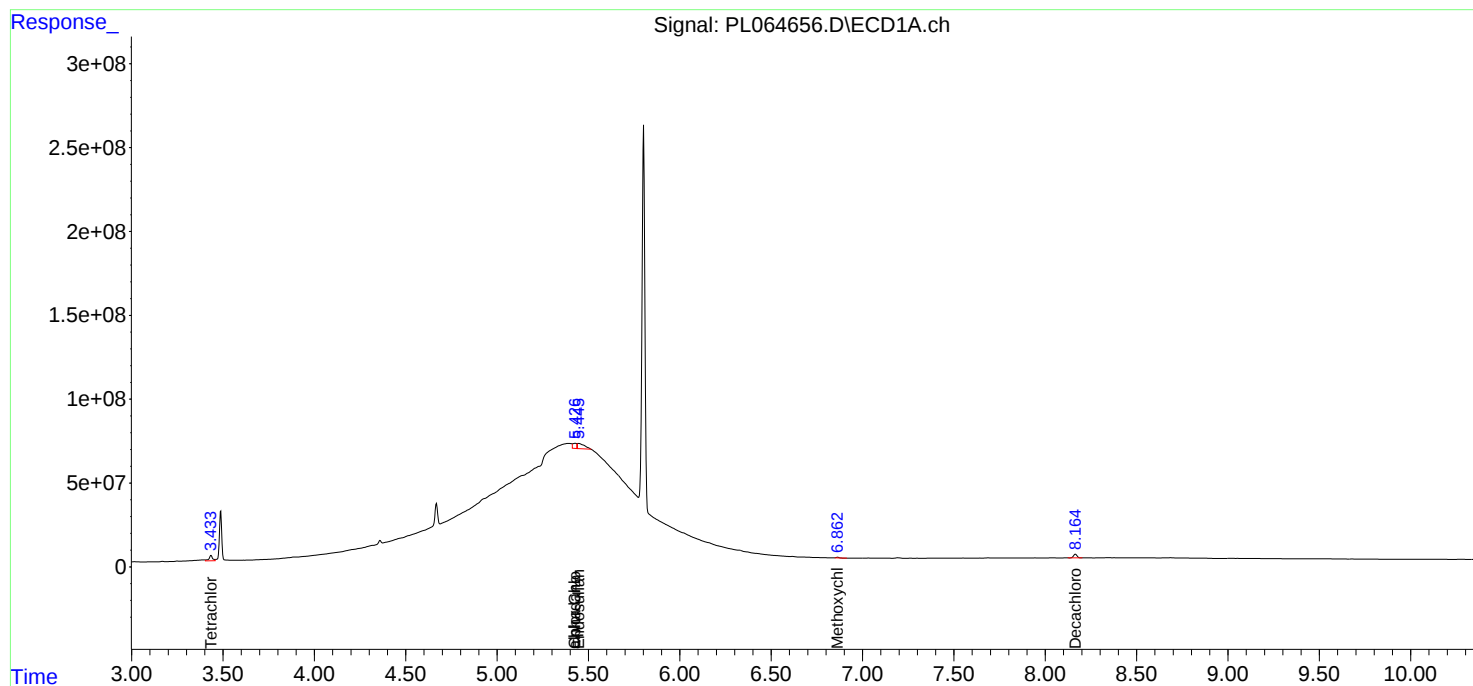


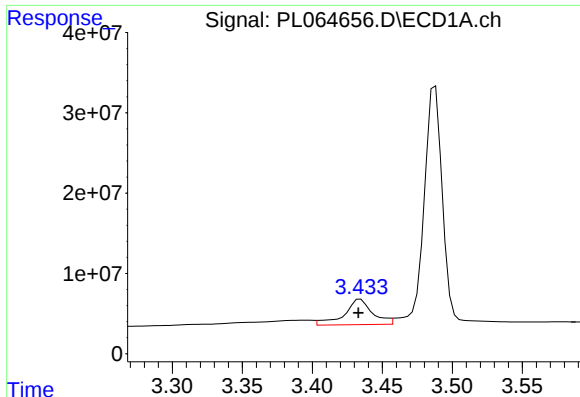

#1 Tetrachloro-m-xylene


R.T.: 3.435 min
Delta R.T.: 0.002 min
Response: 44494340
Conc: 14.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-C

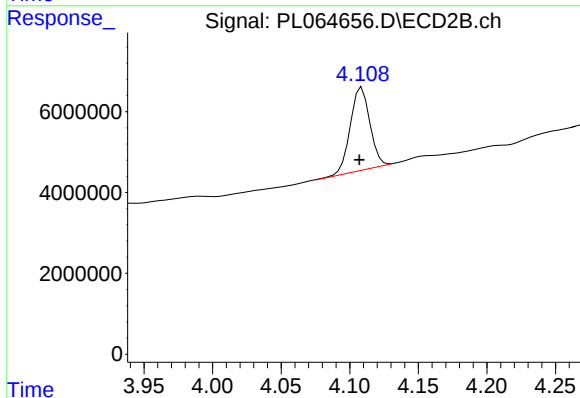


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.002 min
Response: 20259203
Conc: 8.51 ng/ml

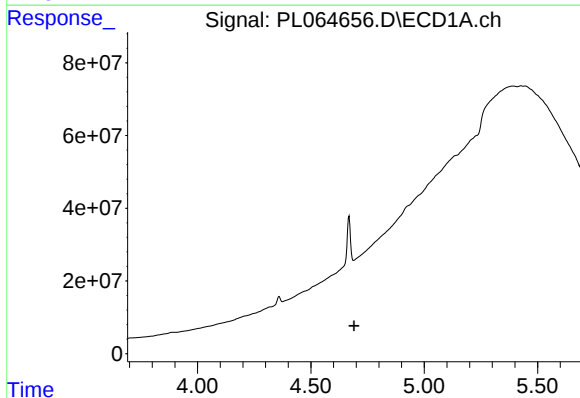


#5 Aldrin

R.T.: 4.668 min
Delta R.T.: -0.022 min
Response: -11080728
Conc: N.D.

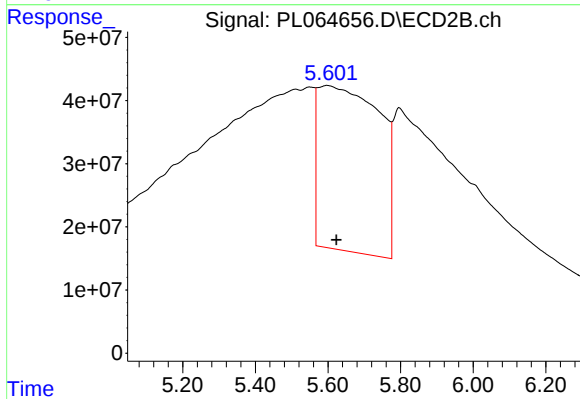

#5 Aldrin


R.T.: 5.597 min
Delta R.T.: -0.026 min
Response: 3063534081
Conc: 1026.38 ng/ml

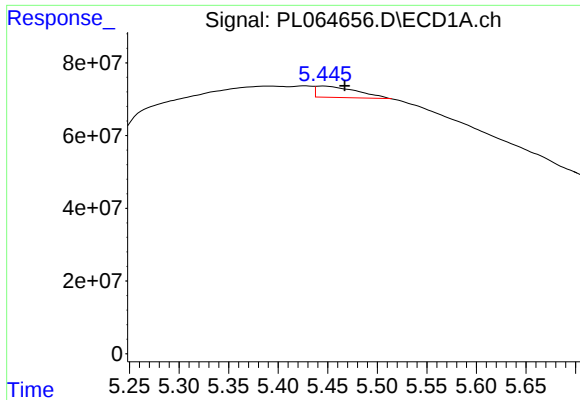

#9 Endosulfan I


R.T.: 5.446 min
Delta R.T.: -0.021 min
Response: 86702565
Conc: 22.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-C

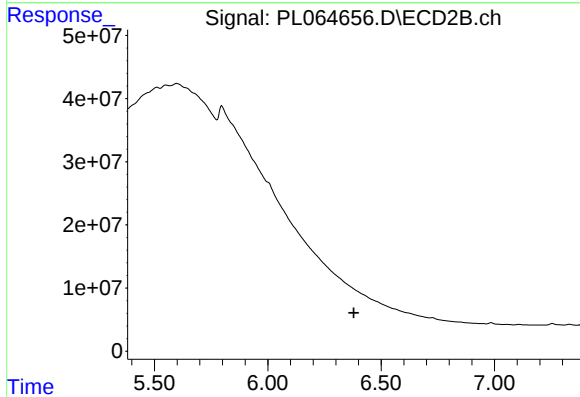


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.379 min
Response: 0
Conc: N.D.

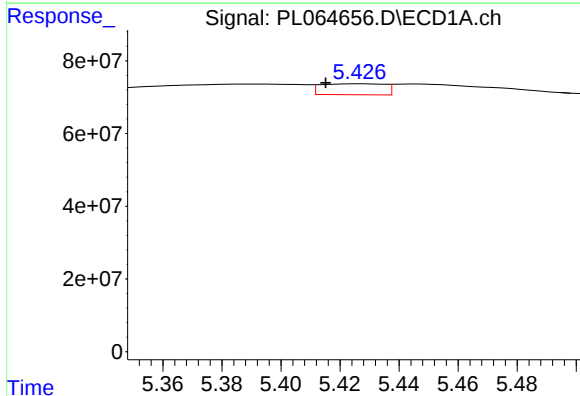


#11 alpha-Chlordane

R.T.: 5.427 min
Delta R.T.: 0.012 min
Response: 44786796
Conc: 10.92 ng/ml

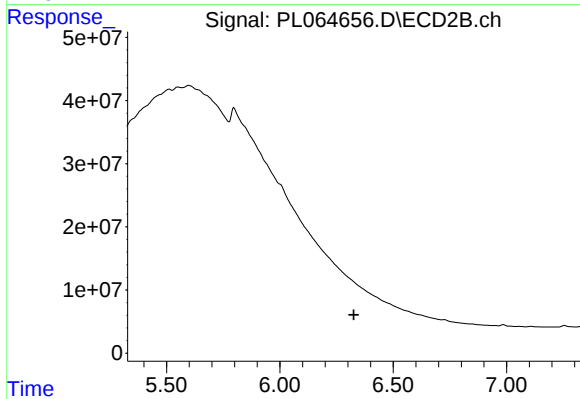

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.326 min
Response: 0
Conc: N.D.

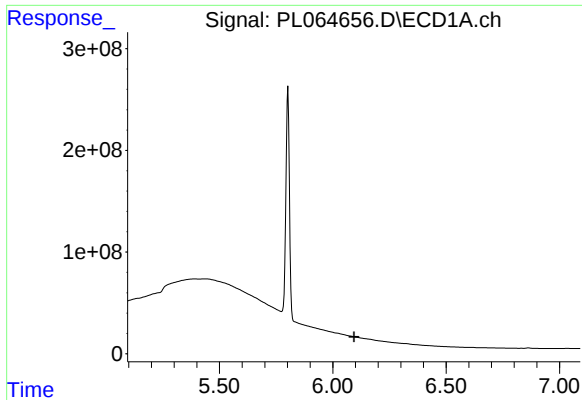

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R-C

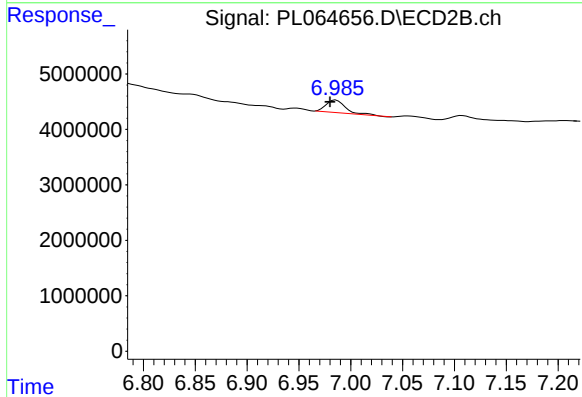


#16 4,4'-DDD

R.T.: 6.986 min
Delta R.T.: 0.006 min
Response: 2998182
Conc: 1.30 ng/ml

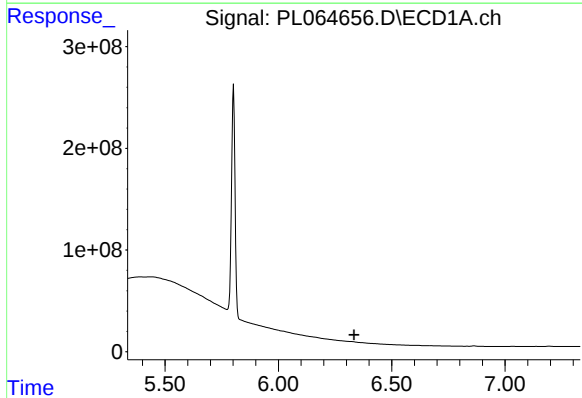


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.334 min
Response: 0
Conc: N.D.

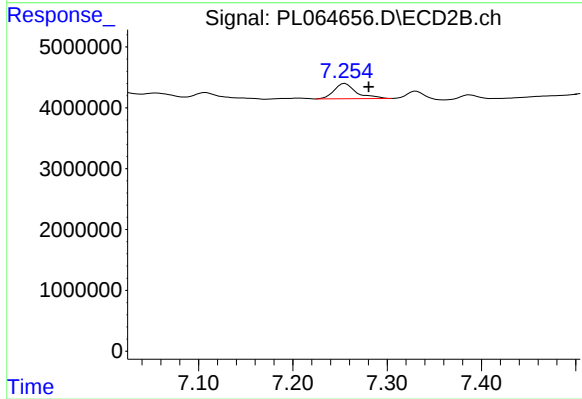

#17 4,4'-DDT


R.T.: 7.255 min
Delta R.T.: -0.025 min
Response: 4130026
Conc: 2.01 ng/ml

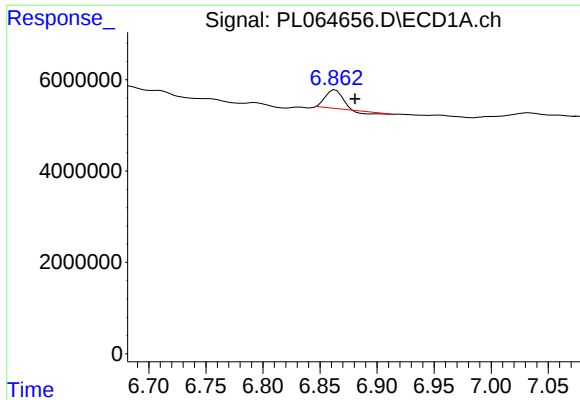

#20 Methoxychlor


R.T.: 6.863 min
Delta R.T.: -0.017 min
Response: 3670483
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-C

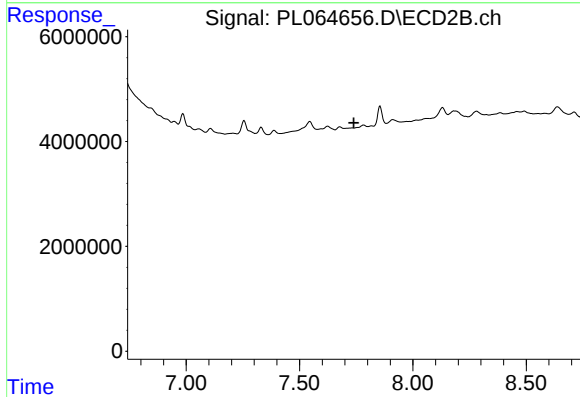


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

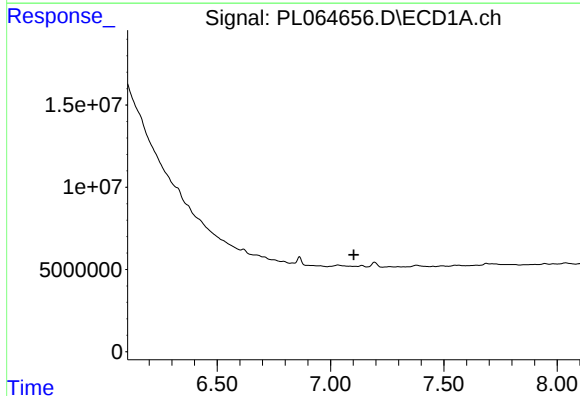


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.103 min
Response: 0
Conc: N.D.

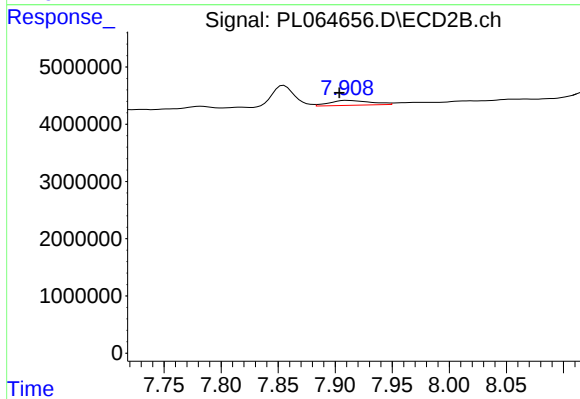

#21 Endrin ketone


R.T.: 7.911 min
Delta R.T.: 0.008 min
Response: 2153959
Conc: 0.89 ng/ml

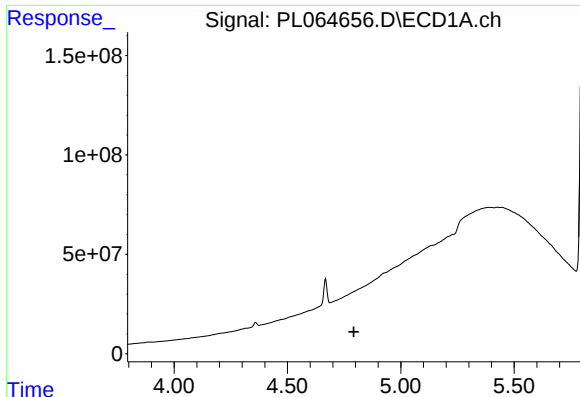

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
R-C

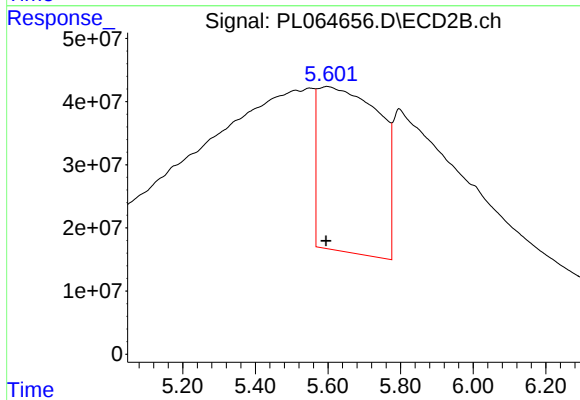


#24 Chlordane-2

R.T.: 5.597 min
Delta R.T.: 0.002 min
Response: 3063534081
Conc: 29536.53 ng/ml

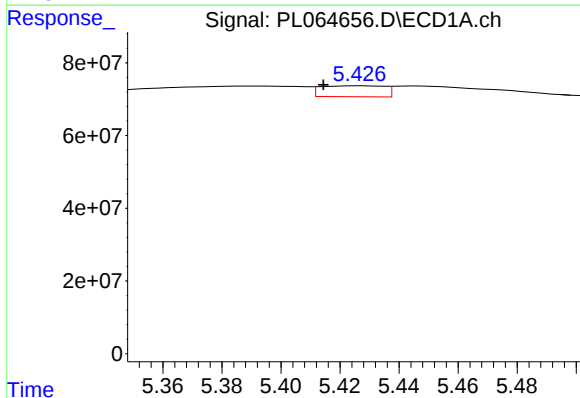


#26 Chlordane-4

R.T.: 5.427 min
Delta R.T.: 0.013 min
Response: 44786796
Conc: 150.57 ng/ml

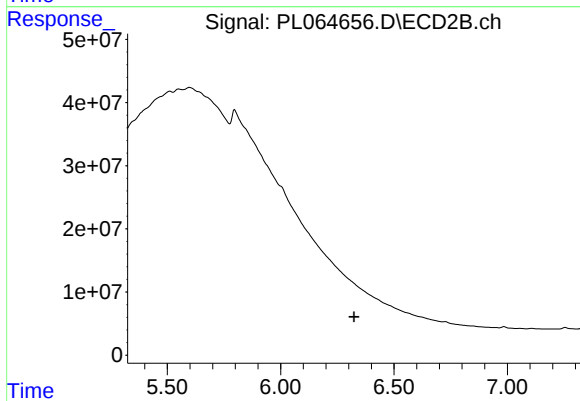

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.324 min
Response: 0
Conc: N.D.

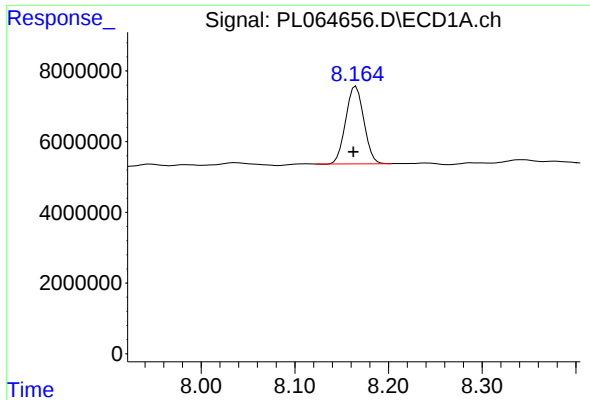

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.003 min
Response: 29592504
Conc: 9.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
R-C

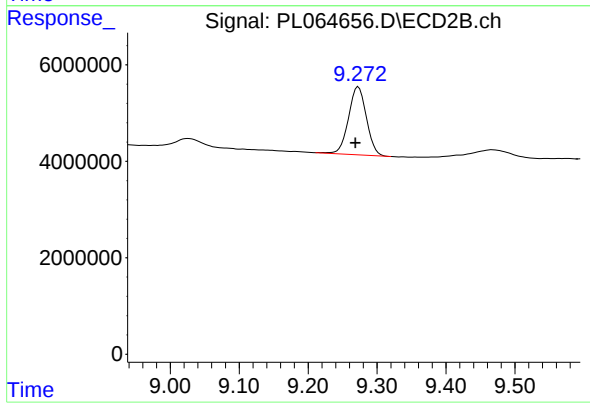

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.004 min
Response: 25292318
Conc: 12.35 ng/ml