

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
 Data File : PL044527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 09:57
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 10:09:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.985	168.2E6	53803577	23.638	22.903
28)	SA Decachlor...	8.051	9.045	157.1E6	46853315	21.543	21.154
Target Compounds							
8)	B Heptachlo...	0.000	5.851	0	2547007	N.D.	1.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
Data File : PL044527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 09:57
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 10:09:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

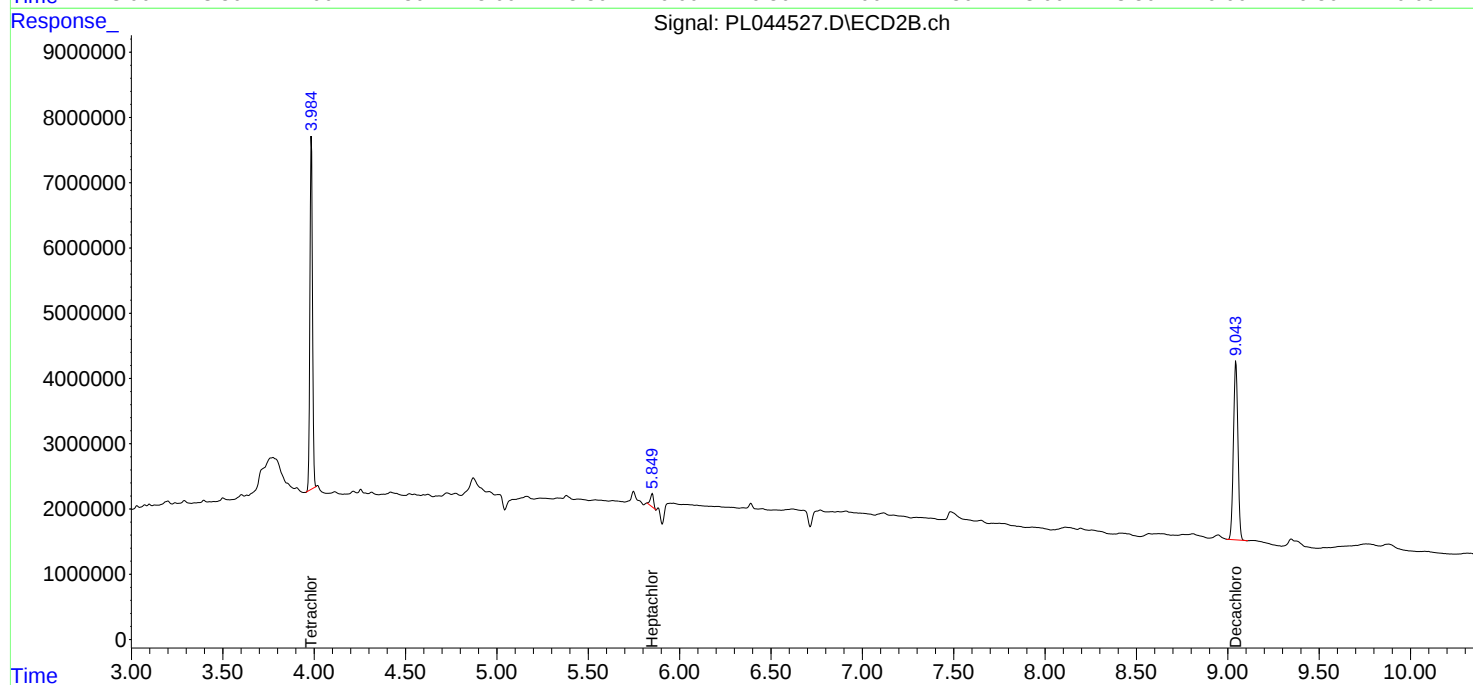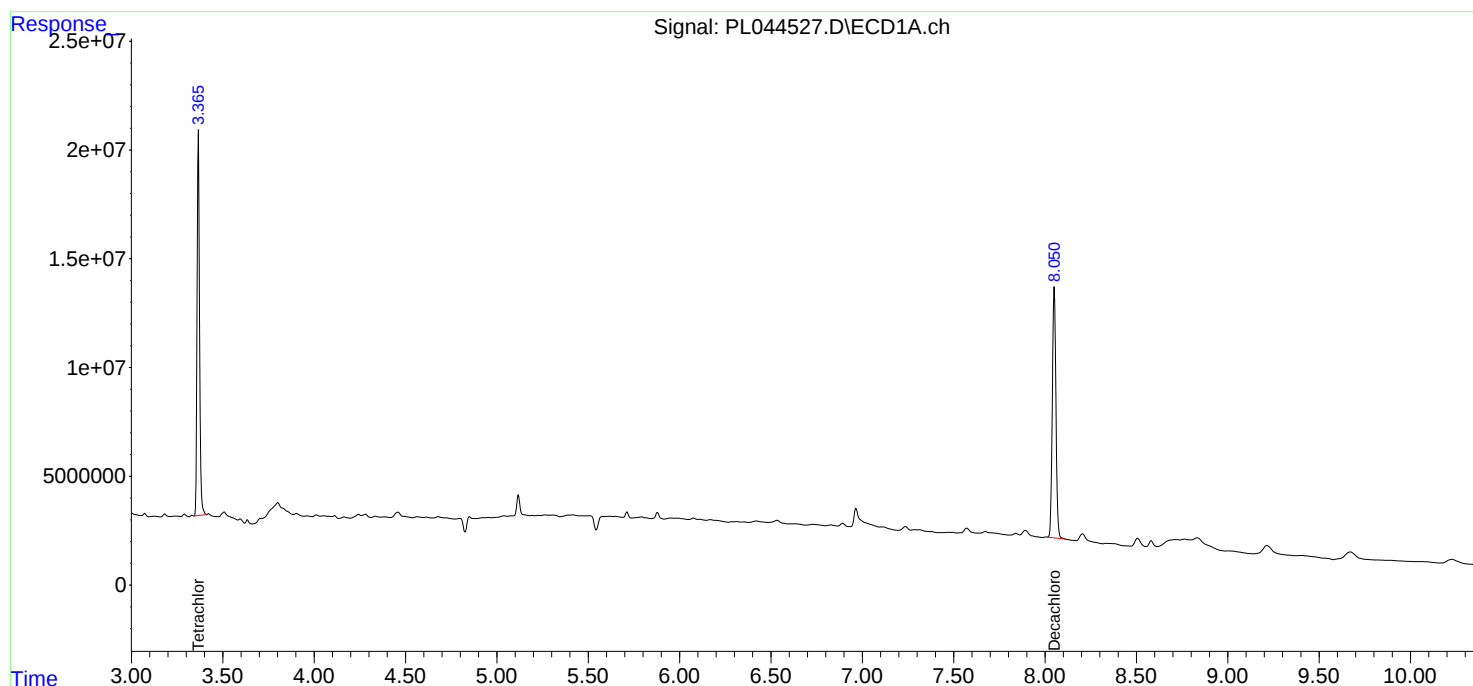


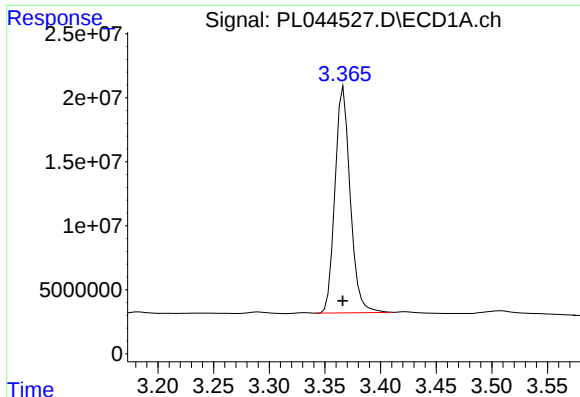

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.000 min
Response: 168207586
Conc: 23.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

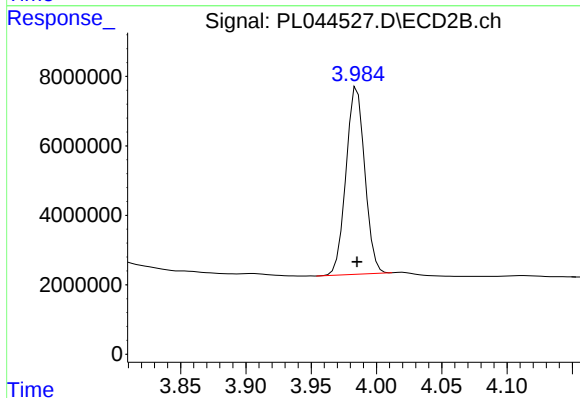


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 53803577
Conc: 22.90 ng/ml

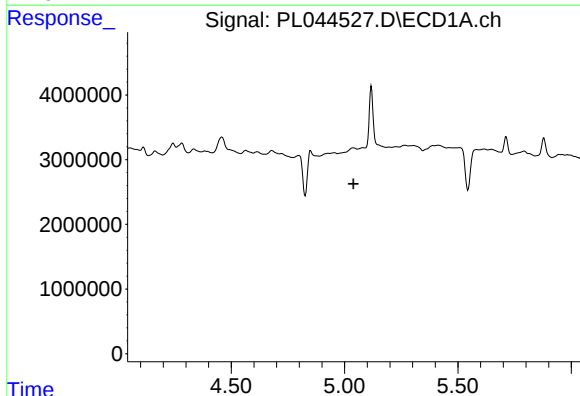


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

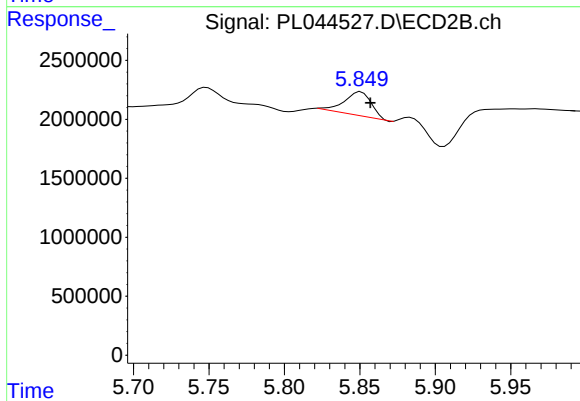

#8 Heptachlor epoxide


R.T.: 5.851 min
Delta R.T.: -0.006 min
Response: 2547007
Conc: 1.02 ng/ml

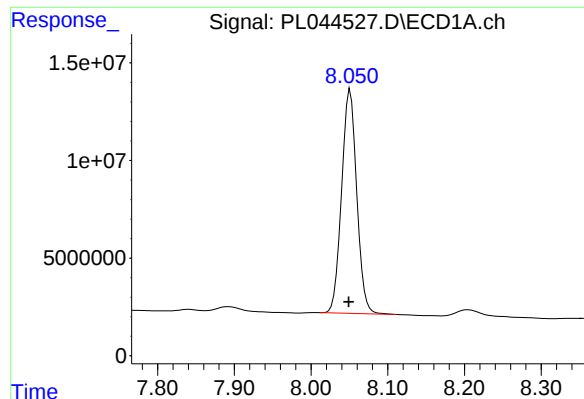

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 157123053
Conc: 21.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

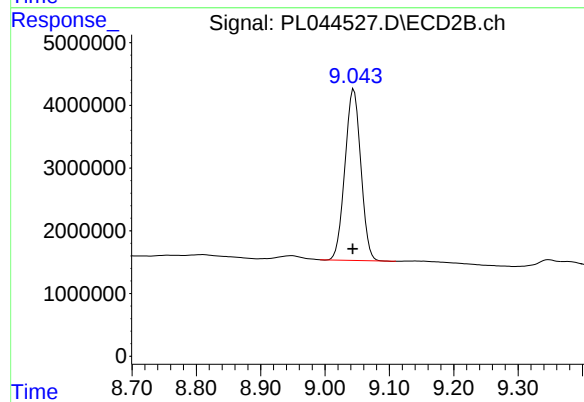

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: 0.002 min
Response: 46853315
Conc: 21.15 ng/ml