

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
 Data File : PL044457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2019 11:26
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 01:13:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:11:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.366	3.985	374.2E6	112.1E6	50.000	50.000
28)	SA Decachlor...	8.049	9.044	358.3E6	107.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.214	4.979	163.2E6	54217041	500.000	500.000
24)	Chlordane-2	4.706	5.446	179.7E6	58804460	500.000	500.000
25)	Chlordane-3	5.264	6.092	548.7E6	194.7E6	500.000	500.000
26)	Chlordane-4	5.320	6.166	515.5E6	233.8E6	500.000	500.000
27)	Chlordane-5	6.145	6.969	168.3E6	44841140	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
Data File : PL044457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2019 11:26
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 01:13:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:11:04 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

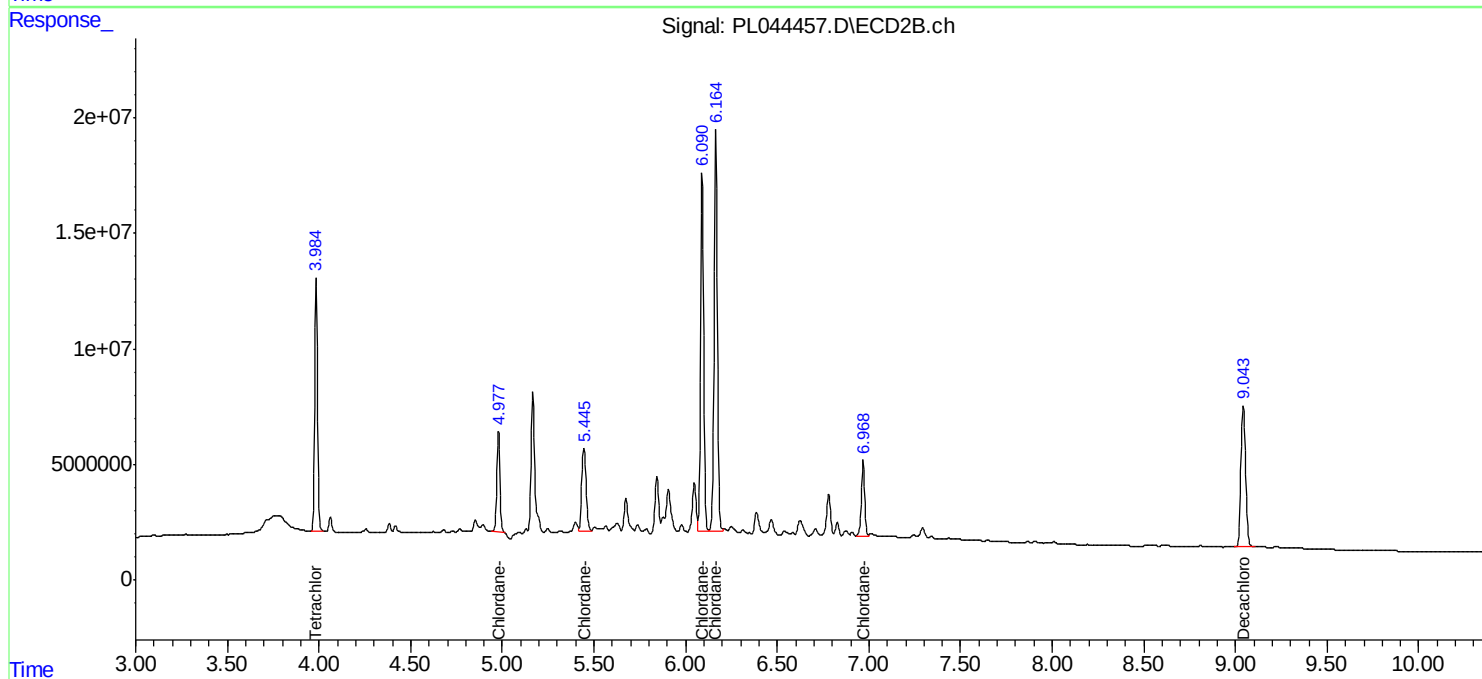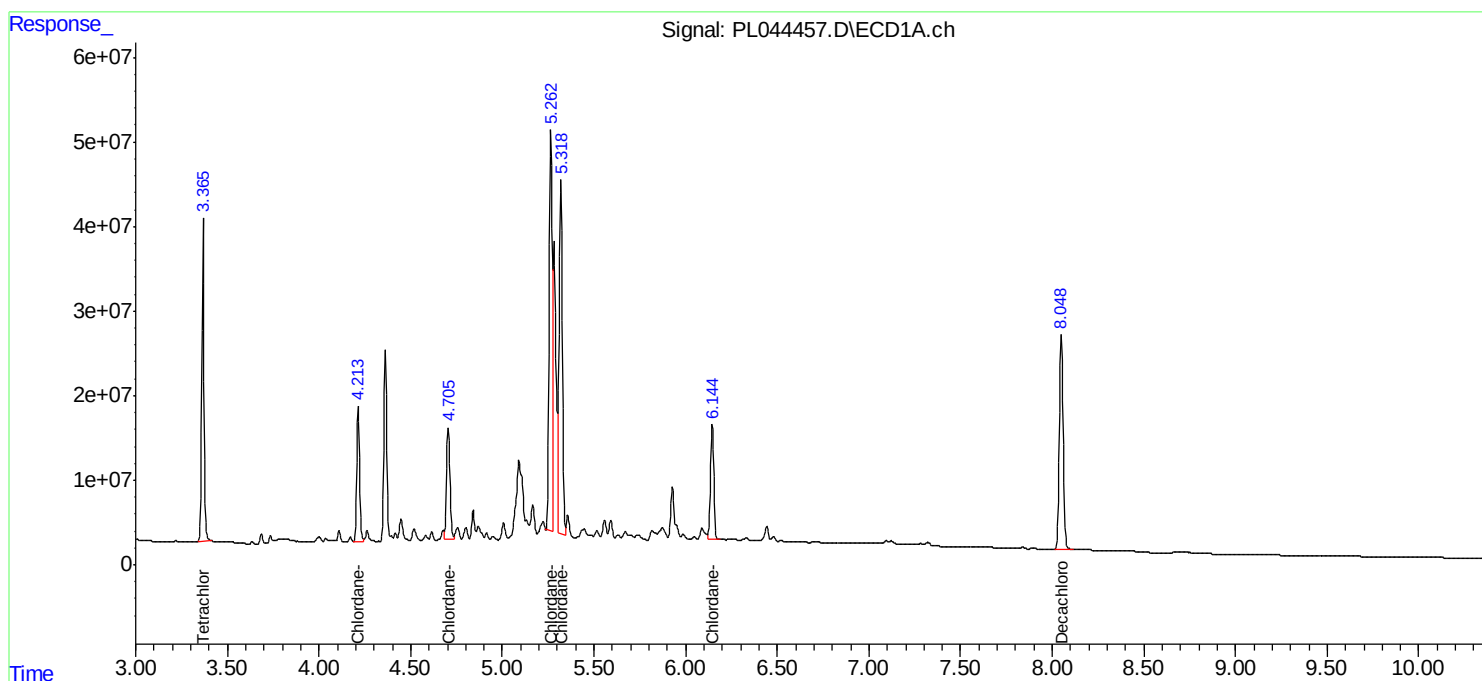


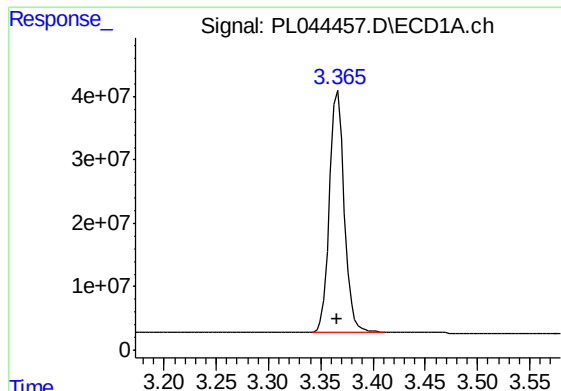

#1 Tetrachloro-m-xylene


R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 374164527
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

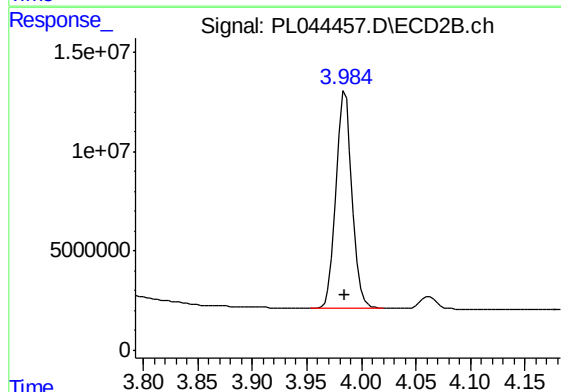


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 112086875
Conc: 50.00 ng/ml

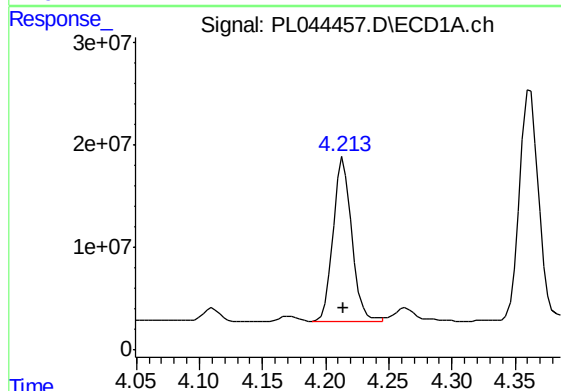


#23 Chlordane-1

R.T.: 4.214 min
Delta R.T.: 0.000 min
Response: 163189960
Conc: 500.00 ng/ml

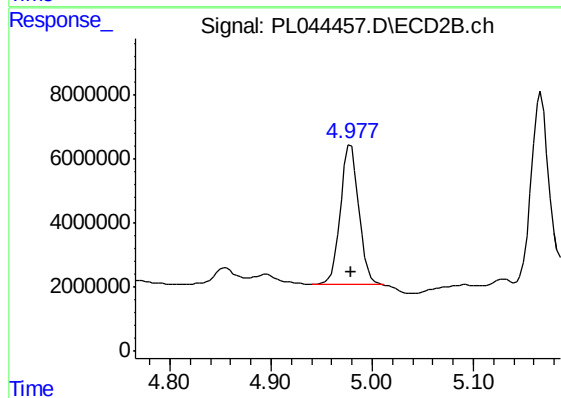

#23 Chlordane-1


R.T.: 4.979 min
Delta R.T.: 0.000 min
Response: 54217041
Conc: 500.00 ng/ml

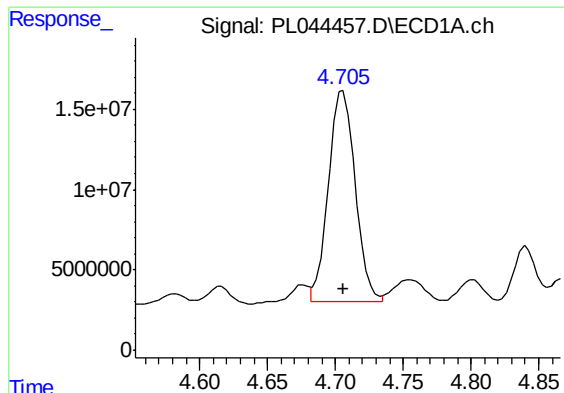

#24 Chlordane-2


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 179733732
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

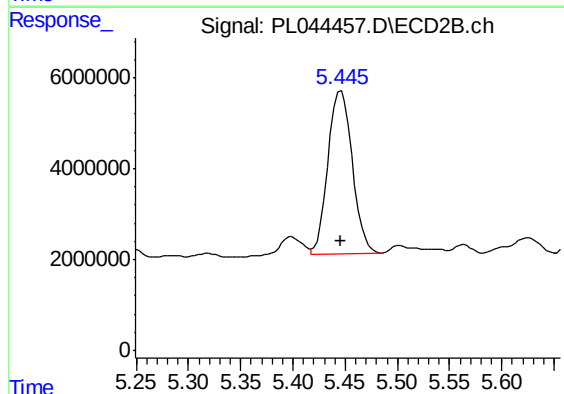


#24 Chlordane-2

R.T.: 5.446 min
Delta R.T.: 0.000 min
Response: 58804460
Conc: 500.00 ng/ml

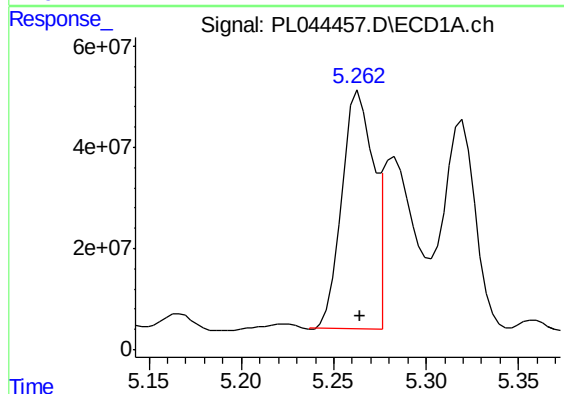


#25 Chlordane-3

R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 548692753
Conc: 500.00 ng/ml

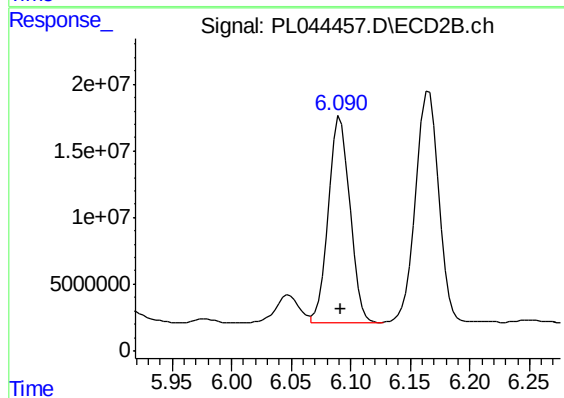

#25 Chlordane-3


R.T.: 6.092 min
Delta R.T.: 0.000 min
Response: 194699312
Conc: 500.00 ng/ml

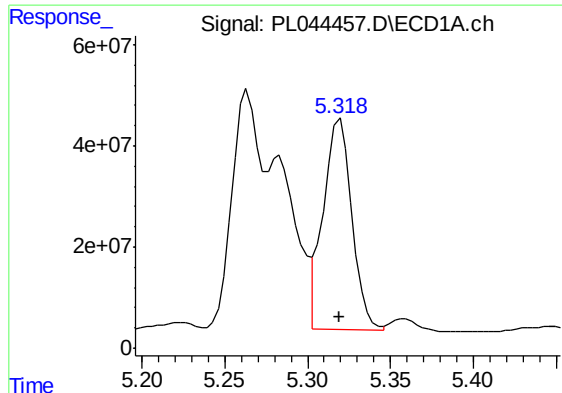

#26 Chlordane-4


R.T.: 5.320 min
Delta R.T.: 0.000 min
Response: 515512708
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

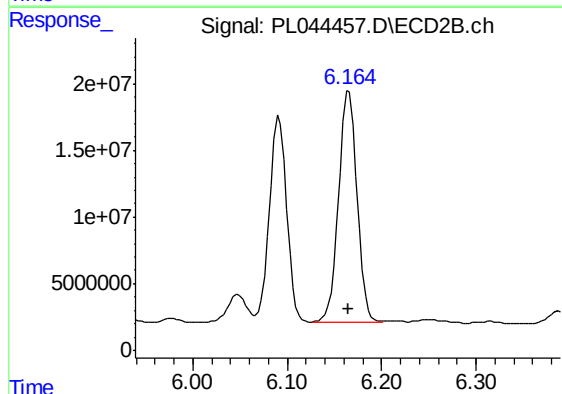


#26 Chlordane-4

R.T.: 6.166 min
Delta R.T.: 0.000 min
Response: 233787416
Conc: 500.00 ng/ml

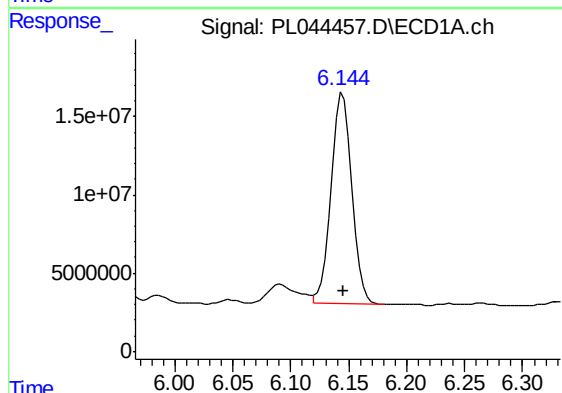


#27 Chlordane-5

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 168262385
Conc: 500.00 ng/ml

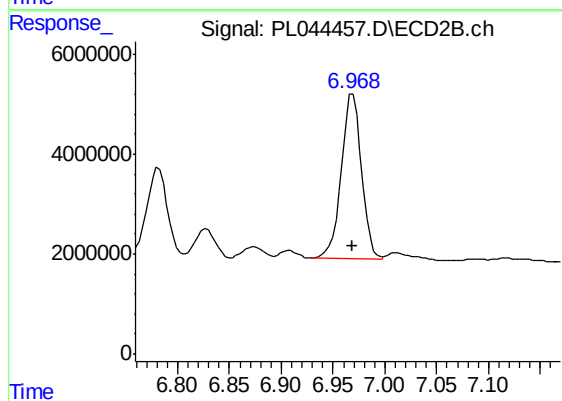

#27 Chlordane-5


R.T.: 6.969 min
Delta R.T.: 0.000 min
Response: 44841140
Conc: 500.00 ng/ml

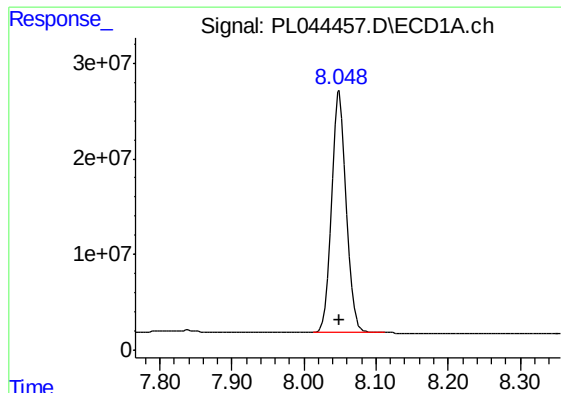

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.000 min
Response: 358257894
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

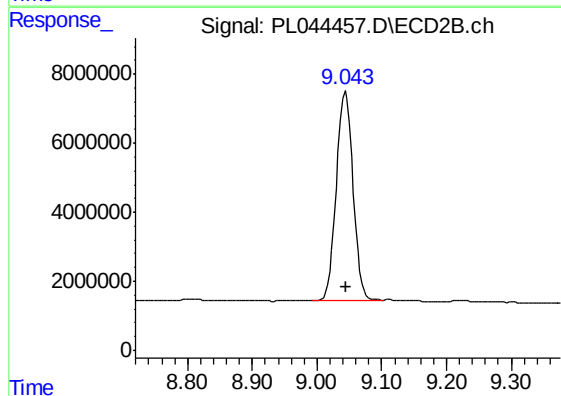

#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.000 min
Response: 107418009
Conc: 50.00 ng/ml