

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
 Data File : PL044511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 00:53
 Operator : AJ\SJ
 Sample : K1338-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-06-020519-A

Manual Integrations
 APPROVED

Sohil
 2/7/2019 12:20:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 03:00:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.366	3.986	85264103	29438884	11.982	12.532
28)	SA Decachlor...	8.051	9.045	91530075	32248062	12.549	14.560
Target Compounds							
12)	B 4,4'-DDE	5.485	6.322	4397984	1759846	0.507m	0.737 #
17)	MA 4,4'-DDT	6.229	7.109	3210472	707236	0.448m	0.361m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
Data File : PL044511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 00:53
Operator : AJ\SJ
Sample : K1338-01
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
AU-06-020519-A


Manual Integrations
APPROVED

Sohil
2/7/2019 12:20:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 03:00:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

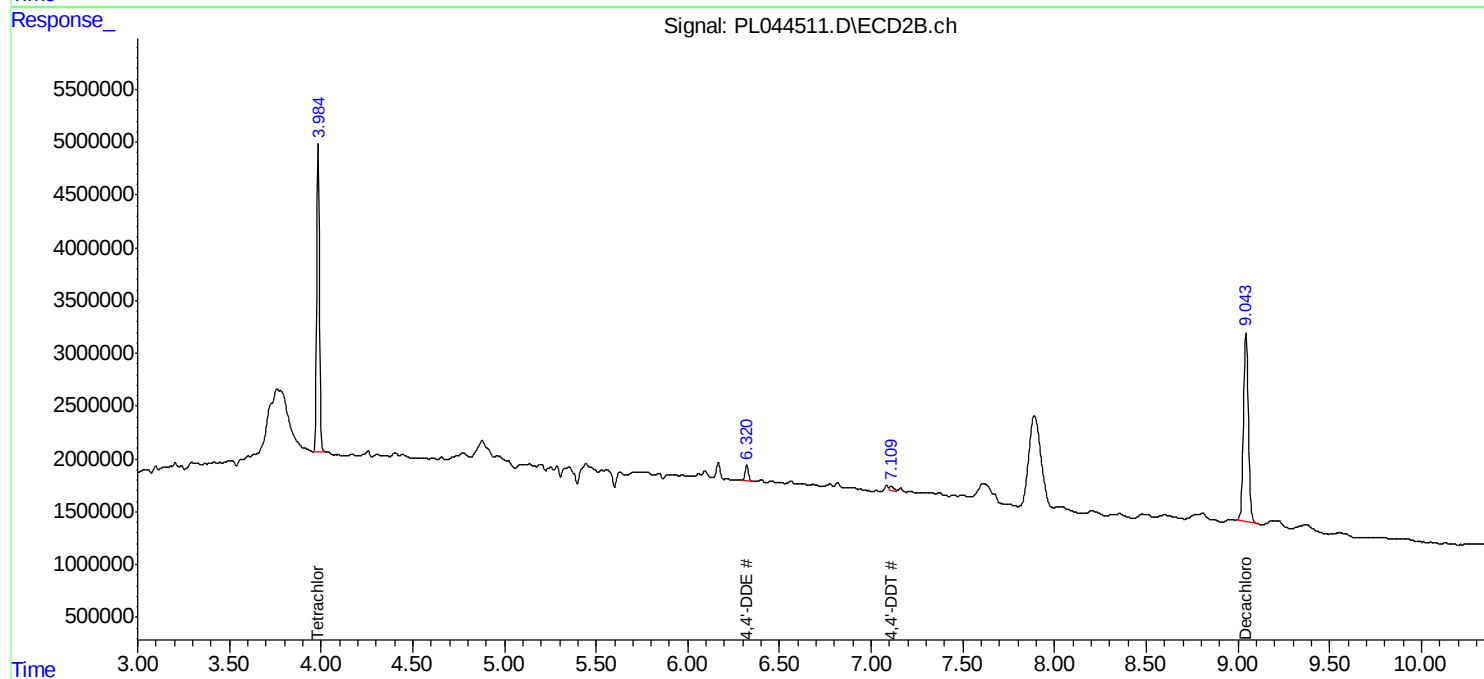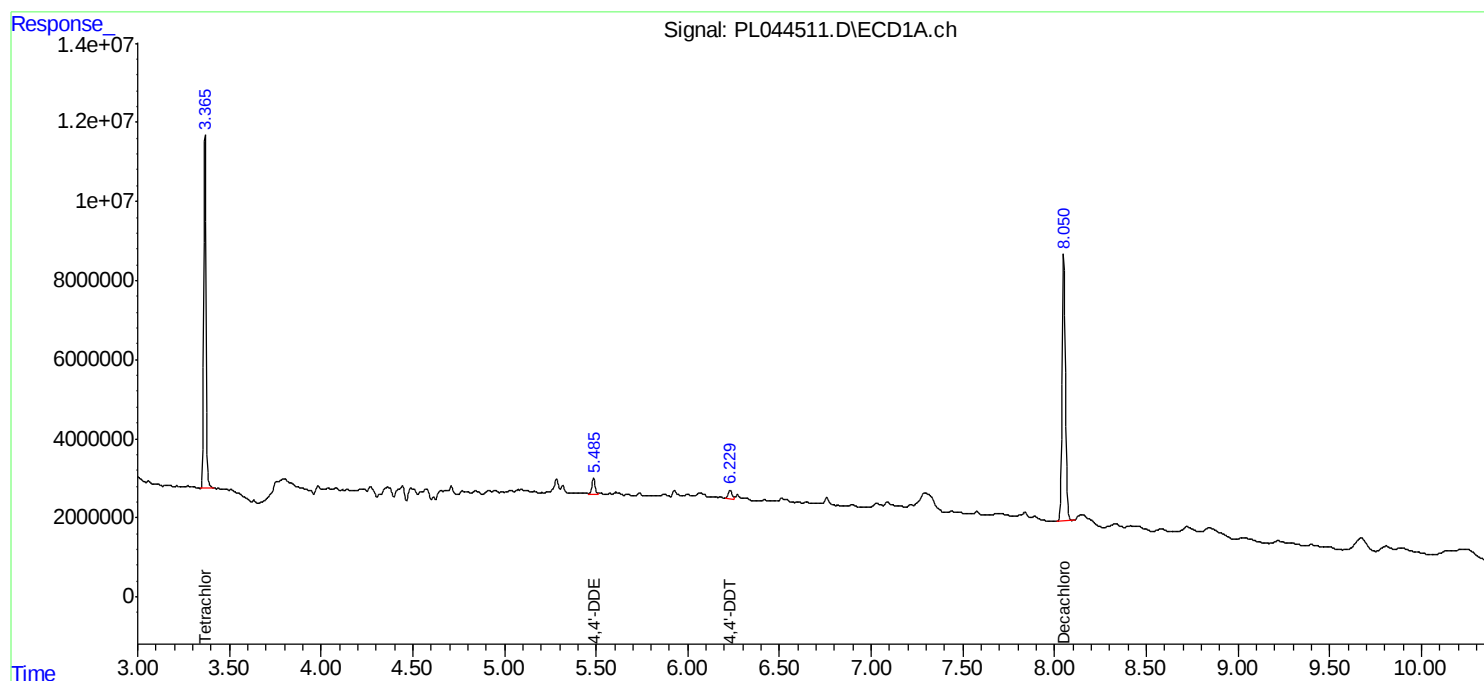

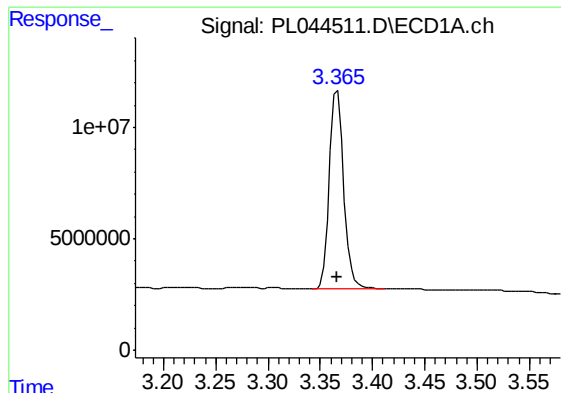


#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 85264103
Conc: 11.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-06-020519-A


Manual Integrations
APPROVED

Sohil
2/7/2019 12:20:43 PM

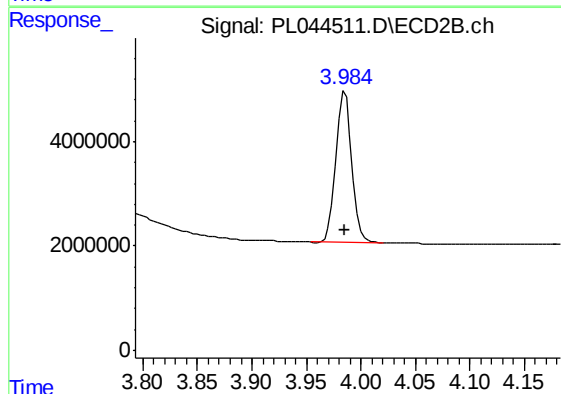


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 29438884
Conc: 12.53 ng/ml

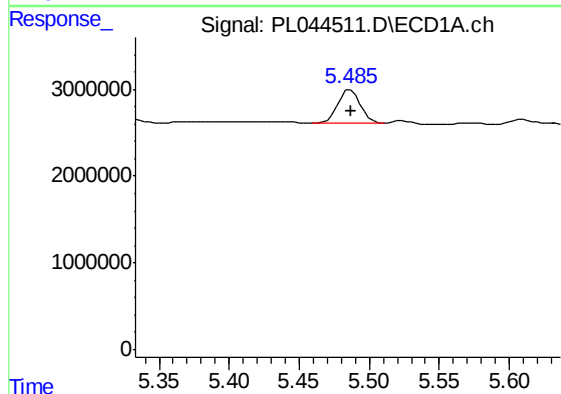


#12 4,4'-DDE

R.T.: 5.485 min
Delta R.T.: -0.001 min
Response: 4397984
Conc: 0.51 ng/ml m

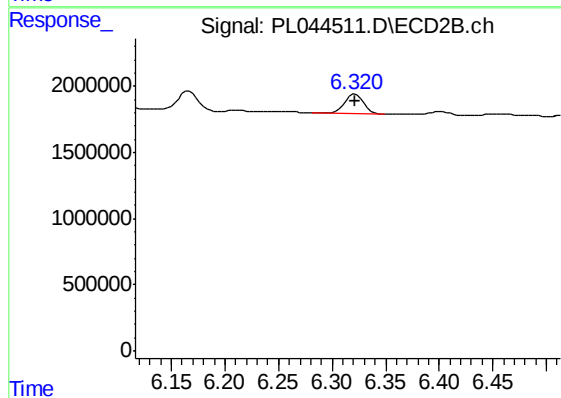

#12 4,4'-DDE

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 1759846
Conc: 0.74 ng/ml

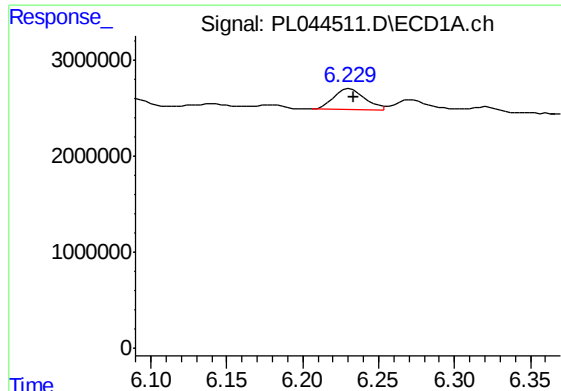


#17 4,4'-DDT

R.T.: 6.229 min
Delta R.T.: -0.004 min
Response: 3210472
Conc: 0.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
AU-06-020519-A


Manual Integrations
APPROVED

Sohil
2/7/2019 12:20:43 PM

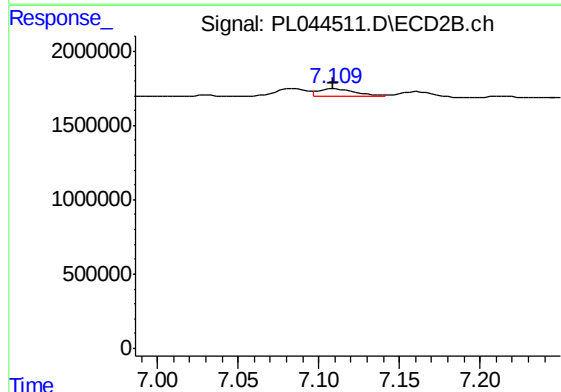


#17 4,4'-DDT

R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 707236
Conc: 0.36 ng/ml m

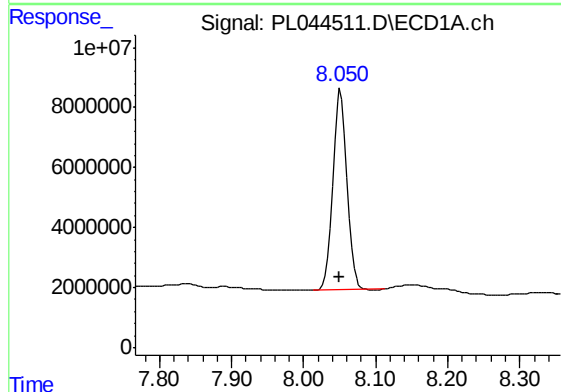

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 91530075
Conc: 12.55 ng/ml

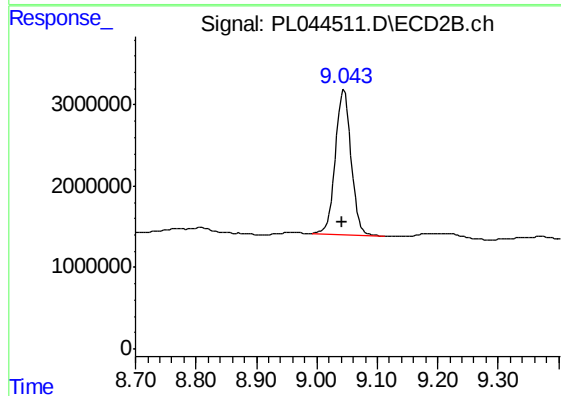

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: 0.002 min
Response: 32248062
Conc: 14.56 ng/ml