

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
 Data File : PL044518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 02:32
 Operator : AJ\SJ
 Sample : K1383-01
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 A0C5B-SS1-0.0-0.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 06:17:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.986	76517968	26305894	10.753	11.198
28)	SA Decachlor...	8.052	9.046	76847476	24179406	10.536	10.917

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020619\
Data File : PL044518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 02:32
Operator : AJ\SJ
Sample : K1383-01
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
A0C5B-SS1-0.0-0.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 06:17:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

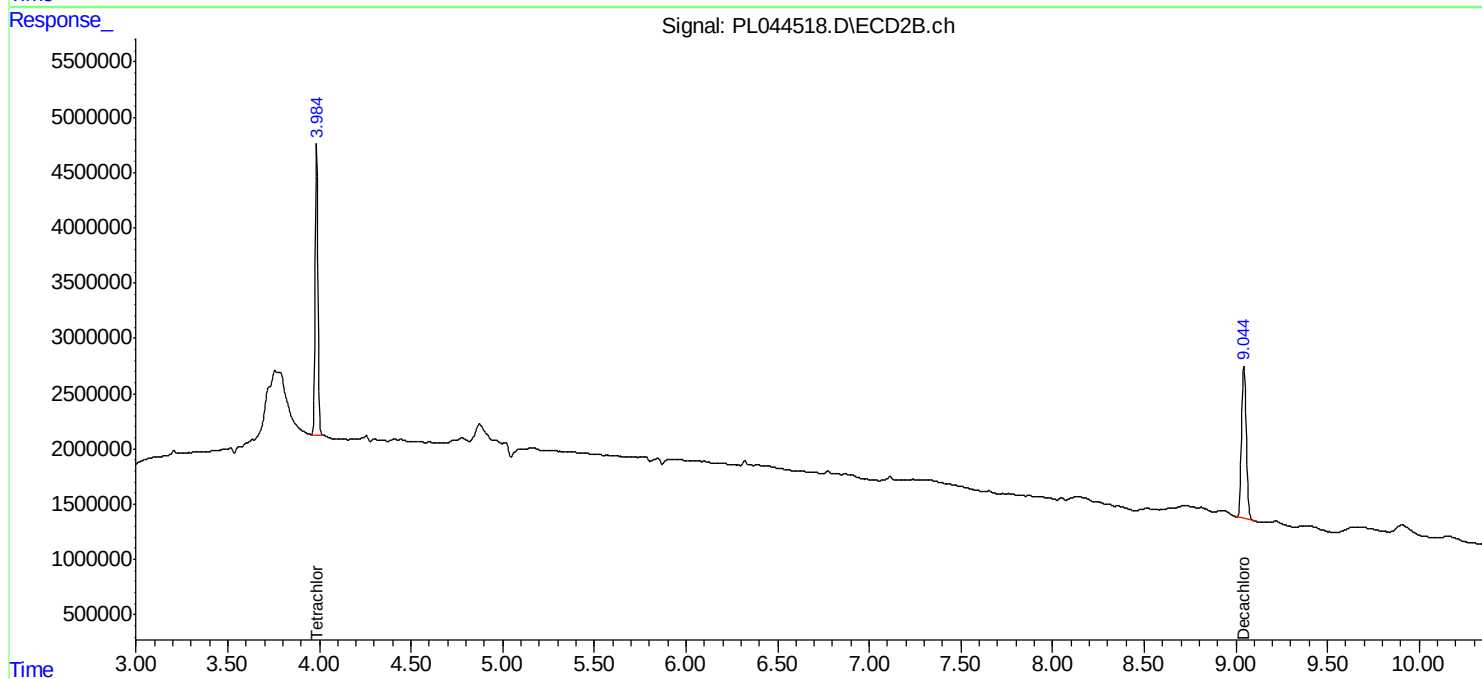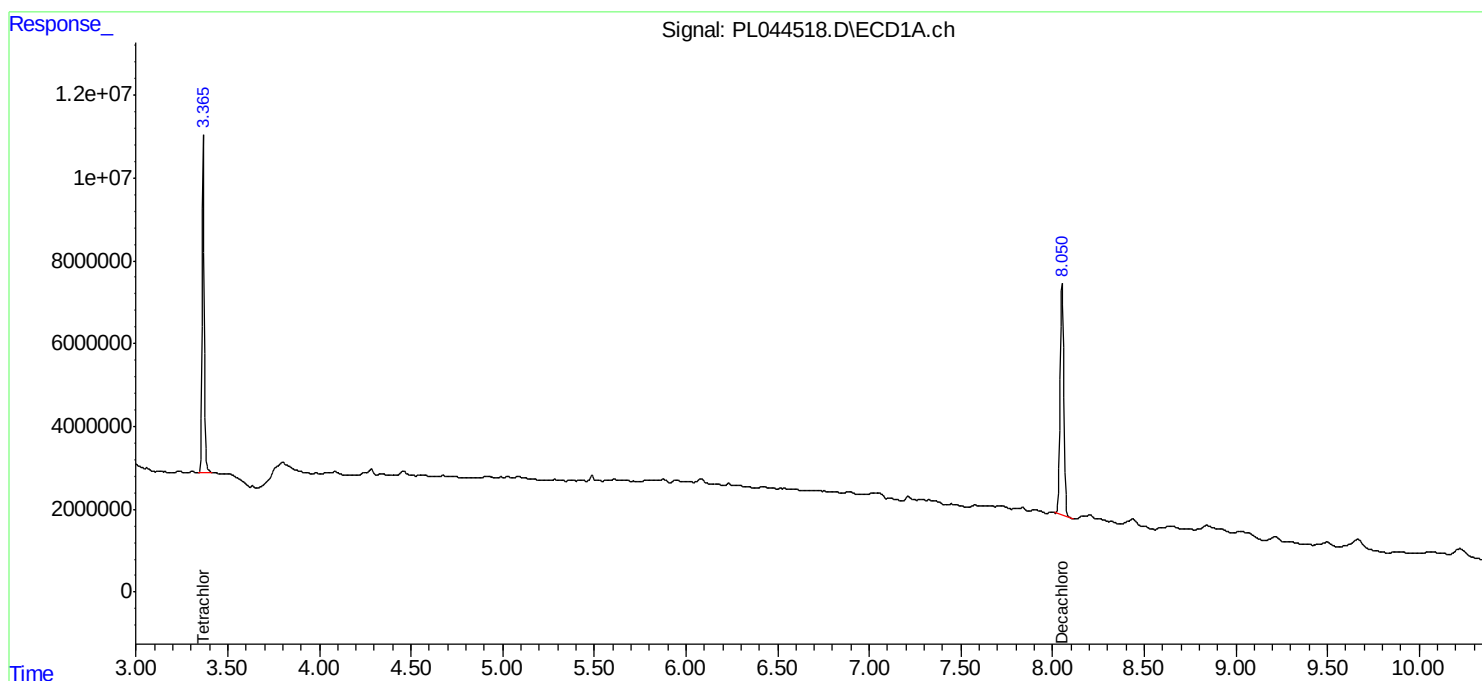


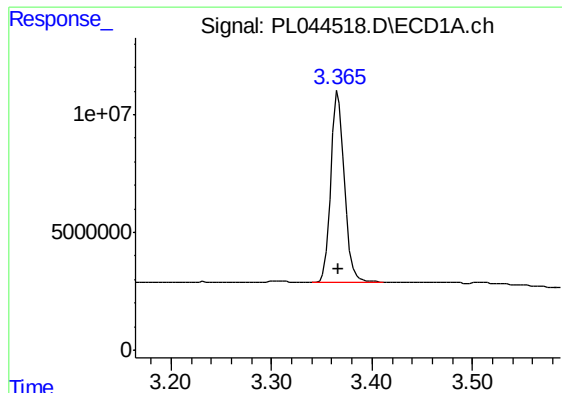

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.000 min
Response: 76517968
Conc: 10.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
A0C5B-SS1-0.0-0.5

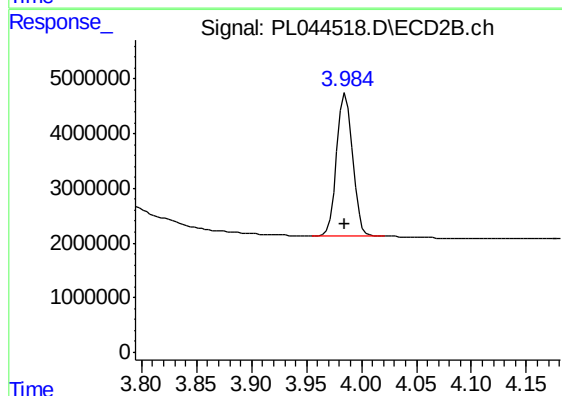


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.001 min
Response: 26305894
Conc: 11.20 ng/ml

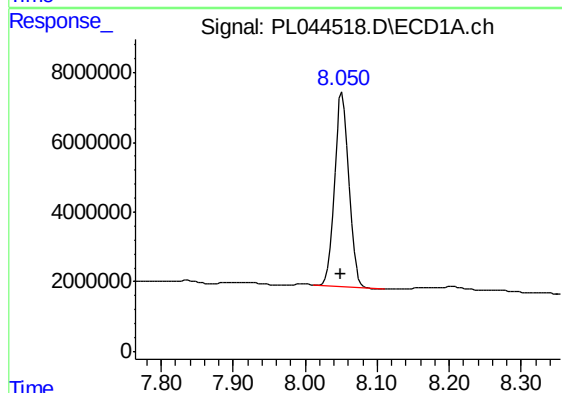

#28 Decachlorobiphenyl

R.T.: 8.052 min
Delta R.T.: 0.002 min
Response: 76847476
Conc: 10.54 ng/ml

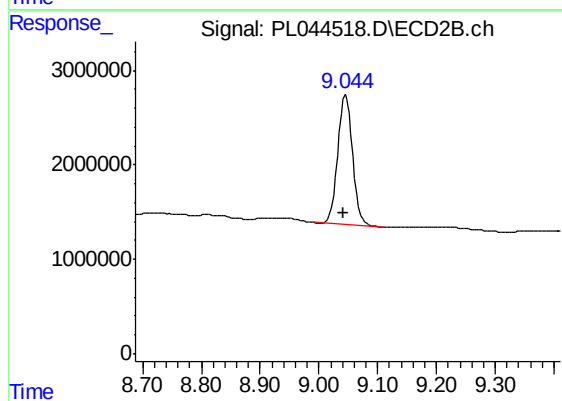

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: 0.003 min
Response: 24179406
Conc: 10.92 ng/ml