

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020620\
 Data File : PL056359.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Feb 2020 13:26
 Operator : AJ\MA
 Sample : PB126623BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB126623BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 06:48:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.016	176.0E6	54488461	16.806	18.634
28)	SA Decachlor...	8.262	9.100	210.8E6	42542083	20.027	18.808
Target Compounds							
4)	MA Heptachlor	4.534	0.000	1467593	0	0.091	N.D. #
7)	B delta-BHC	4.685	0.000	2972247	0	0.185	N.D. #
8)	B Heptachlo...	5.225	0.000	17705916	0	1.151	N.D. #
11)	B alpha-Chl...	5.491	0.000	163.3E6	0	10.619	N.D. #
12)	B 4,4'-DDE	5.678	0.000	73779532	0	5.090	N.D. #
14)	MA Endrin	6.075f	0.000	2357657	0	0.168	N.D. #
16)	A 4,4'-DDD	6.179	0.000	14938306	0	1.390	N.D. #
26)	Chlordane-4	5.491	0.000	163.3E6	0	150.961	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020620\
Data File : PL056359.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Feb 2020 13:26
Operator : AJ\MA
Sample : PB126623BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB126623BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 06:48:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

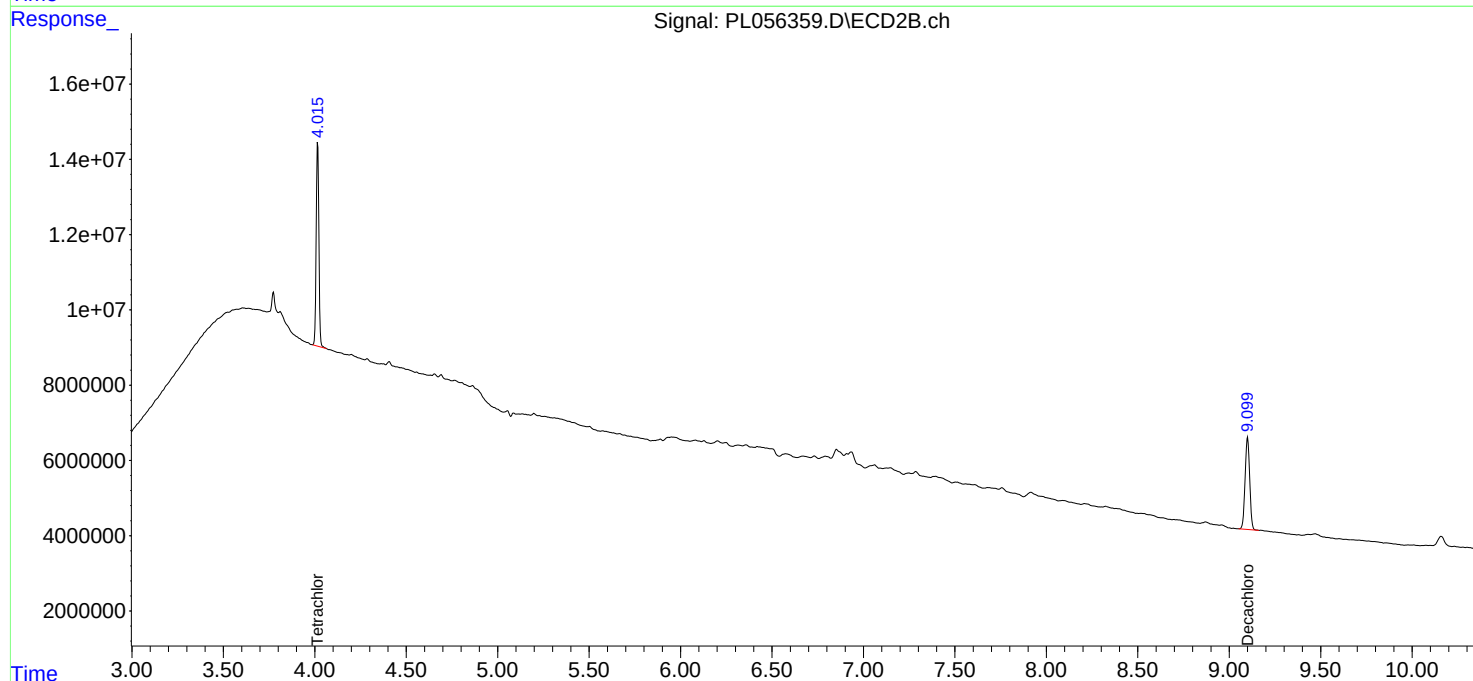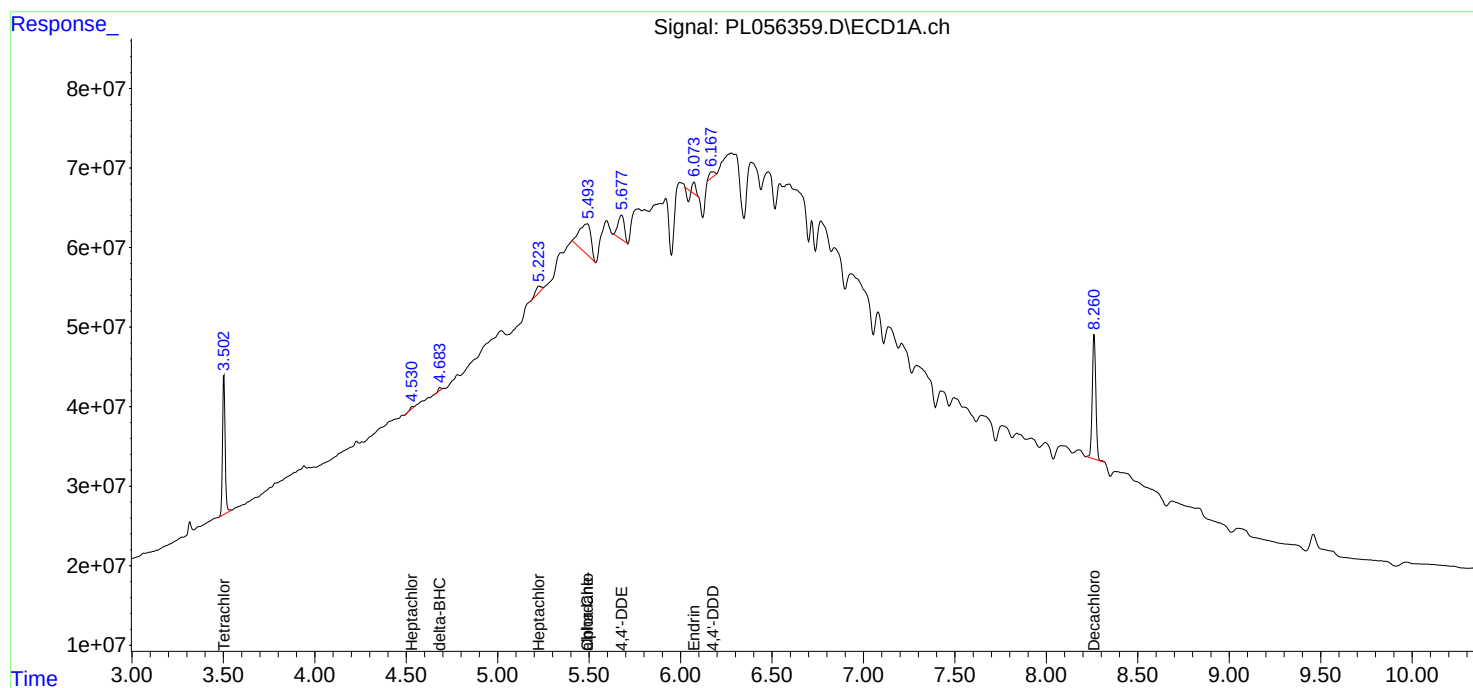


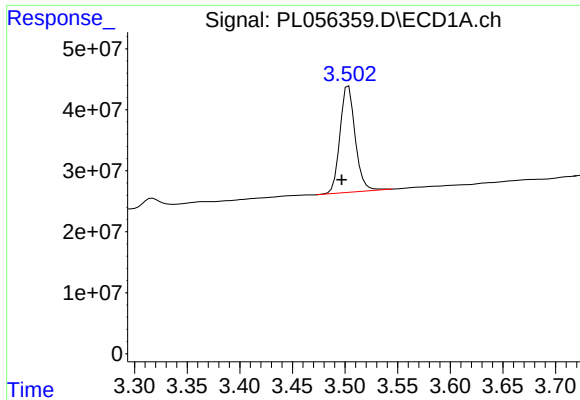

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.006 min
Response: 176007517
Conc: 16.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126623BL

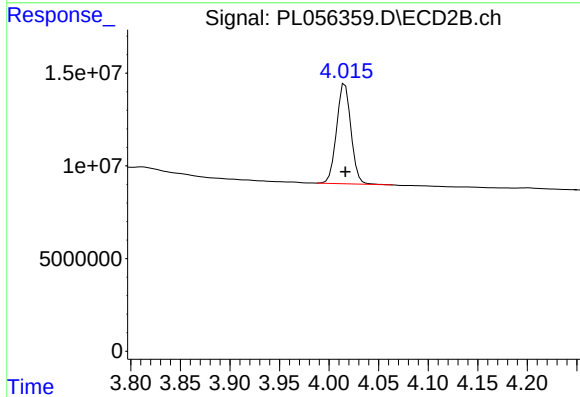


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 54488461
Conc: 18.63 ng/ml

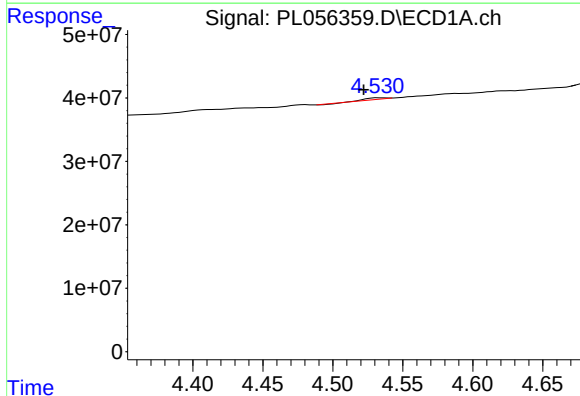


#4 Heptachlor

R.T.: 4.534 min
Delta R.T.: 0.012 min
Response: 1467593
Conc: 0.09 ng/ml

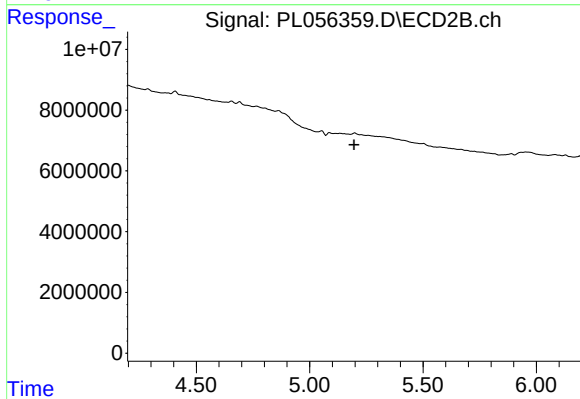

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.197 min
Response: 0
Conc: N.D.

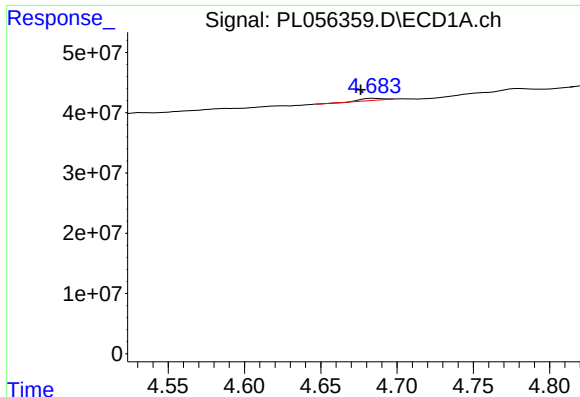

#7 delta-BHC


R.T.: 4.685 min
Delta R.T.: 0.009 min
Response: 2972247
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126623BL

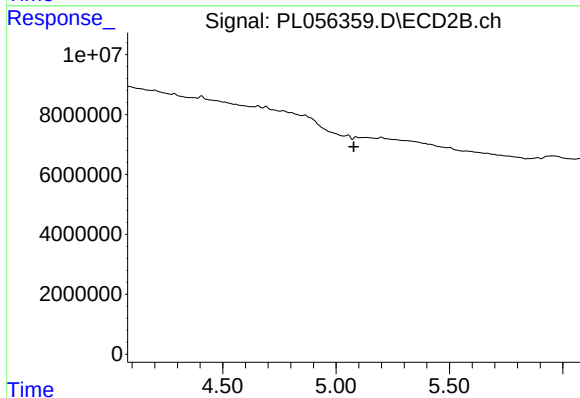


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 5.078 min
Response: 0
Conc: N.D.

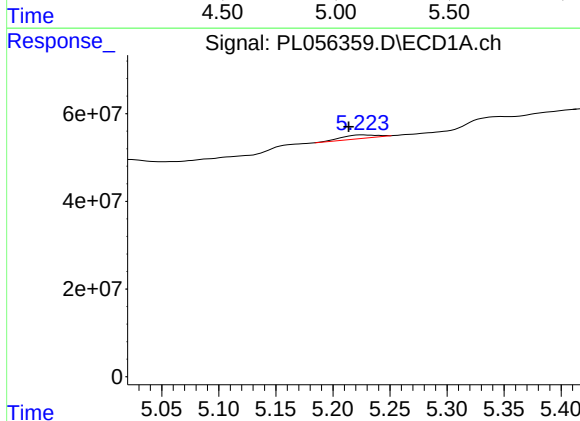


#8 Heptachlor epoxide

R.T.: 5.225 min
Delta R.T.: 0.012 min
Response: 17705916
Conc: 1.15 ng/ml

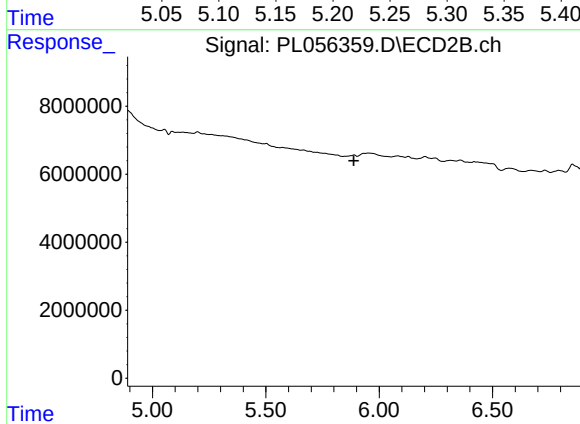

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.889 min
Response: 0
Conc: N.D.

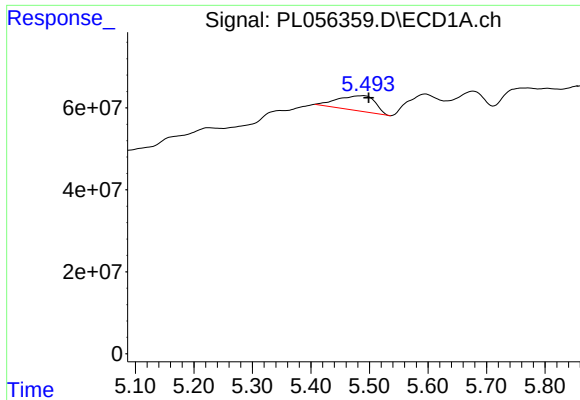

#11 alpha-Chlordane


R.T.: 5.491 min
Delta R.T.: -0.008 min
Response: 163345521
Conc: 10.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126623BL

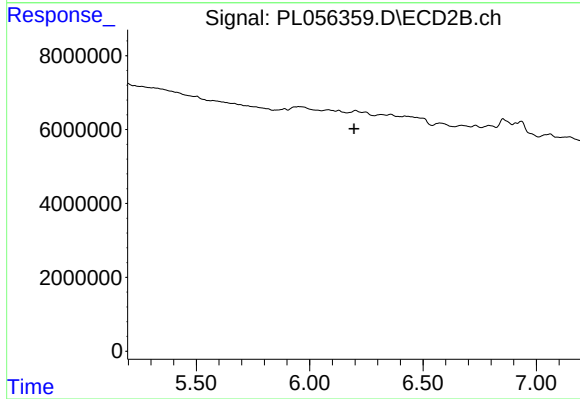


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

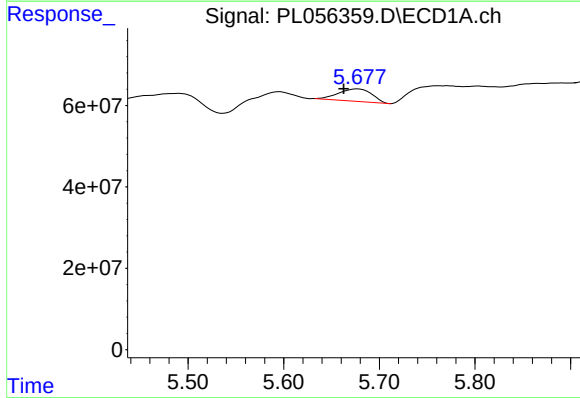


#12 4,4'-DDE

R.T.: 5.678 min
Delta R.T.: 0.015 min
Response: 73779532
Conc: 5.09 ng/ml

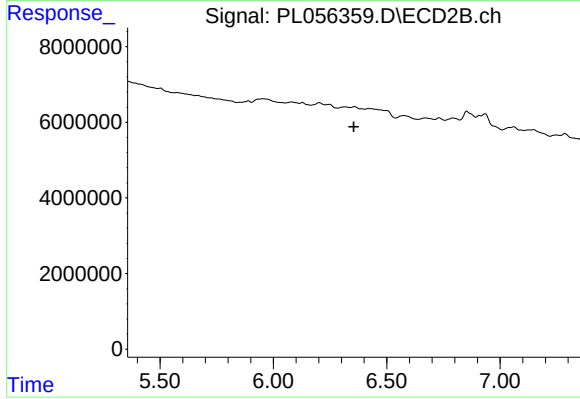

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.355 min
Response: 0
Conc: N.D.

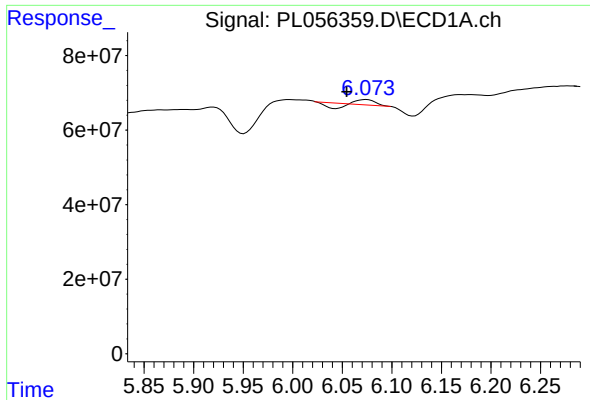

#14 Endrin


R.T.: 6.075 min
Delta R.T.: 0.020 min
Response: 2357657
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126623BL

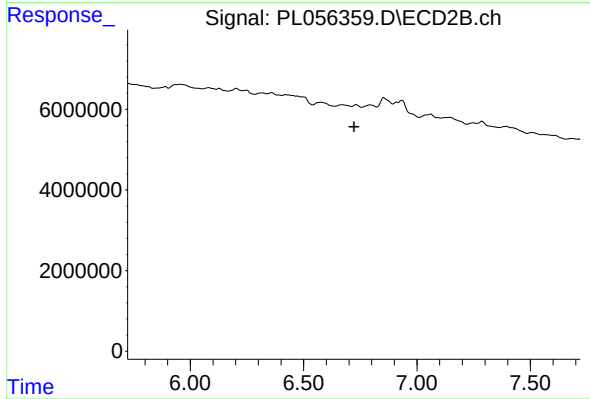


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.723 min
Response: 0
Conc: N.D.

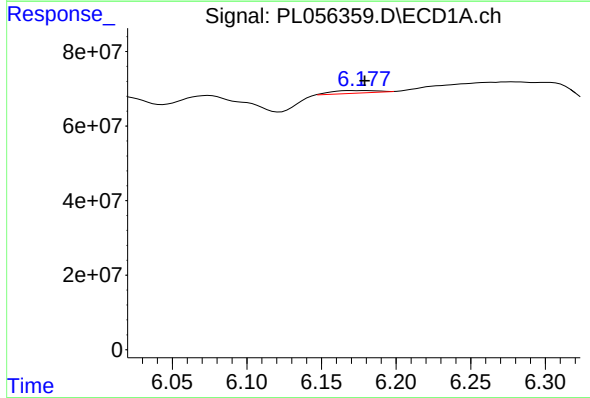


#16 4,4'-DDD

R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 14938306
Conc: 1.39 ng/ml

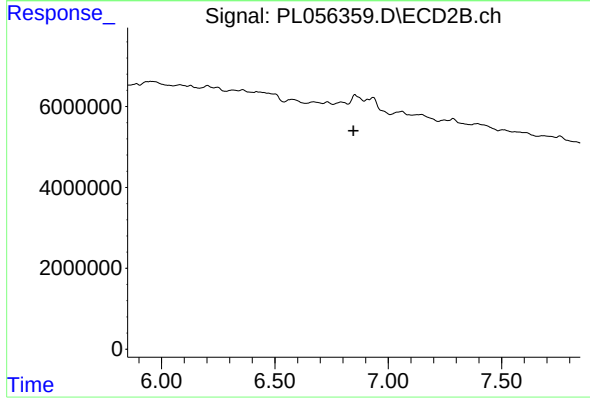

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.847 min
Response: 0
Conc: N.D.

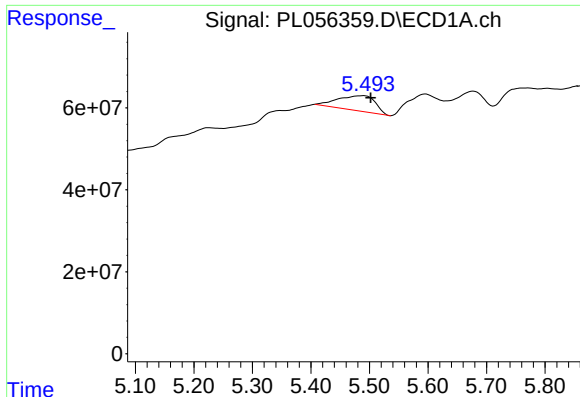

#26 Chlordane-4


R.T.: 5.491 min
Delta R.T.: -0.012 min
Response: 163345521
Conc: 150.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB126623BL

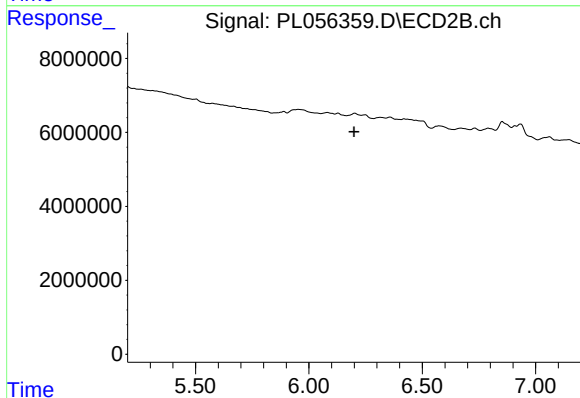


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.199 min
Response: 0
Conc: N.D.

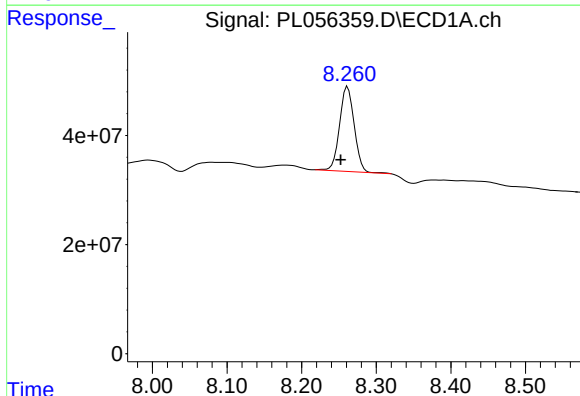

#28 Decachlorobiphenyl

R.T.: 8.262 min
Delta R.T.: 0.010 min
Response: 210846154
Conc: 20.03 ng/ml

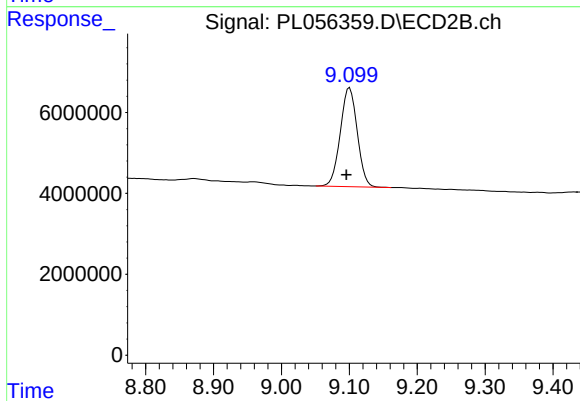

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.005 min
Response: 42542083
Conc: 18.81 ng/ml