

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020719\
 Data File : PL044567.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 21:31
 Operator : AJ\SJ
 Sample : K1394-01
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ISW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 07:53:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.986	123.2E6	39765222	17.310	16.927
28)	SA Decachlor...	8.051	9.045	142.4E6	43053277	19.524	19.438
Target Compounds							
4)	MA Heptachlor	4.353	5.171	65511126	9794968	6.359	3.216 #
6)	B beta-BHC	4.353f	0.000	65511126	0	15.504	N.D. #
7)	B delta-BHC	0.000	5.035	0	8382274	N.D.	4.584 #
8)	B Heptachlo...	0.000	5.843	0	5728992	N.D.	2.291 #
11)	B alpha-Chl...	5.316	0.000	20137405	0	2.106	N.D. #
15)	B Endosulfa...	6.158f	6.912	23028232	146827	2.723	0.064 #
17)	MA 4,4'-DDT	0.000	7.130f	0	3296322	N.D.	1.680 #
18)	B Endrin al...	0.000	6.992f	0	1680065	N.D.	0.828 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020719\
Data File : PL044567.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 21:31
Operator : AJ\SJ
Sample : K1394-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
ISW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 07:53:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

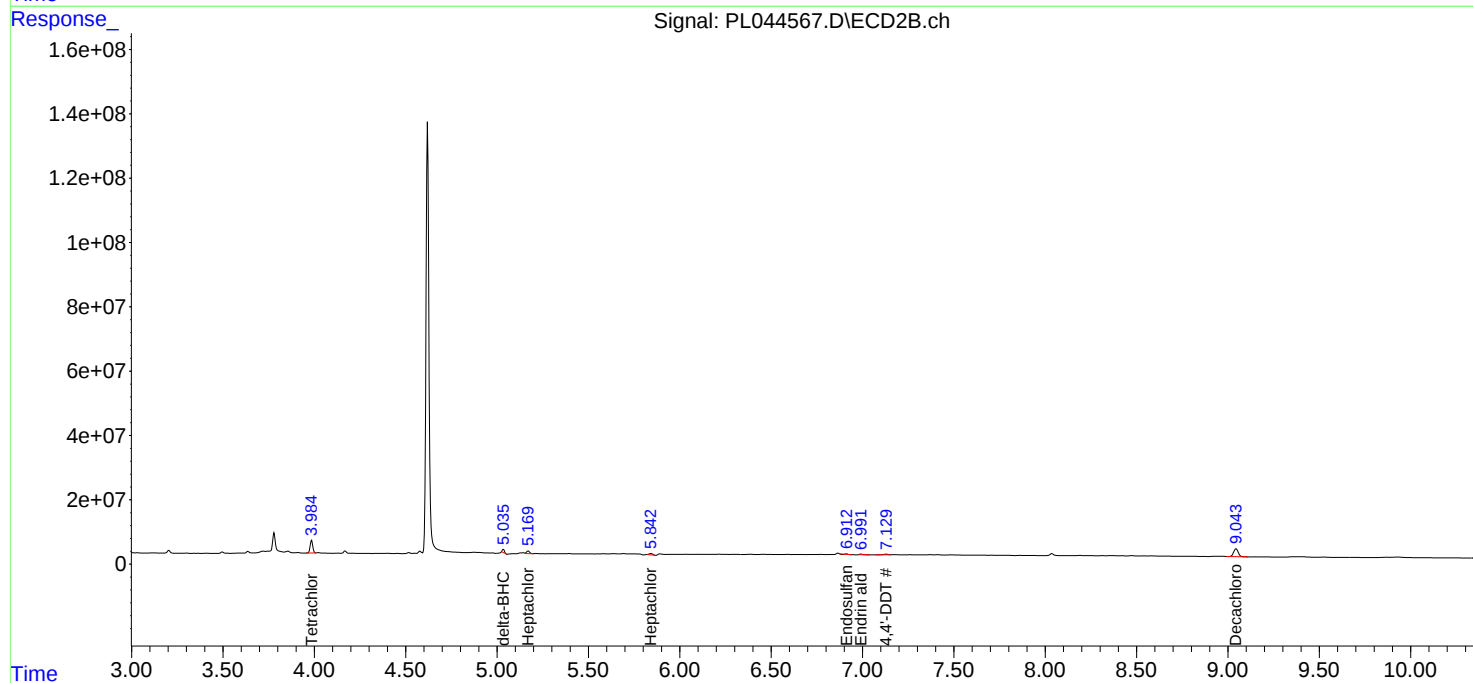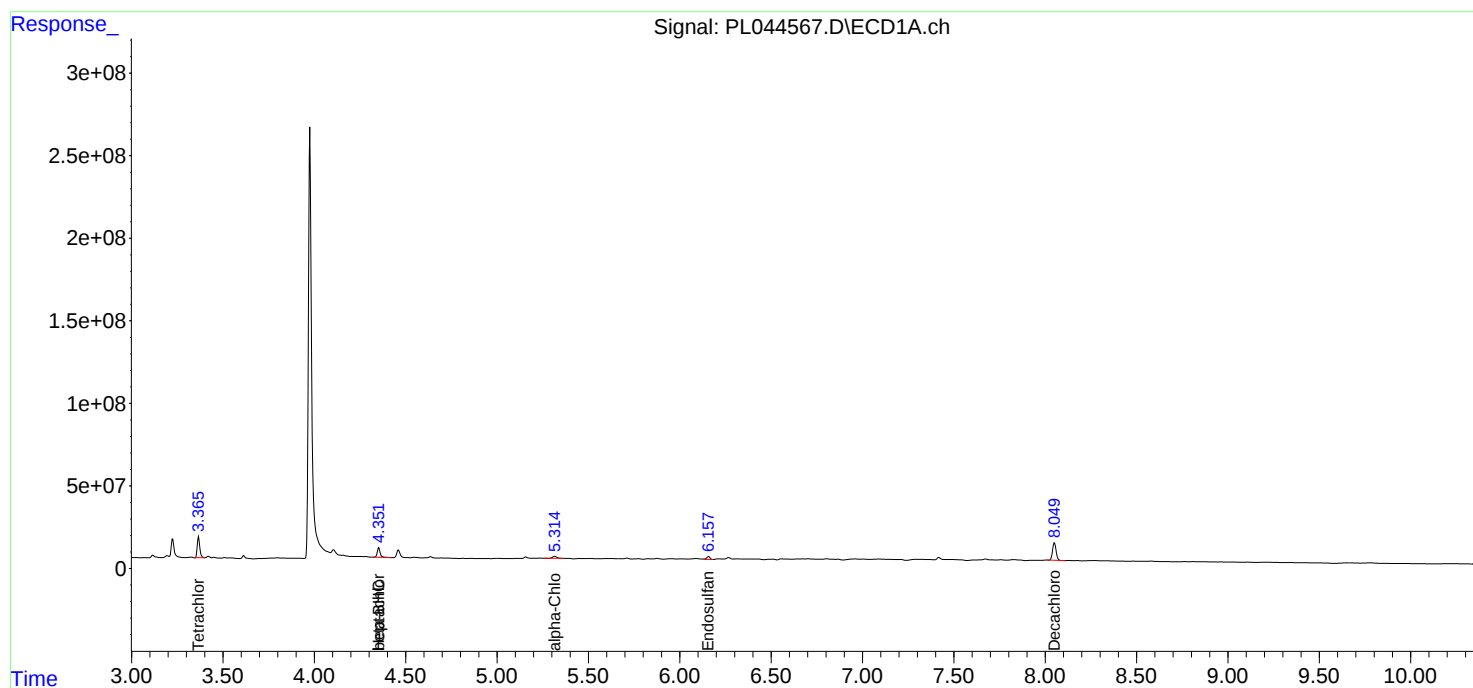


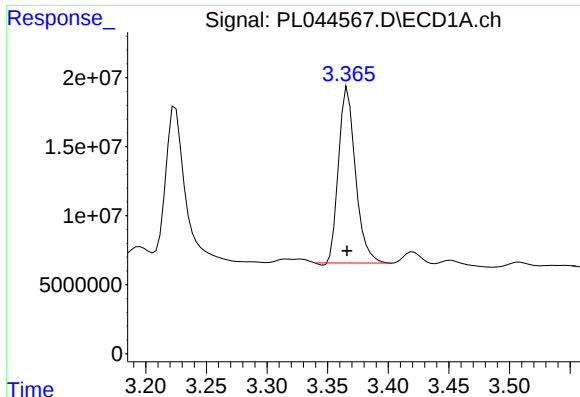

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.000 min
Response: 123176847
Conc: 17.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
ISW

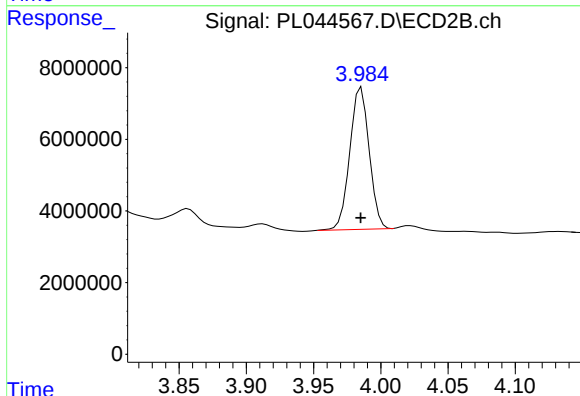


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 39765222
Conc: 16.93 ng/ml

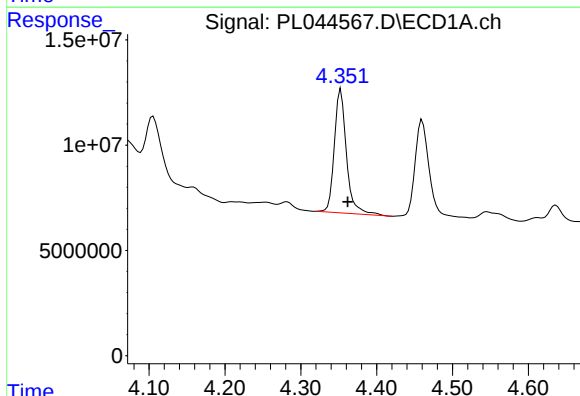


#4 Heptachlor

R.T.: 4.353 min
Delta R.T.: -0.009 min
Response: 65511126
Conc: 6.36 ng/ml

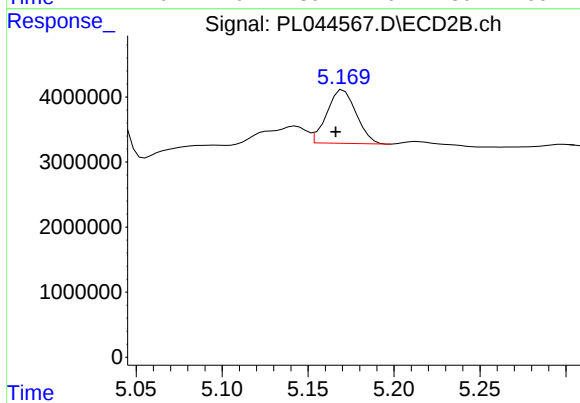

#4 Heptachlor


R.T.: 5.171 min
Delta R.T.: 0.005 min
Response: 9794968
Conc: 3.22 ng/ml

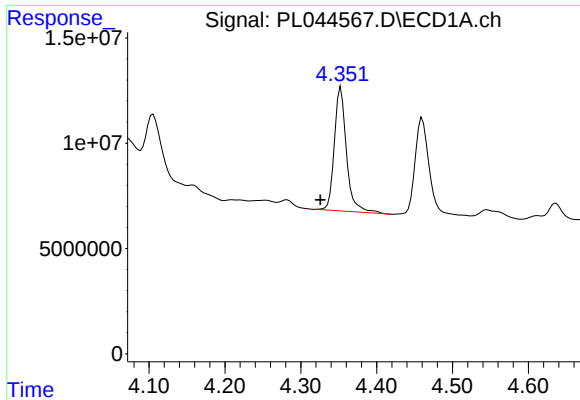

#6 beta-BHC


R.T.: 4.353 min
Delta R.T.: 0.027 min
Response: 65511126
Conc: 15.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
ISW

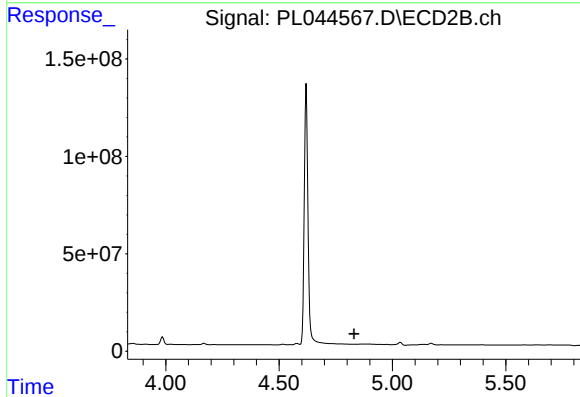


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.831 min
Response: 0
Conc: N.D.

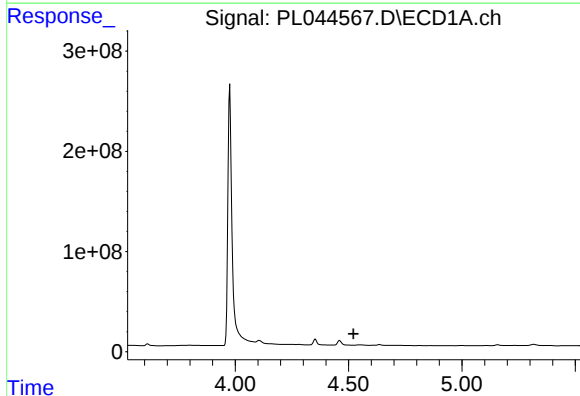


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.522 min
Response: 0
Conc: N.D.

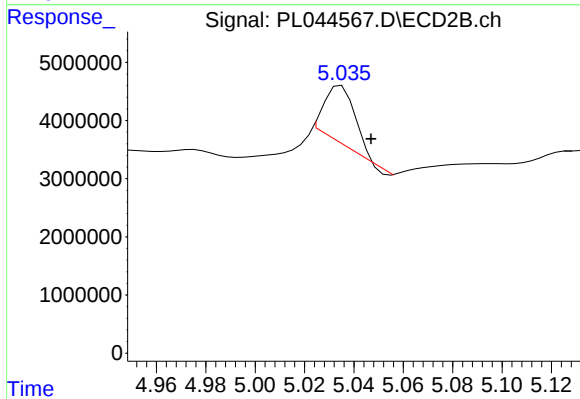

#7 delta-BHC


R.T.: 5.035 min
Delta R.T.: -0.012 min
Response: 8382274
Conc: 4.58 ng/ml

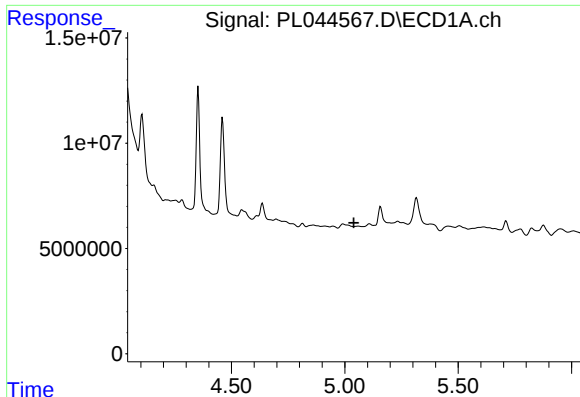

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ISW

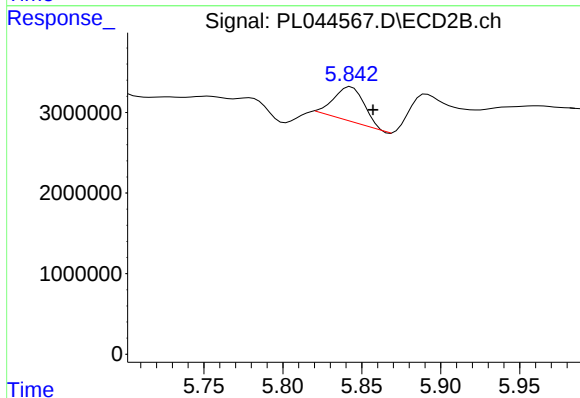


#8 Heptachlor epoxide

R.T.: 5.843 min
Delta R.T.: -0.014 min
Response: 5728992
Conc: 2.29 ng/ml

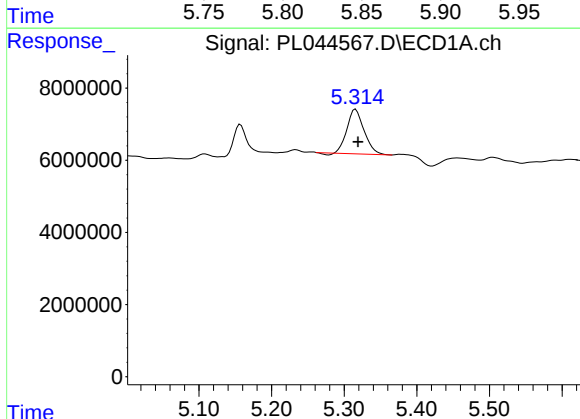


#11 alpha-Chlordane

R.T.: 5.316 min
Delta R.T.: -0.003 min
Response: 20137405
Conc: 2.11 ng/ml

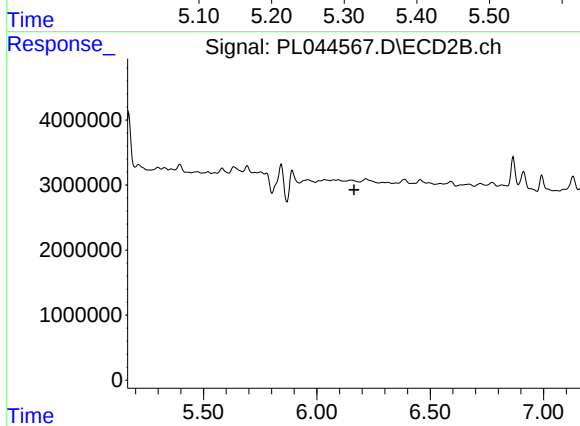

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.164 min
Response: 0
Conc: N.D.

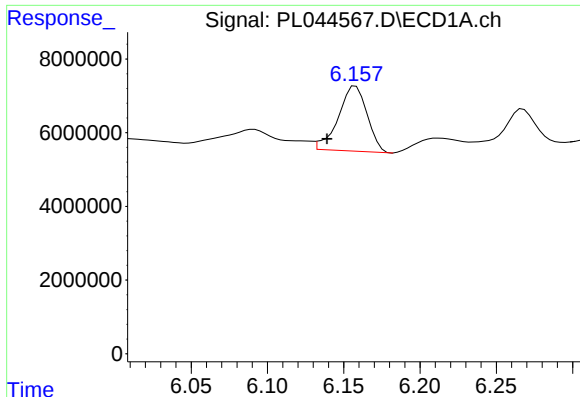

#15 Endosulfan II


R.T.: 6.158 min
Delta R.T.: 0.019 min
Response: 23028232
Conc: 2.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
ISW

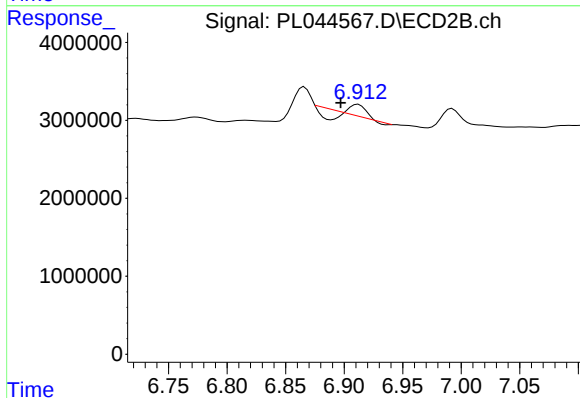


#15 Endosulfan II

R.T.: 6.912 min
Delta R.T.: 0.015 min
Response: 146827
Conc: 0.06 ng/ml

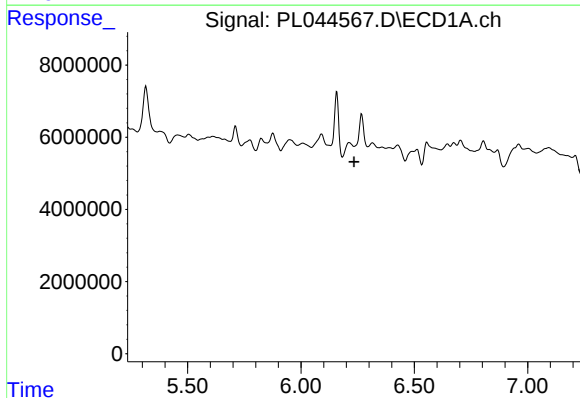


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.234 min
Response: 0
Conc: N.D.

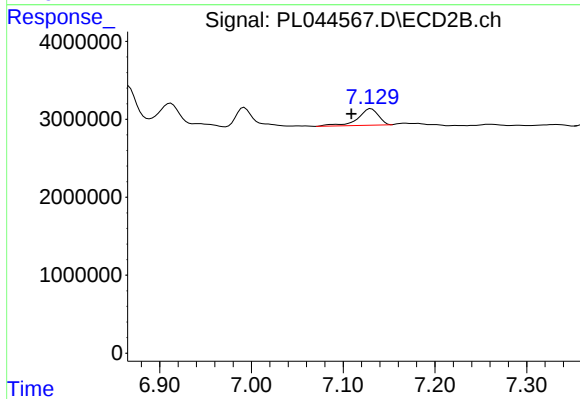

#17 4,4'-DDT


R.T.: 7.130 min
Delta R.T.: 0.021 min
Response: 3296322
Conc: 1.68 ng/ml

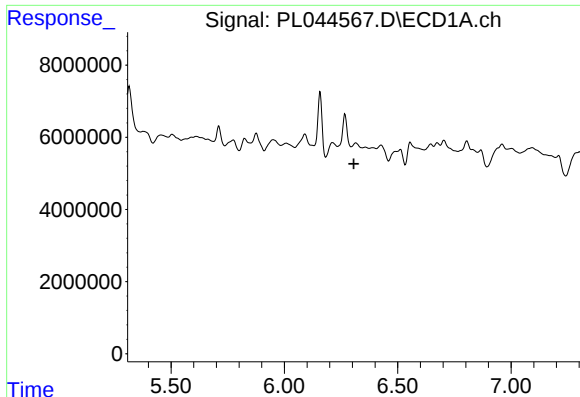

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
ISW

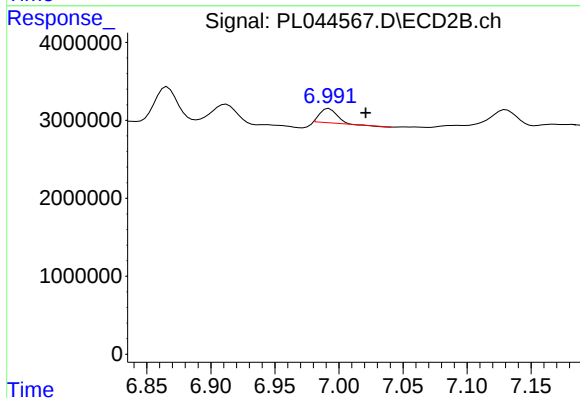


#18 Endrin aldehyde

R.T.: 6.992 min
Delta R.T.: -0.029 min
Response: 1680065
Conc: 0.83 ng/ml

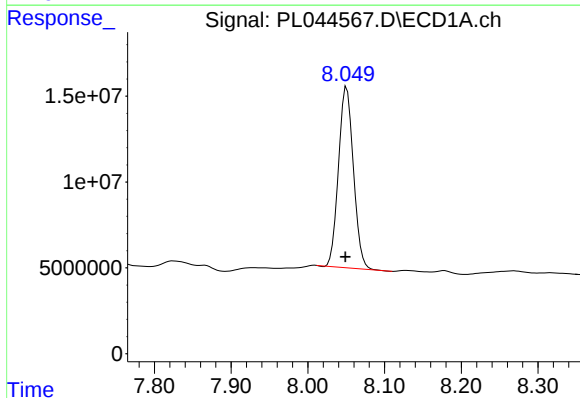

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 142396183
Conc: 19.52 ng/ml

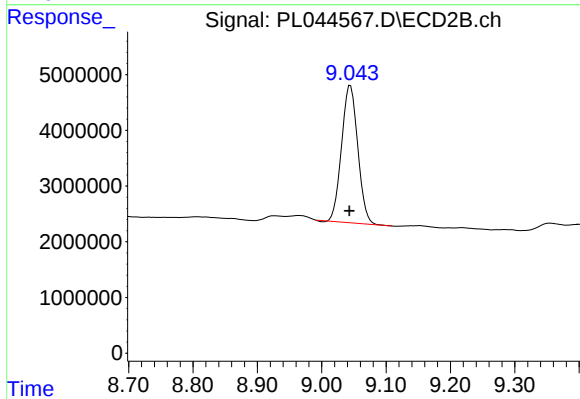

#28 Decachlorobiphenyl

R.T.: 9.045 min
Delta R.T.: 0.002 min
Response: 43053277
Conc: 19.44 ng/ml