

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020719\
 Data File : PL044570.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 22:13
 Operator : AJ\SJ
 Sample : K1401-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 07:53:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.986	115.8E6	41354363	16.268	17.604
28)	SA Decachlor...	8.050	9.046	150.5E6	42450768	20.629	19.166
Target Compounds							
2)	A alpha-BHC	3.826f	0.000	10664213	0	0.999	N.D. #
3)	MA gamma-BHC...	4.081	0.000	24459183	0	2.486	N.D. #
9)	A Endosulfan I	5.401f	6.221	10678475	504011	1.224	0.199 #
10)	B gamma-Chl...	0.000	6.078	0	5432410	N.D.	1.957 #
13)	MA Dieldrin	5.598	6.464	27326428	1460500	2.911	0.566 #
15)	B Endosulfa...	6.125	0.000	16272076	0	1.924	N.D. #
18)	B Endrin al...	0.000	7.015	0	1693139	N.D.	0.835 #
19)	B Endosulfa...	6.547f	0.000	15917792	0	2.190	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020719\
Data File : PL044570.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 22:13
Operator : AJ\SJ
Sample : K1401-04
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 07:53:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

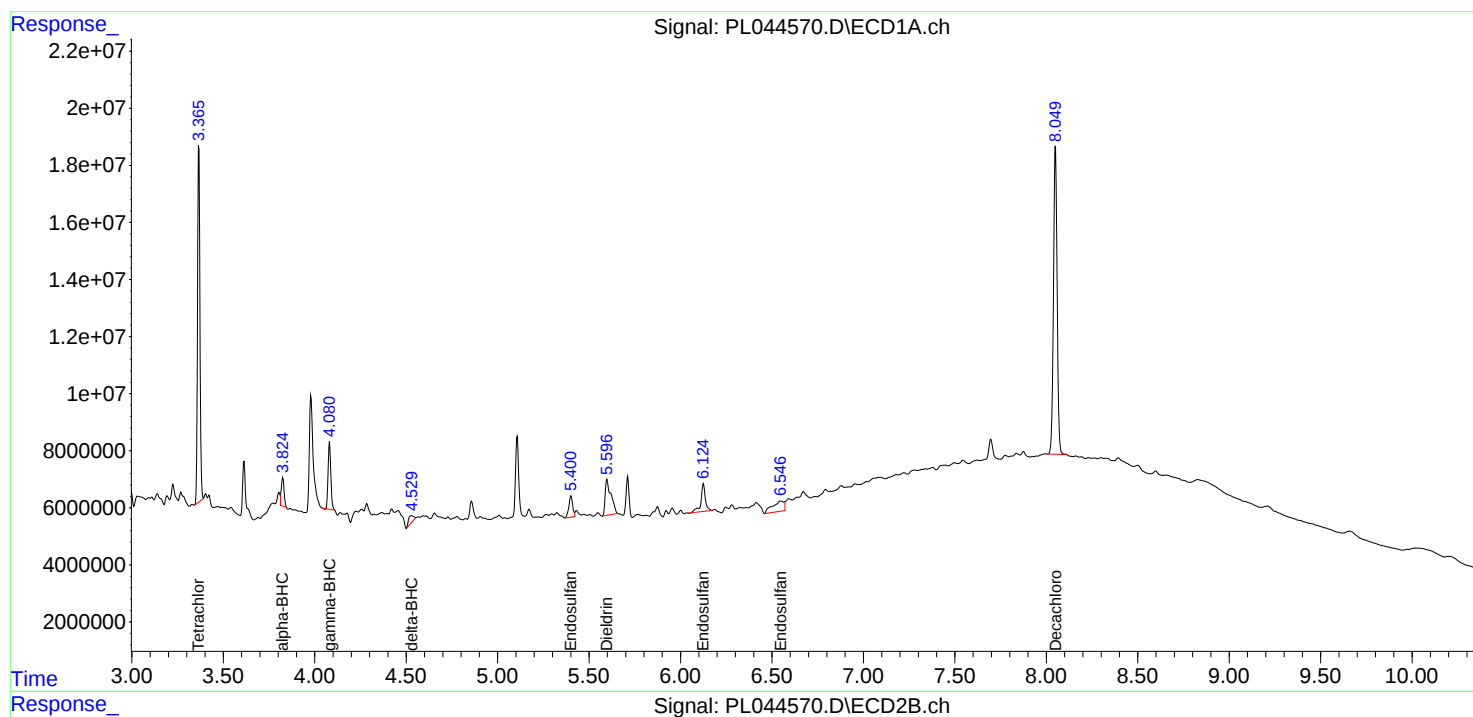


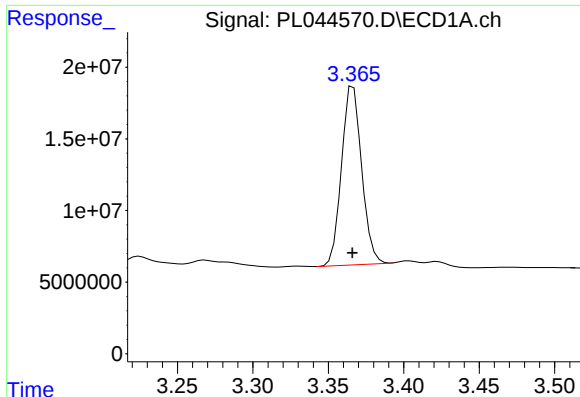

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.000 min
Response: 115758301
Conc: 16.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

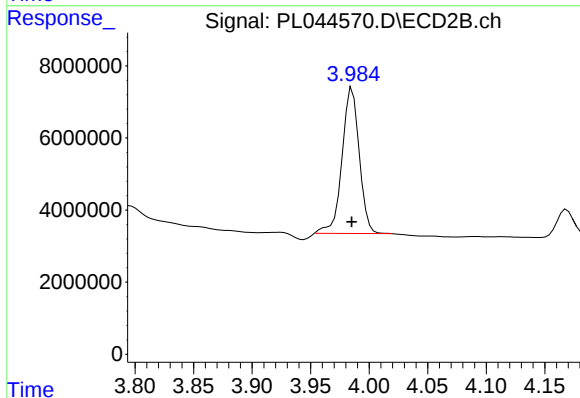


#1 Tetrachloro-m-xylene

R.T.: 3.986 min
Delta R.T.: 0.000 min
Response: 41354363
Conc: 17.60 ng/ml

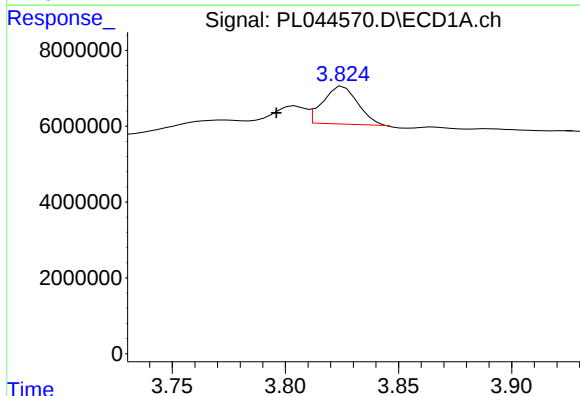


#2 alpha-BHC

R.T.: 3.826 min
Delta R.T.: 0.030 min
Response: 10664213
Conc: 1.00 ng/ml

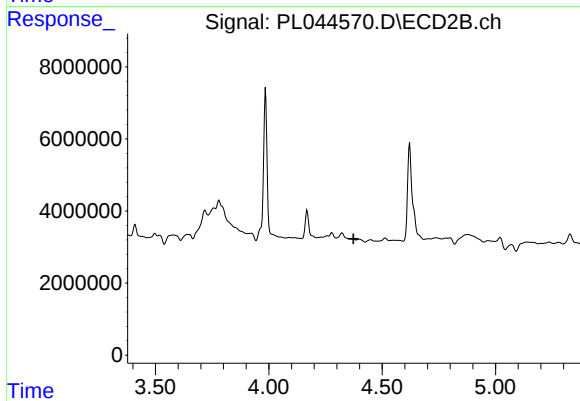

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.374 min
Response: 0
Conc: N.D.

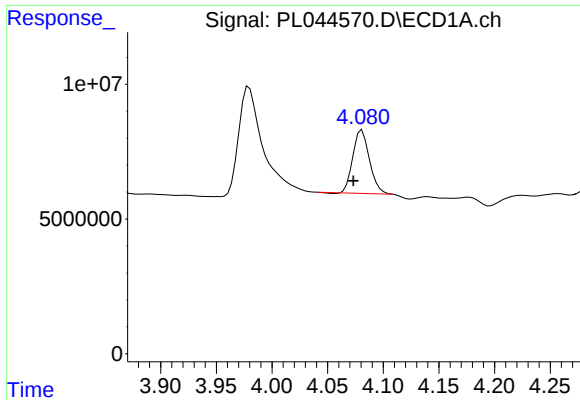

#3 gamma-BHC (Lindane)


R.T.: 4.081 min
Delta R.T.: 0.008 min
Response: 24459183
Conc: 2.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

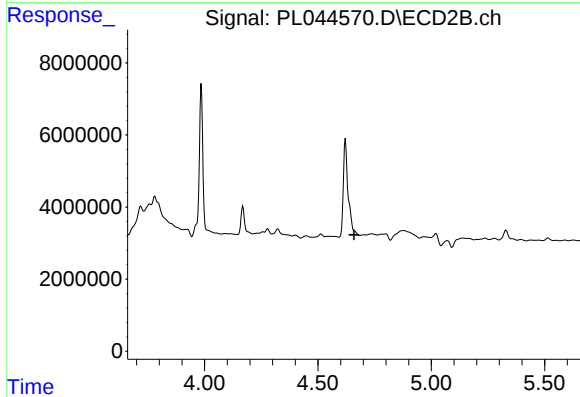


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.659 min
Response: 0
Conc: N.D.

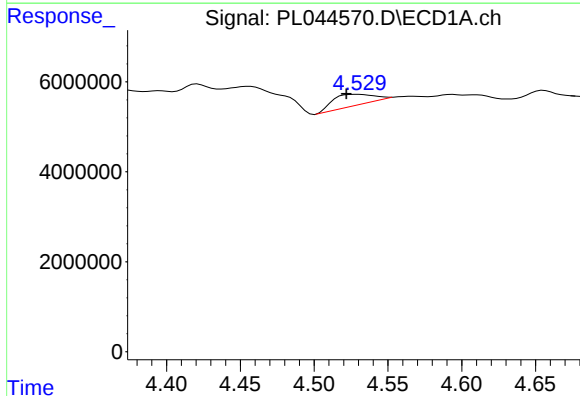


#7 delta-BHC

R.T.: 4.530 min
Delta R.T.: 0.008 min
Response: 4677627
Conc: 0.58 ng/ml

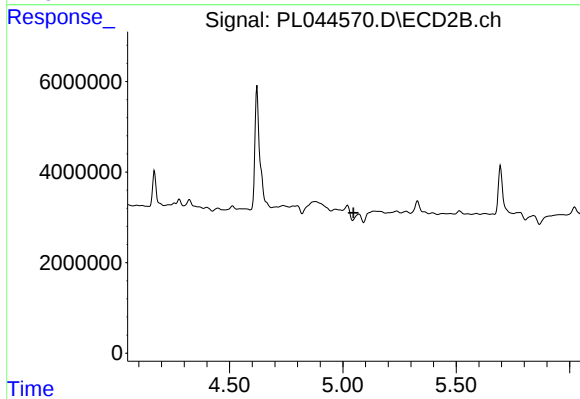

#7 delta-BHC


R.T.: 5.071 min
Delta R.T.: 0.024 min
Response: -1085730
Conc: N.D.

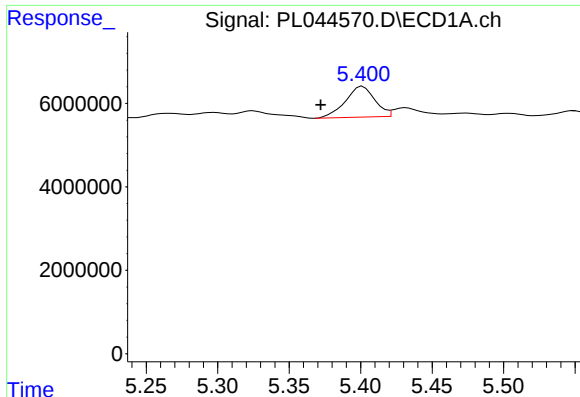

#9 Endosulfan I


R.T.: 5.401 min
Delta R.T.: 0.029 min
Response: 10678475
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

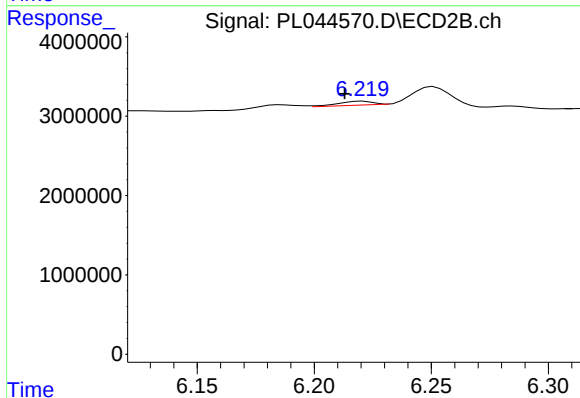


#9 Endosulfan I

R.T.: 6.221 min
Delta R.T.: 0.008 min
Response: 504011
Conc: 0.20 ng/ml

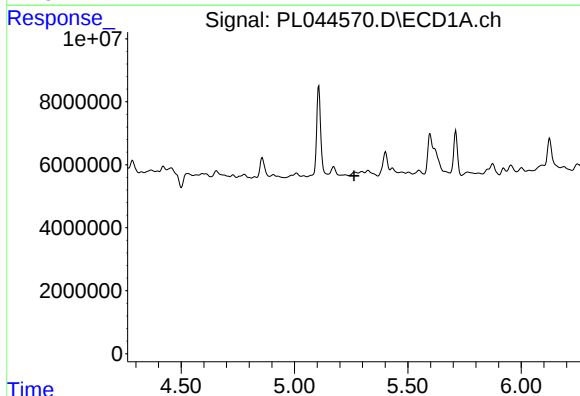


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.263 min
Response: 0
Conc: N.D.

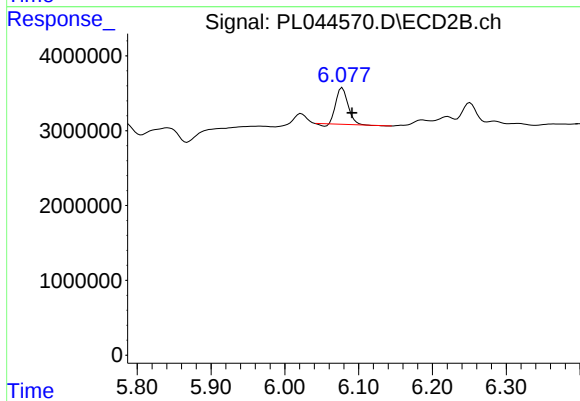

#10 gamma-Chlordane


R.T.: 6.078 min
Delta R.T.: -0.013 min
Response: 5432410
Conc: 1.96 ng/ml

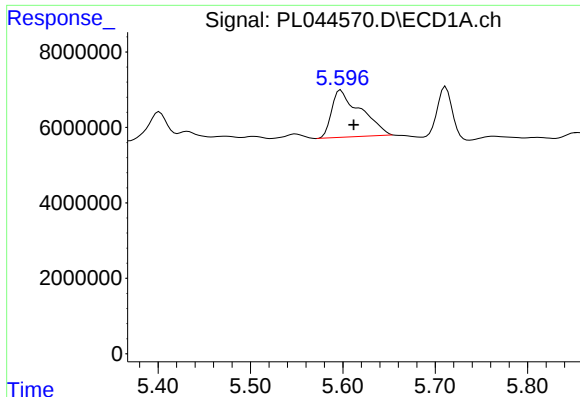

#13 Dieldrin


R.T.: 5.598 min
Delta R.T.: -0.014 min
Response: 27326428
Conc: 2.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

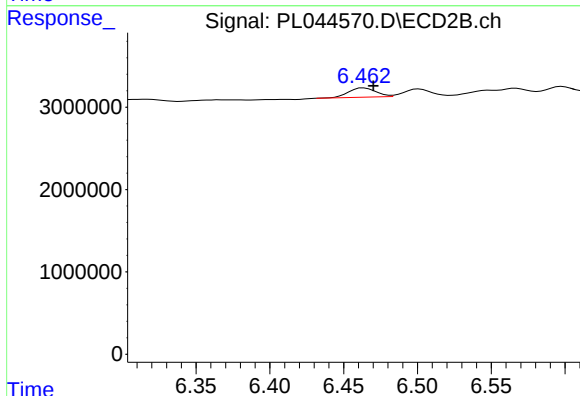


#13 Dieldrin

R.T.: 6.464 min
Delta R.T.: -0.006 min
Response: 1460500
Conc: 0.57 ng/ml

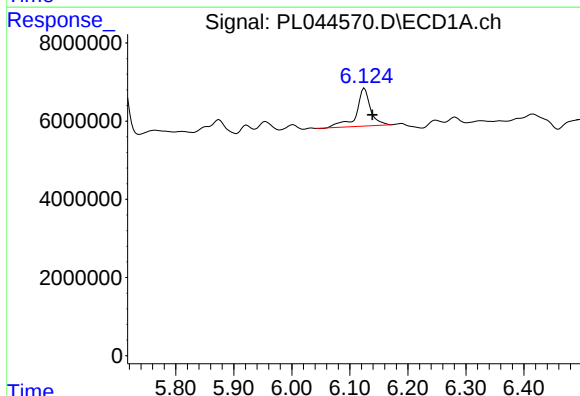


#15 Endosulfan II

R.T.: 6.125 min
Delta R.T.: -0.014 min
Response: 16272076
Conc: 1.92 ng/ml

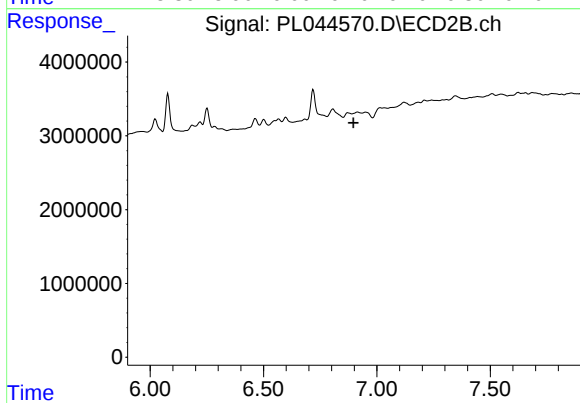

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.897 min
Response: 0
Conc: N.D.

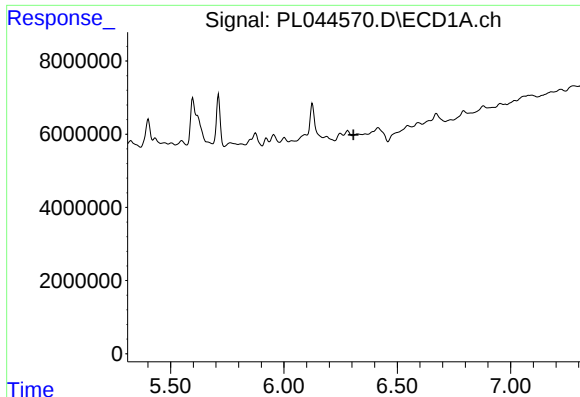

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

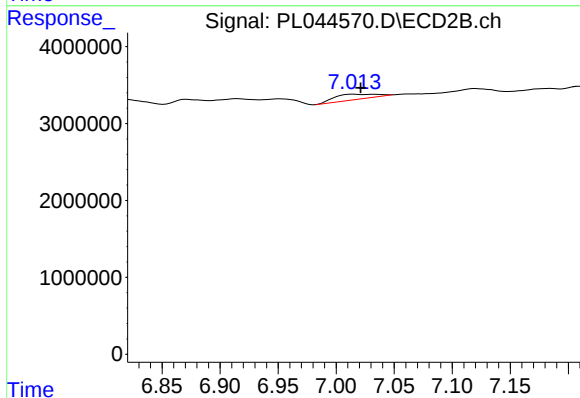


#18 Endrin aldehyde

R.T.: 7.015 min
Delta R.T.: -0.006 min
Response: 1693139
Conc: 0.83 ng/ml

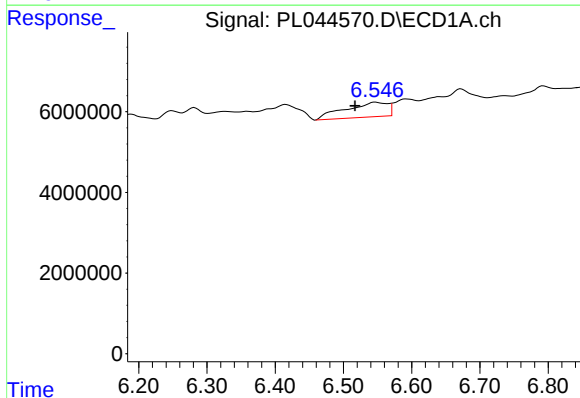


#19 Endosulfan Sulfate

R.T.: 6.547 min
Delta R.T.: 0.030 min
Response: 15917792
Conc: 2.19 ng/ml

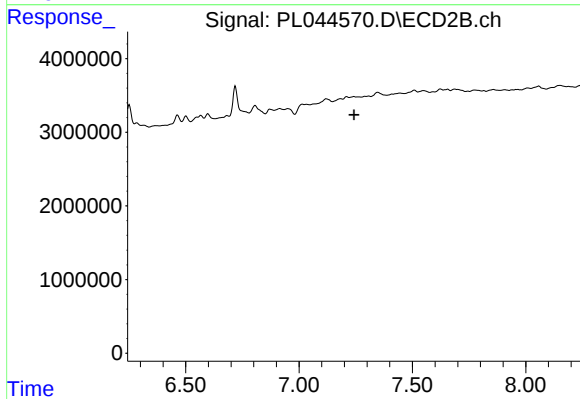

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.243 min
Response: 0
Conc: N.D.

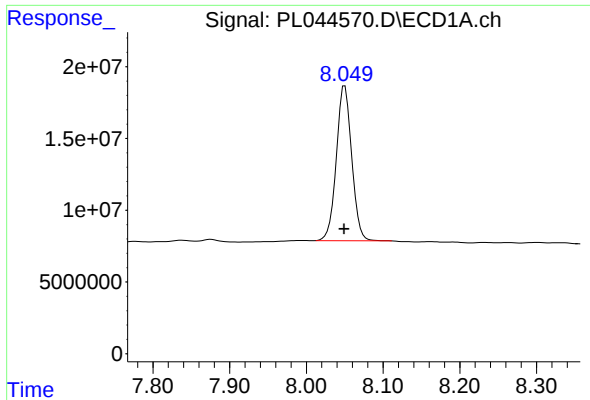

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.001 min
Response: 150461581
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

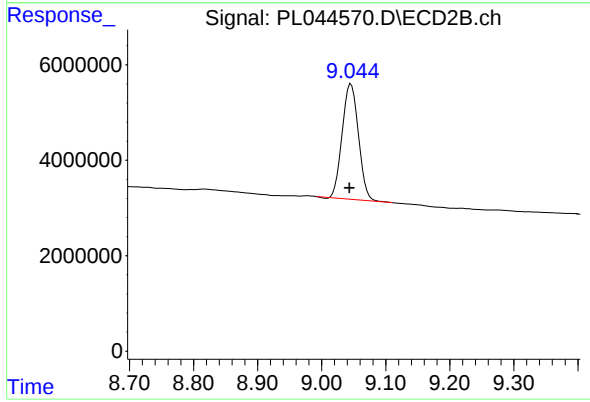

#28 Decachlorobiphenyl

R.T.: 9.046 min
Delta R.T.: 0.003 min
Response: 42450768
Conc: 19.17 ng/ml