

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020719\
 Data File : PL044550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2019 17:31
 Operator : AJ\SJ
 Sample : K1401-07
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RT-3451

Manual Integrations
 APPROVED

Sohil
 2/8/2019 5:09:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 07:51:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.366	3.985	70379786	24213372	9.891	10.307
28) SA Decachlor...	8.050	9.044	75217214	22386732	10.313	10.108
Target Compounds						
12) B 4,4'-DDE	5.486	6.321	4970660	1593818	0.573	0.668
17) MA 4,4'-DDT	6.230	7.109	4968471	1102194	0.693	0.562m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : X:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020719\
Data File : PL044550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2019 17:31
Operator : AJ\SJ
Sample : K1401-07
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
RT-3451


Manual Integrations
APPROVED

Sohil
2/8/2019 5:09:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 07:51:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

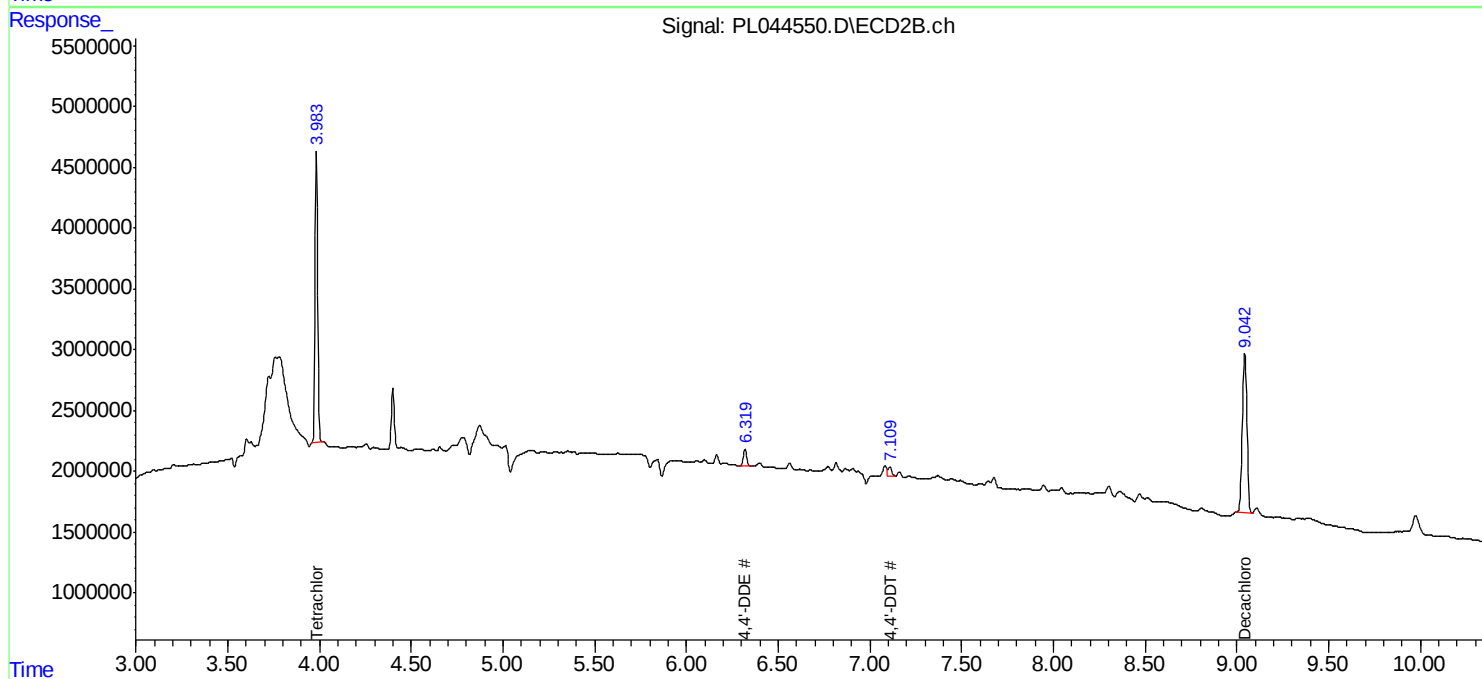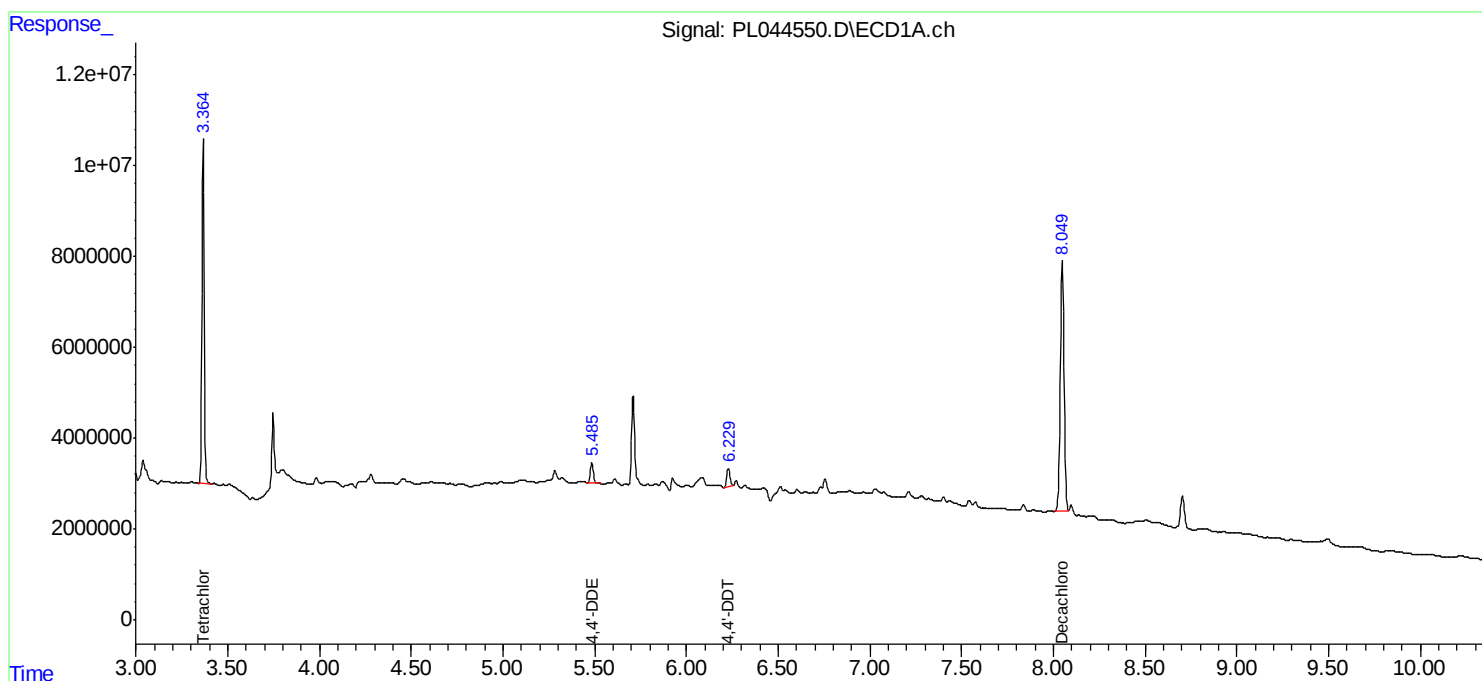

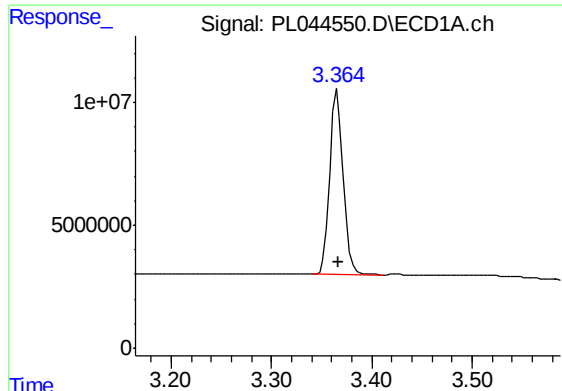


#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: 0.000 min
Response: 70379786
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3451


Manual Integrations
APPROVED

Sohil
2/8/2019 5:09:51 PM

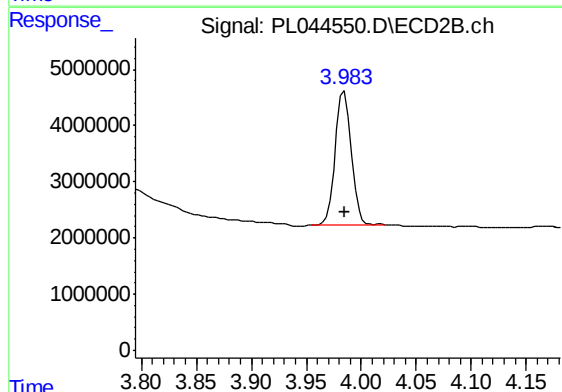


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 24213372
Conc: 10.31 ng/ml

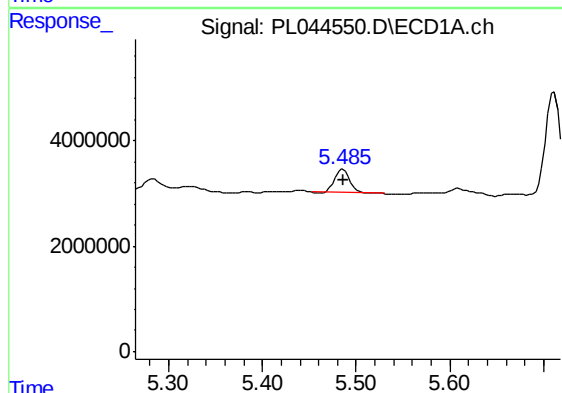


#12 4,4'-DDE

R.T.: 5.486 min
Delta R.T.: -0.001 min
Response: 4970660
Conc: 0.57 ng/ml

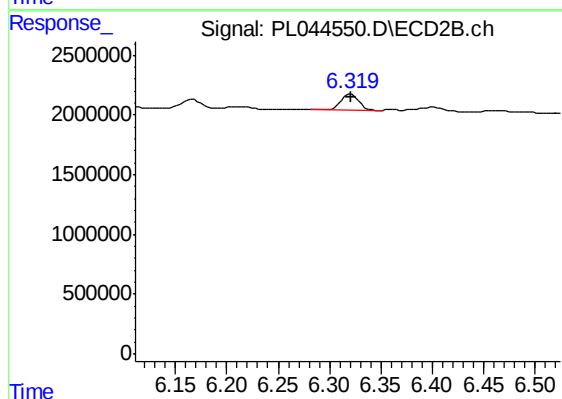

#12 4,4'-DDE

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 1593818
Conc: 0.67 ng/ml

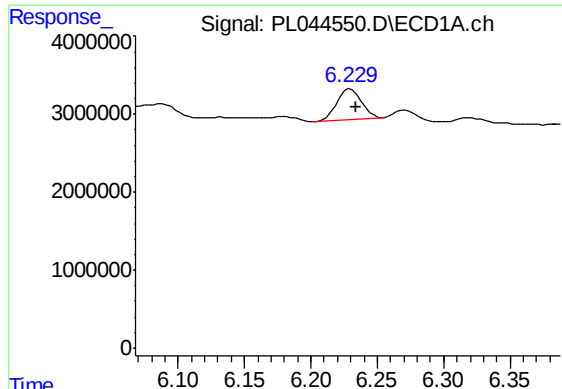


#17 4,4'-DDT

R.T.: 6.230 min
Delta R.T.: -0.004 min
Response: 4968471
Conc: 0.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
RT-3451


Manual Integrations
APPROVED

Sohil
2/8/2019 5:09:51 PM

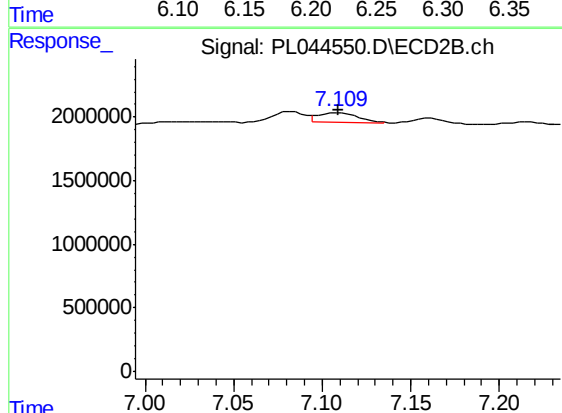


#17 4,4'-DDT

R.T.: 7.109 min
Delta R.T.: 0.000 min
Response: 1102194
Conc: 0.56 ng/ml m

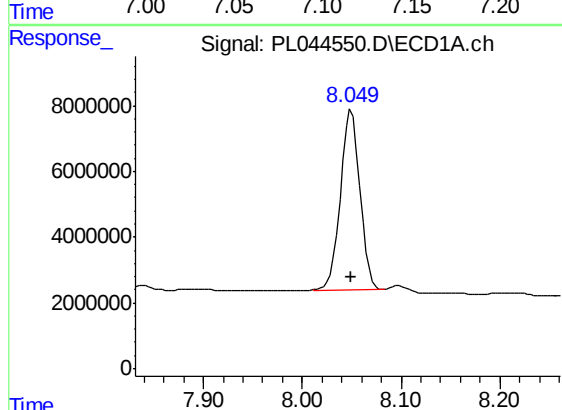

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.000 min
Response: 75217214
Conc: 10.31 ng/ml

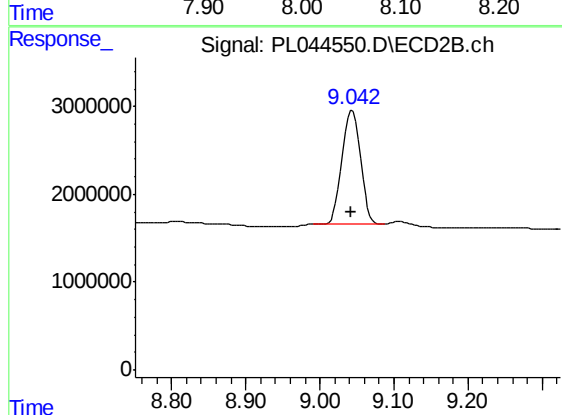

#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.000 min
Response: 22386732
Conc: 10.11 ng/ml