

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 18:19
 Operator : AJ\MA
 Sample : L1431-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:33:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.018	180.2E6	58209212	17.207	19.907
28)	SA Decachlor...	8.255	9.098	227.7E6	44577891	21.625	19.708
Target Compounds							
7)	B delta-BHC	0.000	5.050f	0	11352273	N.D.	3.540 #
8)	B Heptachlo...	5.217	0.000	4022240	0	0.262	N.D. #
17)	MA 4,4'-DDT	6.417	0.000	9563371	0	0.875	N.D. #
23)	Chlordane-1	4.374	0.000	11335571	0	29.945	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 18:19
Operator : AJ\MA
Sample : L1431-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:33:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

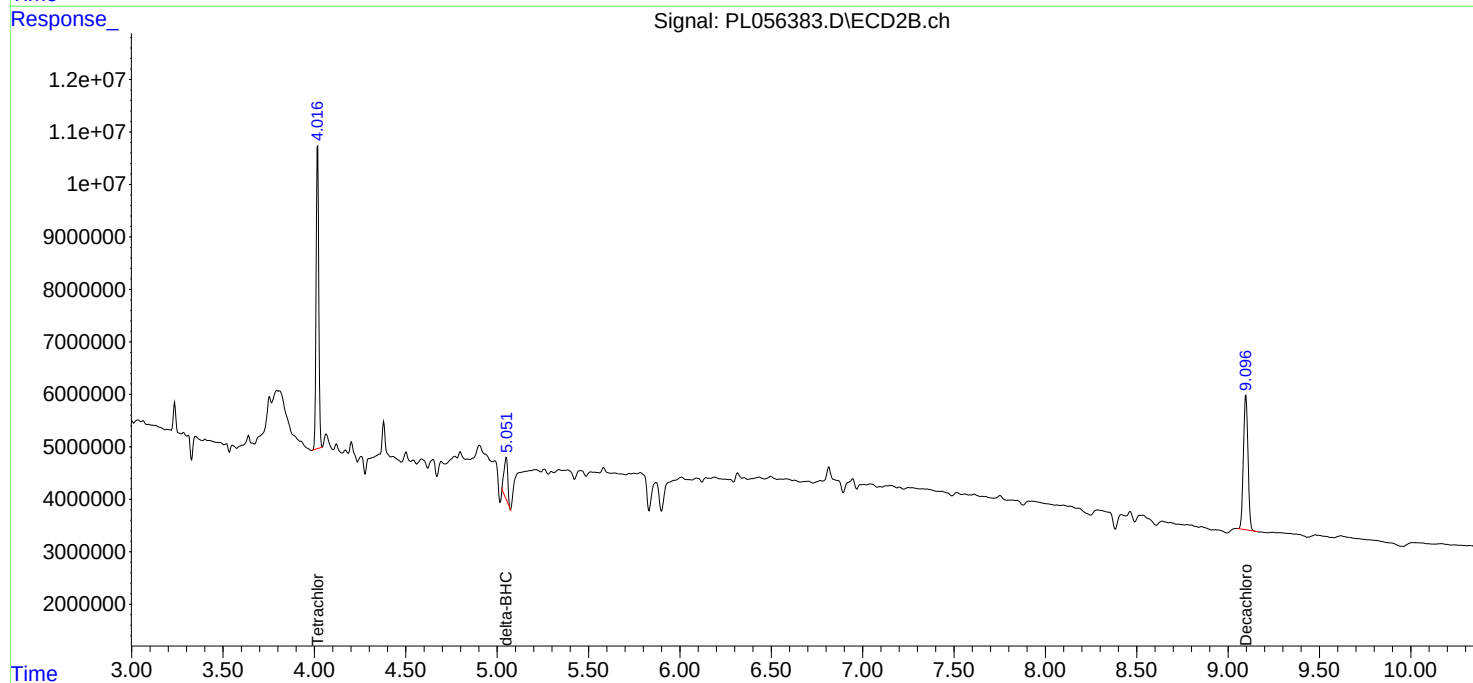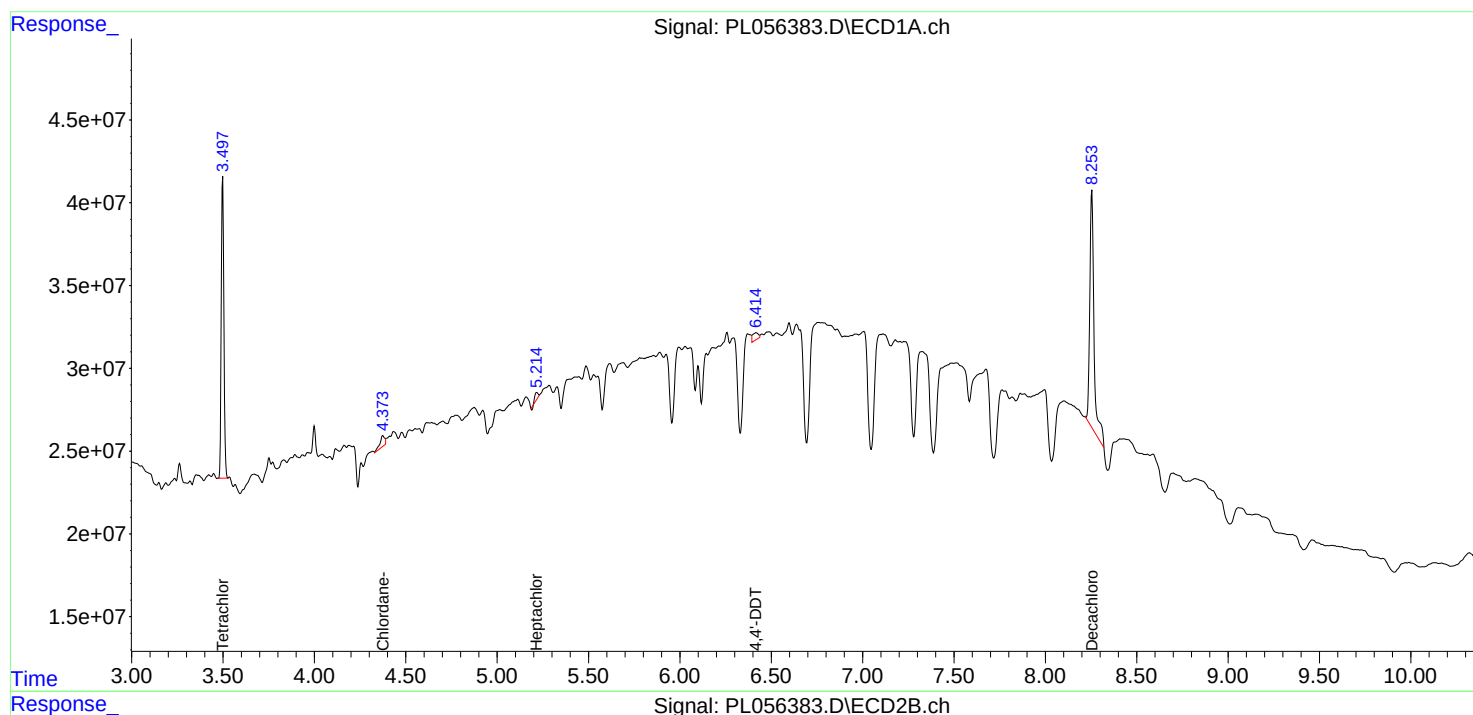


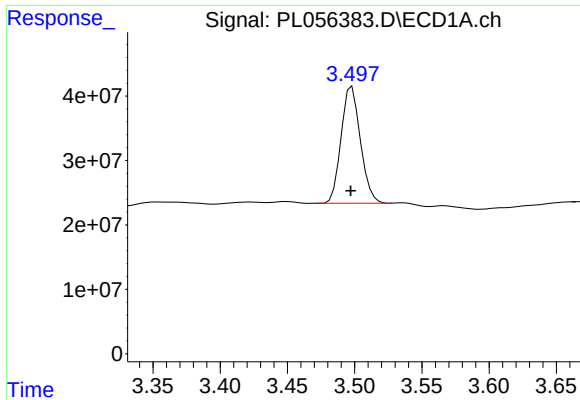

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 180213641
Conc: 17.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

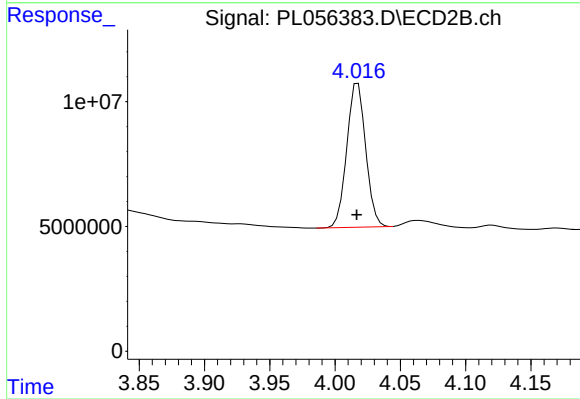


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: 0.001 min
Response: 58209212
Conc: 19.91 ng/ml

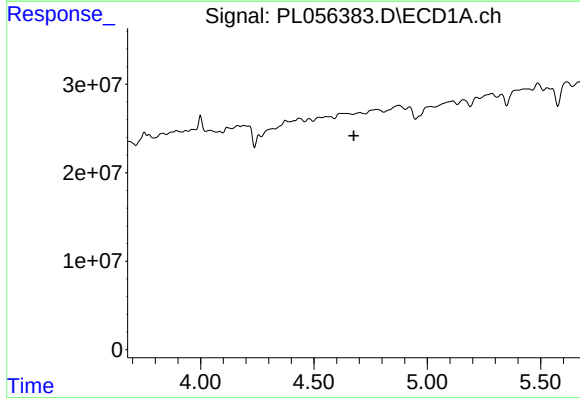


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

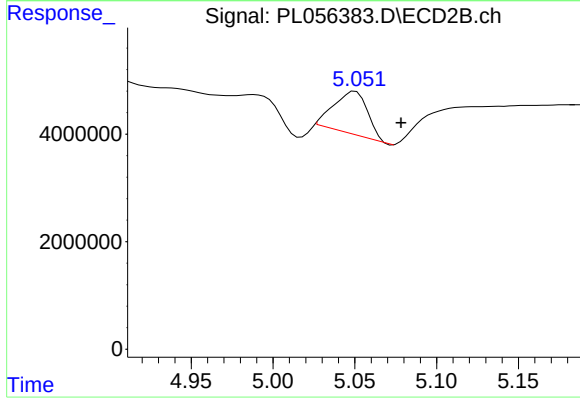

#7 delta-BHC


R.T.: 5.050 min
Delta R.T.: -0.028 min
Response: 11352273
Conc: 3.54 ng/ml

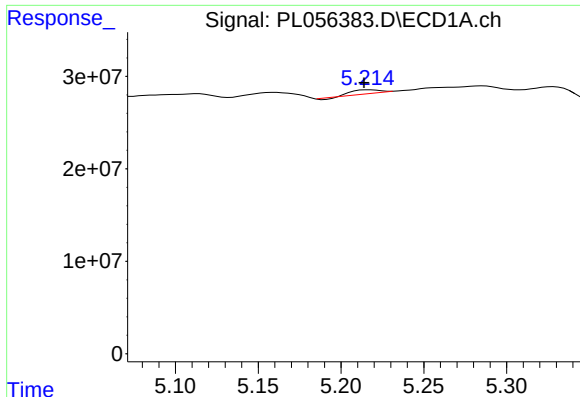

#8 Heptachlor epoxide


R.T.: 5.217 min
Delta R.T.: 0.003 min
Response: 4022240
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

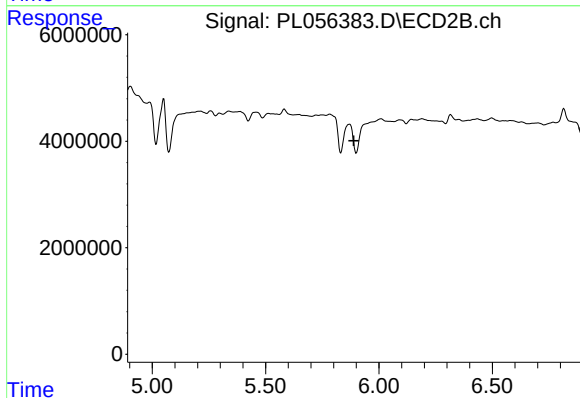


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.889 min
Response: 0
Conc: N.D.

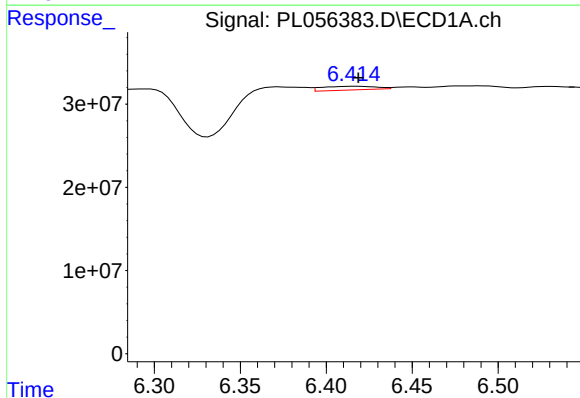


#17 4,4'-DDT

R.T.: 6.417 min
Delta R.T.: -0.002 min
Response: 9563371
Conc: 0.88 ng/ml

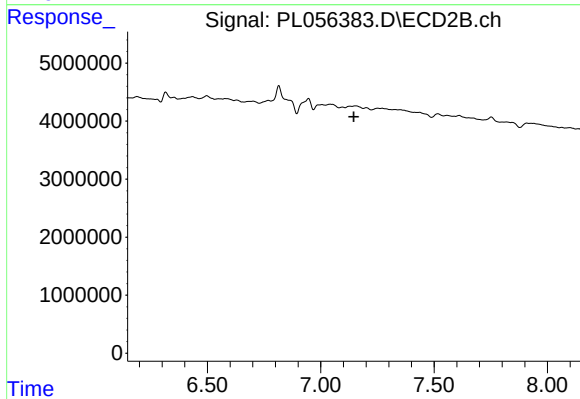

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

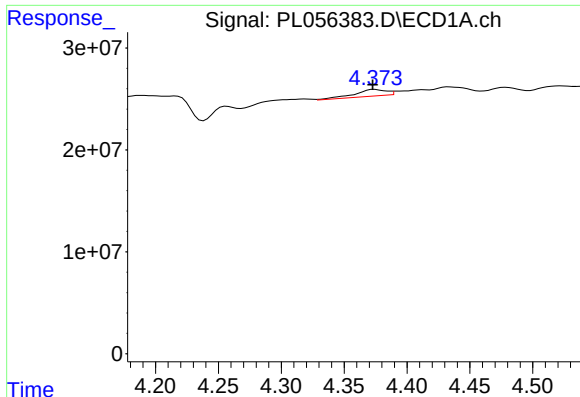

#23 Chlordane-1


R.T.: 4.374 min
Delta R.T.: 0.002 min
Response: 11335571
Conc: 29.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

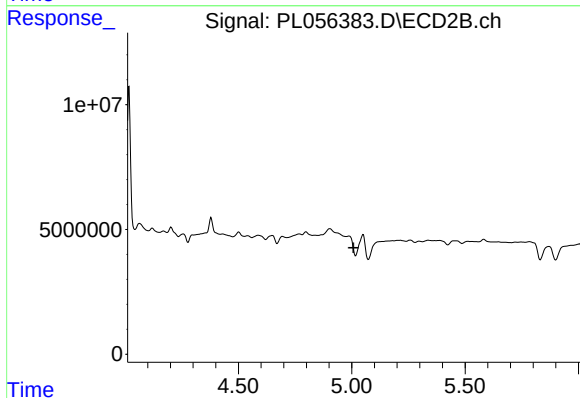


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

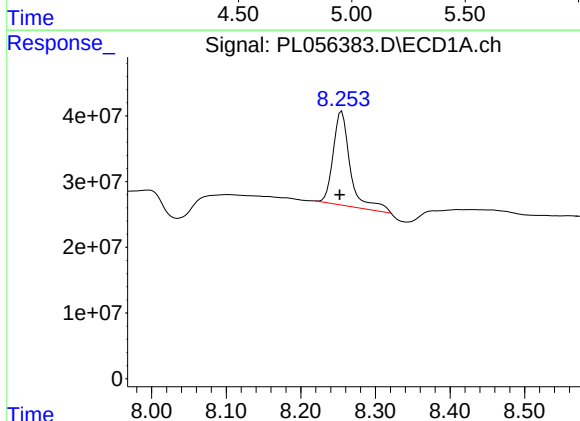

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: 0.003 min
Response: 227670536
Conc: 21.63 ng/ml

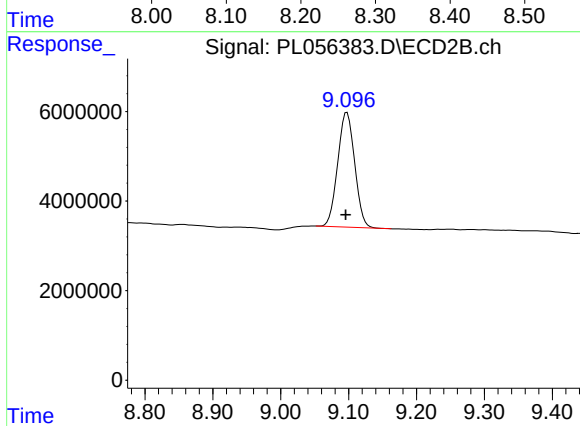

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.002 min
Response: 44577891
Conc: 19.71 ng/ml