

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 18:33
 Operator : AJ\MA
 Sample : L1431-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:33:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.017	178.8E6	60670600	17.075	20.749
28)	SA Decachlor...	8.256	9.098	206.8E6	50576147	19.646	22.360
Target Compounds							
4)	MA Heptachlor	4.523	0.000	7534484	0	0.469	N.D. #
5)	MB Aldrin	4.771	0.000	21504469	0	1.322	N.D. #
7)	B delta-BHC	0.000	5.052f	0	10031505	N.D.	3.128 #
8)	B Heptachlo...	5.216	0.000	8616160	0	0.560	N.D. #
11)	B alpha-Chl...	5.495	0.000	28071084	0	1.825	N.D. #
12)	B 4,4'-DDE	5.663	0.000	15279346	0	1.054	N.D. #
17)	MA 4,4'-DDT	6.422	0.000	463245	0	0.042	N.D. #
23)	Chlordane-1	4.377	0.000	16178828	0	42.740	N.D. #
26)	Chlordane-4	5.495	0.000	28071084	0	25.943	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 18:33
Operator : AJ\MA
Sample : L1431-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:33:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

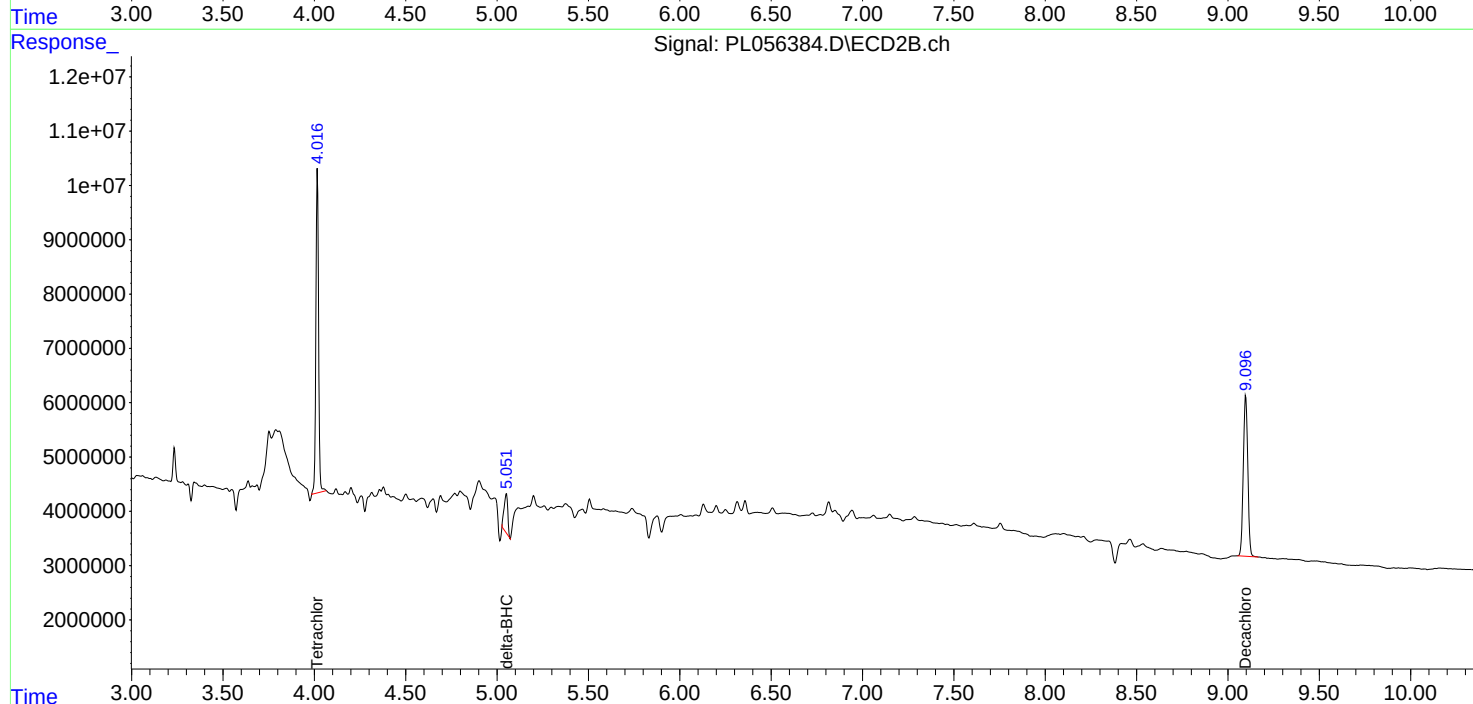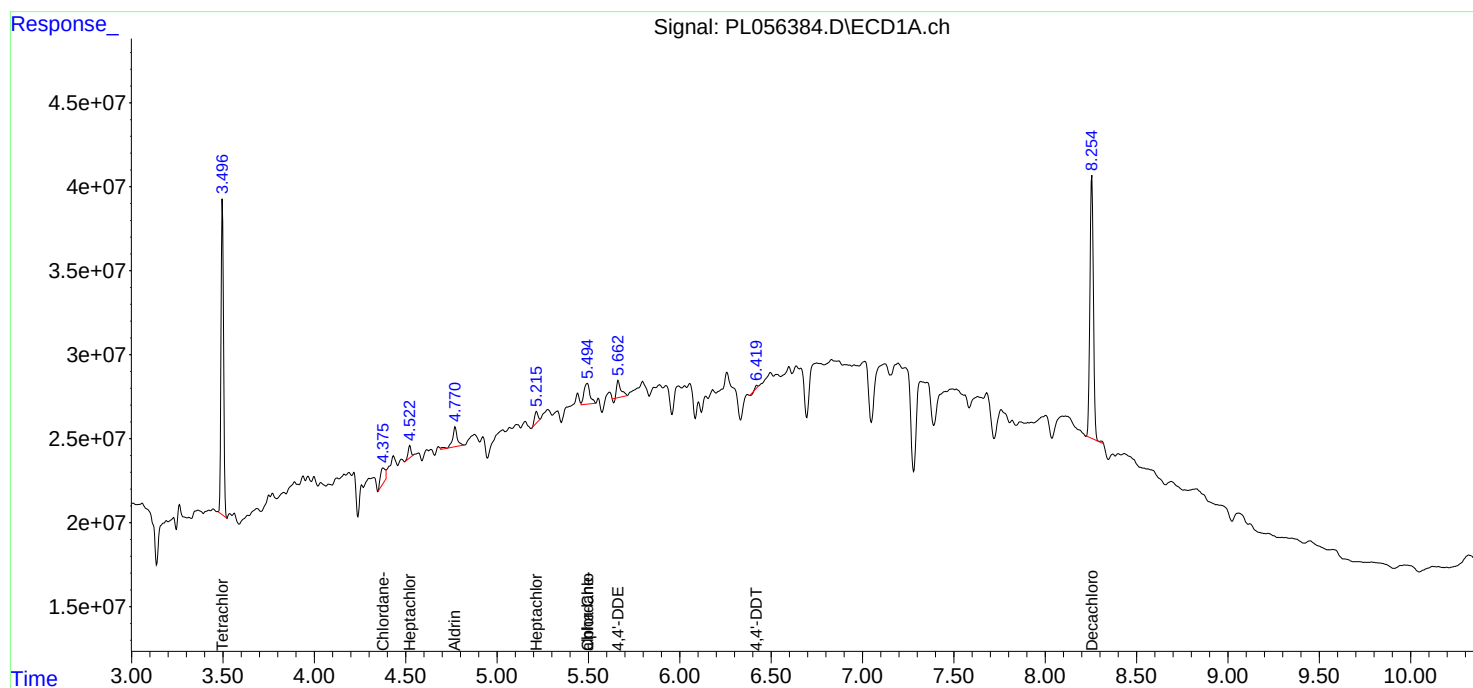


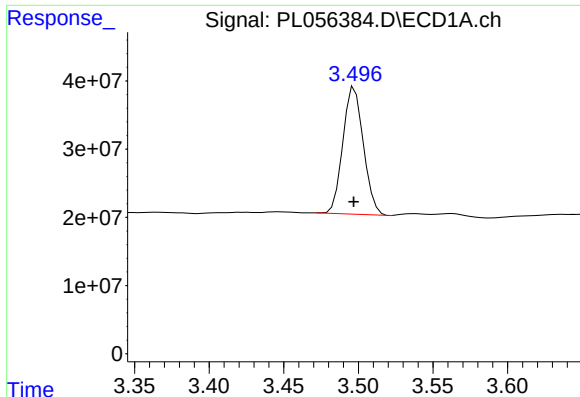

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 178823340
Conc: 17.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

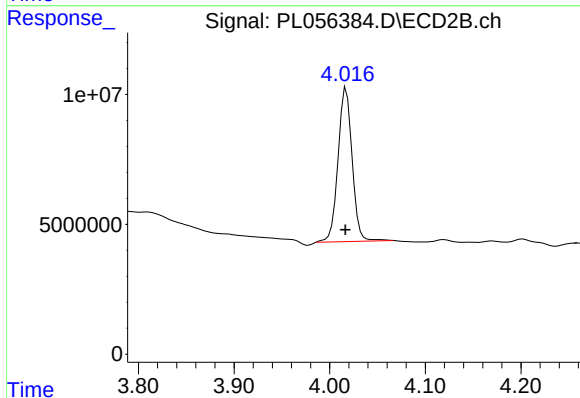


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 60670600
Conc: 20.75 ng/ml

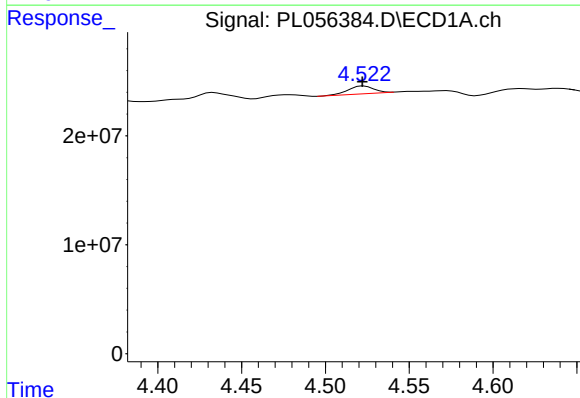


#4 Heptachlor

R.T.: 4.523 min
Delta R.T.: 0.001 min
Response: 7534484
Conc: 0.47 ng/ml

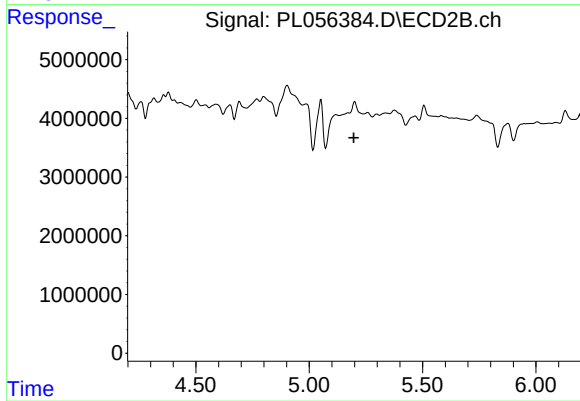

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.197 min
Response: 0
Conc: N.D.

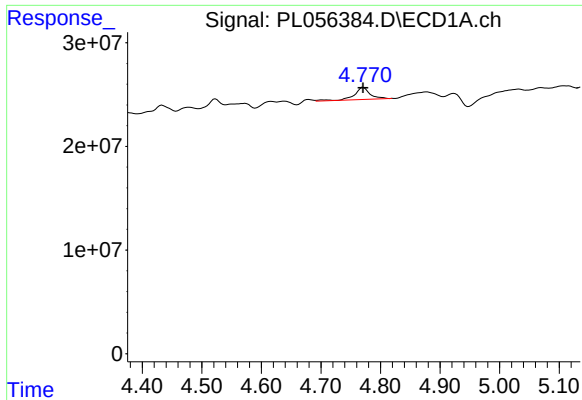

#5 Aldrin


R.T.: 4.771 min
Delta R.T.: 0.000 min
Response: 21504469
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

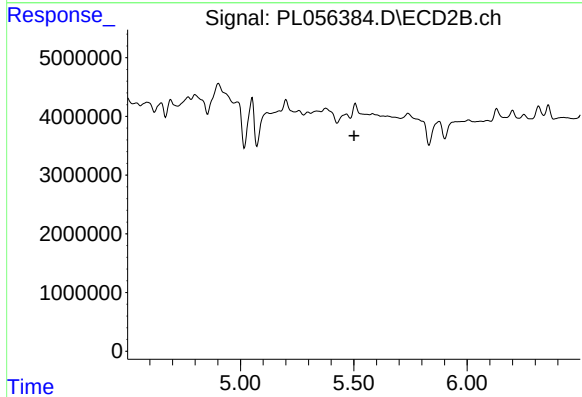


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.501 min
Response: 0
Conc: N.D.

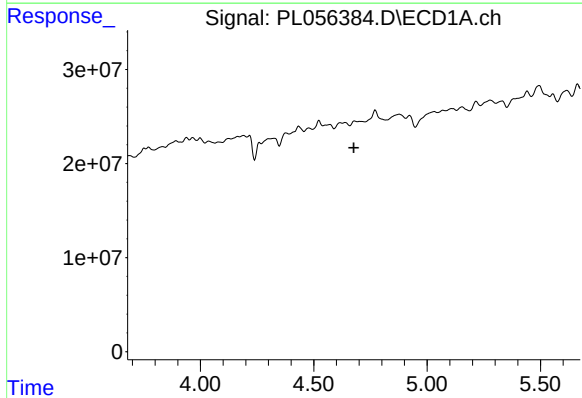


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.676 min
Response: 0
Conc: N.D.

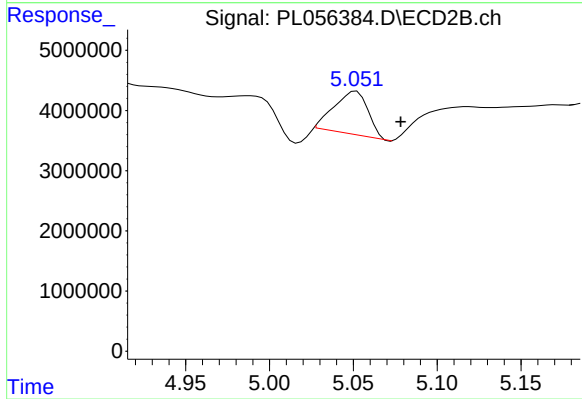

#7 delta-BHC


R.T.: 5.052 min
Delta R.T.: -0.027 min
Response: 10031505
Conc: 3.13 ng/ml

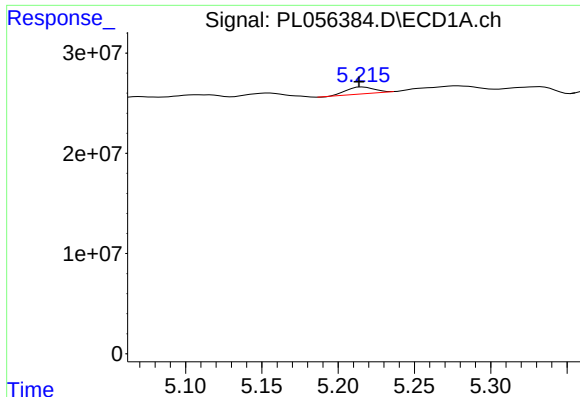

#8 Heptachlor epoxide


R.T.: 5.216 min
Delta R.T.: 0.002 min
Response: 8616160
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

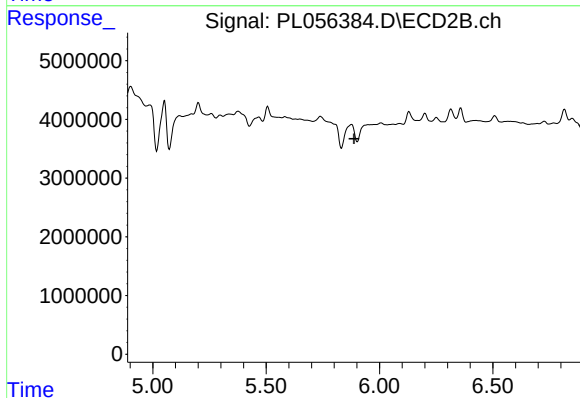


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.889 min
Response: 0
Conc: N.D.

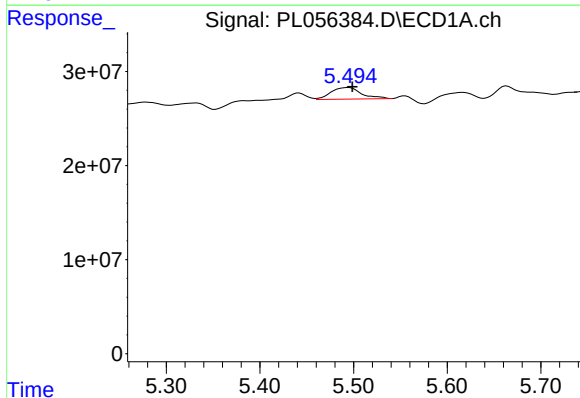


#11 alpha-Chlordane

R.T.: 5.495 min
Delta R.T.: -0.004 min
Response: 28071084
Conc: 1.82 ng/ml

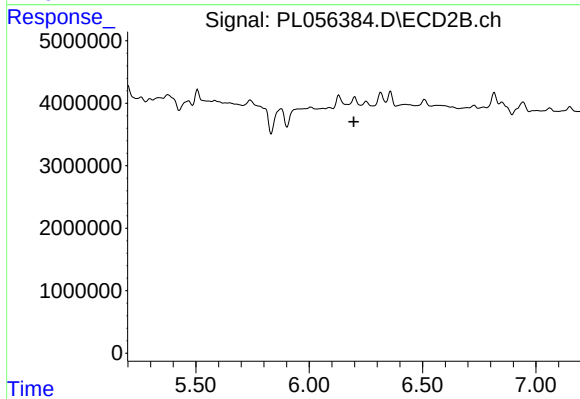

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.196 min
Response: 0
Conc: N.D.

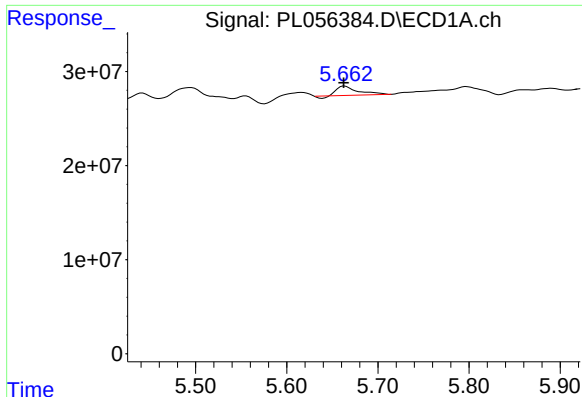

#12 4,4'-DDE


R.T.: 5.663 min
Delta R.T.: 0.000 min
Response: 15279346
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

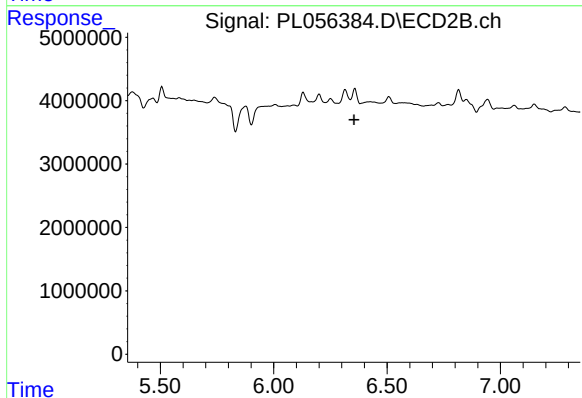


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

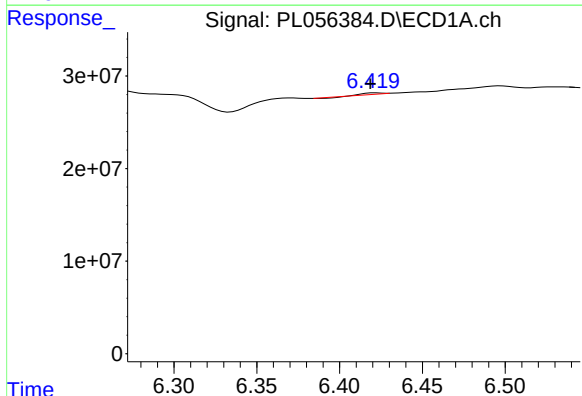


#17 4,4'-DDT

R.T.: 6.422 min
Delta R.T.: 0.003 min
Response: 463245
Conc: 0.04 ng/ml

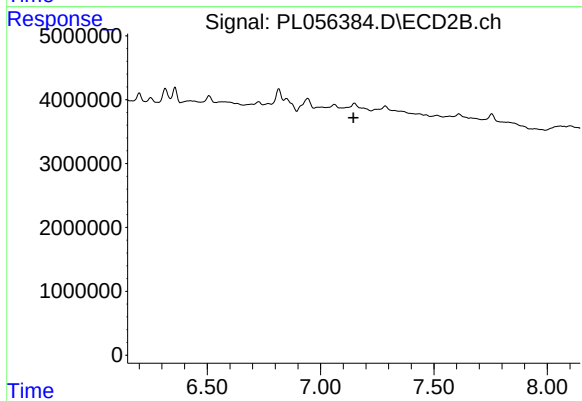

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

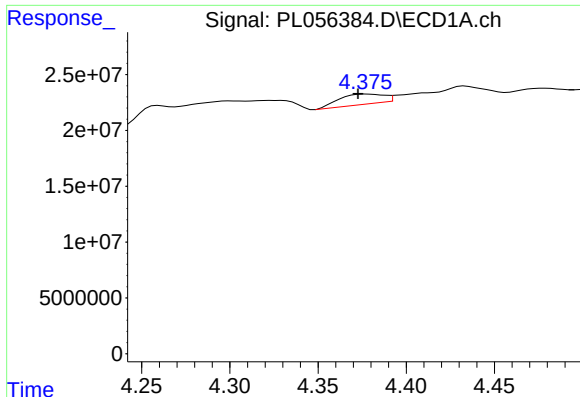

#23 Chlordane-1


R.T.: 4.377 min
Delta R.T.: 0.004 min
Response: 16178828
Conc: 42.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

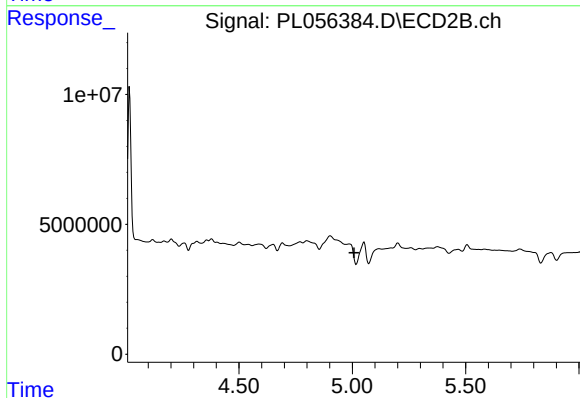


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

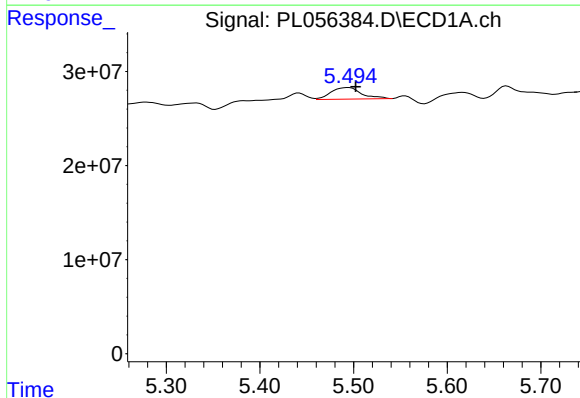


#26 Chlordane-4

R.T.: 5.495 min
Delta R.T.: -0.008 min
Response: 28071084
Conc: 25.94 ng/ml

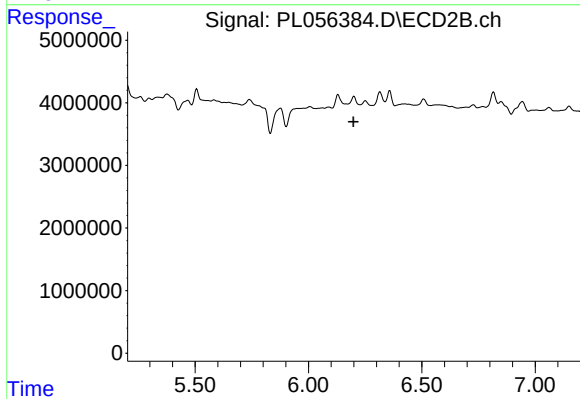

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

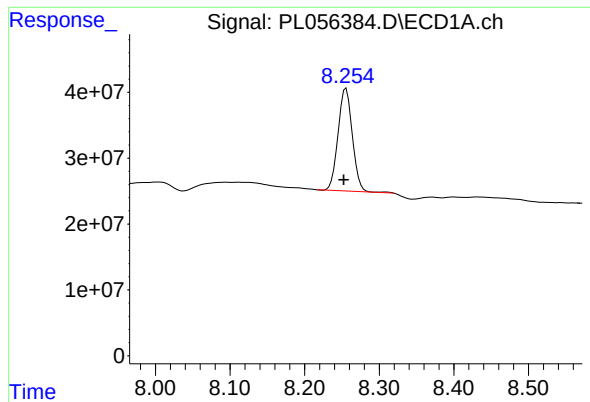

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: 0.003 min
Response: 206835210
Conc: 19.65 ng/ml

Instrument :
ECD_L
ClientSampleId :

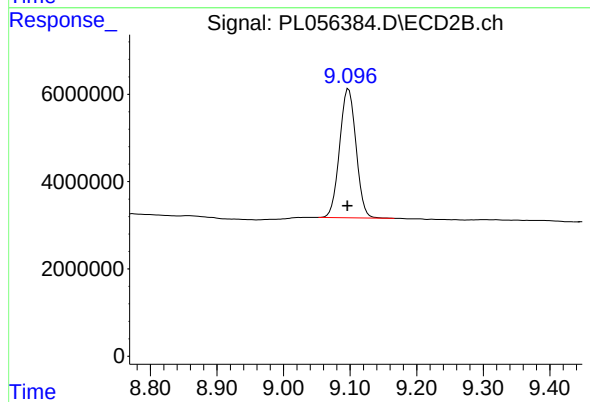

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.002 min
Response: 50576147
Conc: 22.36 ng/ml