

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 20:11
 Operator : AJ\MA
 Sample : L1437-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 07 22:34:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.018	170.9E6	61580170	16.318	21.060 #
28)	SA Decachlor...	8.255	9.097	97995241	20923682	9.308	9.250
Target Compounds							
5)	MB Aldrin	4.767	0.000	22490863	0	1.383	N.D. #
7)	B delta-BHC	0.000	5.055f	0	10612499	N.D.	3.309 #
8)	B Heptachlo...	5.212	5.888	33933961	38498360	2.206	12.369 #
9)	A Endosulfan I	0.000	6.254	0	60635382	N.D.	20.261 #
11)	B alpha-Chl...	5.493	0.000	449.7E6	0	29.235	N.D. #
15)	B Endosulfa...	6.320	0.000	44475869	0	3.401	N.D. #
26)	Chlordane-4	5.493	0.000	449.7E6	0	415.626	N.D. #
27)	Chlordane-5	6.320f	0.000	44475869	0	107.214	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 20:11
Operator : AJ\MA
Sample : L1437-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 07 22:34:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

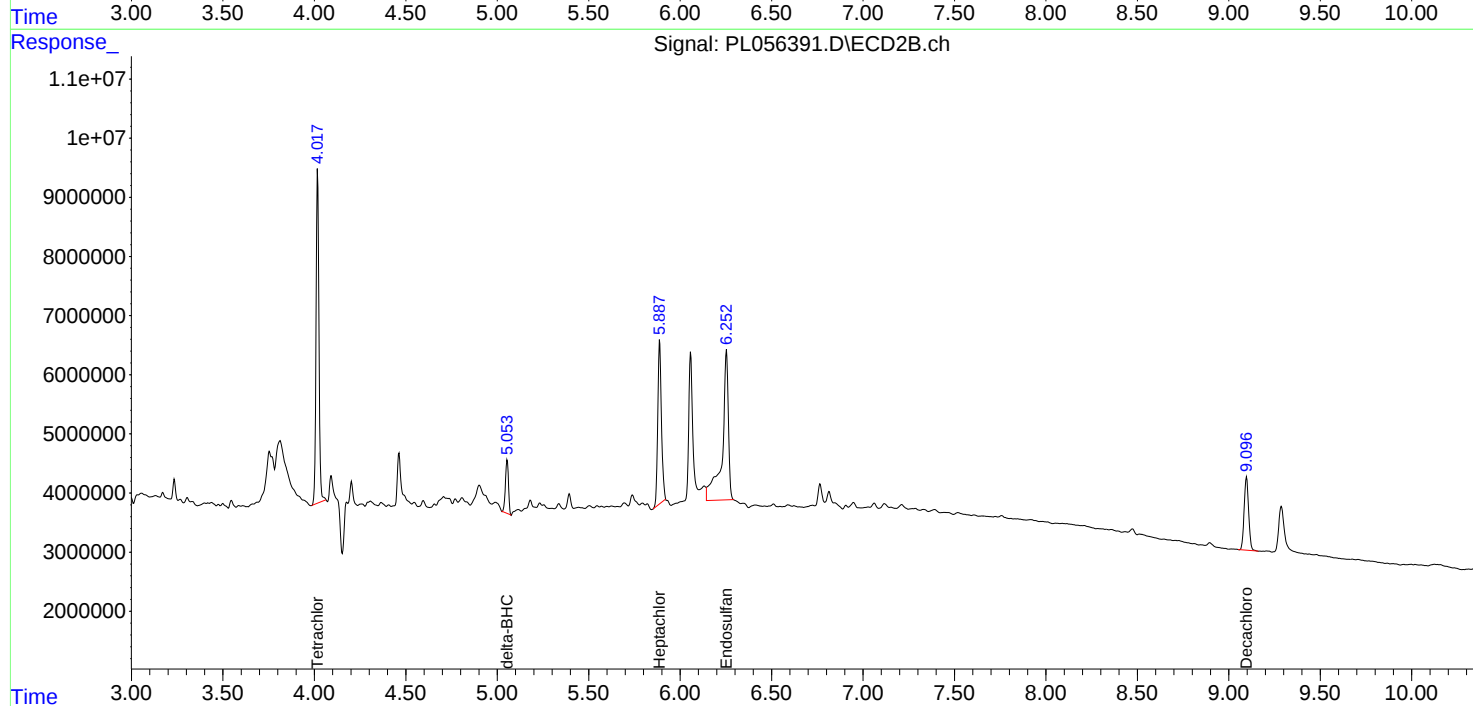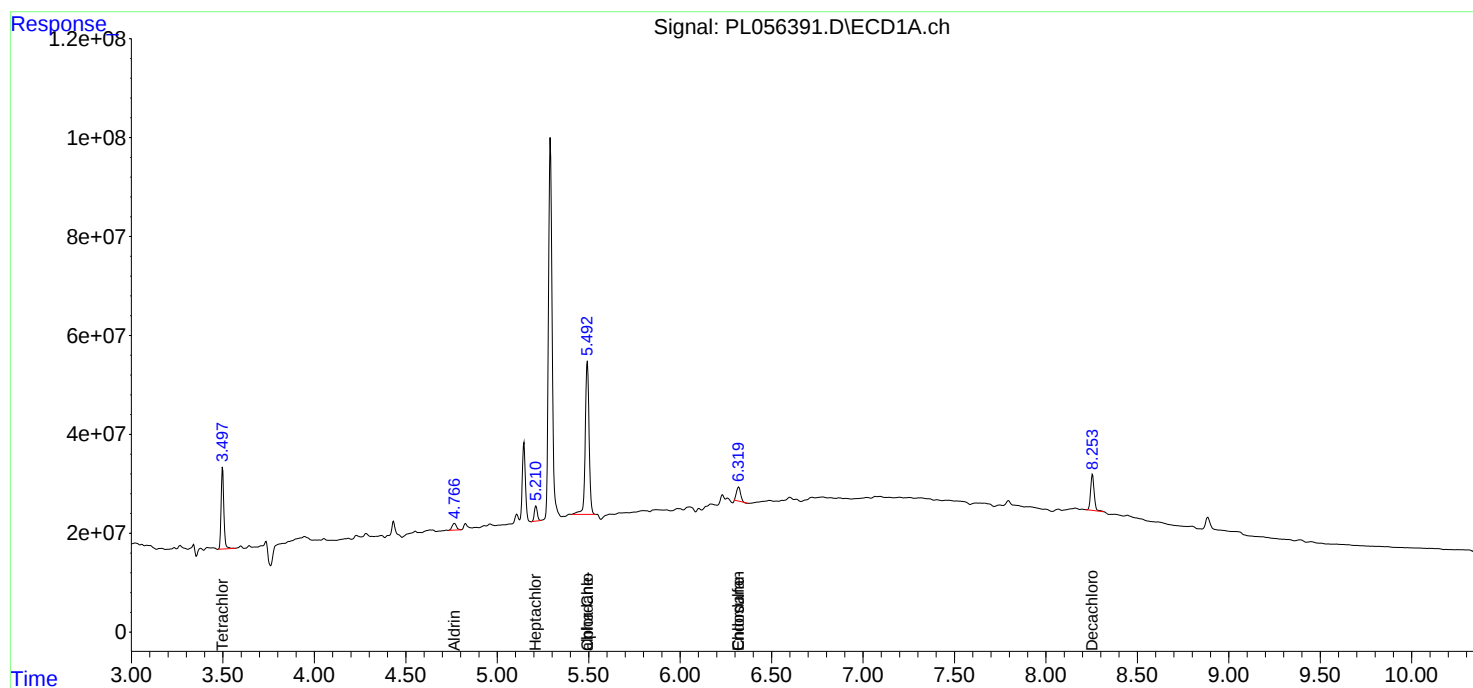


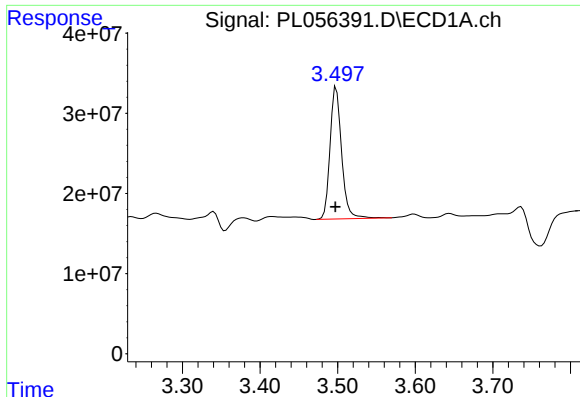

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.001 min
Response: 170896302
Conc: 16.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

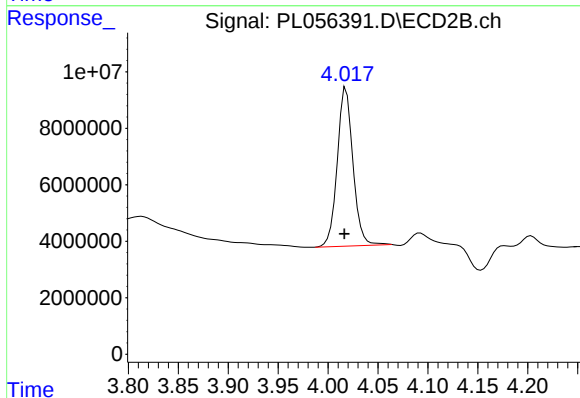


#1 Tetrachloro-m-xylene

R.T.: 4.018 min
Delta R.T.: 0.002 min
Response: 61580170
Conc: 21.06 ng/ml

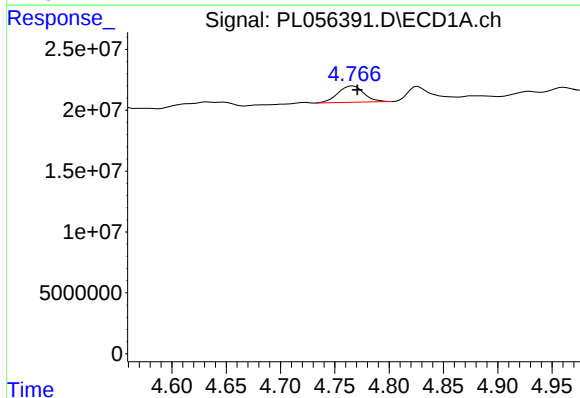


#5 Aldrin

R.T.: 4.767 min
Delta R.T.: -0.004 min
Response: 22490863
Conc: 1.38 ng/ml

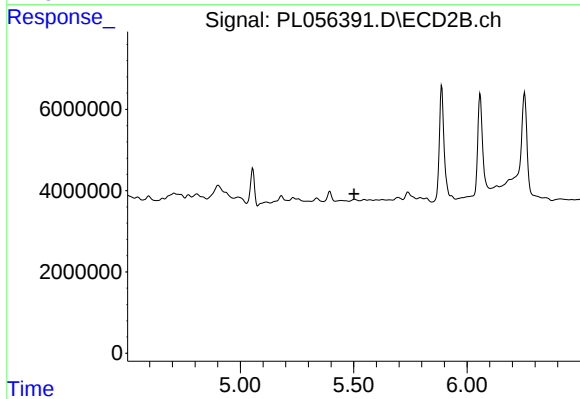

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

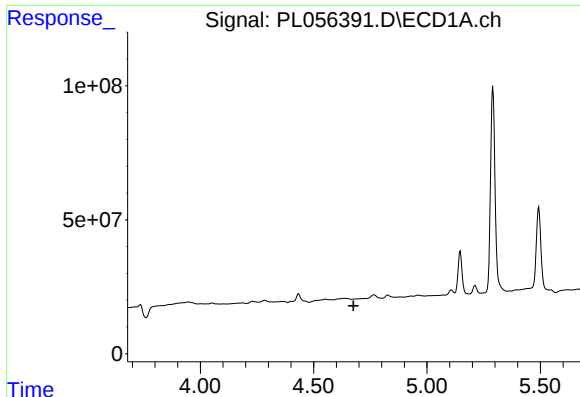

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

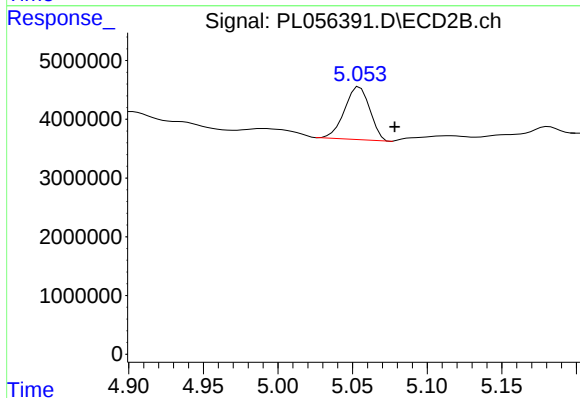


#7 delta-BHC

R.T.: 5.055 min
Delta R.T.: -0.024 min
Response: 10612499
Conc: 3.31 ng/ml

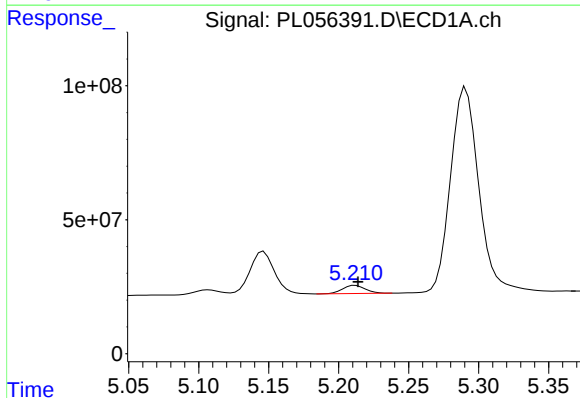


#8 Heptachlor epoxide

R.T.: 5.212 min
Delta R.T.: -0.002 min
Response: 33933961
Conc: 2.21 ng/ml

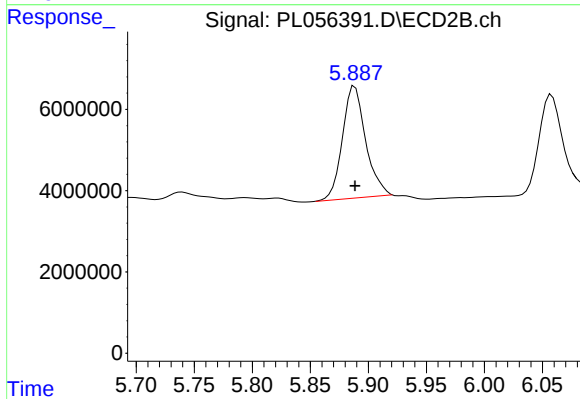

#8 Heptachlor epoxide


R.T.: 5.888 min
Delta R.T.: 0.000 min
Response: 38498360
Conc: 12.37 ng/ml

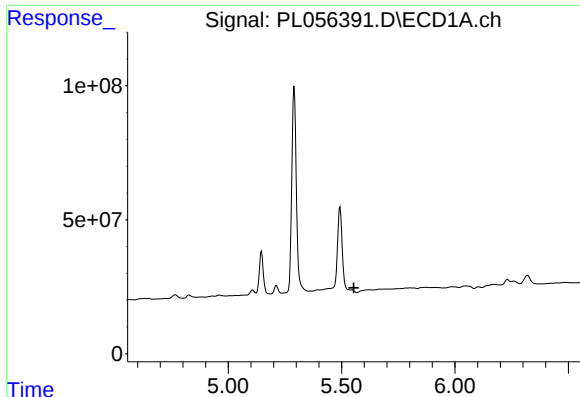

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.553 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

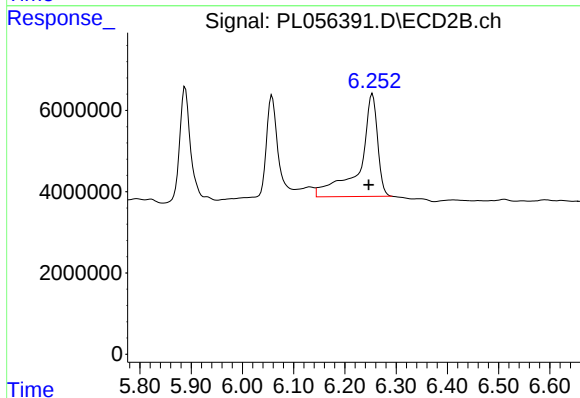


#9 Endosulfan I

R.T.: 6.254 min
Delta R.T.: 0.007 min
Response: 60635382
Conc: 20.26 ng/ml

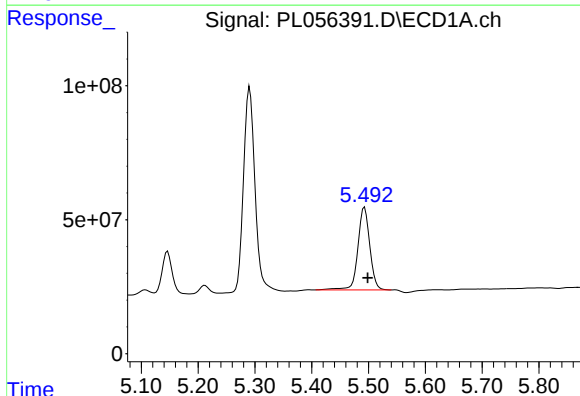


#11 alpha-Chlordane

R.T.: 5.493 min
Delta R.T.: -0.006 min
Response: 449722813
Conc: 29.24 ng/ml

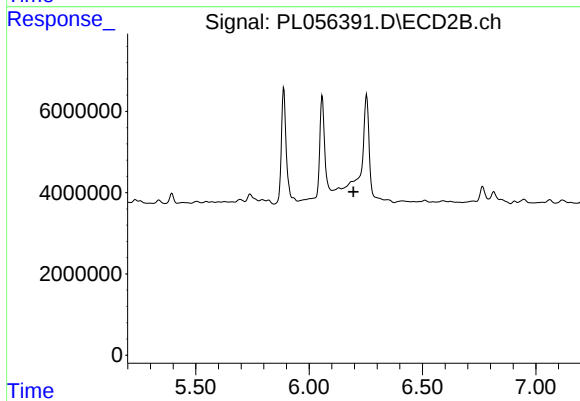

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

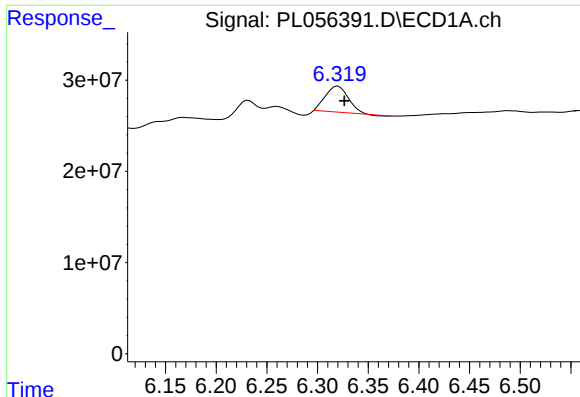

#15 Endosulfan II


R.T.: 6.320 min
Delta R.T.: -0.006 min
Response: 44475869
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

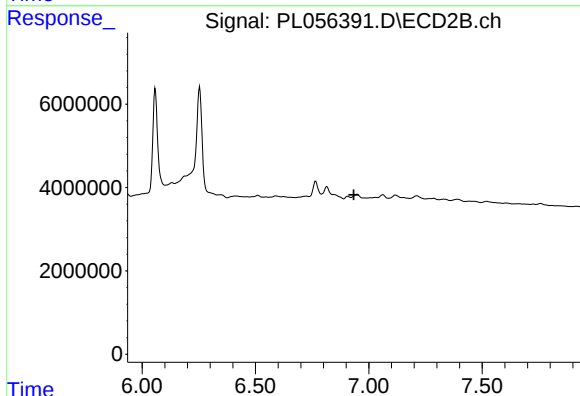


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.934 min
Response: 0
Conc: N.D.

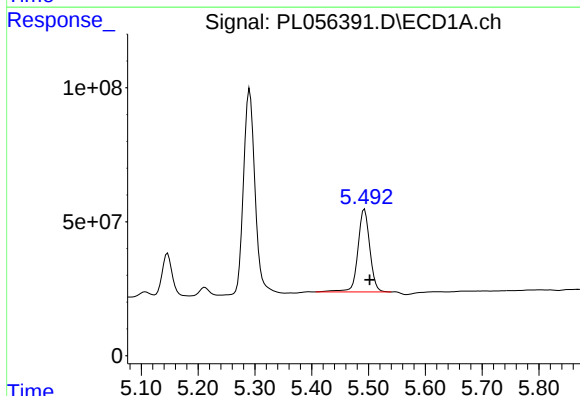


#26 Chlordane-4

R.T.: 5.493 min
Delta R.T.: -0.009 min
Response: 449722813
Conc: 415.63 ng/ml

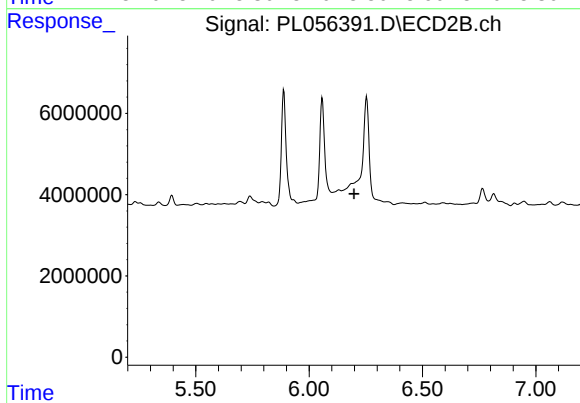

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

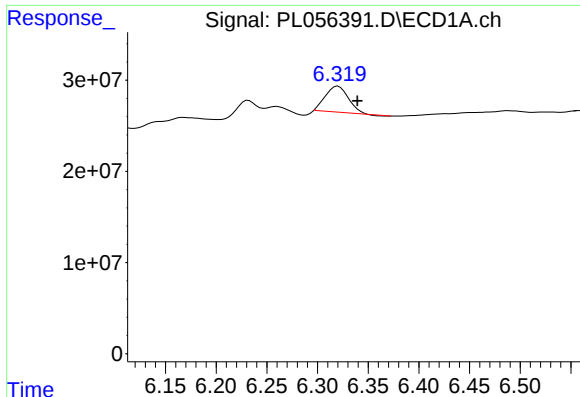

#27 Chlordane-5


R.T.: 6.320 min
Delta R.T.: -0.019 min
Response: 44475869
Conc: 107.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

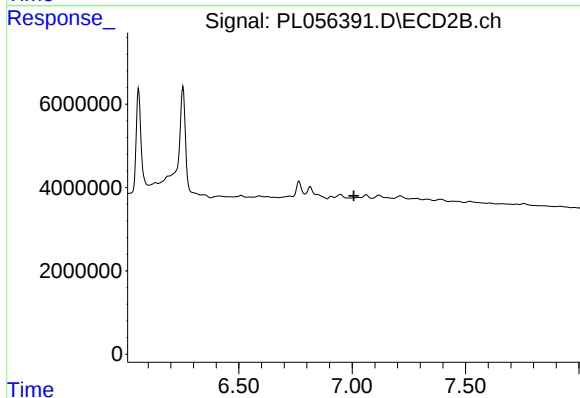


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

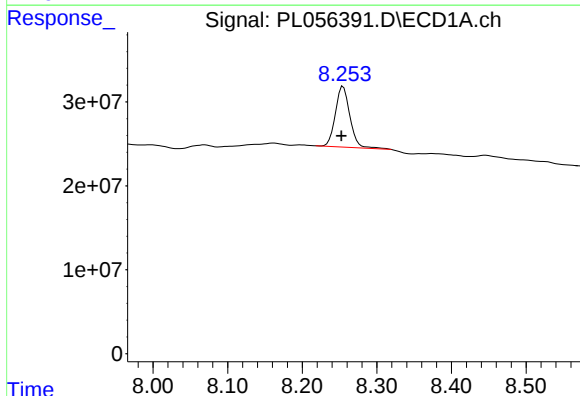

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: 0.003 min
Response: 97995241
Conc: 9.31 ng/ml

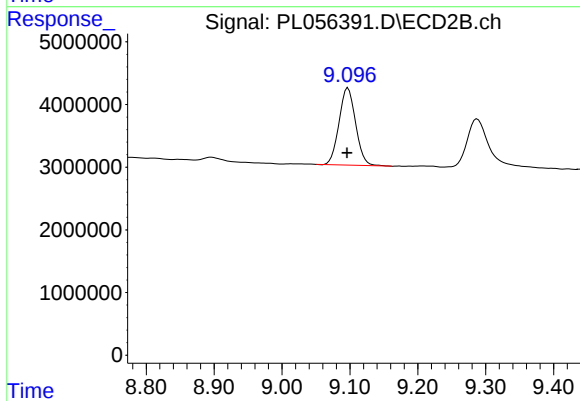

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.001 min
Response: 20923682
Conc: 9.25 ng/ml