

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2020 23:57
 Operator : AJ\MA
 Sample : L1439-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 00:53:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.017	118.7E6	39836429	11.333	13.624
28)	SA Decachlor...	8.253	9.095	135.9E6	32154802	12.911	14.216
Target Compounds							
5)	MB Aldrin	4.772	0.000	10113235	0	0.622	N.D. #
10)	B gamma-Chl...	5.462f	0.000	20325747	0	1.296	N.D. #
11)	B alpha-Chl...	5.499	6.201	13328316	8782364	0.866	2.771 #
12)	B 4,4'-DDE	5.662	6.357	24616874	9850987	1.698	3.289 #
13)	MA Dieldrin	5.790	0.000	37452233	0	2.435	N.D. #
17)	MA 4,4'-DDT	6.418	0.000	40185974	0	3.677	N.D. #
25)	Chlordane-3	5.462f	0.000	20325747	0	16.099	N.D. #
26)	Chlordane-4	5.499	6.201	13328316	8782364	12.318	19.989 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2020 23:57
Operator : AJ\MA
Sample : L1439-02
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 00:53:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

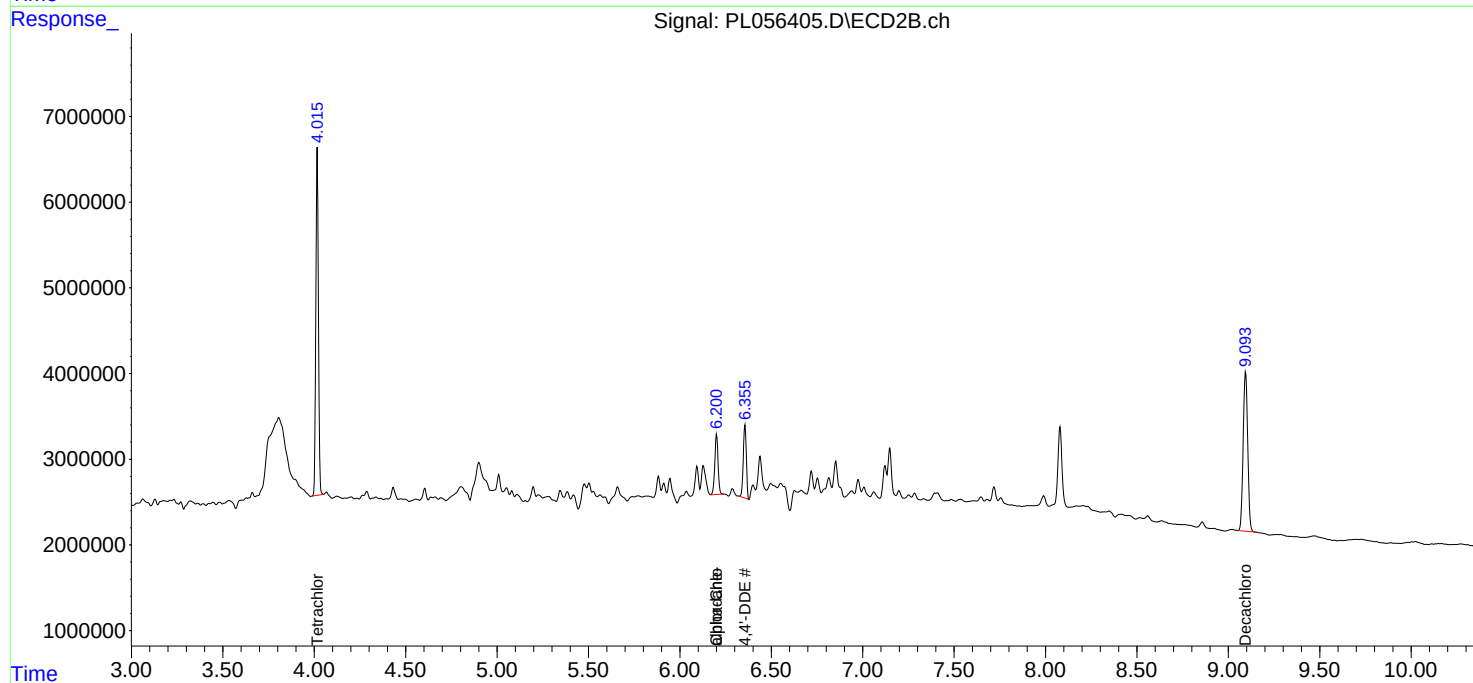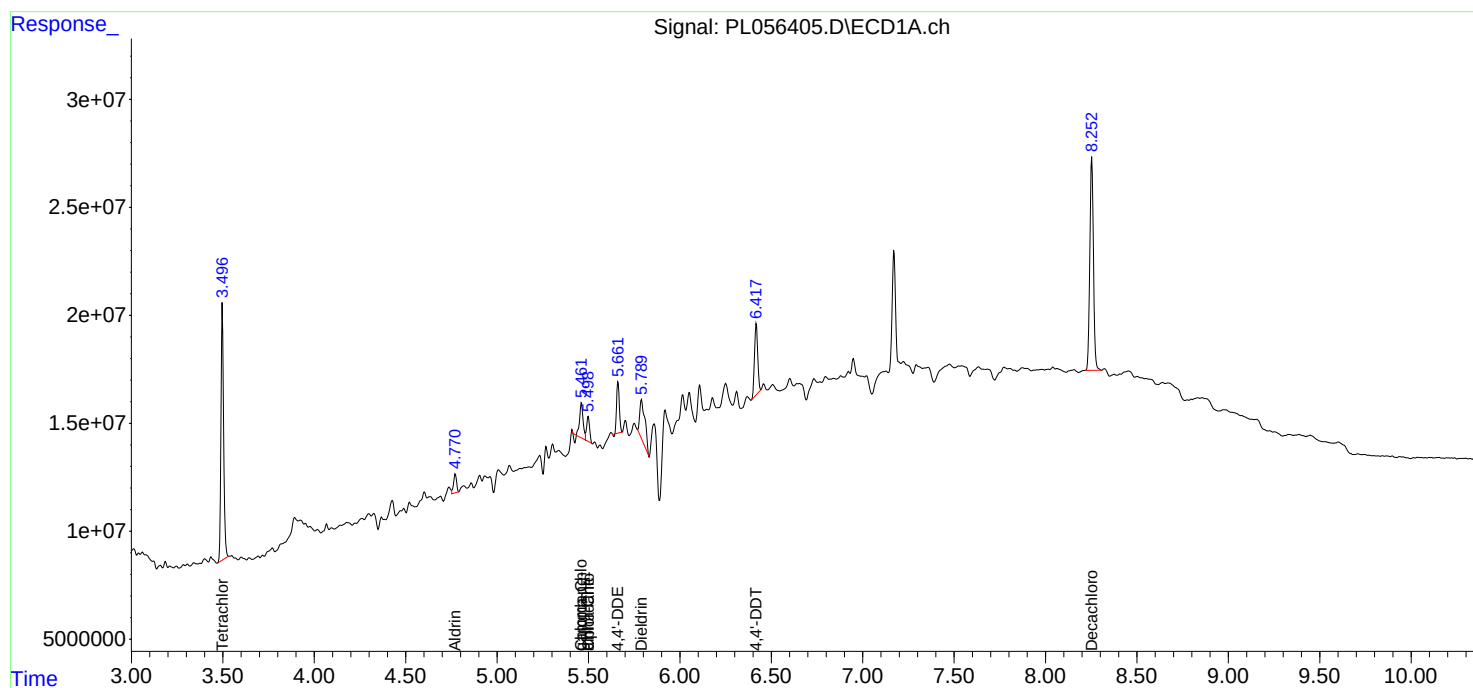


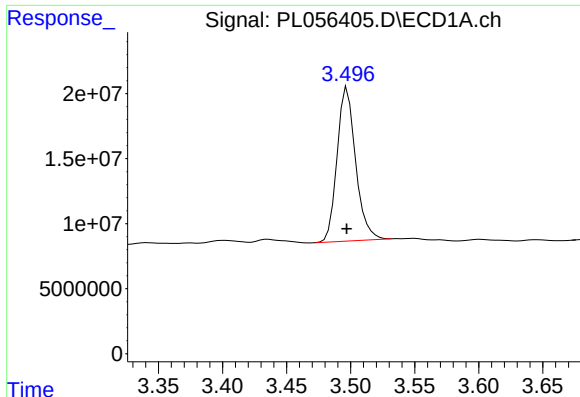

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 118687710
Conc: 11.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

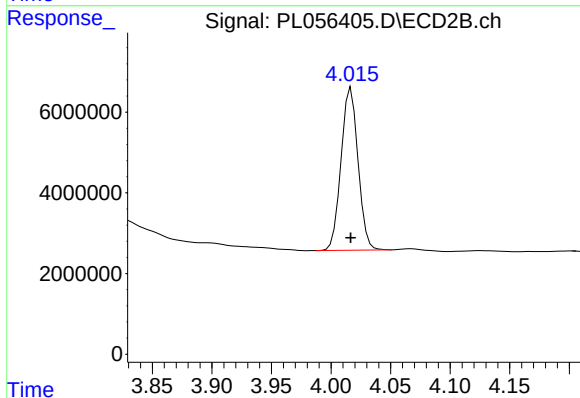


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 39836429
Conc: 13.62 ng/ml

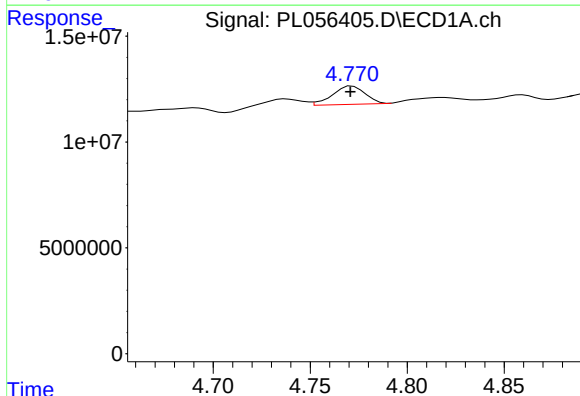


#5 Aldrin

R.T.: 4.772 min
Delta R.T.: 0.000 min
Response: 10113235
Conc: 0.62 ng/ml

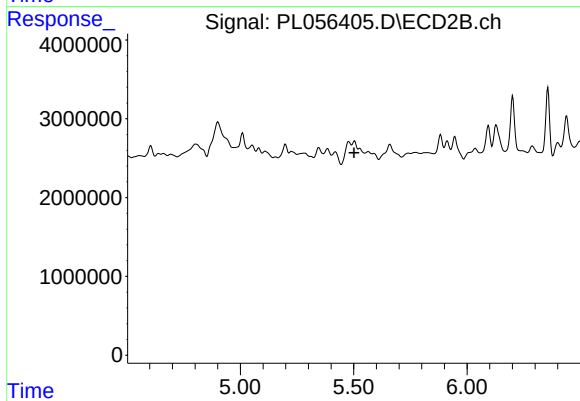

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

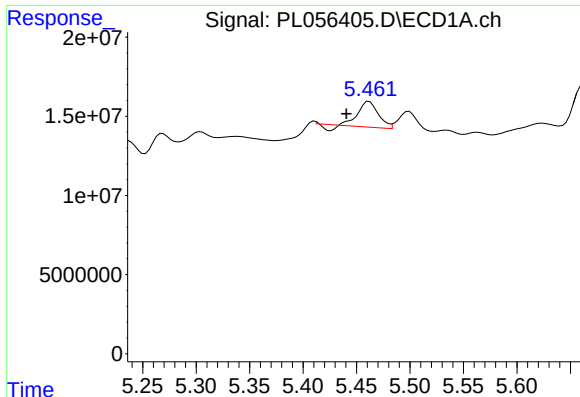

#10 gamma-Chlordane


R.T.: 5.462 min
Delta R.T.: 0.021 min
Response: 20325747
Conc: 1.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

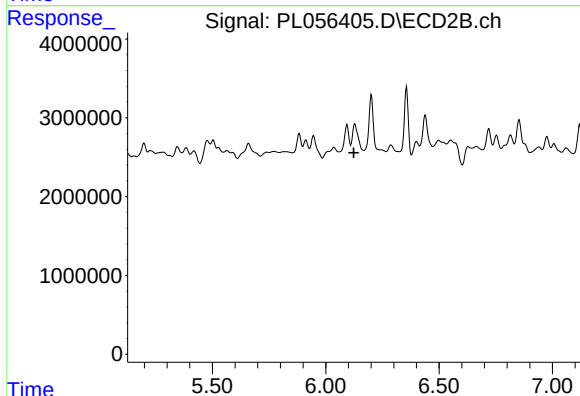


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.124 min
Response: 0
Conc: N.D.

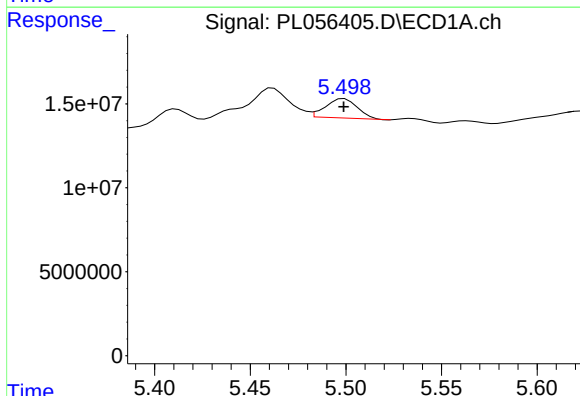


#11 alpha-Chlordane

R.T.: 5.499 min
Delta R.T.: 0.000 min
Response: 13328316
Conc: 0.87 ng/ml

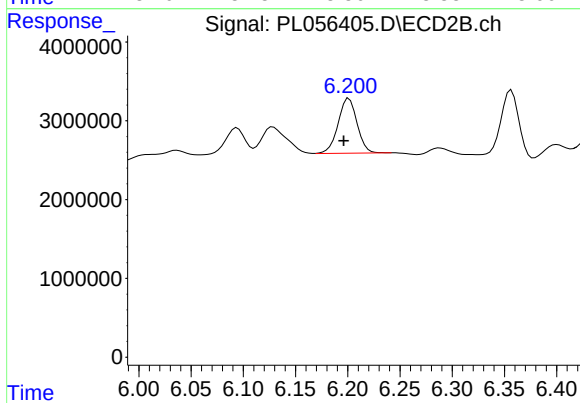

#11 alpha-Chlordane


R.T.: 6.201 min
Delta R.T.: 0.005 min
Response: 8782364
Conc: 2.77 ng/ml

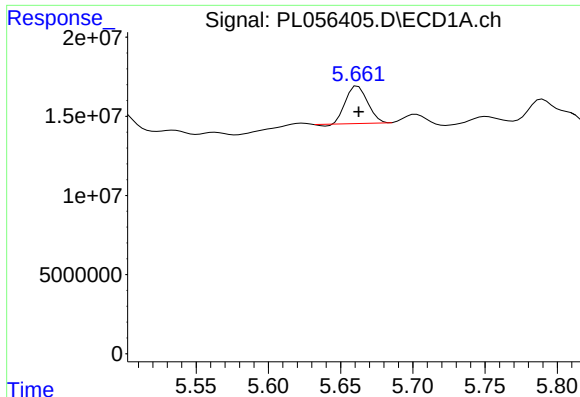

#12 4,4'-DDE


R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 24616874
Conc: 1.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

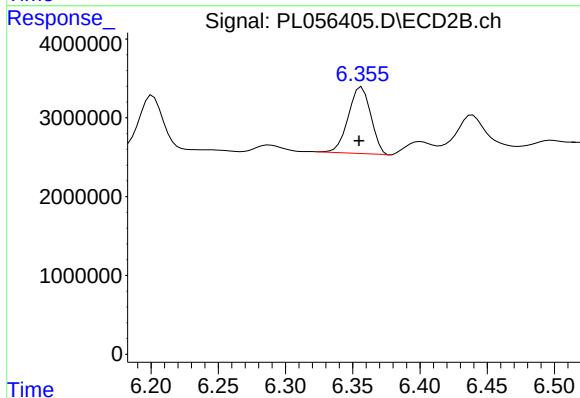


#12 4,4'-DDE

R.T.: 6.357 min
Delta R.T.: 0.002 min
Response: 9850987
Conc: 3.29 ng/ml

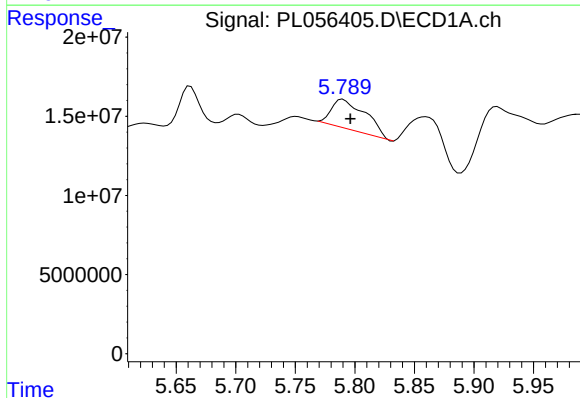


#13 Dieldrin

R.T.: 5.790 min
Delta R.T.: -0.006 min
Response: 37452233
Conc: 2.44 ng/ml

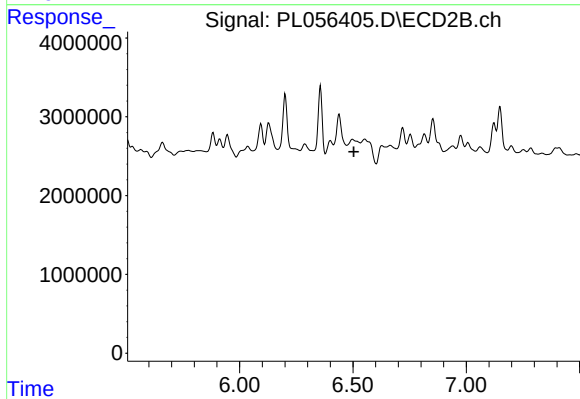

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.504 min
Response: 0
Conc: N.D.

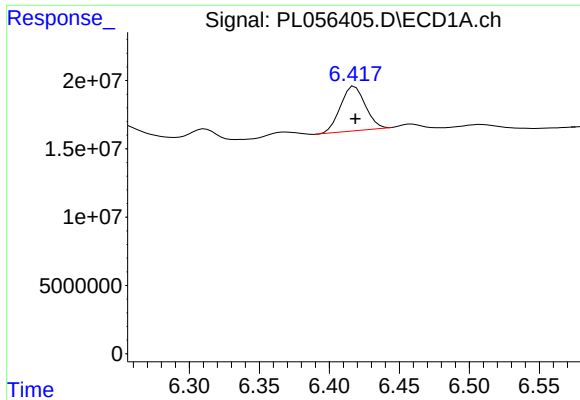

#17 4,4'-DDT


R.T.: 6.418 min
Delta R.T.: 0.000 min
Response: 40185974
Conc: 3.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

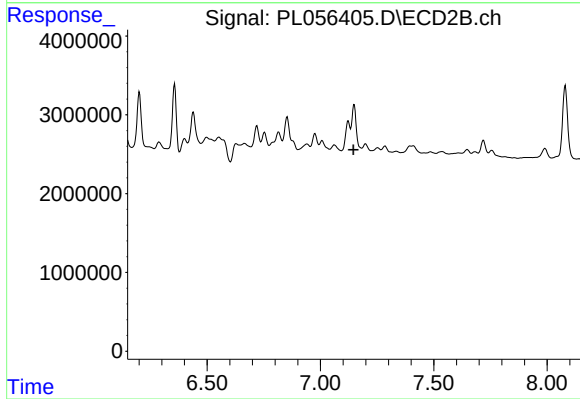


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

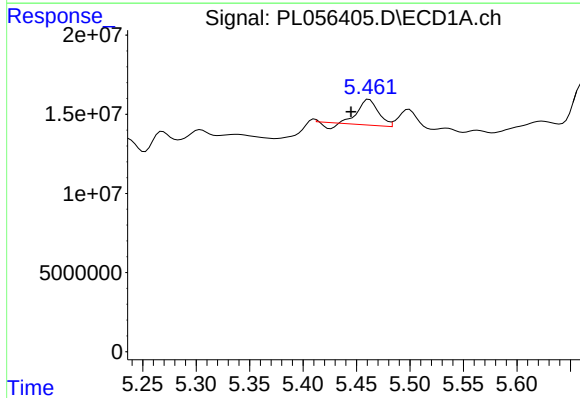


#25 Chlordane-3

R.T.: 5.462 min
Delta R.T.: 0.017 min
Response: 20325747
Conc: 16.10 ng/ml

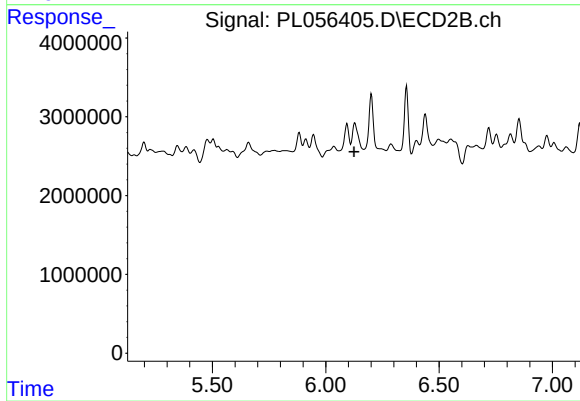

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

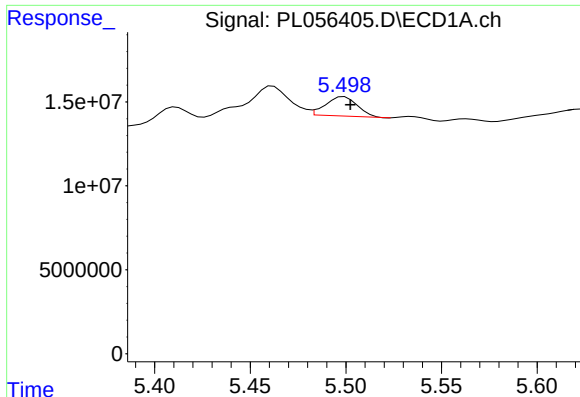

#26 Chlordane-4


R.T.: 5.499 min
Delta R.T.: -0.003 min
Response: 13328316
Conc: 12.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

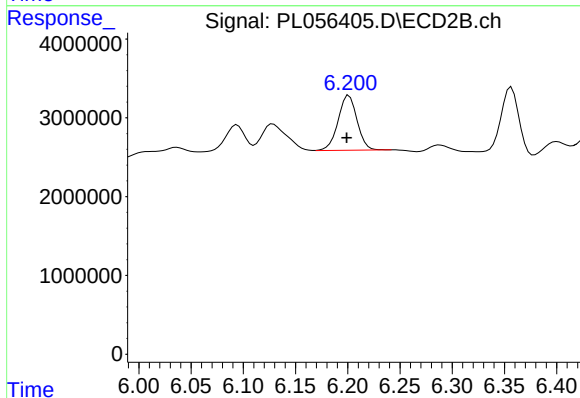


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: 0.002 min
Response: 8782364
Conc: 19.99 ng/ml

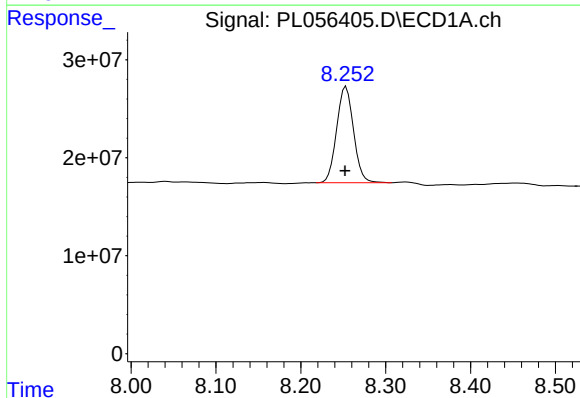

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.001 min
Response: 135932860
Conc: 12.91 ng/ml

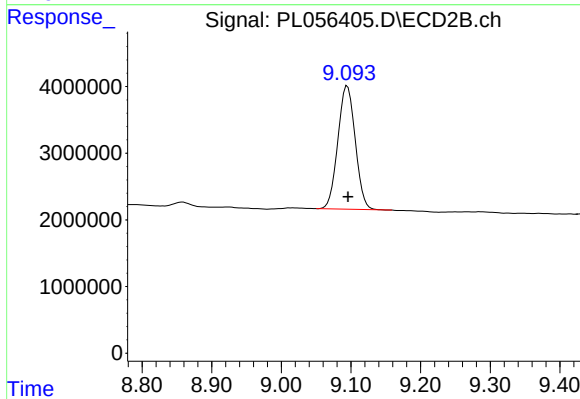

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: -0.001 min
Response: 32154802
Conc: 14.22 ng/ml