

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2020 00:25
 Operator : AJ\MA
 Sample : L1439-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 00:53:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.017	117.6E6	35943124	11.225	12.292
28)	SA Decachlor...	8.253	9.096	102.4E6	25521713	9.729	11.283
Target Compounds							
10)	B gamma-Chl...	5.439	6.097f	7638426	9131434	0.487	2.871 #
11)	B alpha-Chl...	0.000	6.201	0	10671453	N.D.	3.367 #
12)	B 4,4'-DDE	5.662	6.358	32974897	11060136	2.275	3.692 #
13)	MA Dieldrin	5.789	0.000	30652218	0	1.993	N.D. #
16)	A 4,4'-DDD	0.000	6.854	0	4189153	N.D.	1.775 #
17)	MA 4,4'-DDT	6.417	0.000	50499144	0	4.621	N.D. #
20)	A Methoxychlor	6.949	0.000	11116213	0	2.093	N.D. #
23)	Chlordane-1	4.370	0.000	10762455	0	28.431	N.D. #
25)	Chlordane-3	5.439	6.097f	7638426	9131434	6.050	24.296 #
26)	Chlordane-4	0.000	6.201	0	10671453	N.D.	24.289 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2020 00:25
Operator : AJ\MA
Sample : L1439-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 00:53:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

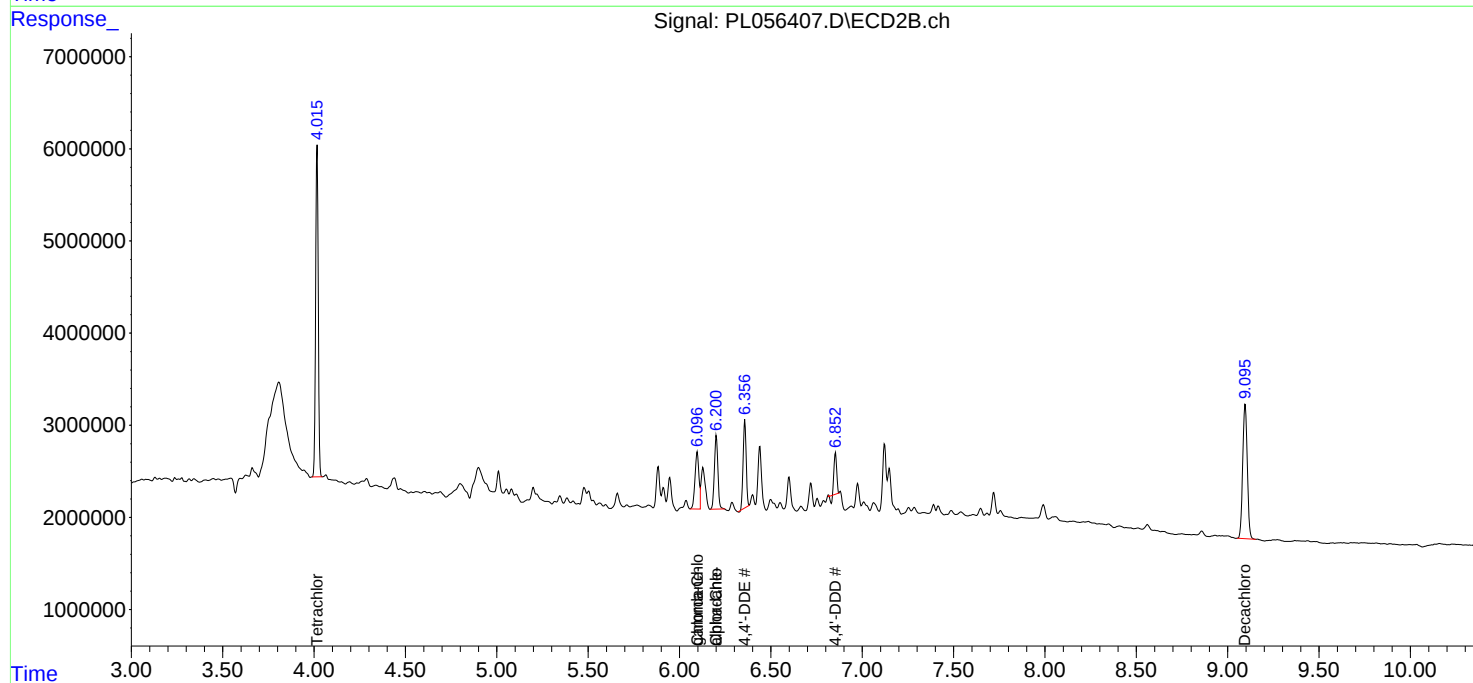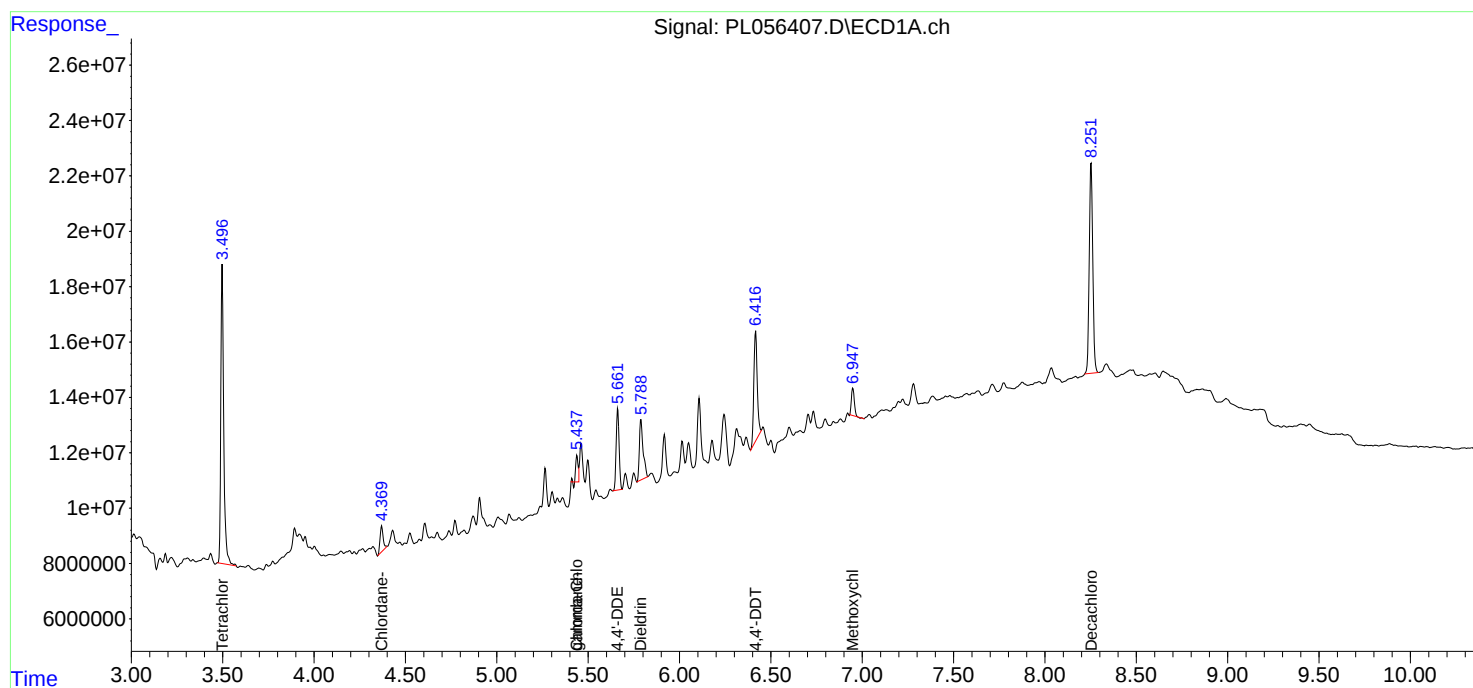


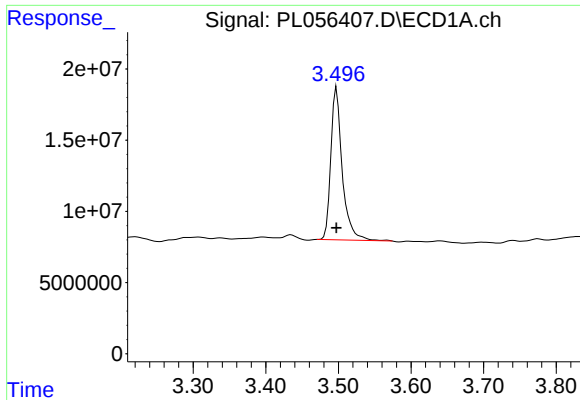

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 117558081
Conc: 11.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

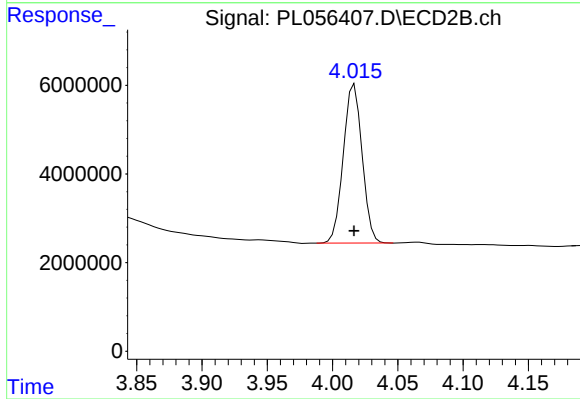


#1 Tetrachloro-m-xylene

R.T.: 4.017 min
Delta R.T.: 0.000 min
Response: 35943124
Conc: 12.29 ng/ml

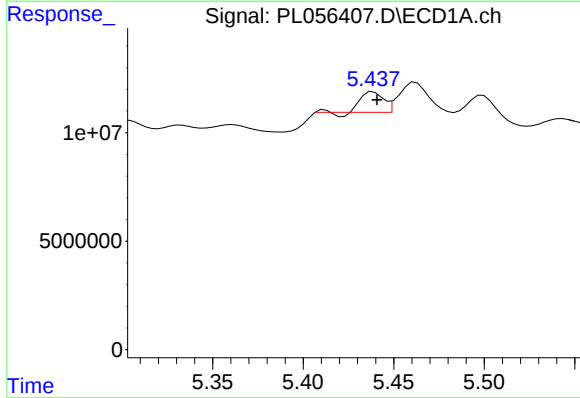


#10 gamma-Chlordane

R.T.: 5.439 min
Delta R.T.: -0.002 min
Response: 7638426
Conc: 0.49 ng/ml

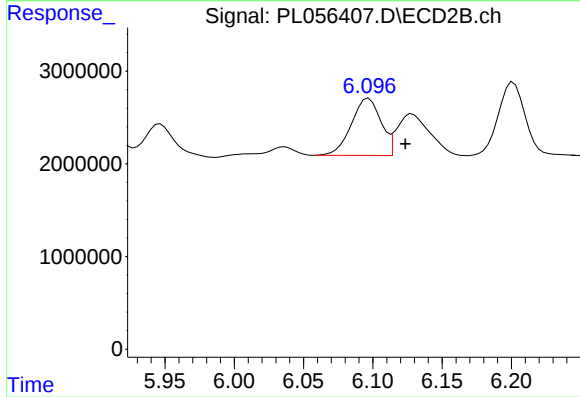

#10 gamma-Chlordane


R.T.: 6.097 min
Delta R.T.: -0.027 min
Response: 9131434
Conc: 2.87 ng/ml

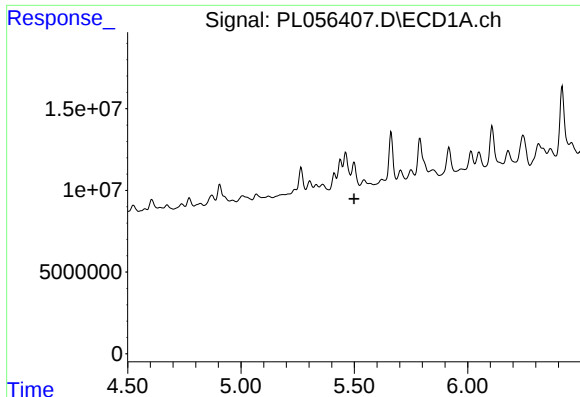

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

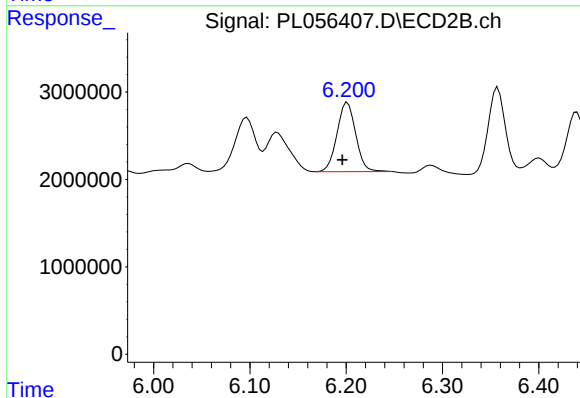


#11 alpha-Chlordane

R.T.: 6.201 min
Delta R.T.: 0.005 min
Response: 10671453
Conc: 3.37 ng/ml

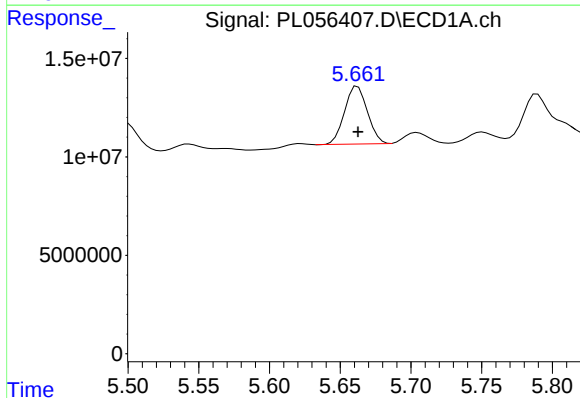


#12 4,4'-DDE

R.T.: 5.662 min
Delta R.T.: 0.000 min
Response: 32974897
Conc: 2.28 ng/ml

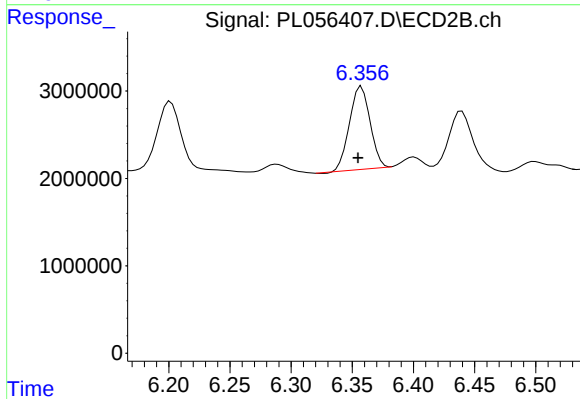

#12 4,4'-DDE


R.T.: 6.358 min
Delta R.T.: 0.003 min
Response: 11060136
Conc: 3.69 ng/ml

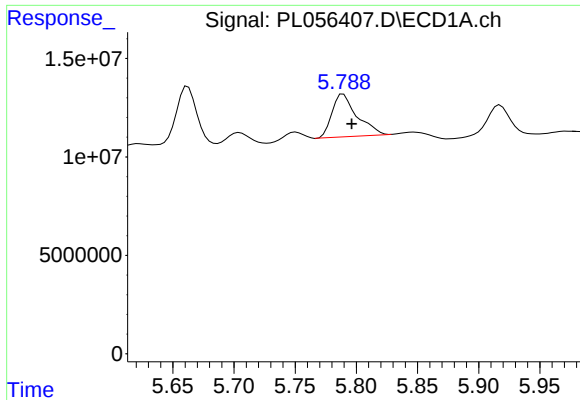

#13 Dieldrin


R.T.: 5.789 min
Delta R.T.: -0.007 min
Response: 30652218
Conc: 1.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

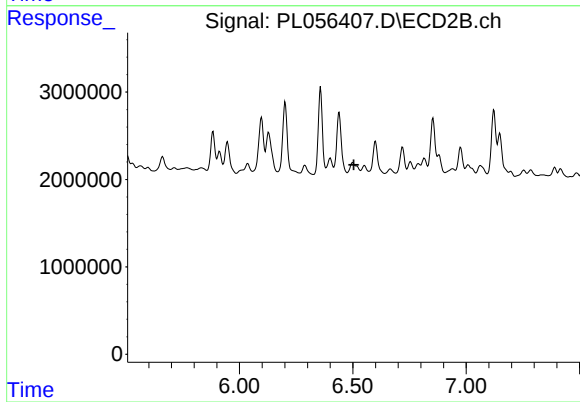


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.504 min
Response: 0
Conc: N.D.

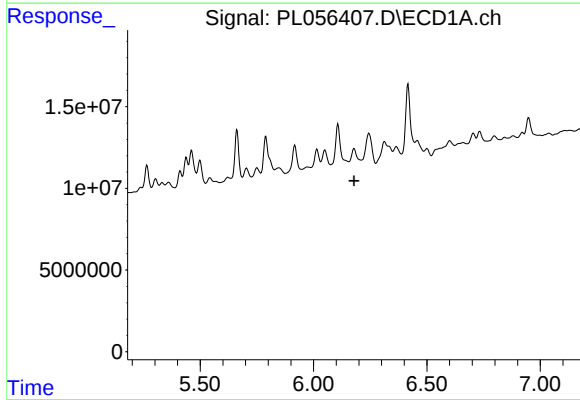


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.179 min
Response: 0
Conc: N.D.

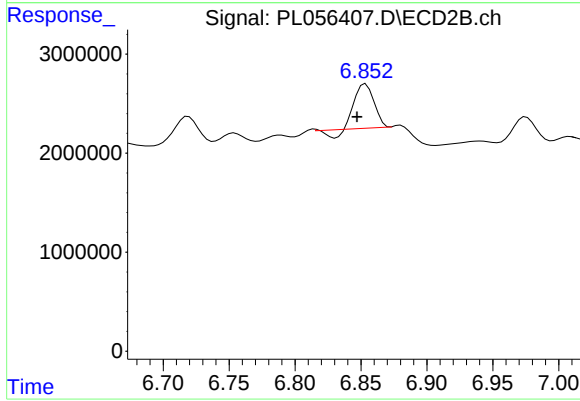

#16 4,4'-DDD


R.T.: 6.854 min
Delta R.T.: 0.006 min
Response: 4189153
Conc: 1.78 ng/ml

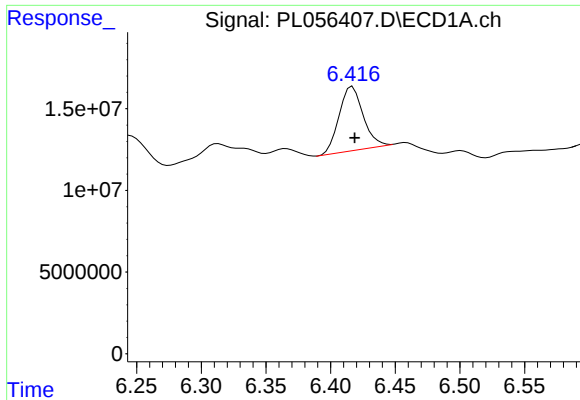

#17 4,4'-DDT


R.T.: 6.417 min
Delta R.T.: -0.002 min
Response: 50499144
Conc: 4.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

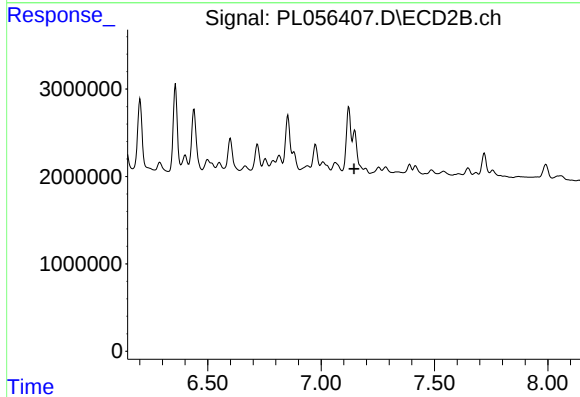


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

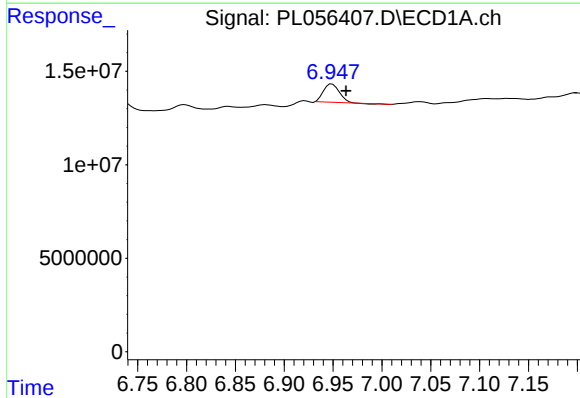


#20 Methoxychlor

R.T.: 6.949 min
Delta R.T.: -0.014 min
Response: 11116213
Conc: 2.09 ng/ml

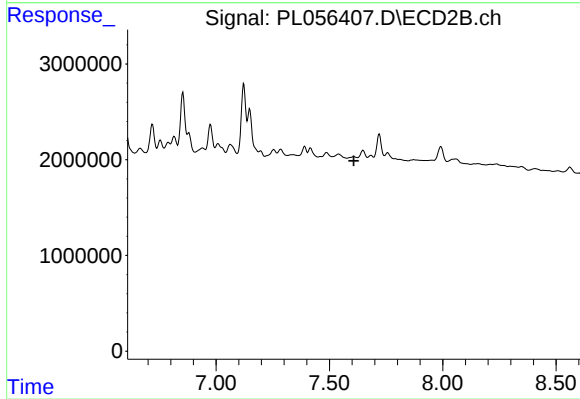

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.607 min
Response: 0
Conc: N.D.

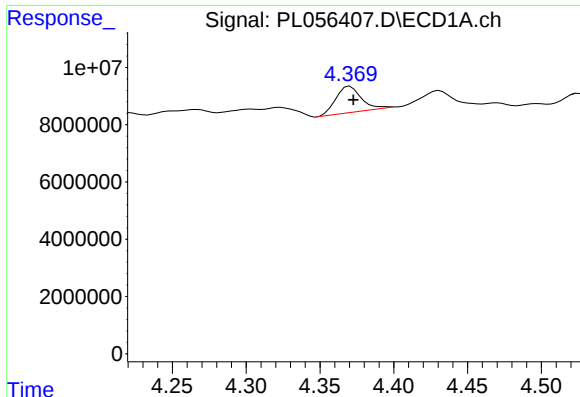

#23 Chlordane-1


R.T.: 4.370 min
Delta R.T.: -0.002 min
Response: 10762455
Conc: 28.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

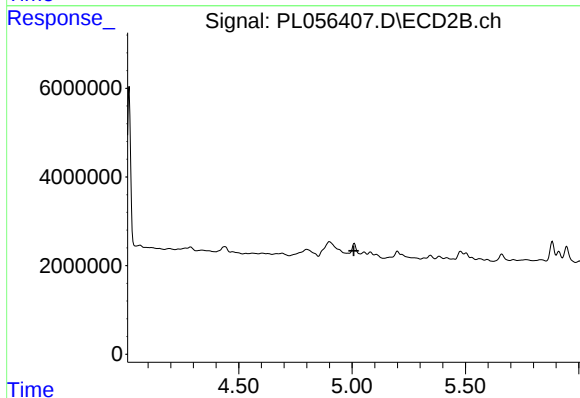


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

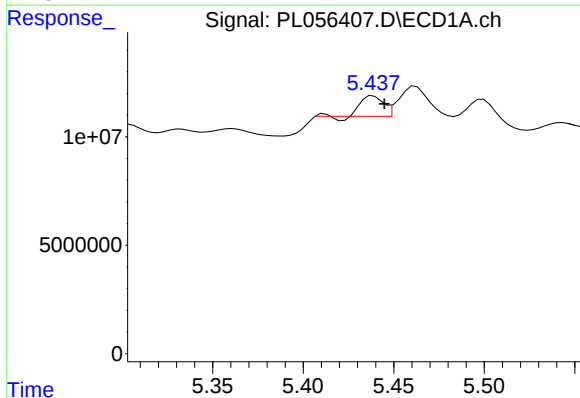


#25 Chlordane-3

R.T.: 5.439 min
Delta R.T.: -0.006 min
Response: 7638426
Conc: 6.05 ng/ml

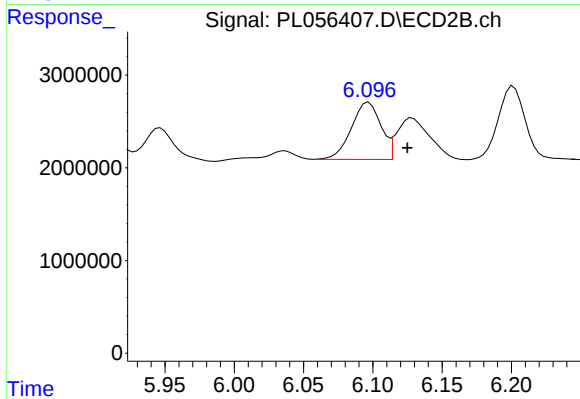

#25 Chlordane-3


R.T.: 6.097 min
Delta R.T.: -0.028 min
Response: 9131434
Conc: 24.30 ng/ml

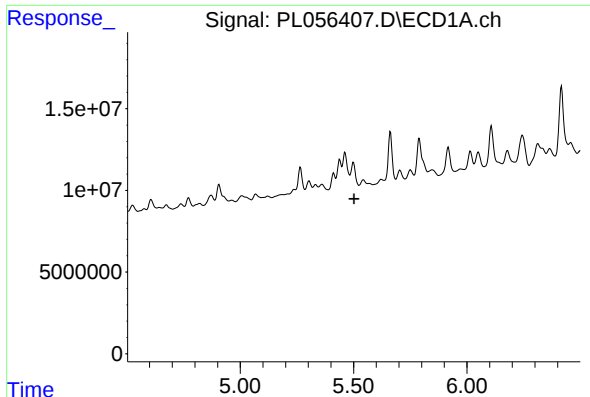

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

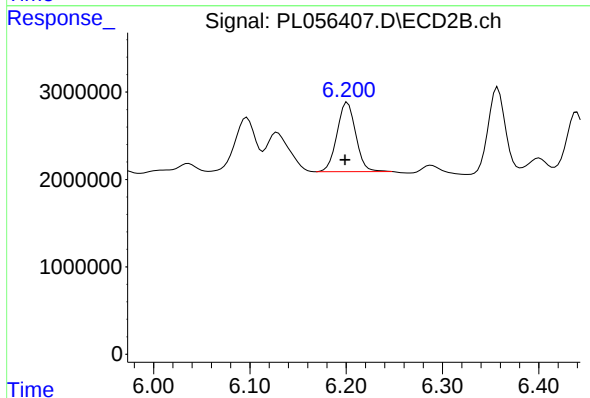


#26 Chlordane-4

R.T.: 6.201 min
Delta R.T.: 0.002 min
Response: 10671453
Conc: 24.29 ng/ml

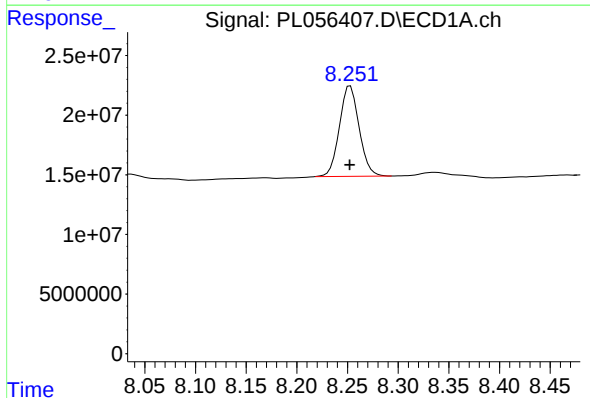

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 102423200
Conc: 9.73 ng/ml

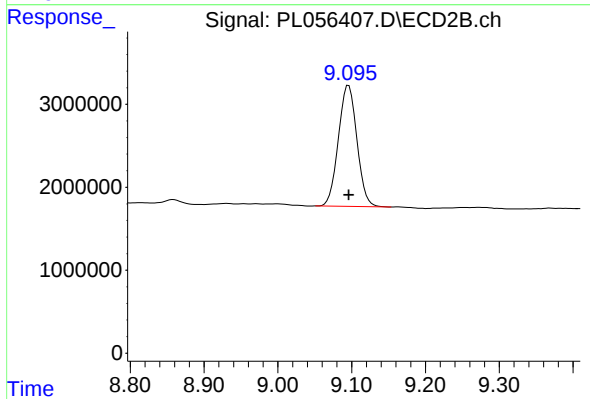

#28 Decachlorobiphenyl

R.T.: 9.096 min
Delta R.T.: 0.000 min
Response: 25521713
Conc: 11.28 ng/ml