

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2020 00:39
 Operator : AJ\MA
 Sample : L1446-05
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 00:53:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.016	216.0E6	67170388	20.628	22.971
28)	SA Decachlor...	8.252	9.095	151.7E6	36428235	14.409	16.105
Target Compounds							
3)	MA gamma-BHC...	4.230	0.000	3449945	0	0.211	N.D. #
4)	MA Heptachlor	0.000	5.202	0	6947940	N.D.	1.942 #
5)	MB Aldrin	4.760	0.000	4373245	0	0.269	N.D. #
7)	B delta-BHC	0.000	5.052f	0	12836179	N.D.	4.002 #
11)	B alpha-Chl...	5.491	0.000	21271323	0	1.383	N.D. #
15)	B Endosulfa...	6.335	6.949	14315832	3705004	1.095	1.376 #
26)	Chlordane-4	5.491	0.000	21271323	0	19.659	N.D. #
27)	Chlordane-5	6.335	0.000	14315832	0	34.510	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2020 00:39
Operator : AJ\MA
Sample : L1446-05
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 00:53:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

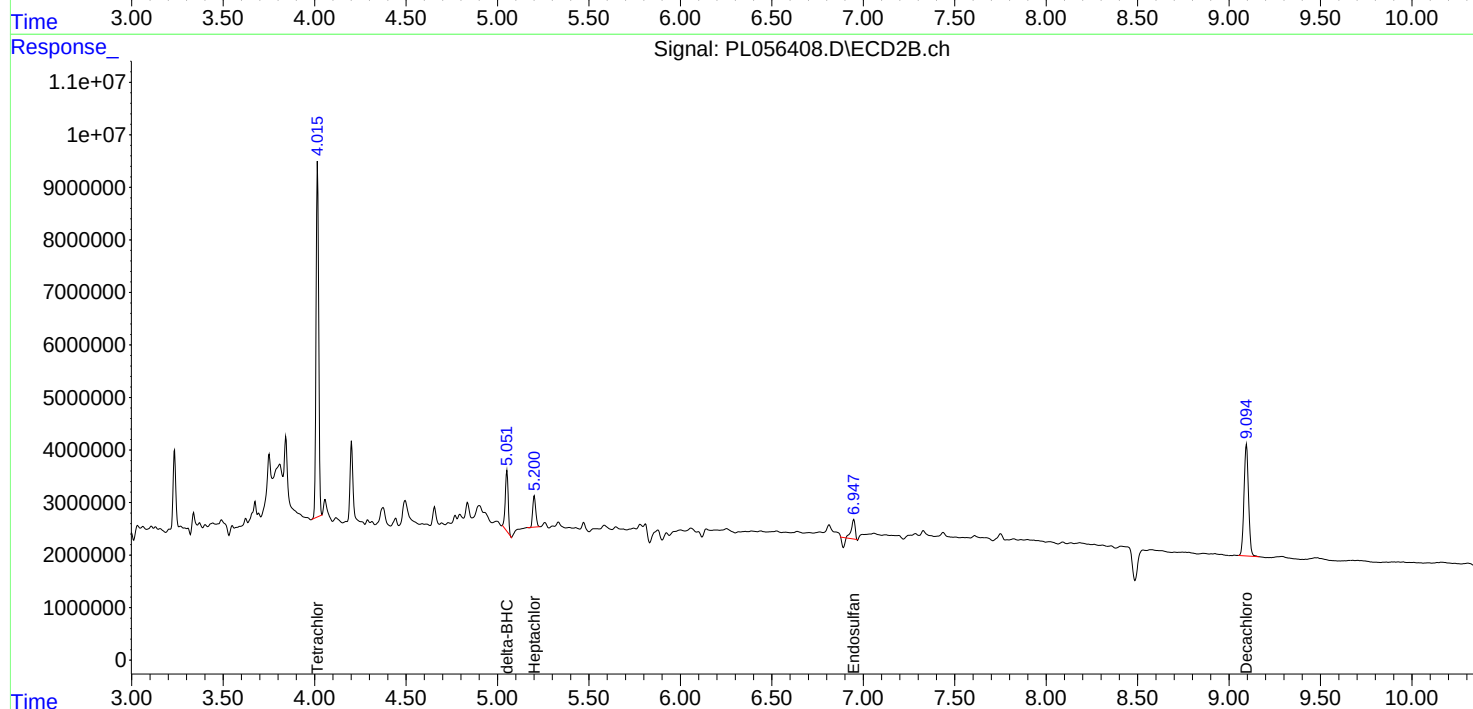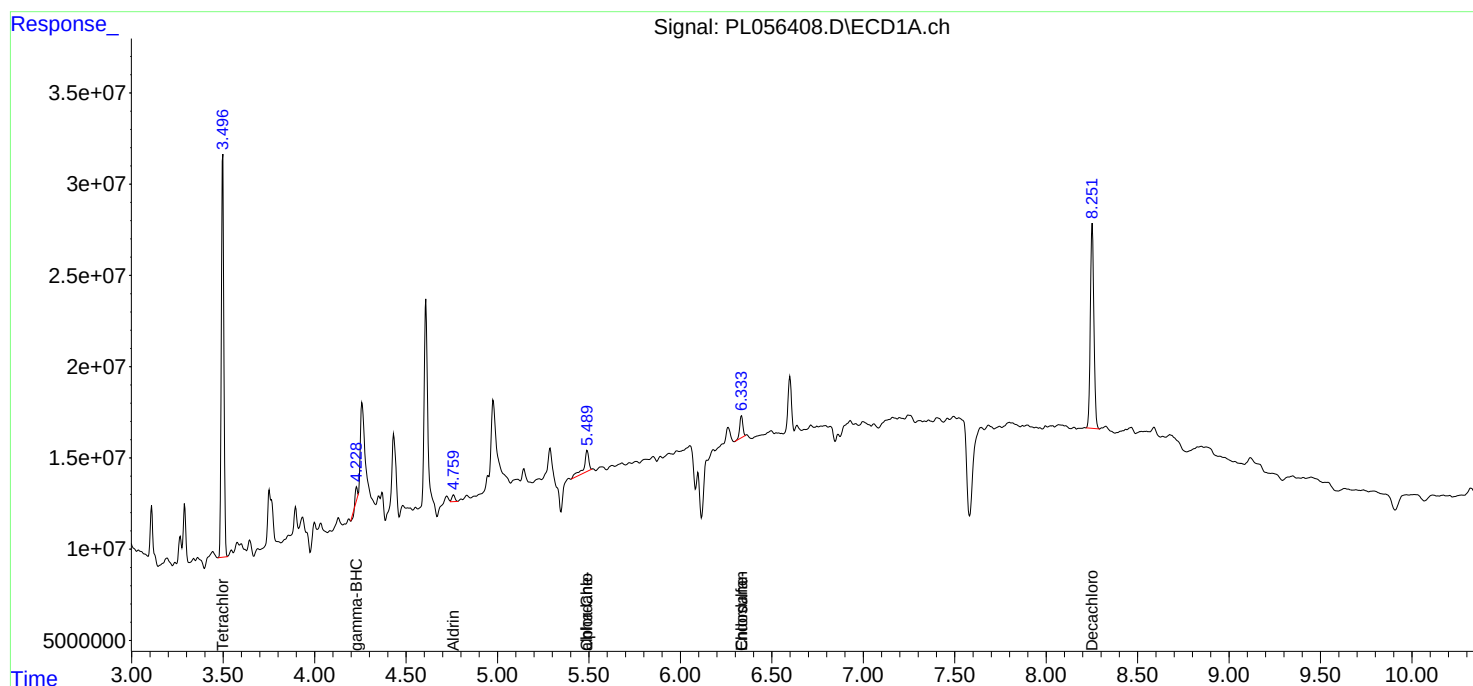


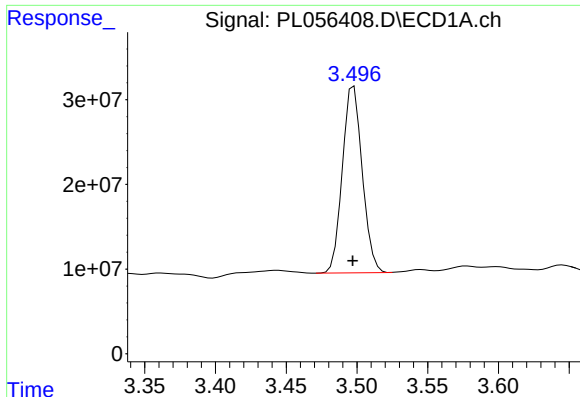

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 216041951
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :

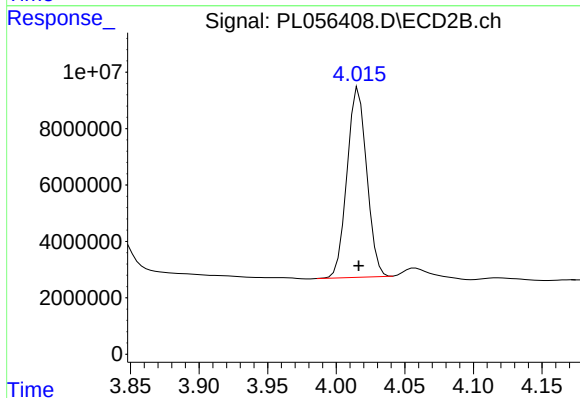


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 67170388
Conc: 22.97 ng/ml

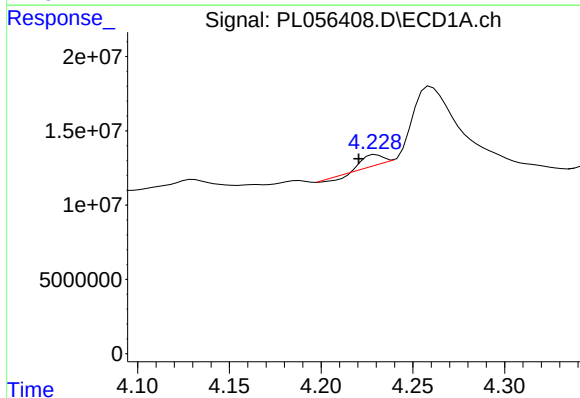


#3 gamma-BHC (Lindane)

R.T.: 4.230 min
Delta R.T.: 0.009 min
Response: 3449945
Conc: 0.21 ng/ml

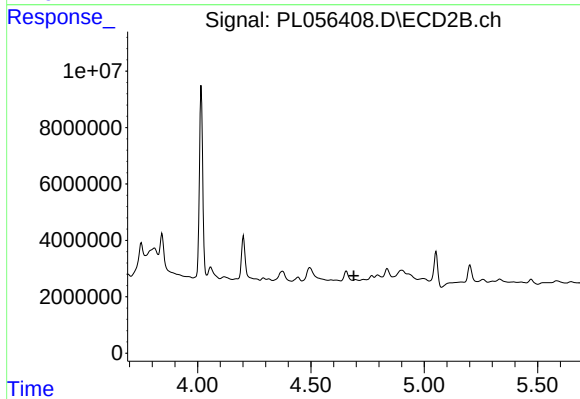

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.689 min
Response: 0
Conc: N.D.

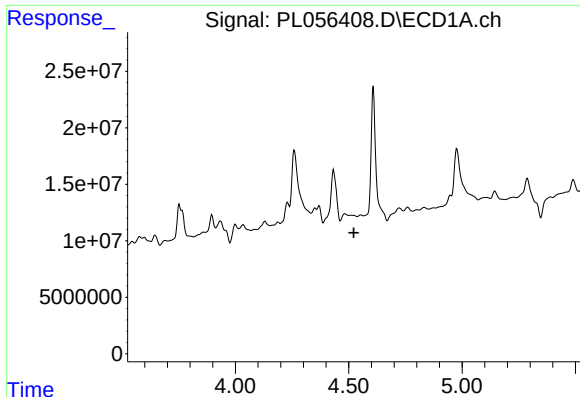

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.522 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

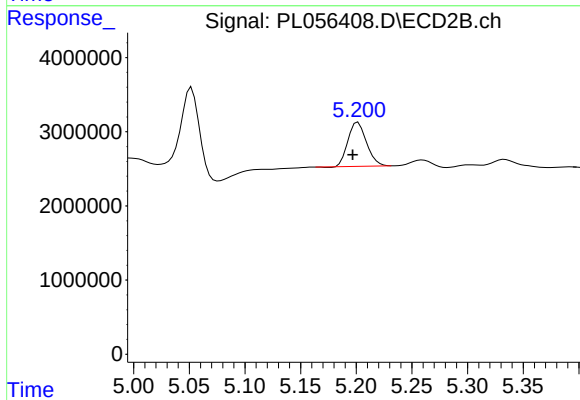


#4 Heptachlor

R.T.: 5.202 min
Delta R.T.: 0.005 min
Response: 6947940
Conc: 1.94 ng/ml

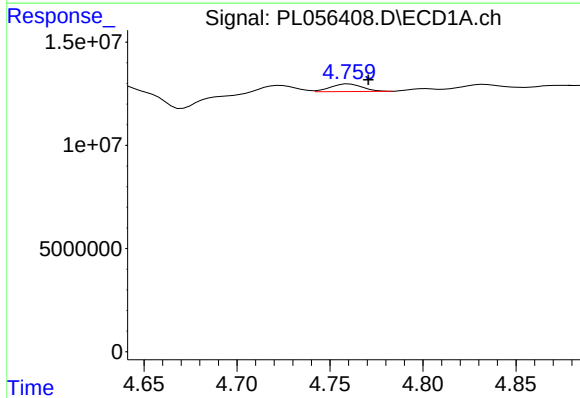


#5 Aldrin

R.T.: 4.760 min
Delta R.T.: -0.010 min
Response: 4373245
Conc: 0.27 ng/ml

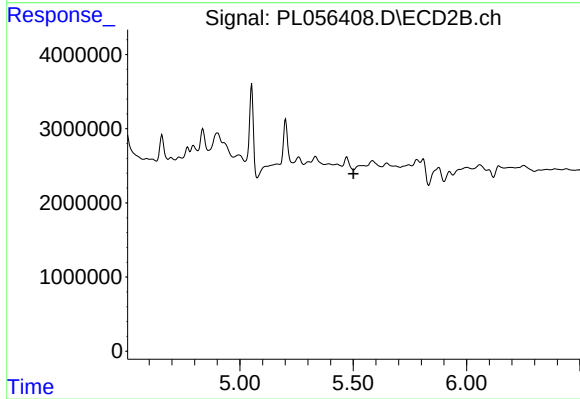

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.501 min
Response: 0
Conc: N.D.

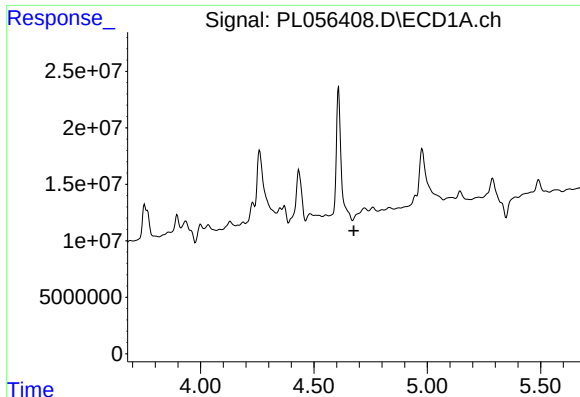

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.676 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

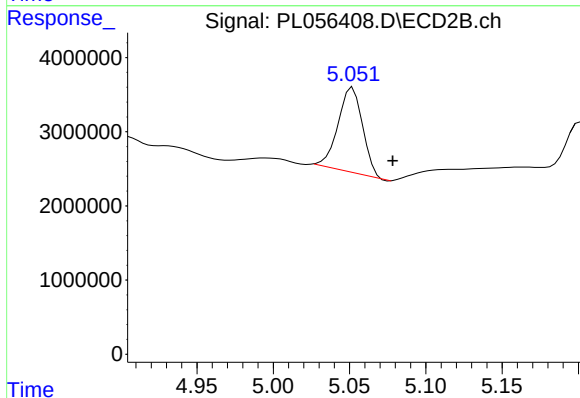


#7 delta-BHC

R.T.: 5.052 min
Delta R.T.: -0.026 min
Response: 12836179
Conc: 4.00 ng/ml

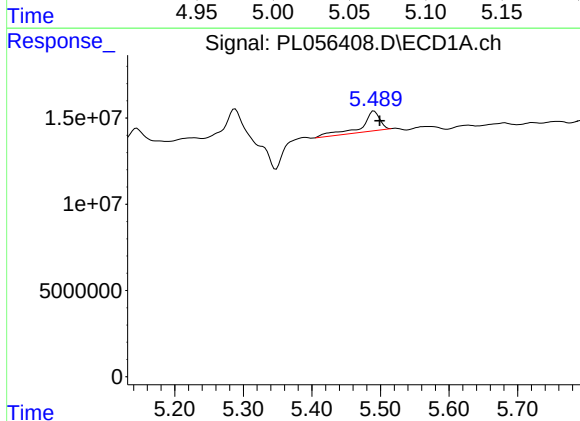


#11 alpha-Chlordane

R.T.: 5.491 min
Delta R.T.: -0.008 min
Response: 21271323
Conc: 1.38 ng/ml

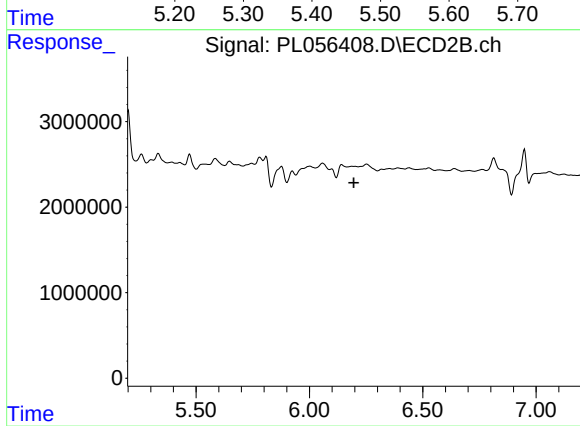

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

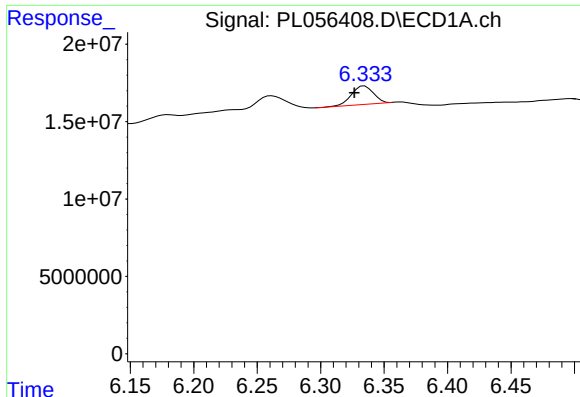

#15 Endosulfan II


R.T.: 6.335 min
Delta R.T.: 0.008 min
Response: 14315832
Conc: 1.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

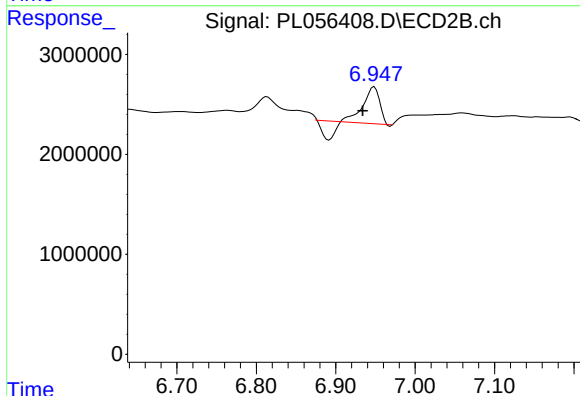


#15 Endosulfan II

R.T.: 6.949 min
Delta R.T.: 0.015 min
Response: 3705004
Conc: 1.38 ng/ml

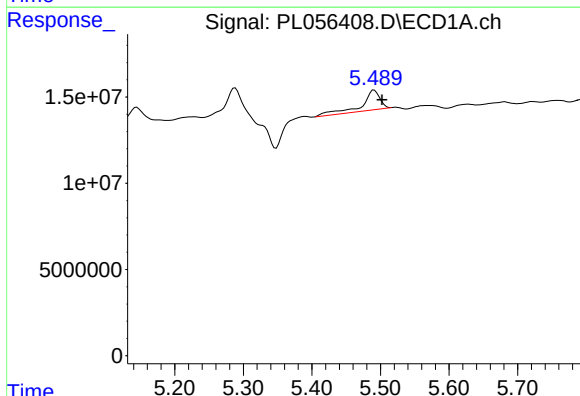


#26 Chlordane-4

R.T.: 5.491 min
Delta R.T.: -0.012 min
Response: 21271323
Conc: 19.66 ng/ml

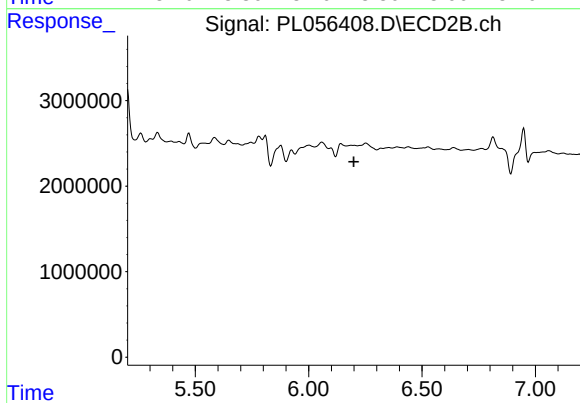

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

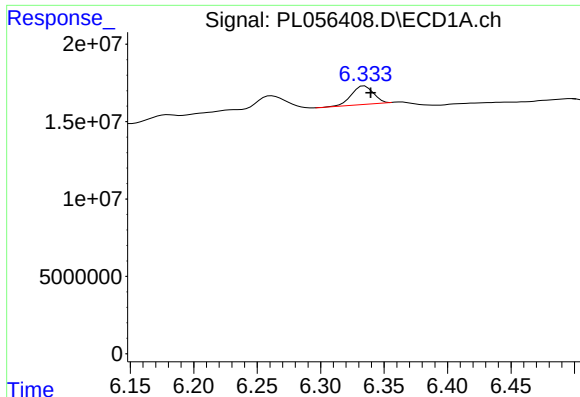

#27 Chlordane-5


R.T.: 6.335 min
Delta R.T.: -0.005 min
Response: 14315832
Conc: 34.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

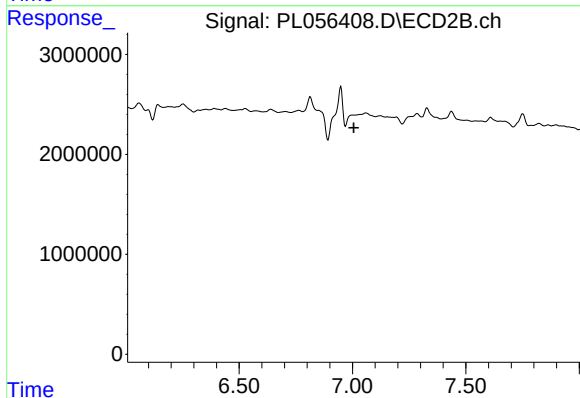


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.007 min
Response: 0
Conc: N.D.

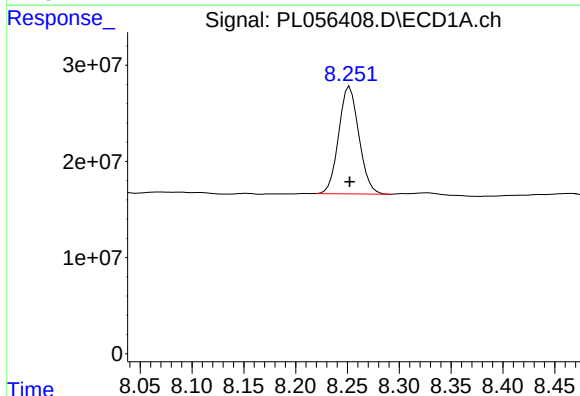

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 151703005
Conc: 14.41 ng/ml

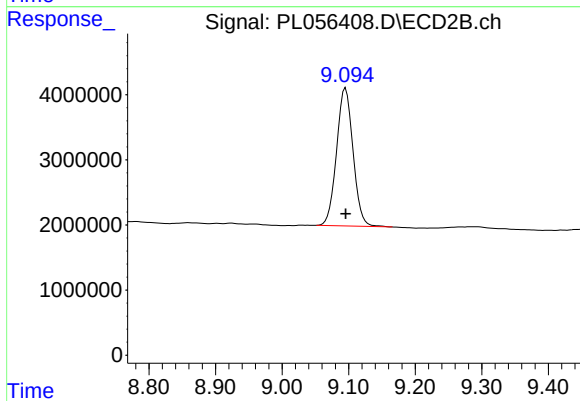

#28 Decachlorobiphenyl

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 36428235
Conc: 16.10 ng/ml