

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2020 00:53
 Operator : AJ\MA
 Sample : L1446-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HP-640-X

Manual Integrations
 APPROVED

mohammad
 2/11/2020 11:07:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 03:04:54 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.015	393.9E6	36074957	37.614m	12.337m#
28)	SA Decachlor...	8.253	9.094	187.8E6	39955541	17.834	17.664
Target Compounds							
15)	B Endosulfa...	6.336	6.949f	11672.4E6	1810.4E6	892.493	672.498m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2020 00:53
Operator : AJ\MA
Sample : L1446-04
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640-X


Manual Integrations
APPROVED

mohammad
2/11/2020 11:07:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 03:04:54 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

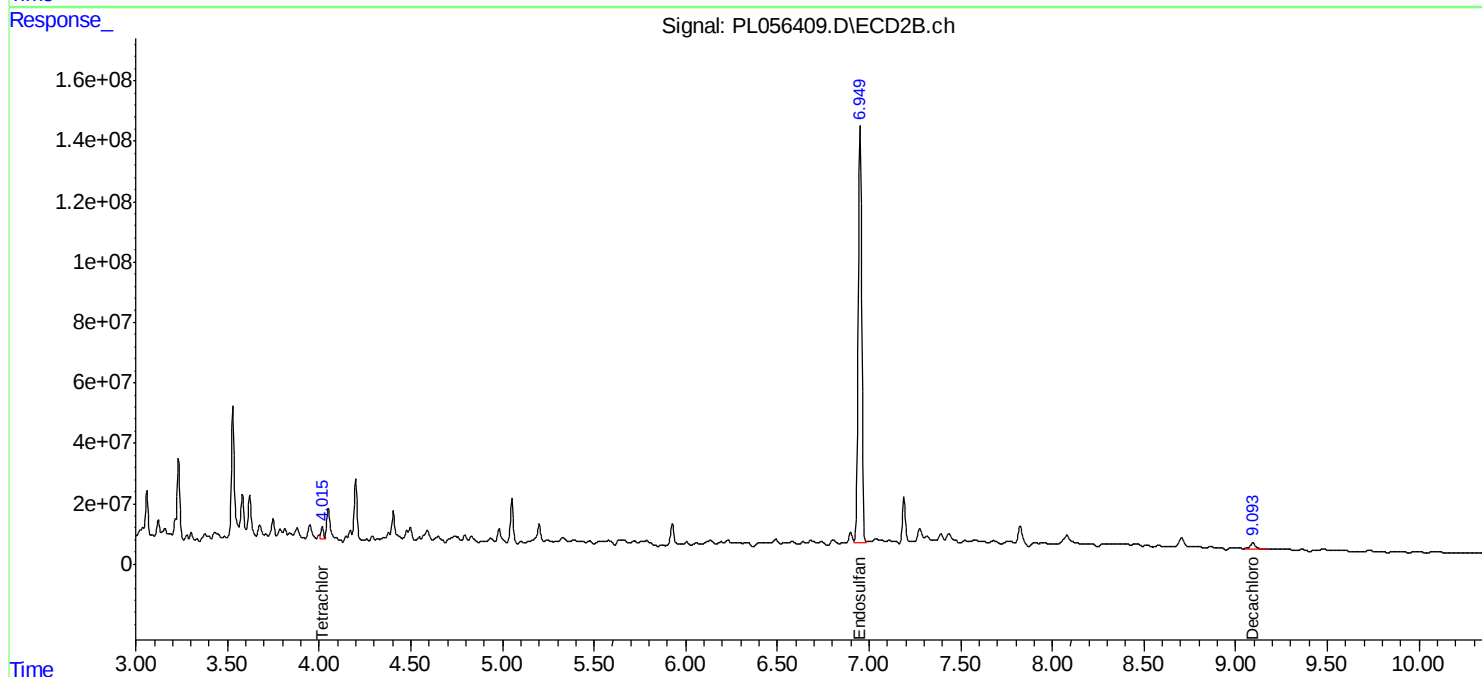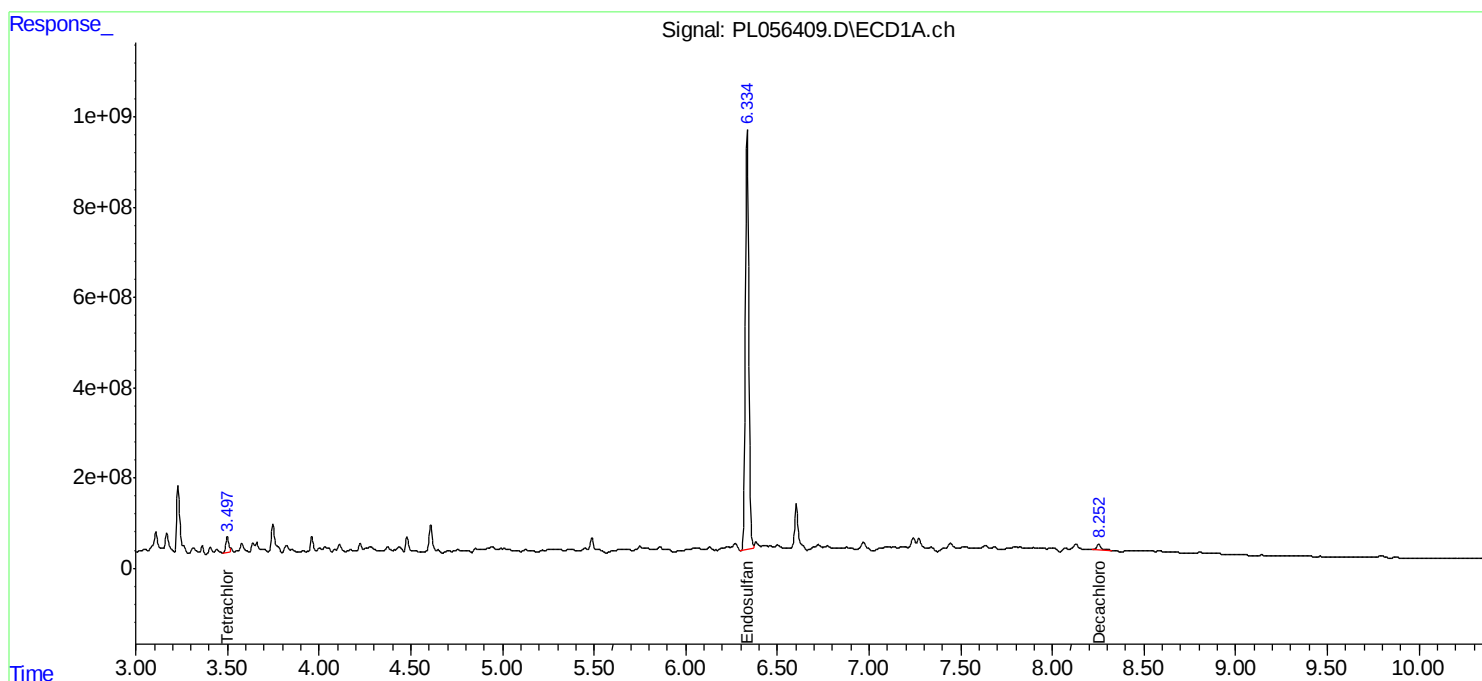

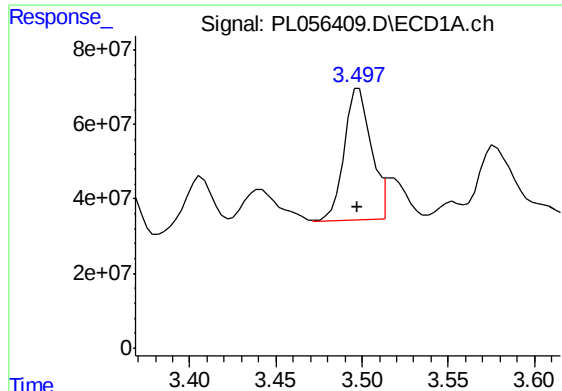


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 393927285
Conc: 37.61 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HP-640-X


Manual Integrations
APPROVED

mohammad
2/11/2020 11:07:05 AM

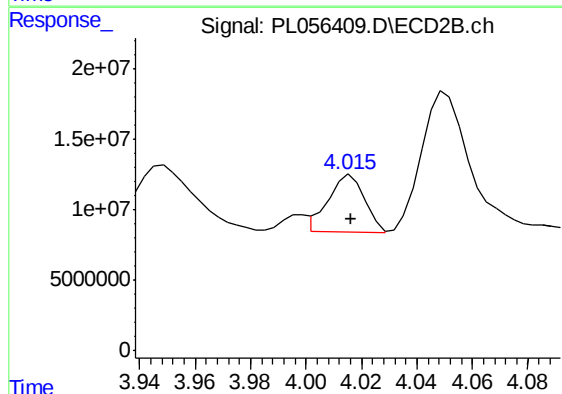


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.001 min
Response: 36074957
Conc: 12.34 ng/ml m

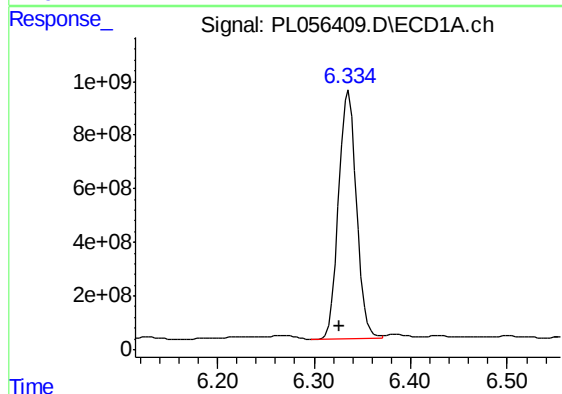


#15 Endosulfan II

R.T.: 6.336 min
Delta R.T.: 0.009 min
Response: 11672405425
Conc: 892.49 ng/ml

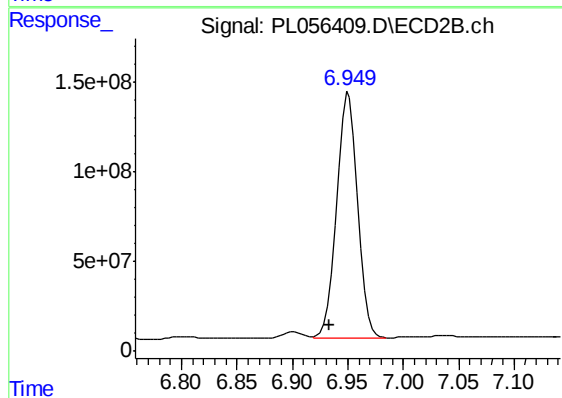

#15 Endosulfan II

R.T.: 6.949 min
Delta R.T.: 0.016 min
Response: 1810423029
Conc: 672.50 ng/ml m

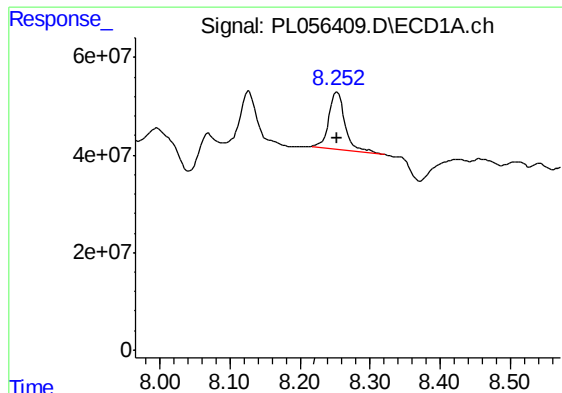


#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 187756508
Conc: 17.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640-X

Manual Integrations
APPROVED

mohammad
2/11/2020 11:07:05 AM

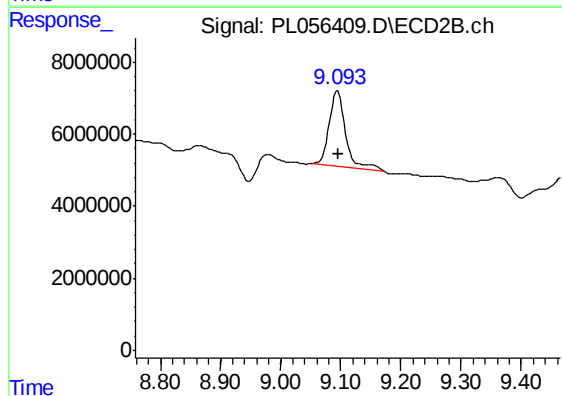

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.002 min
Response: 39955541
Conc: 17.66 ng/ml