

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
 Data File : PL056410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2020 01:07
 Operator : AJ\MA
 Sample : L1446-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleID :
 HP-640

Manual Integrations
 APPROVED

mohammad
 2/11/2020 11:06:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 03:08:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.016	379.2E6	27657248	36.204	9.458m#
28)	SA Decachlor...	8.252	9.093	167.6E6	33508286	15.921	14.814
Target Compounds							
15)	B Endosulfa...	6.335	6.950f	10644.9E6	1687.5E6	813.929	626.840m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020720\
Data File : PL056410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2020 01:07
Operator : AJ\MA
Sample : L1446-01
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HP-640


Manual Integrations
APPROVED

mohammad
2/11/2020 11:06:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 03:08:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

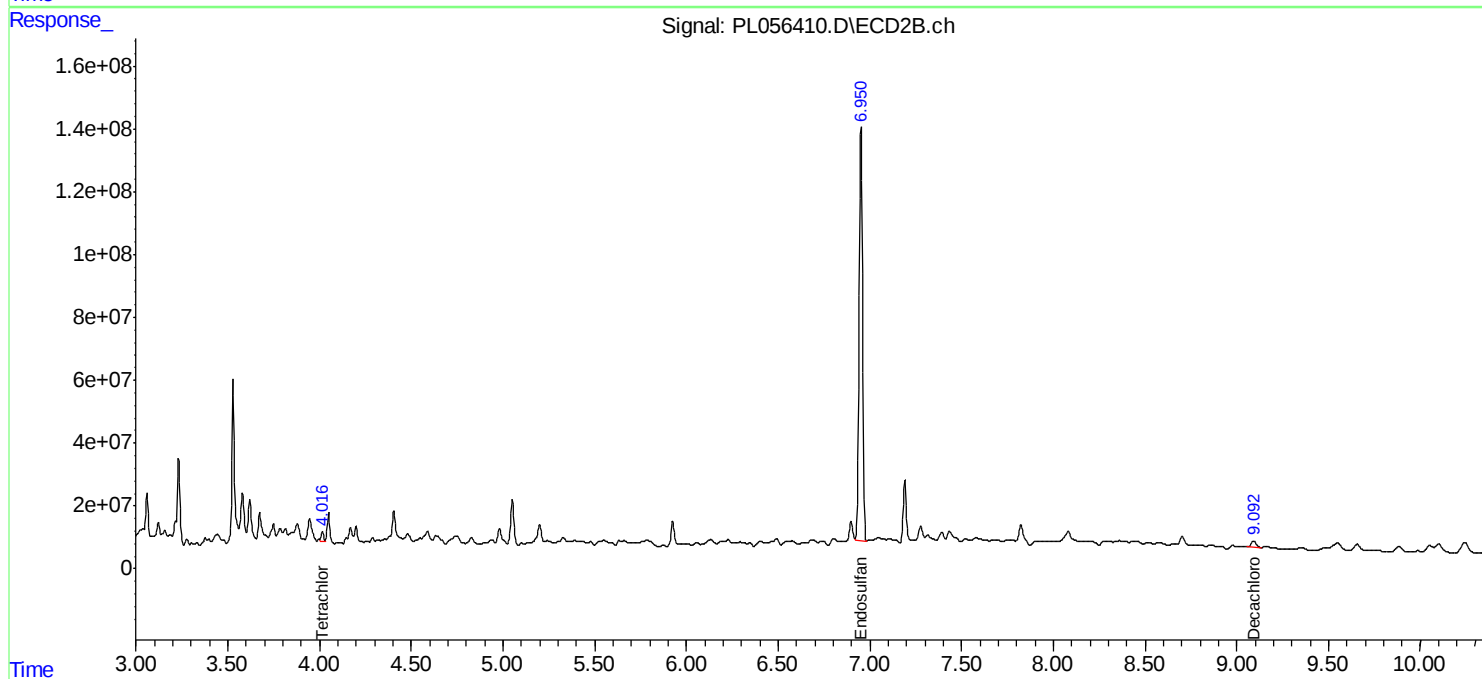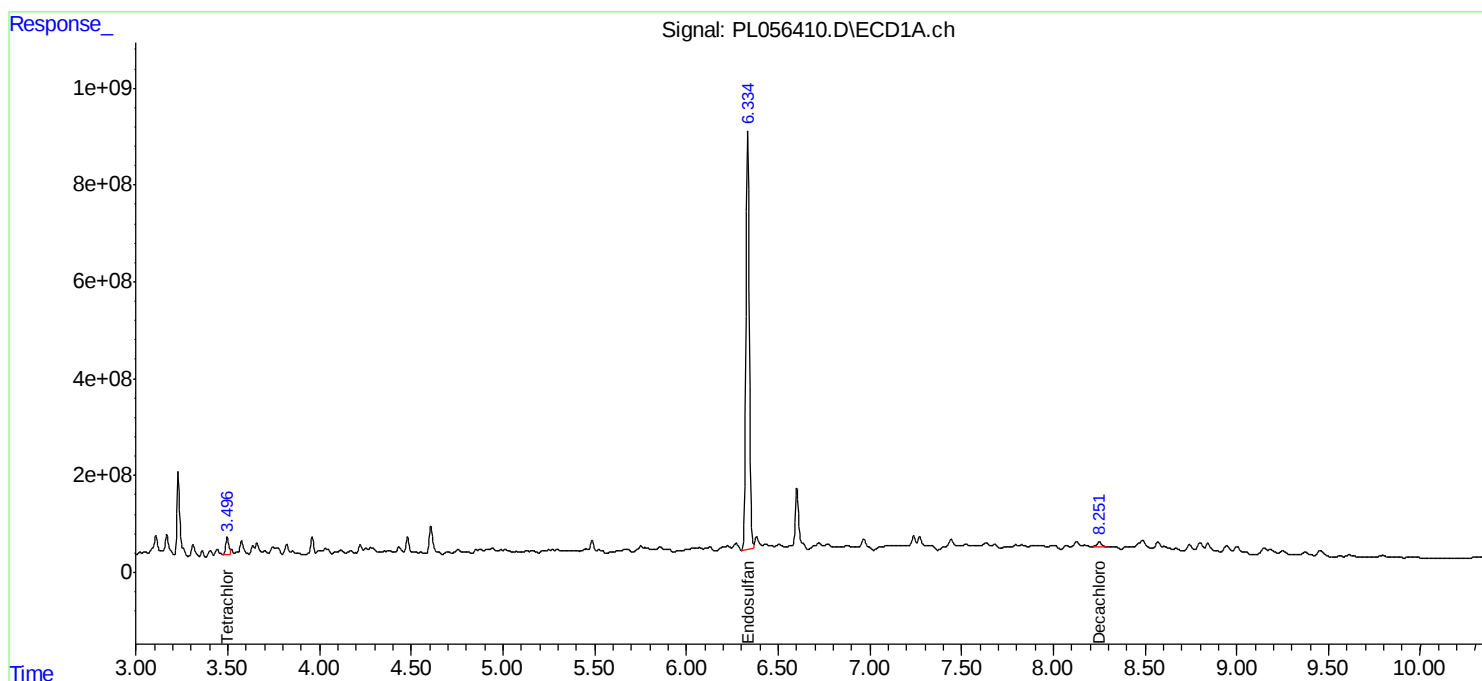

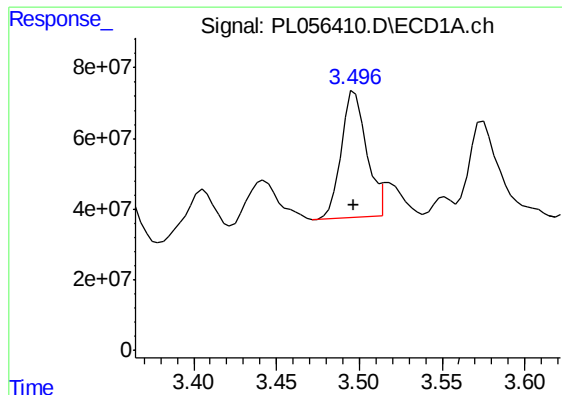


#1 Tetrachloro-m-xylene

R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 379159816
Conc: 36.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640


Manual Integrations
APPROVED

mohammad
2/11/2020 11:06:57 AM

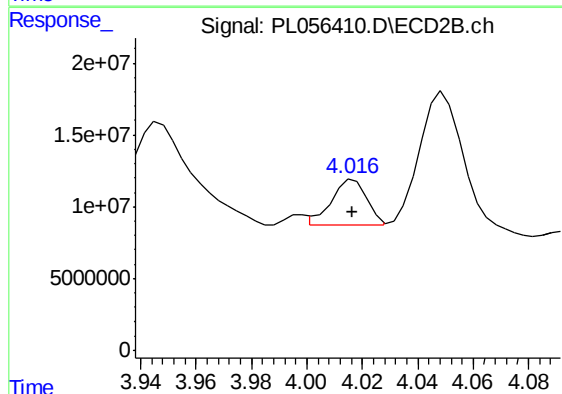


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 27657248
Conc: 9.46 ng/ml m

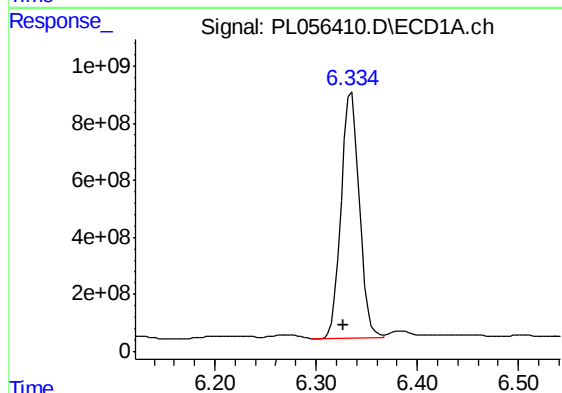


#15 Endosulfan II

R.T.: 6.335 min
Delta R.T.: 0.008 min
Response: 10644908798
Conc: 813.93 ng/ml

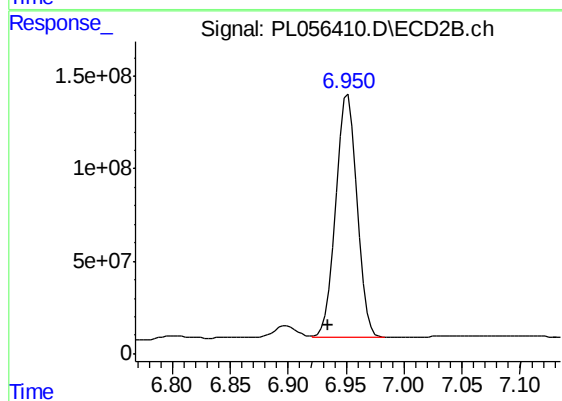

#15 Endosulfan II

R.T.: 6.950 min
Delta R.T.: 0.016 min
Response: 1687508442
Conc: 626.84 ng/ml m

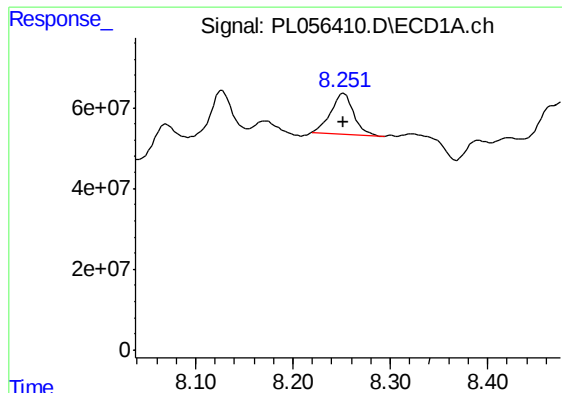


#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 167618318
Conc: 15.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
HP-640

Manual Integrations
APPROVED

mohammad
2/11/2020 11:06:57 AM

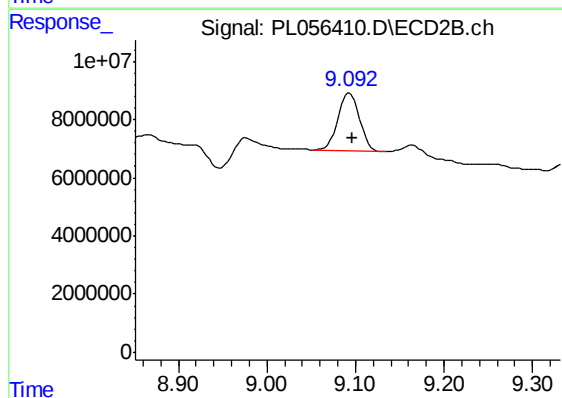

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.003 min
Response: 33508286
Conc: 14.81 ng/ml