

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020722\
 Data File : PL072496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2022 21:45
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 01:03:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 01:03:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.492	51394121	178.8E6	100.425	100.077
28)	SA Decachlor...	10.317	11.385	74152950	160.7E6	97.810	99.522
Target Compounds							
23)	Chlordane-1	5.881	6.874	18887818	72490319	994.778	997.204
24)	Chlordane-2	6.570	7.467	24246607	73423844	970.423	972.373
25)	Chlordane-3	7.271	8.224	69515124	307.2E6	999.715	997.516
26)	Chlordane-4	7.338	8.306	75129744	360.5E6	998.615	991.382
27)	Chlordane-5	8.288	9.193	25255307	61054038	984.558	986.455



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020722\
Data File : PL072496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2022 21:45
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 01:03:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 01:03:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

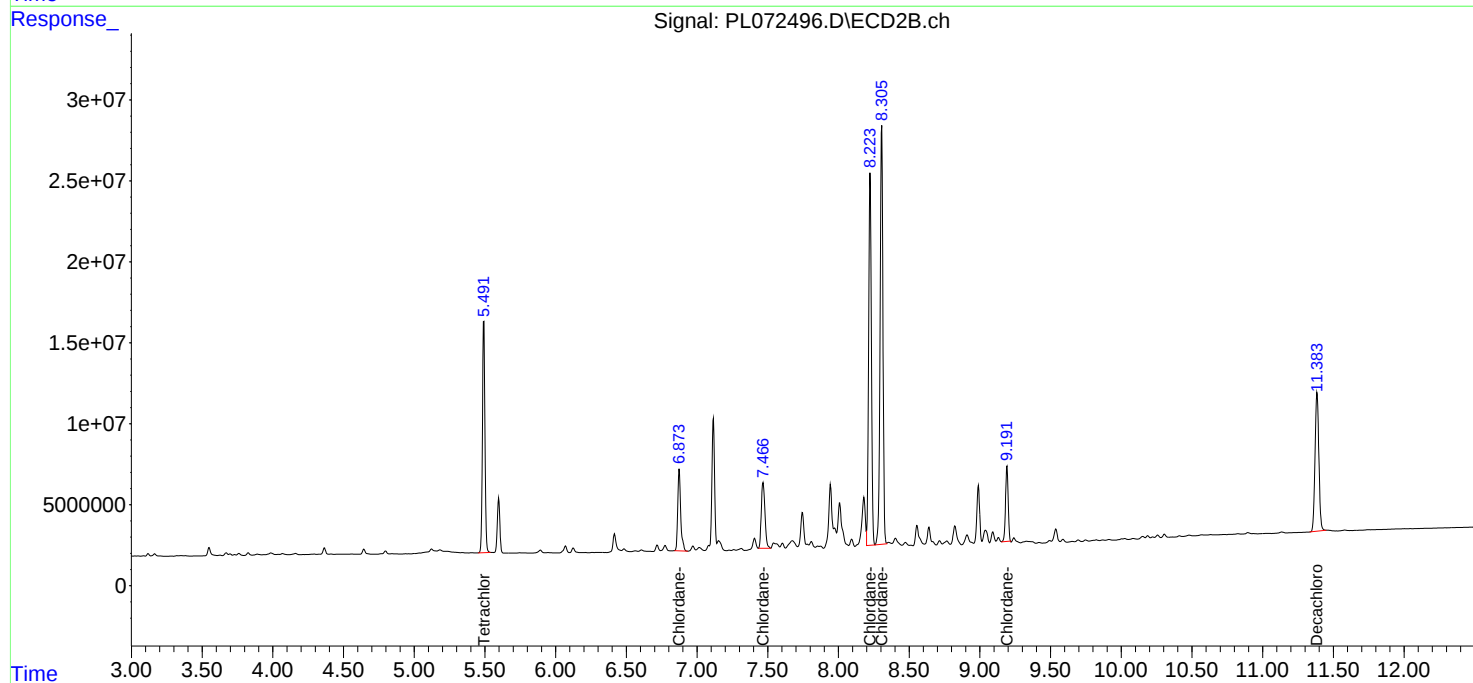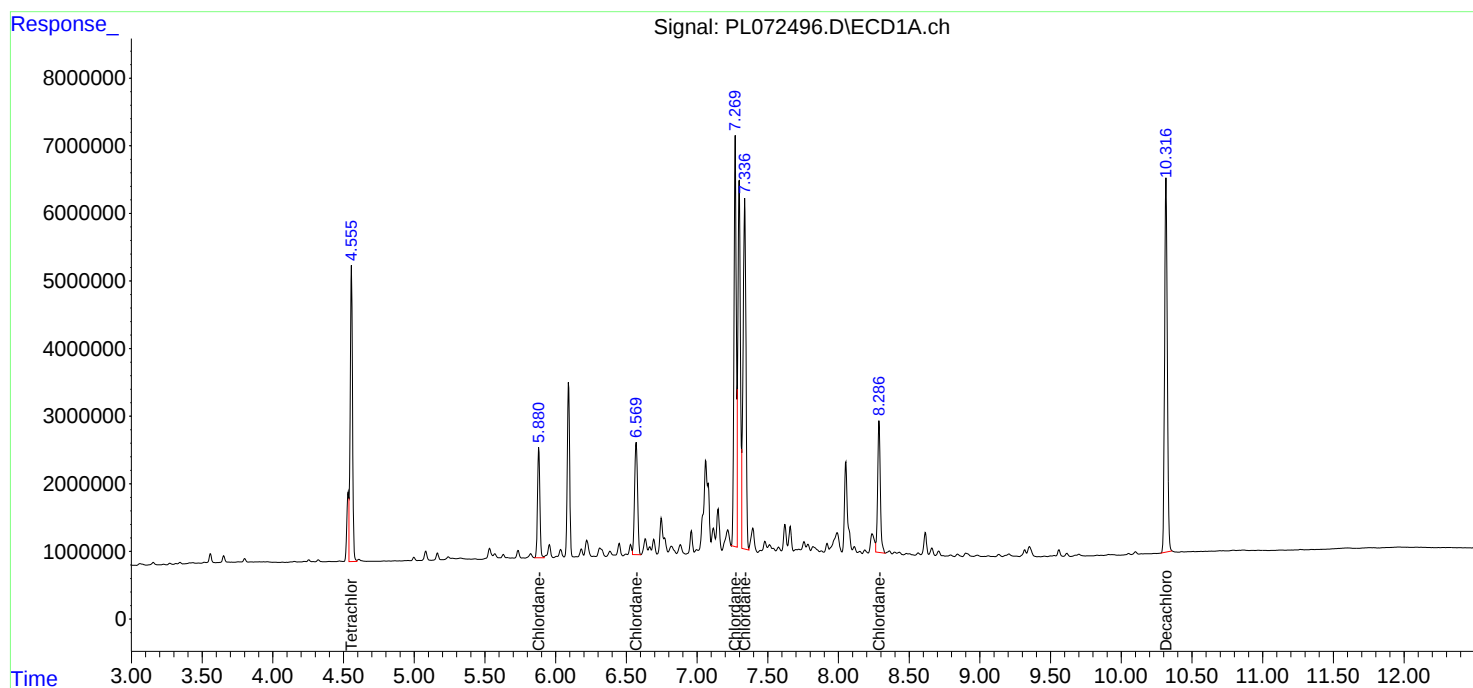


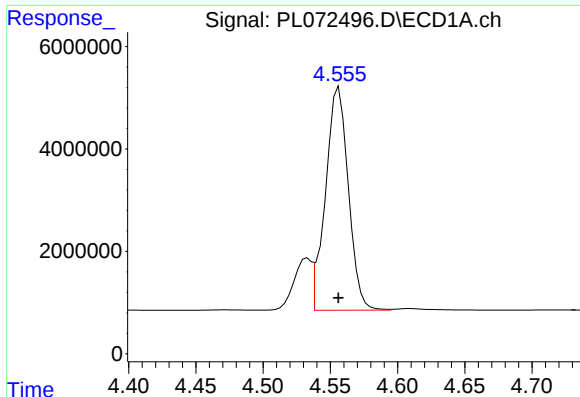

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: 0.000 min
Response: 51394121
Conc: 100.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

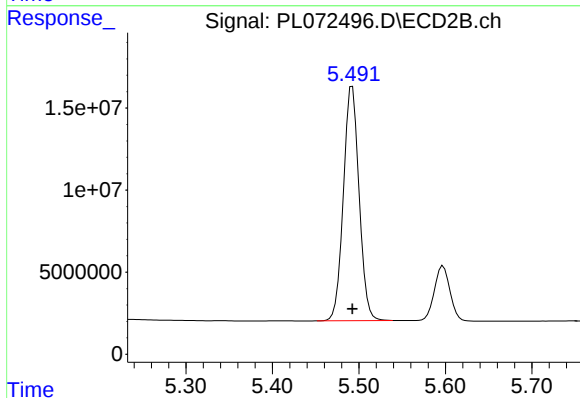


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 178810680
Conc: 100.08 ng/ml

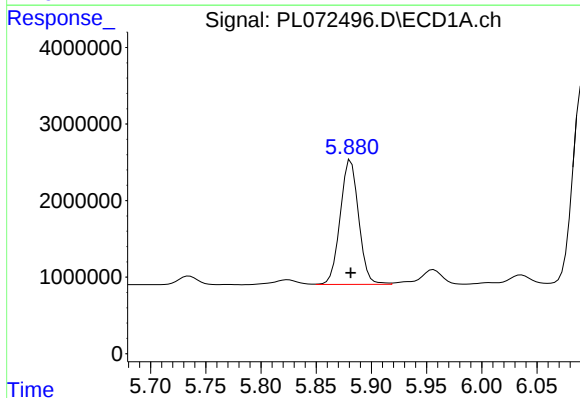


#23 Chlordane-1

R.T.: 5.881 min
Delta R.T.: 0.000 min
Response: 18887818
Conc: 994.78 ng/ml

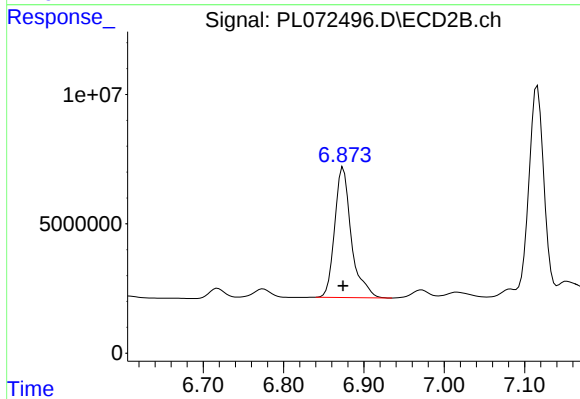

#23 Chlordane-1


R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 72490319
Conc: 997.20 ng/ml

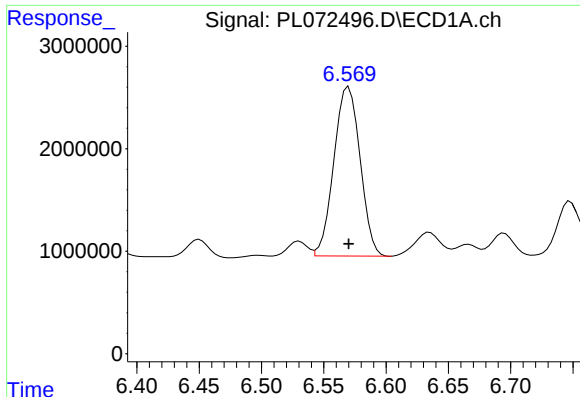

#24 Chlordane-2


R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 24246607
Conc: 970.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

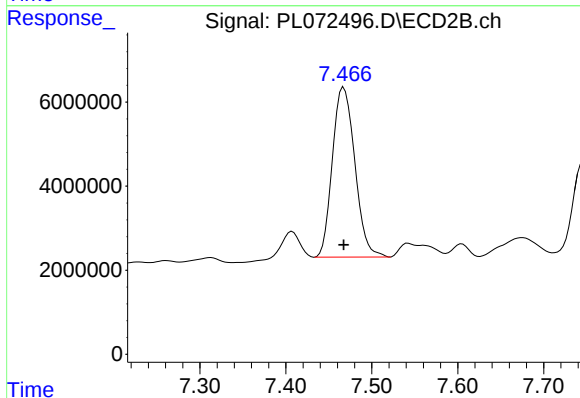


#24 Chlordane-2

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 73423844
Conc: 972.37 ng/ml

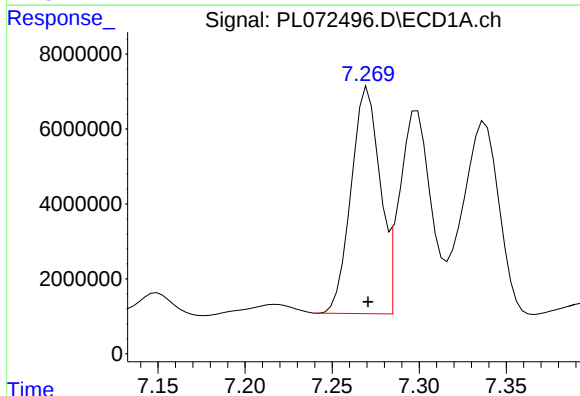


#25 Chlordane-3

R.T.: 7.271 min
Delta R.T.: 0.000 min
Response: 69515124
Conc: 999.72 ng/ml

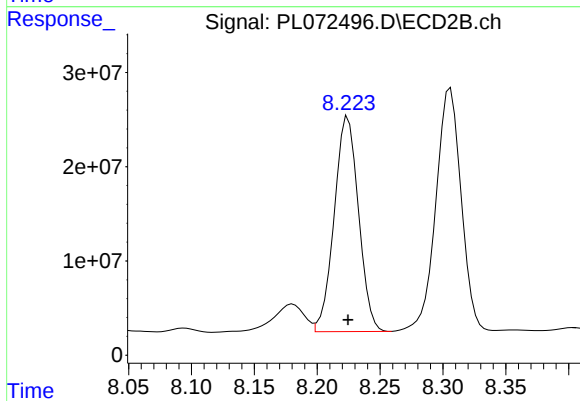

#25 Chlordane-3


R.T.: 8.224 min
Delta R.T.: 0.000 min
Response: 307156844
Conc: 997.52 ng/ml

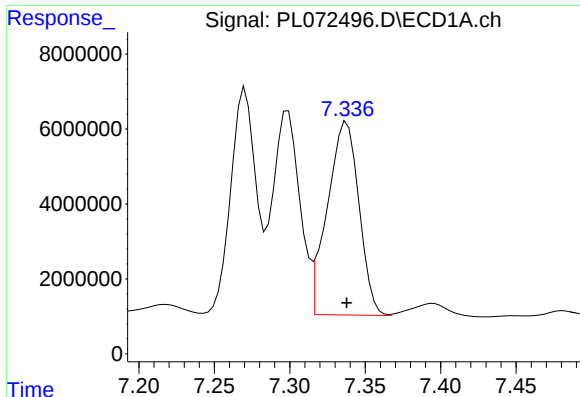

#26 Chlordane-4


R.T.: 7.338 min
Delta R.T.: 0.000 min
Response: 75129744
Conc: 998.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

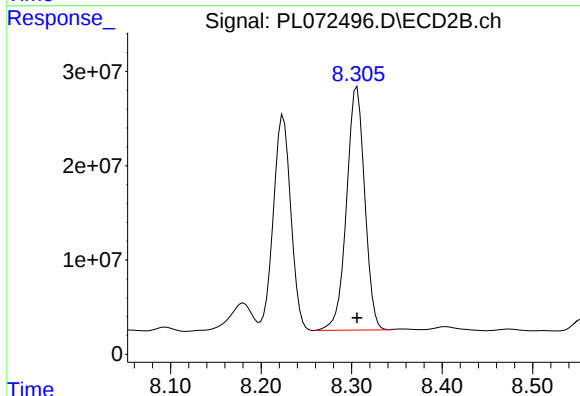


#26 Chlordane-4

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 360509392
Conc: 991.38 ng/ml

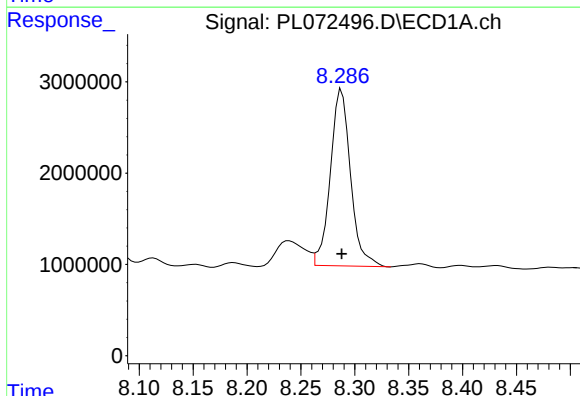


#27 Chlordane-5

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 25255307
Conc: 984.56 ng/ml

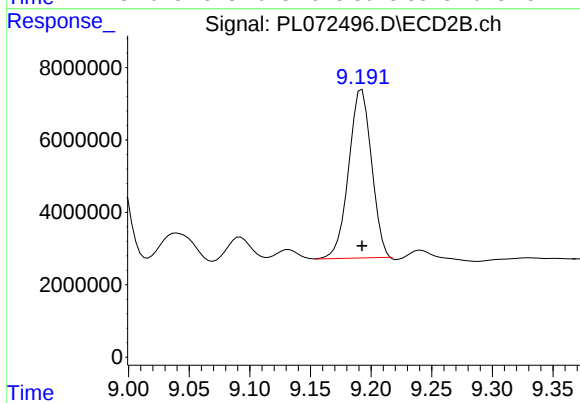

#27 Chlordane-5


R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 61054038
Conc: 986.46 ng/ml

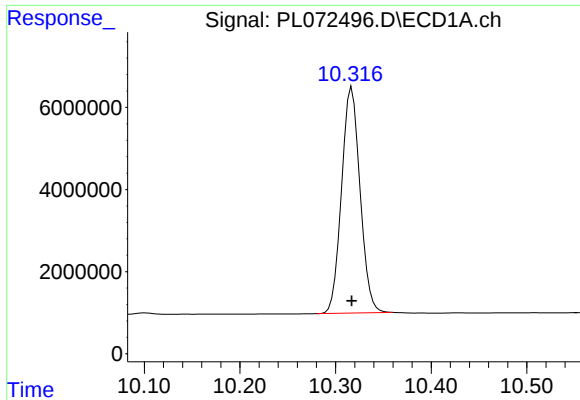

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: 0.000 min
Response: 74152950
Conc: 97.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

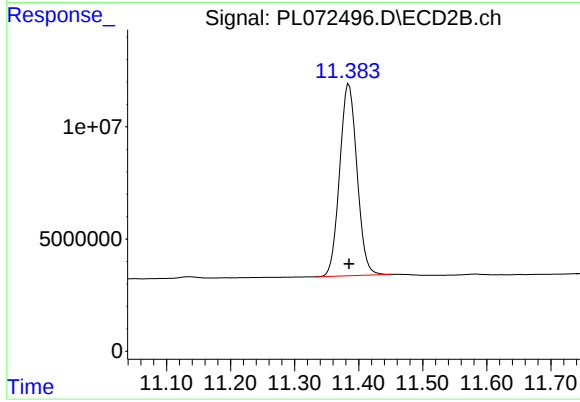

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: 0.000 min
Response: 160693894
Conc: 99.52 ng/ml