

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020722\
 Data File : PL072497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Feb 2022 22:02
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 01:05:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 01:05:00 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	37964925	134.1E6	74.454	75.045
28)	SA Decachlor...	10.317	11.386	57885762	123.6E6	75.896	76.045
Target Compounds							
23)	Chlordane-1	5.882	6.875	14328464	54706734	753.092	751.709
24)	Chlordane-2	6.571	7.467	18767373	56655318	750.751	750.202
25)	Chlordane-3	7.270	8.225	52065056	231.1E6	749.174	750.247
26)	Chlordane-4	7.339	8.306	56690290	272.7E6	752.343	749.954
27)	Chlordane-5	8.288	9.192	19385394	46692561	753.806	752.938



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020722\
Data File : PL072497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Feb 2022 22:02
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 01:05:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 01:05:00 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

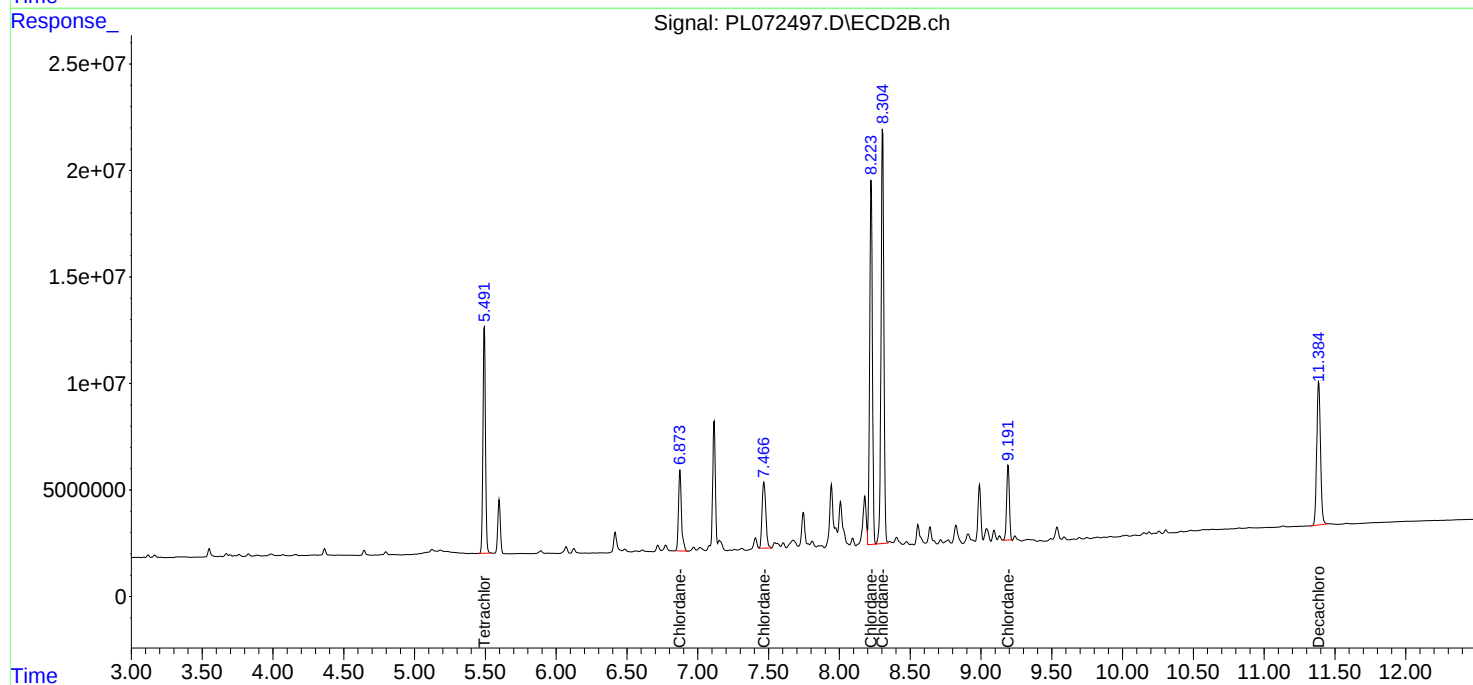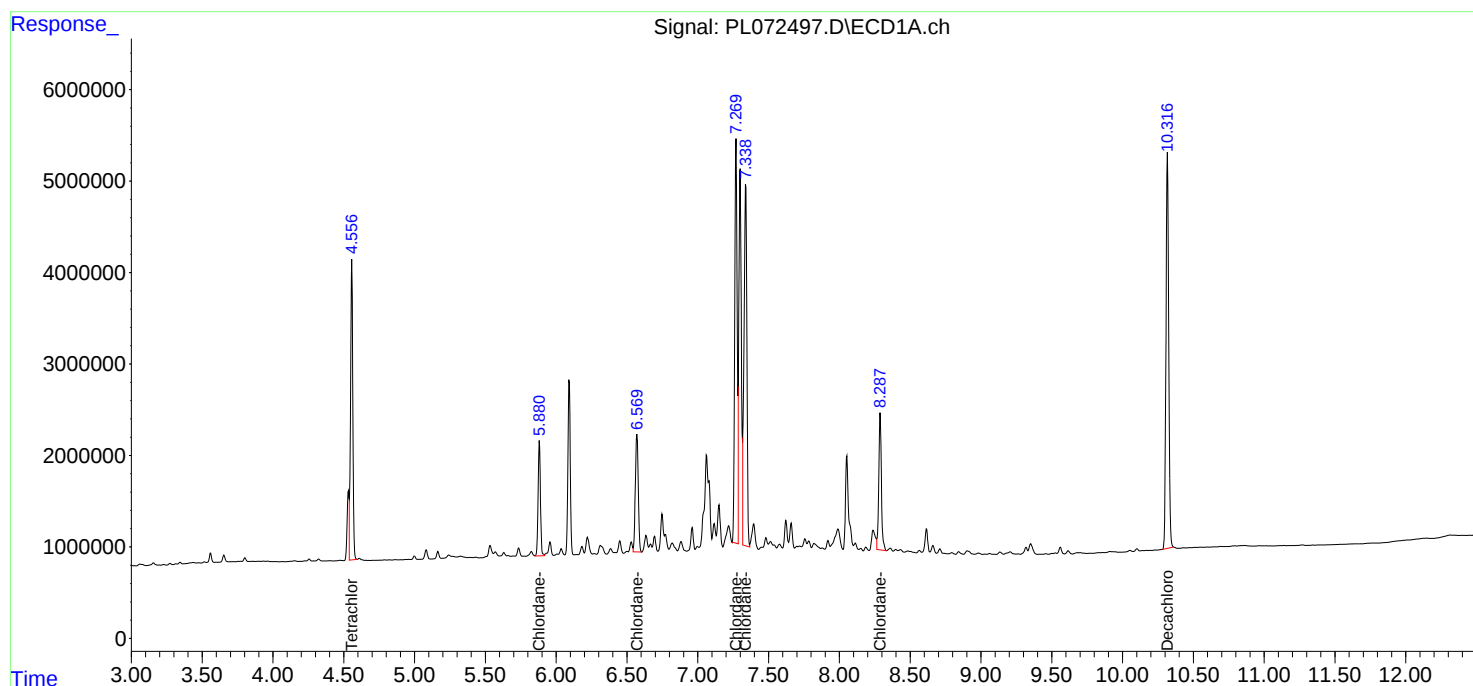


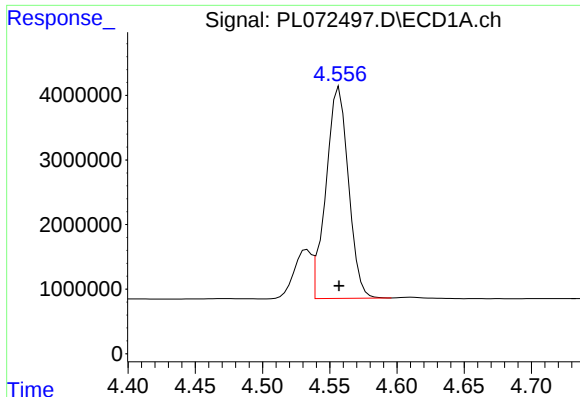

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 37964925
Conc: 74.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

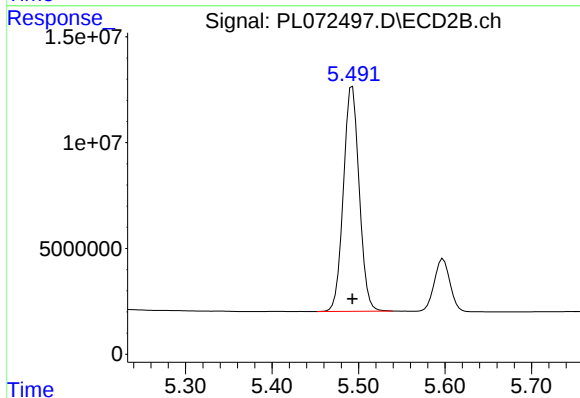


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 134124282
Conc: 75.04 ng/ml

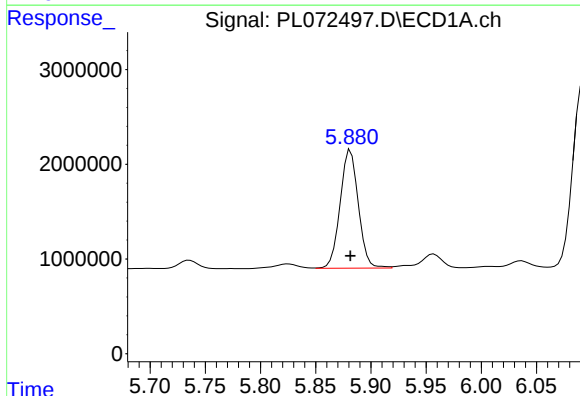


#23 Chlordane-1

R.T.: 5.882 min
Delta R.T.: 0.000 min
Response: 14328464
Conc: 753.09 ng/ml

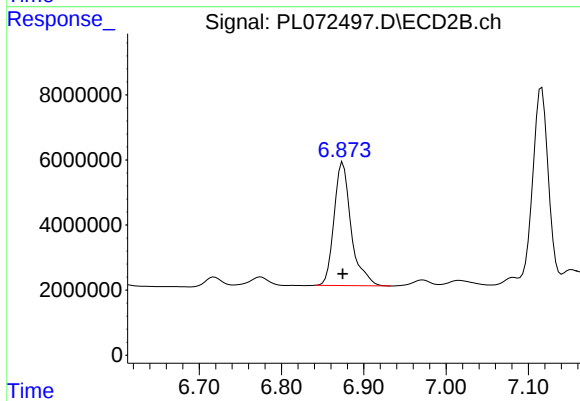

#23 Chlordane-1


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 54706734
Conc: 751.71 ng/ml

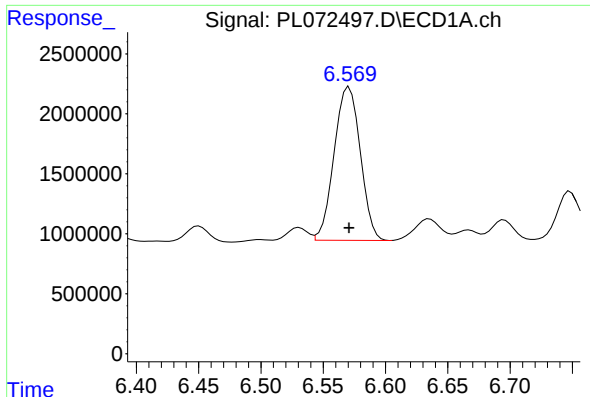

#24 Chlordane-2


R.T.: 6.571 min
Delta R.T.: 0.000 min
Response: 18767373
Conc: 750.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

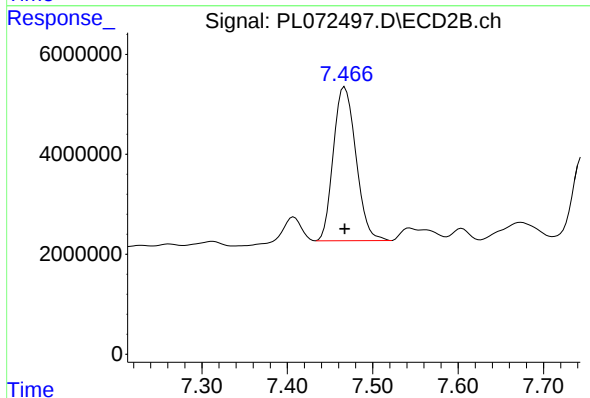


#24 Chlordane-2

R.T.: 7.467 min
Delta R.T.: 0.000 min
Response: 56655318
Conc: 750.20 ng/ml

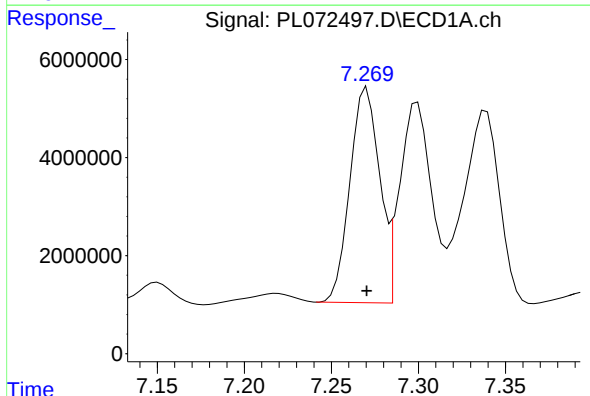


#25 Chlordane-3

R.T.: 7.270 min
Delta R.T.: 0.000 min
Response: 52065056
Conc: 749.17 ng/ml

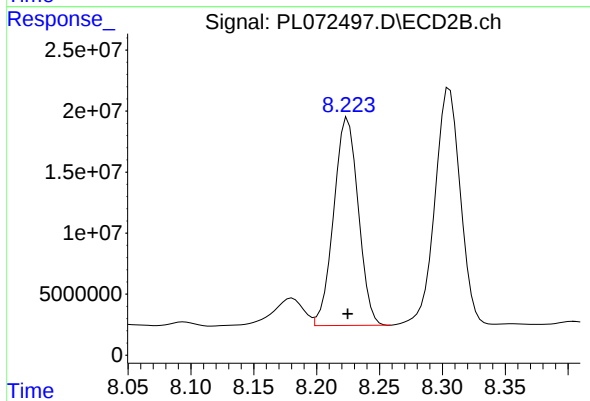

#25 Chlordane-3


R.T.: 8.225 min
Delta R.T.: 0.000 min
Response: 231055228
Conc: 750.25 ng/ml

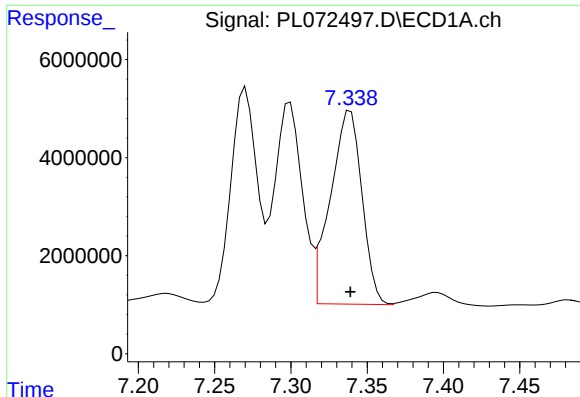

#26 Chlordane-4


R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 56690290
Conc: 752.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

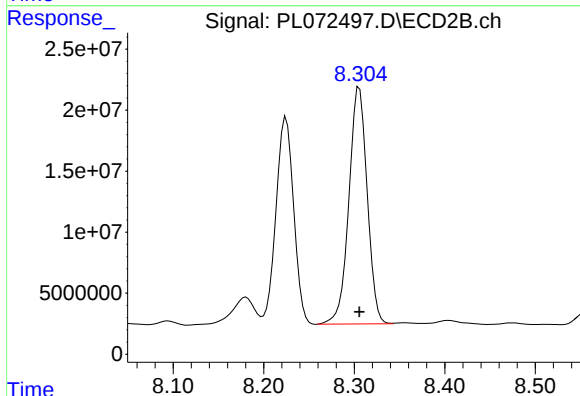


#26 Chlordane-4

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 272707430
Conc: 749.95 ng/ml

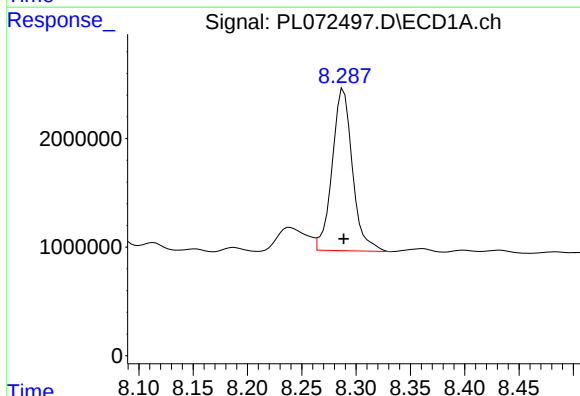


#27 Chlordane-5

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 19385394
Conc: 753.81 ng/ml

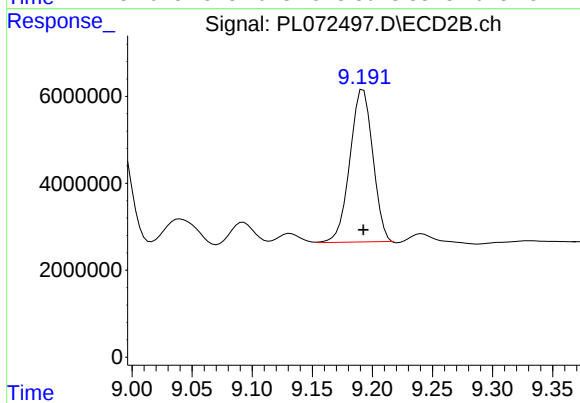

#27 Chlordane-5


R.T.: 9.192 min
Delta R.T.: 0.000 min
Response: 46692561
Conc: 752.94 ng/ml

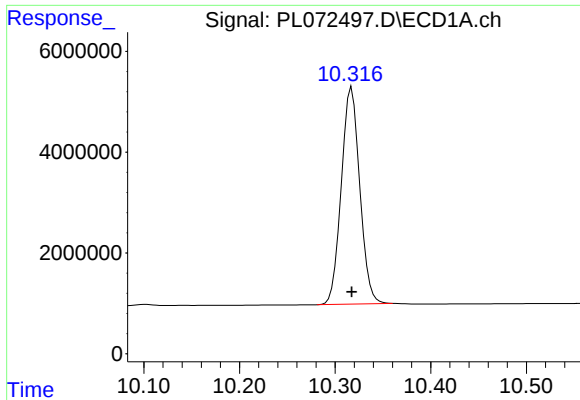

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: 0.000 min
Response: 57885762
Conc: 75.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

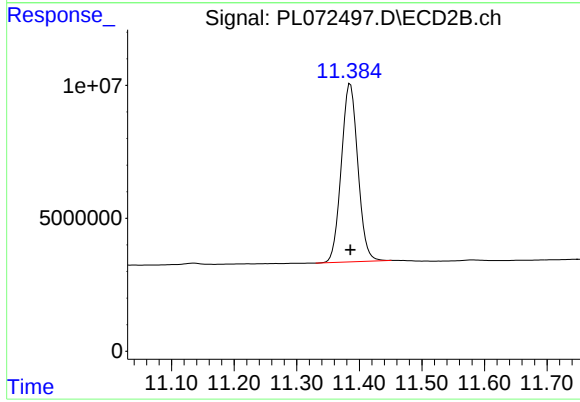

#28 Decachlorobiphenyl

R.T.: 11.386 min
Delta R.T.: 0.000 min
Response: 123647763
Conc: 76.04 ng/ml