

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020722\
 Data File : PL072507.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2022 00:54
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL020722CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 01:12:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 01:10:06 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.557	5.493	25982404	90547795	49.779	50.623
28)	SA Decachlor...	10.318	11.387	39429176	83891774	49.829	50.699
Target Compounds							
23)	Chlordane-1	5.882	6.875	9631069	36889024	520.410	513.240
24)	Chlordane-2	6.571	7.468	12975673	39138554	513.149	508.220
25)	Chlordane-3	7.271	8.225	35259839	156.5E6	523.136	523.793
26)	Chlordane-4	7.339	8.306	37956548	186.0E6	517.289	521.264
27)	Chlordane-5	8.289	9.193	13123974	30697727	511.547	505.774



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020722\
Data File : PL072507.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2022 00:54
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL020722CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 01:12:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 01:10:06 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

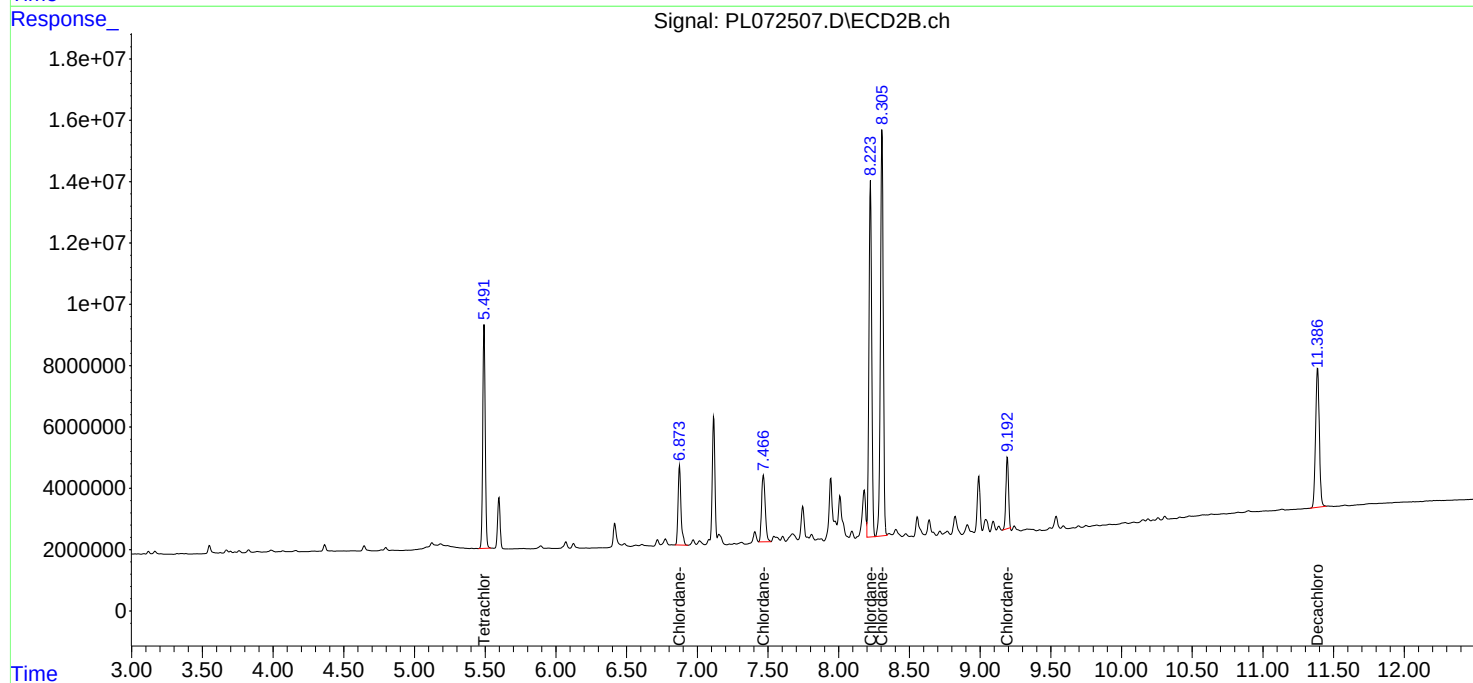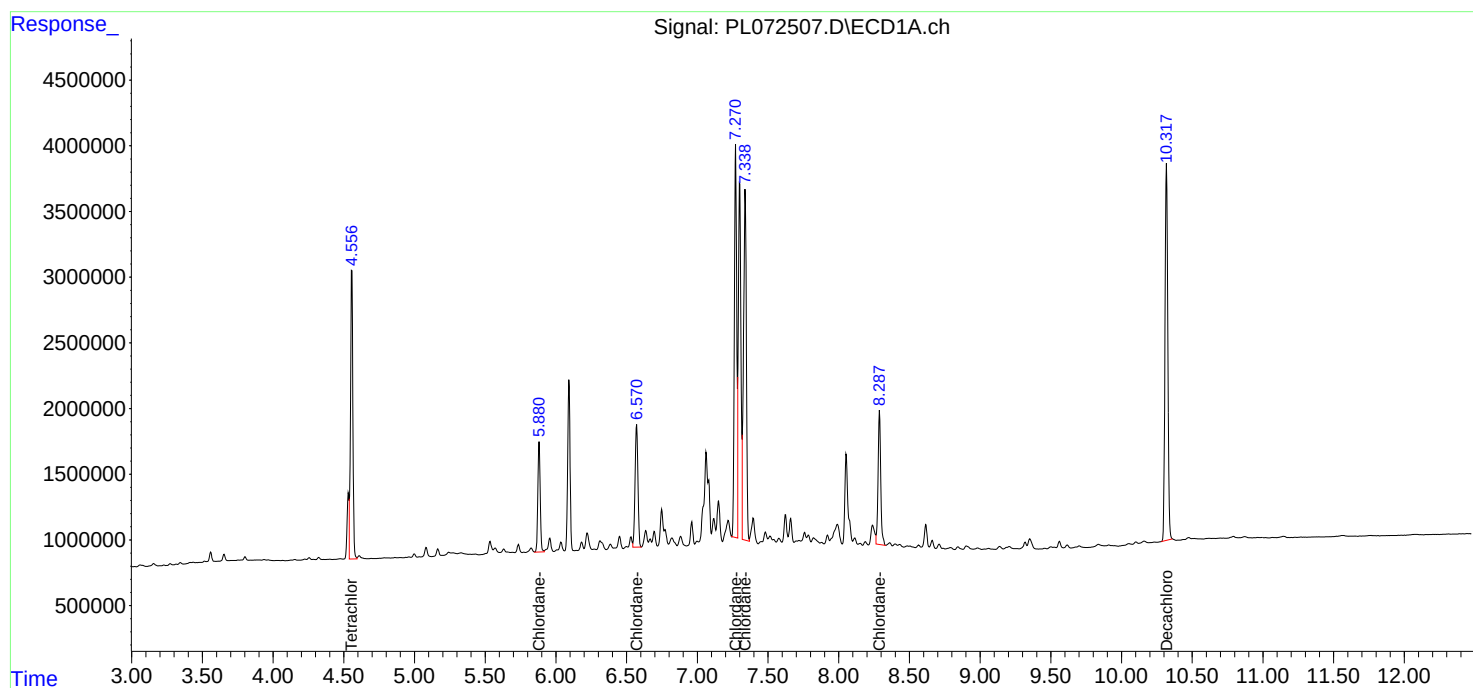


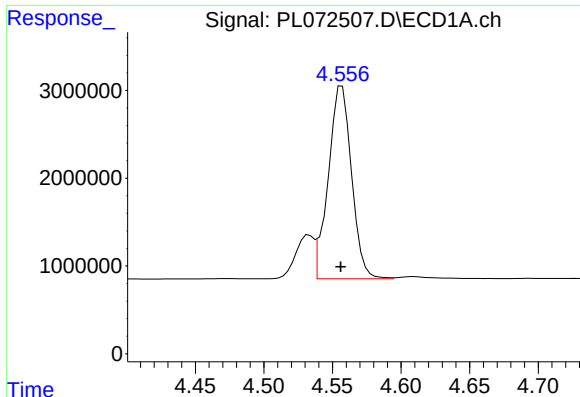

#1 Tetrachloro-m-xylene


R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 25982404
Conc: 49.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020722CHLOR

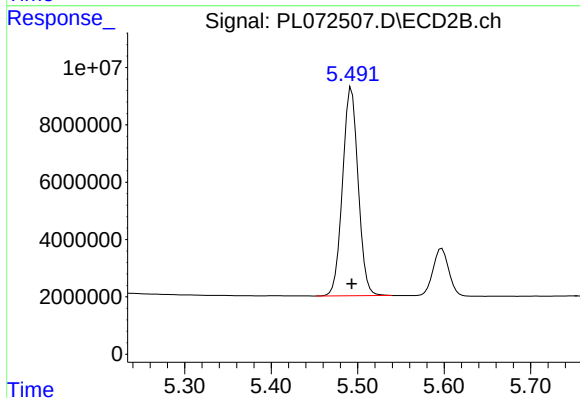


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 90547795
Conc: 50.62 ng/ml

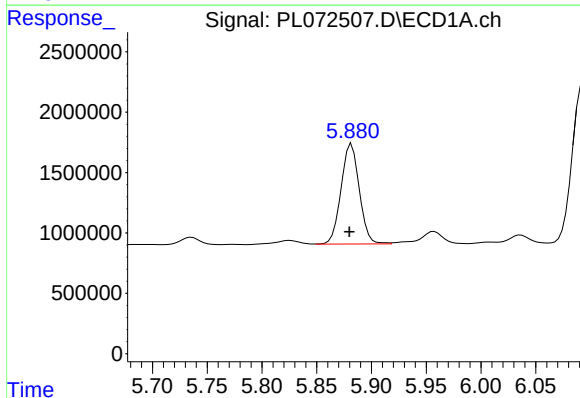


#23 Chlordane-1

R.T.: 5.882 min
Delta R.T.: 0.002 min
Response: 9631069
Conc: 520.41 ng/ml

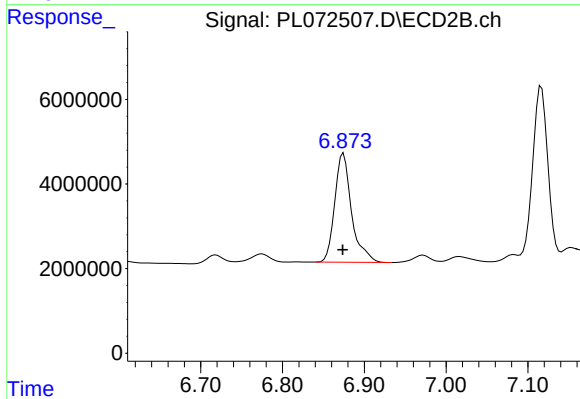

#23 Chlordane-1


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 36889024
Conc: 513.24 ng/ml

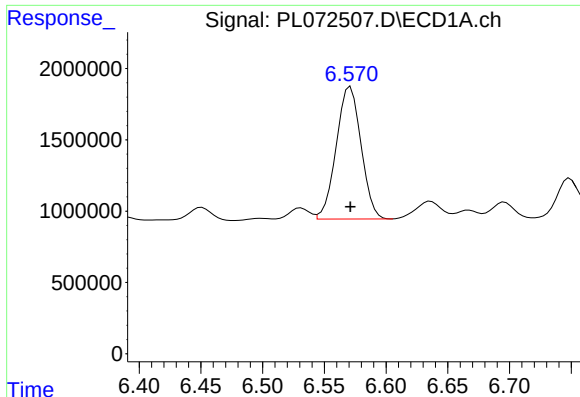

#24 Chlordane-2


R.T.: 6.571 min
Delta R.T.: 0.000 min
Response: 12975673
Conc: 513.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020722CHLOR

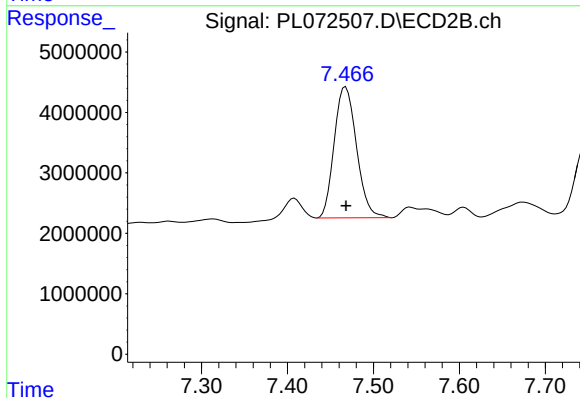


#24 Chlordane-2

R.T.: 7.468 min
Delta R.T.: 0.000 min
Response: 39138554
Conc: 508.22 ng/ml

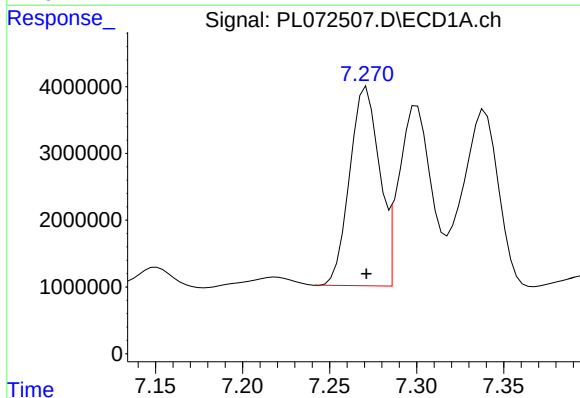


#25 Chlordane-3

R.T.: 7.271 min
Delta R.T.: 0.000 min
Response: 35259839
Conc: 523.14 ng/ml

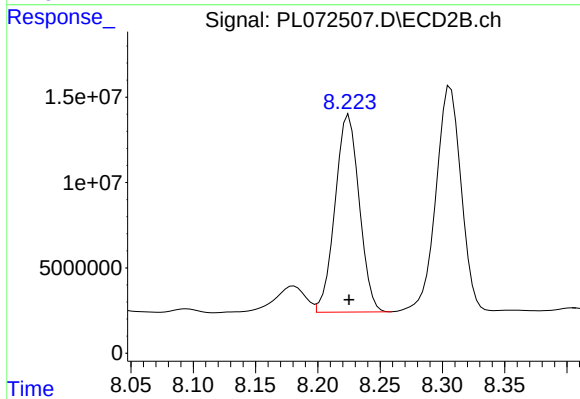

#25 Chlordane-3


R.T.: 8.225 min
Delta R.T.: 0.000 min
Response: 156529404
Conc: 523.79 ng/ml

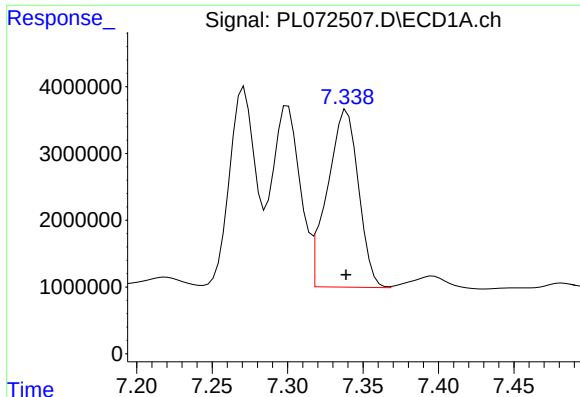

#26 Chlordane-4


R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 37956548
Conc: 517.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020722CHLOR

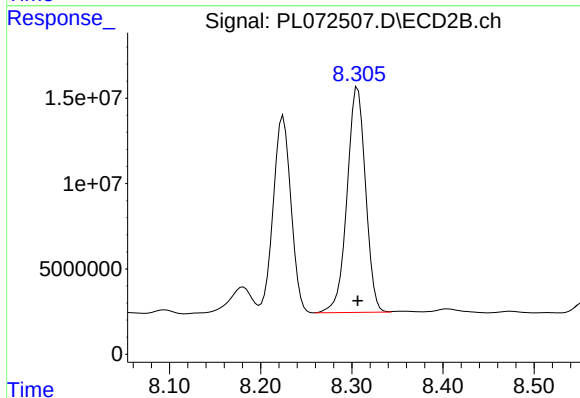


#26 Chlordane-4

R.T.: 8.306 min
Delta R.T.: 0.000 min
Response: 185984773
Conc: 521.26 ng/ml

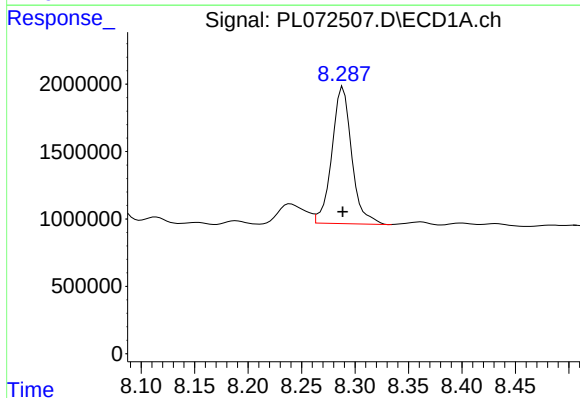


#27 Chlordane-5

R.T.: 8.289 min
Delta R.T.: 0.000 min
Response: 13123974
Conc: 511.55 ng/ml

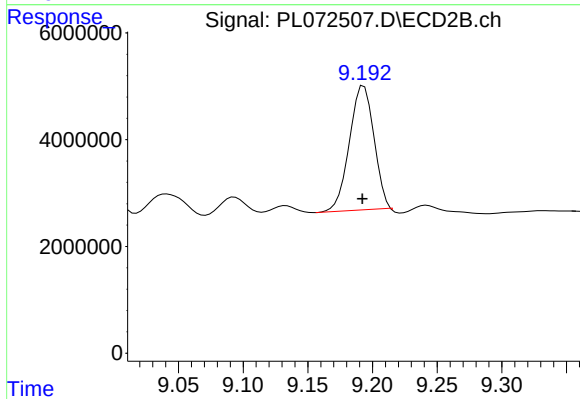

#27 Chlordane-5


R.T.: 9.193 min
Delta R.T.: 0.001 min
Response: 30697727
Conc: 505.77 ng/ml

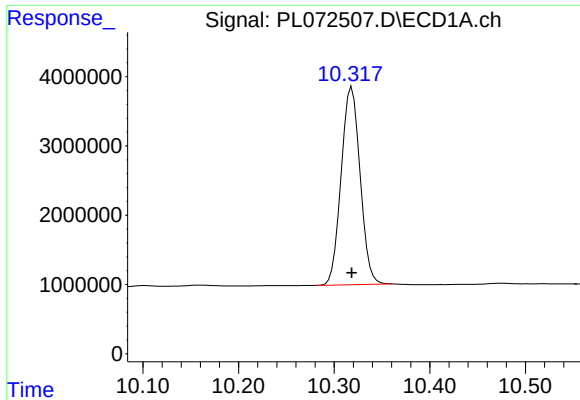

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.000 min
Response: 39429176
Conc: 49.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020722CHLOR

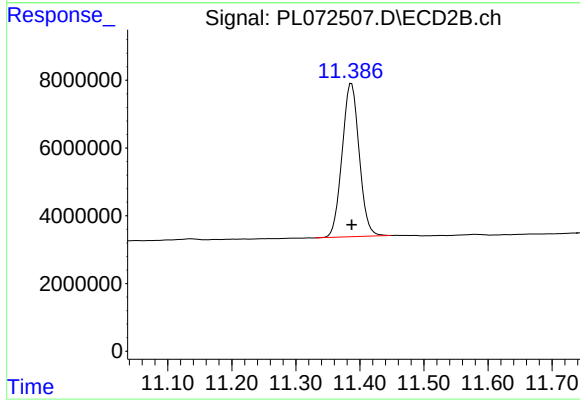

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: 0.000 min
Response: 83891774
Conc: 50.70 ng/ml