

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
 Data File : PL064669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2021 18:58
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 02:55:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 02:54:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.103	249.2E6	169.3E6	79.484	77.317
28)	SA Decachlor...	8.149	9.260	171.3E6	144.6E6	74.408	75.480
Target Compounds							
23)	Chlordane-1	4.287	5.116	80596549	63370944	799.164	743.035
24)	Chlordane-2	4.784	5.592	86076354	63541235	737.822	754.851
25)	Chlordane-3	5.349	6.249	245.9E6	229.0E6	771.712	779.293
26)	Chlordane-4	5.406	6.322	205.2E6	274.5E6	784.484	771.183
27)	Chlordane-5	6.234	7.141	75925403	44482445	771.274	789.156


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
Data File : PL064669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2021 18:58
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 02:55:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 02:54:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

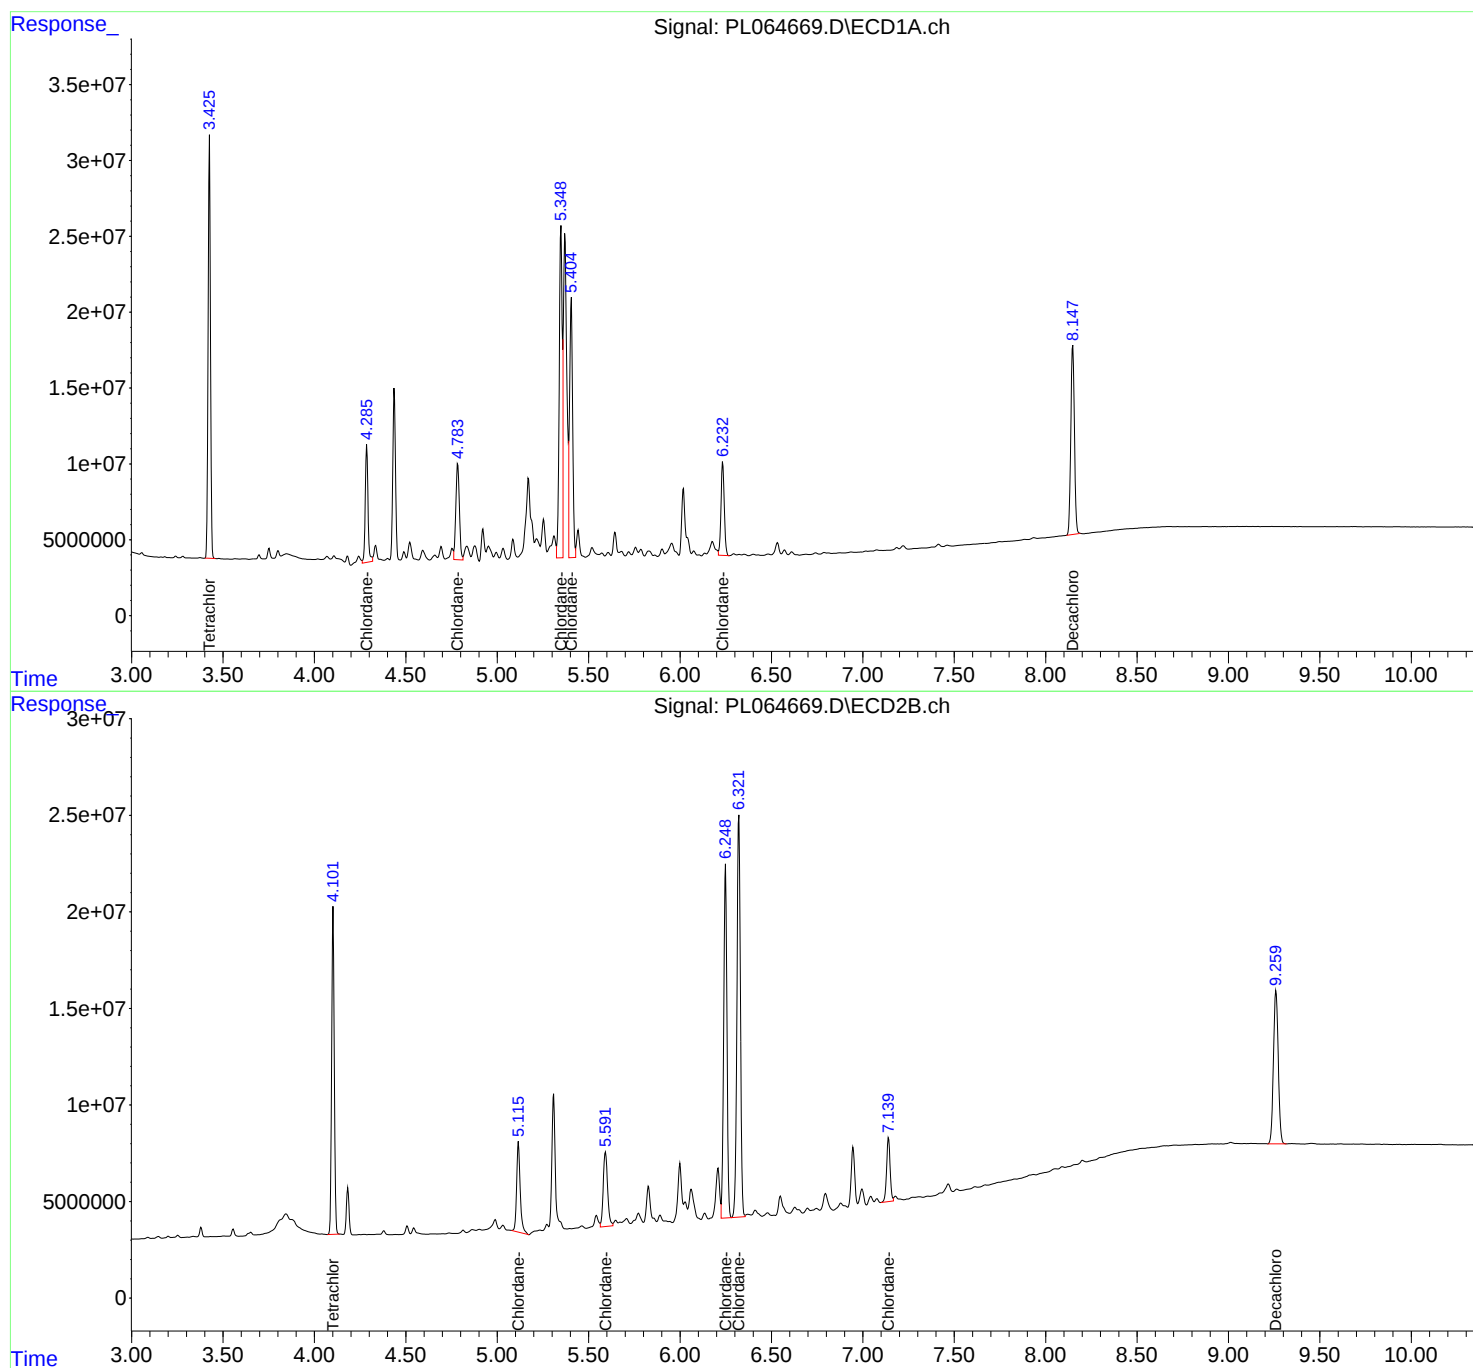


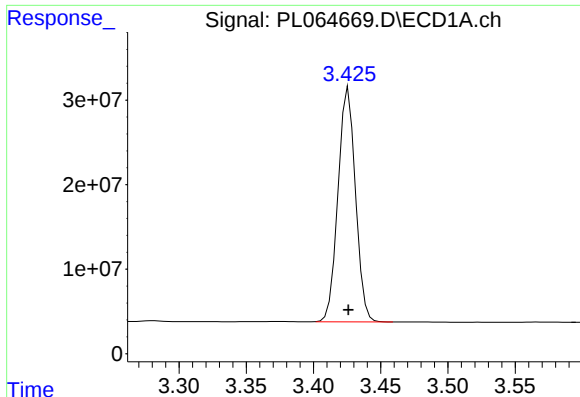

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 249175800
Conc: 79.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

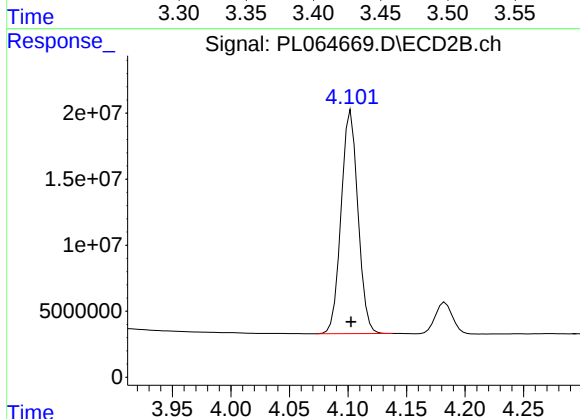


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 169294713
Conc: 77.32 ng/ml

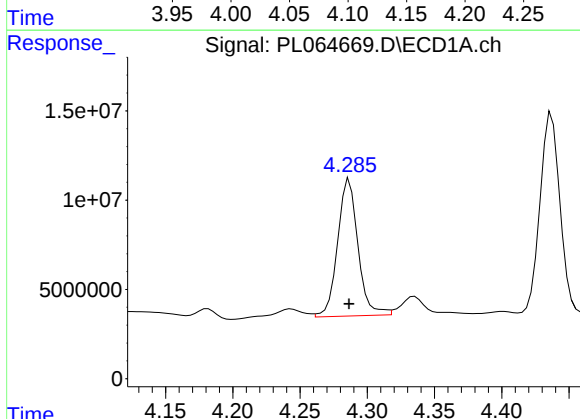


#23 Chlordane-1

R.T.: 4.287 min
Delta R.T.: 0.000 min
Response: 80596549
Conc: 799.16 ng/ml

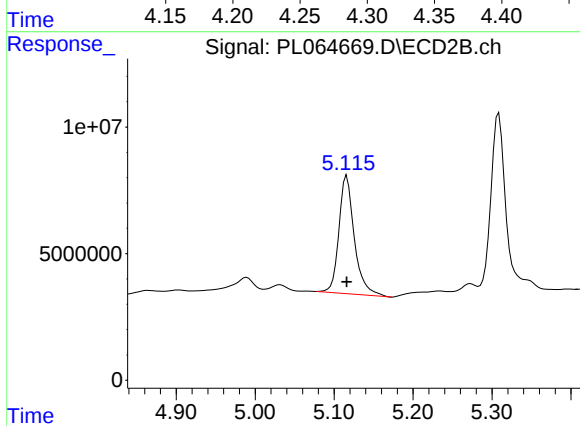

#23 Chlordane-1


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 63370944
Conc: 743.04 ng/ml

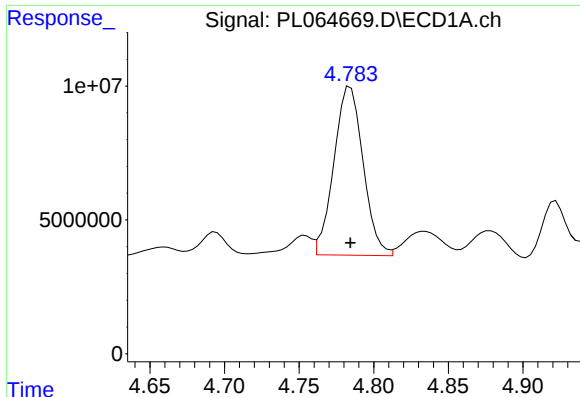

#24 Chlordane-2


R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 86076354
Conc: 737.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

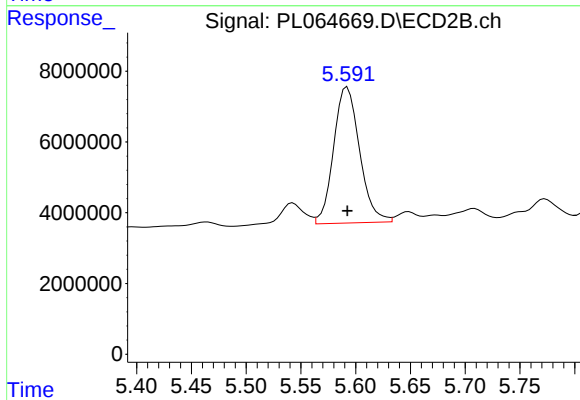


#24 Chlordane-2

R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 63541235
Conc: 754.85 ng/ml

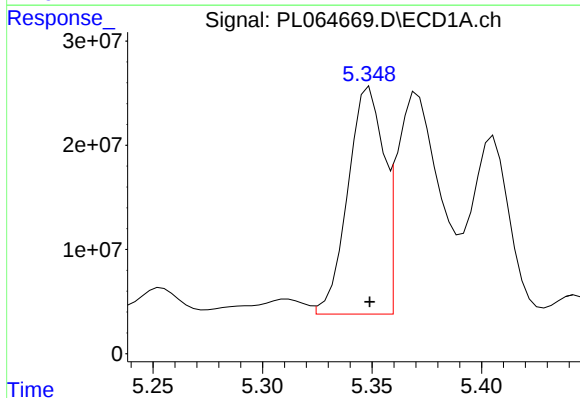


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 245934782
Conc: 771.71 ng/ml

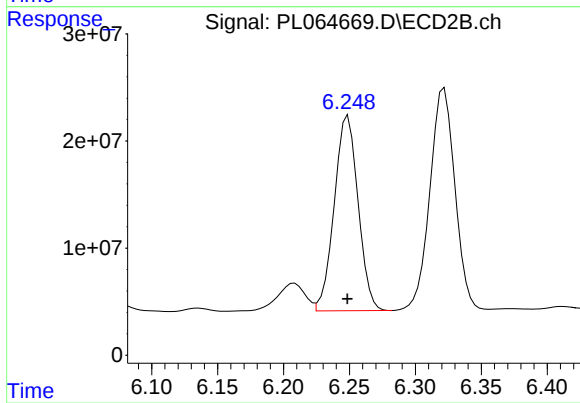

#25 Chlordane-3


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 228998199
Conc: 779.29 ng/ml

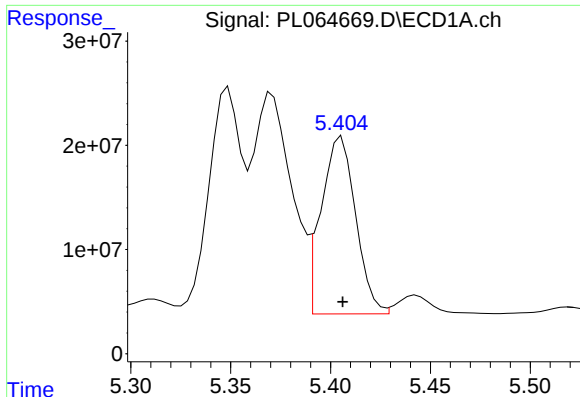

#26 Chlordane-4


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 205245966
Conc: 784.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

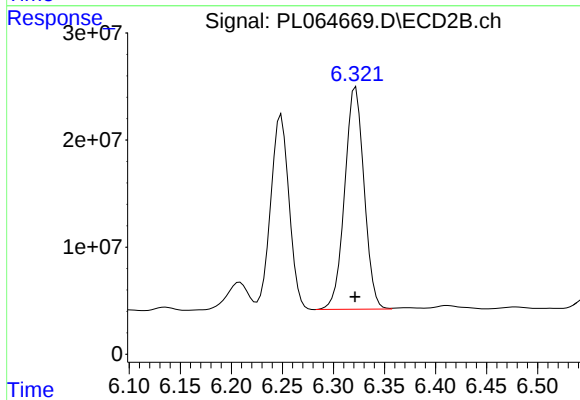


#26 Chlordane-4

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 274489121
Conc: 771.18 ng/ml

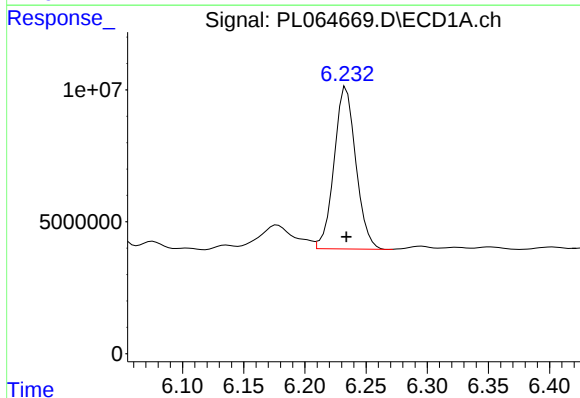


#27 Chlordane-5

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 75925403
Conc: 771.27 ng/ml

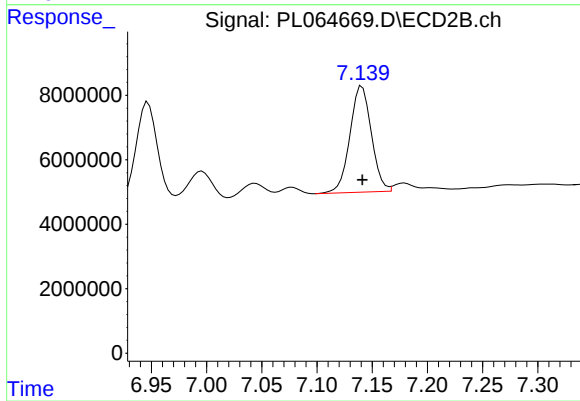

#27 Chlordane-5


R.T.: 7.141 min
Delta R.T.: 0.000 min
Response: 44482445
Conc: 789.16 ng/ml

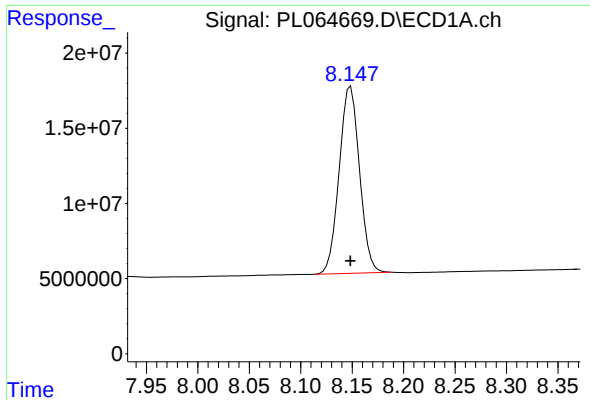

#28 Decachlorobiphenyl

R.T.: 8.149 min
Delta R.T.: 0.000 min
Response: 171347395
Conc: 74.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

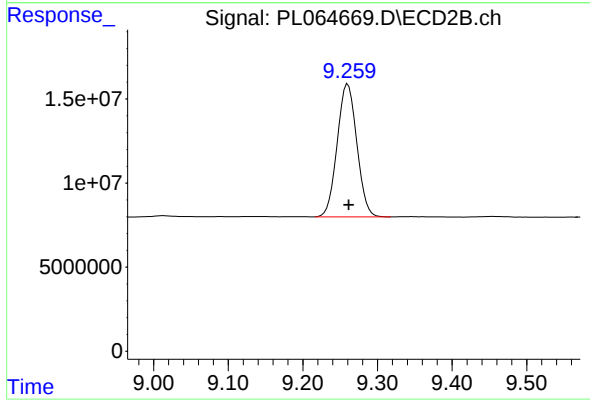

#28 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: 0.000 min
Response: 144620666
Conc: 75.48 ng/ml