

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
 Data File : PL064670.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2021 19:12
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 02:56:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 02:54:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.103	156.7E6	109.5E6	50.000	50.000
28)	SA Decachlor...	8.148	9.261	115.1E6	95800236	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.286	5.116	50425538	42643283	500.000	500.000
24)	Chlordane-2	4.784	5.593	58331354	42088594	500.000	500.000
25)	Chlordane-3	5.349	6.248	159.3E6	146.9E6	500.000	500.000
26)	Chlordane-4	5.406	6.321	130.8E6	178.0E6	500.000	500.000
27)	Chlordane-5	6.234	7.141	49220799	28183557	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
Data File : PL064670.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2021 19:12
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 02:56:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 02:54:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

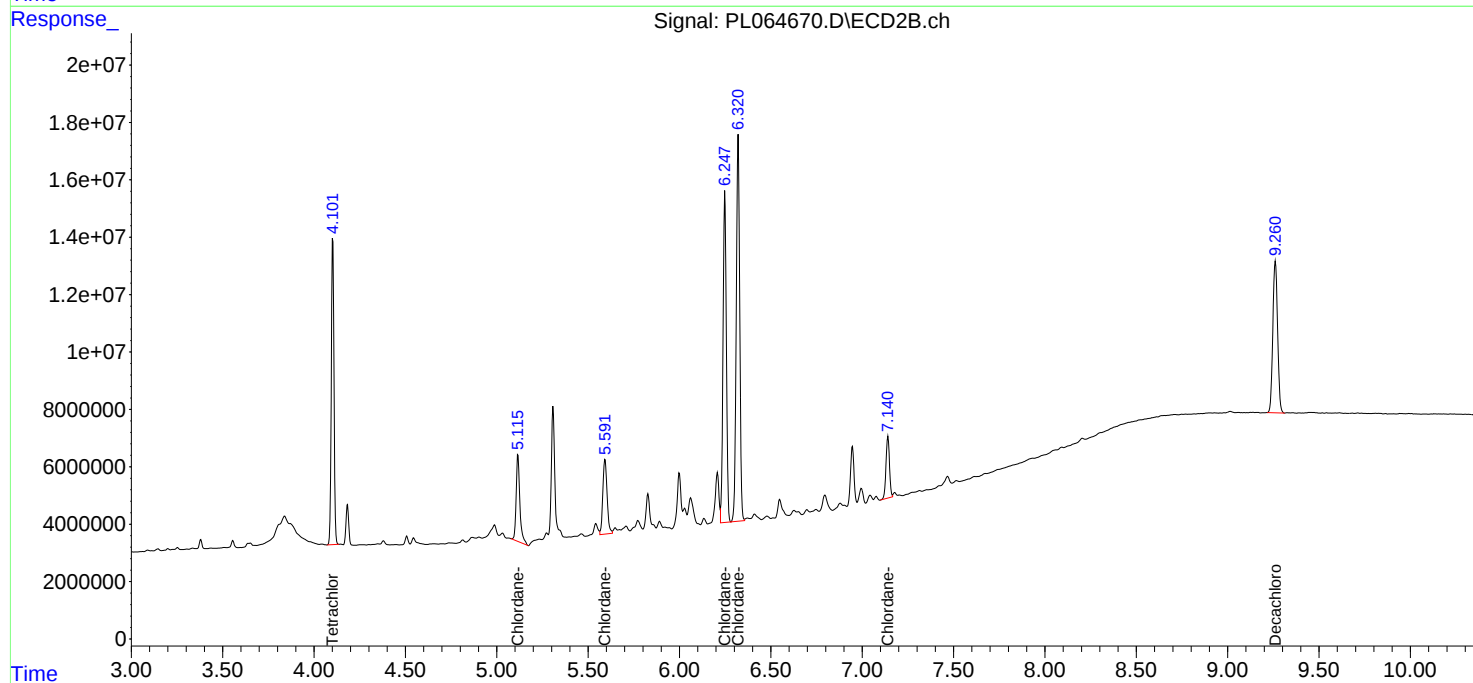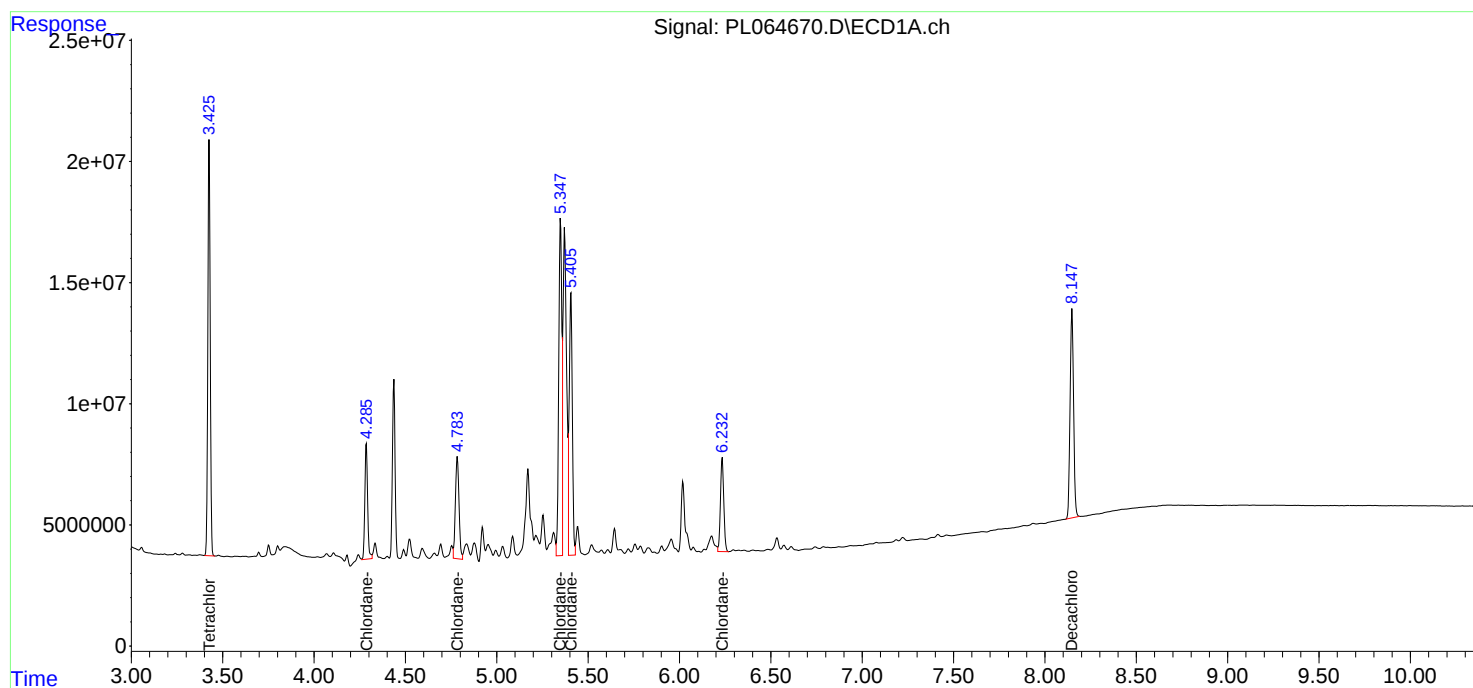


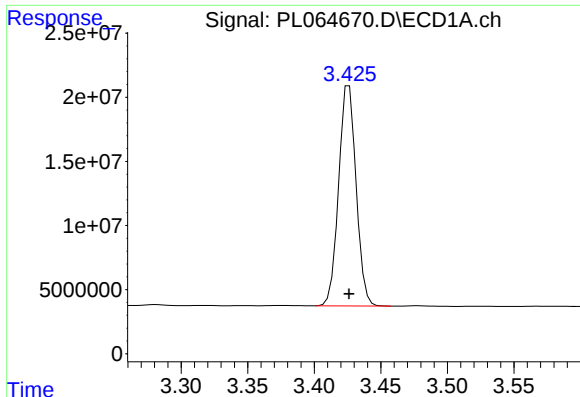

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 156745764
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

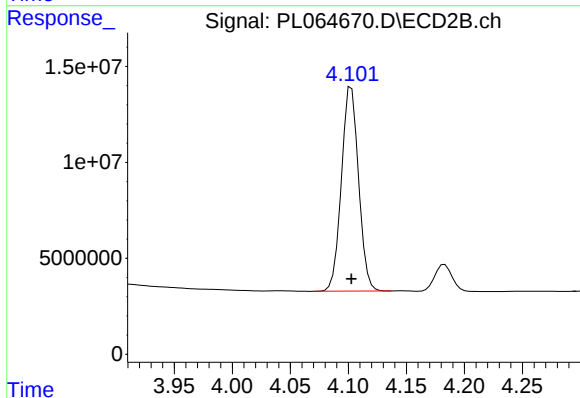


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 109480749
Conc: 50.00 ng/ml

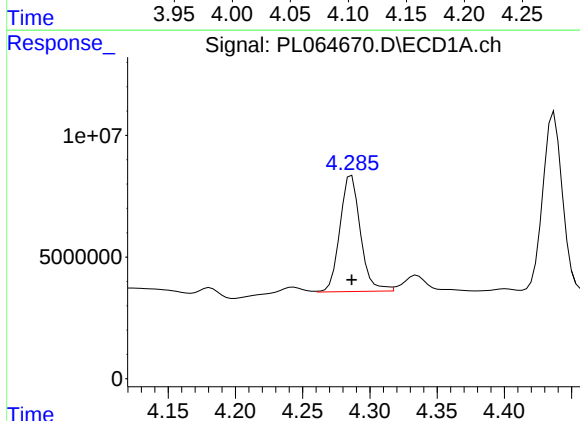


#23 Chlordane-1

R.T.: 4.286 min
Delta R.T.: 0.000 min
Response: 50425538
Conc: 500.00 ng/ml

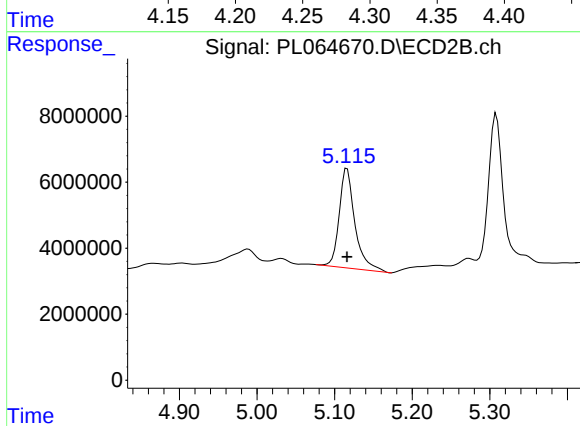

#23 Chlordane-1


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 42643283
Conc: 500.00 ng/ml

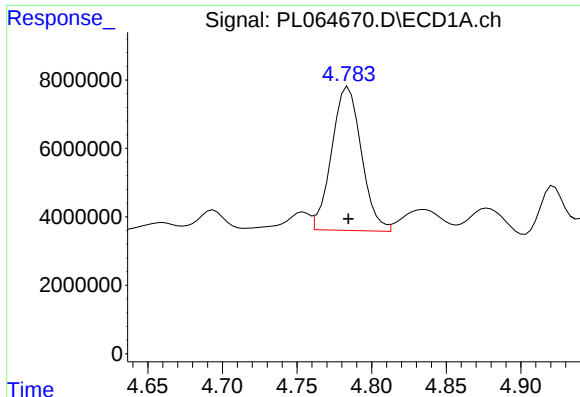

#24 Chlordane-2


R.T.: 4.784 min
Delta R.T.: 0.000 min
Response: 58331354
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

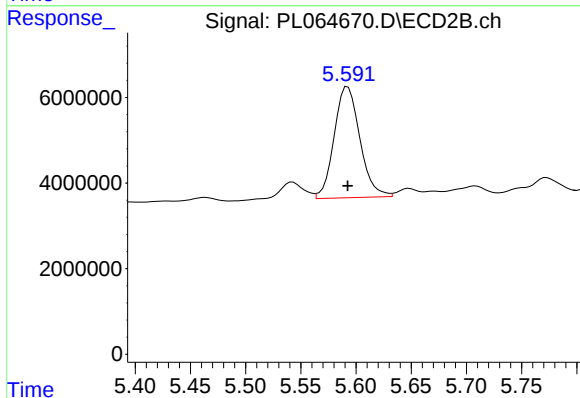


#24 Chlordane-2

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 42088594
Conc: 500.00 ng/ml

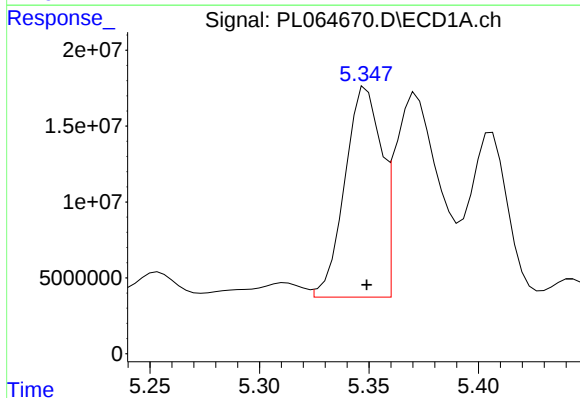


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 159343657
Conc: 500.00 ng/ml

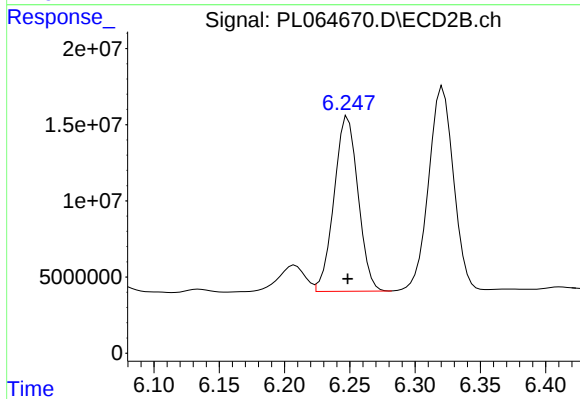

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 146926964
Conc: 500.00 ng/ml

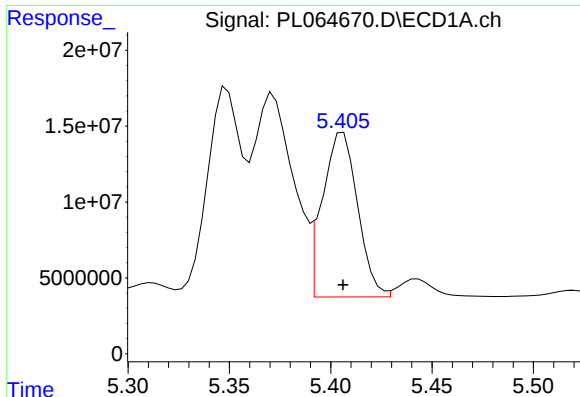

#26 Chlordane-4


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 130815866
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

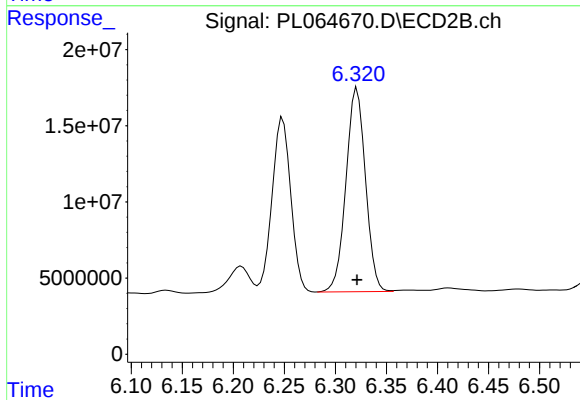


#26 Chlordane-4

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 177966282
Conc: 500.00 ng/ml

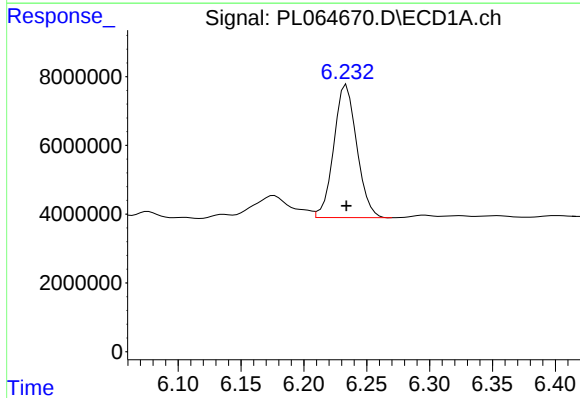


#27 Chlordane-5

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 49220799
Conc: 500.00 ng/ml

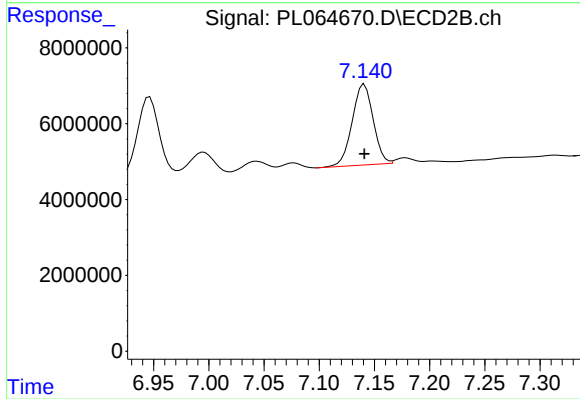

#27 Chlordane-5


R.T.: 7.141 min
Delta R.T.: 0.000 min
Response: 28183557
Conc: 500.00 ng/ml

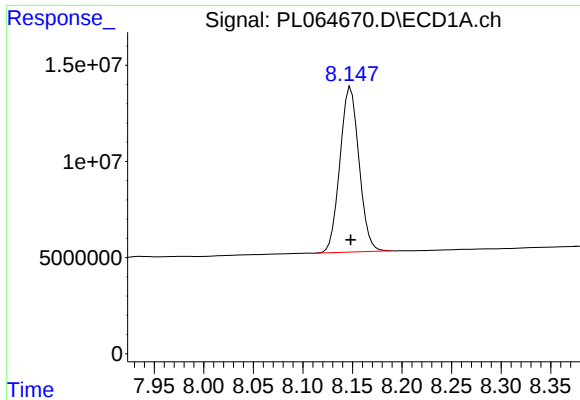

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 115140911
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

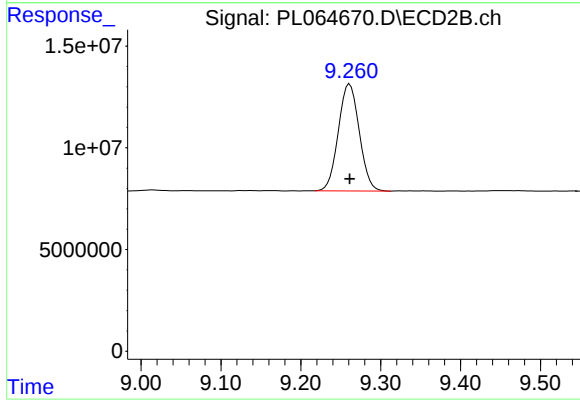

#28 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 95800236
Conc: 50.00 ng/ml