

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
 Data File : PL064668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2021 18:44
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 02:55:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 02:54:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.103	327.9E6	218.1E6	104.594	99.588
28)	SA Decachlor...	8.147	9.261	223.1E6	183.9E6	96.881	95.962
Target Compounds							
23)	Chlordane-1	4.287	5.116	103.2E6	84872420	1023.340	995.144
24)	Chlordane-2	4.785	5.593	111.1E6	81133343	951.941	963.840
25)	Chlordane-3	5.348	6.249	319.7E6	300.2E6	1003.328	1021.668
26)	Chlordane-4	5.405	6.322	271.5E6	358.5E6	1037.687	1007.280
27)	Chlordane-5	6.234	7.141	100.3E6	56887834	1018.488	1009.238



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
Data File : PL064668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2021 18:44
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 02:55:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 02:54:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

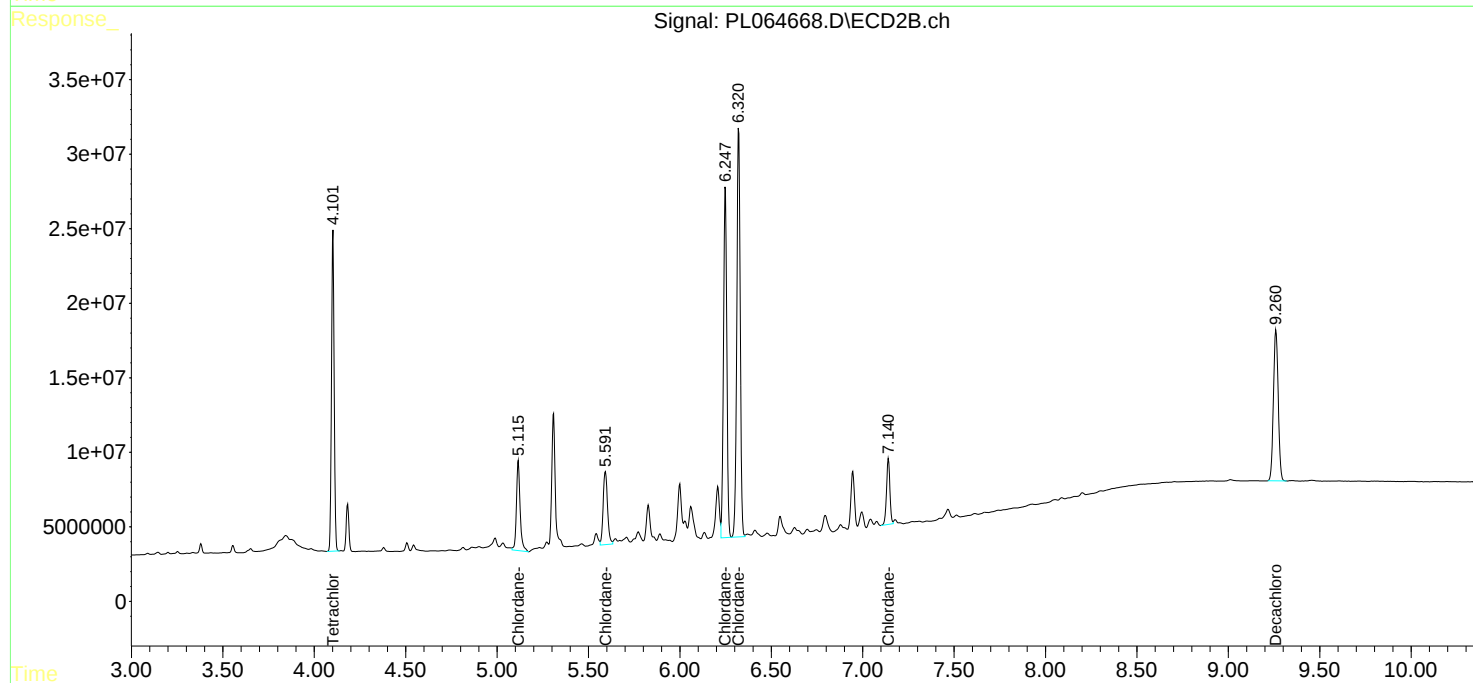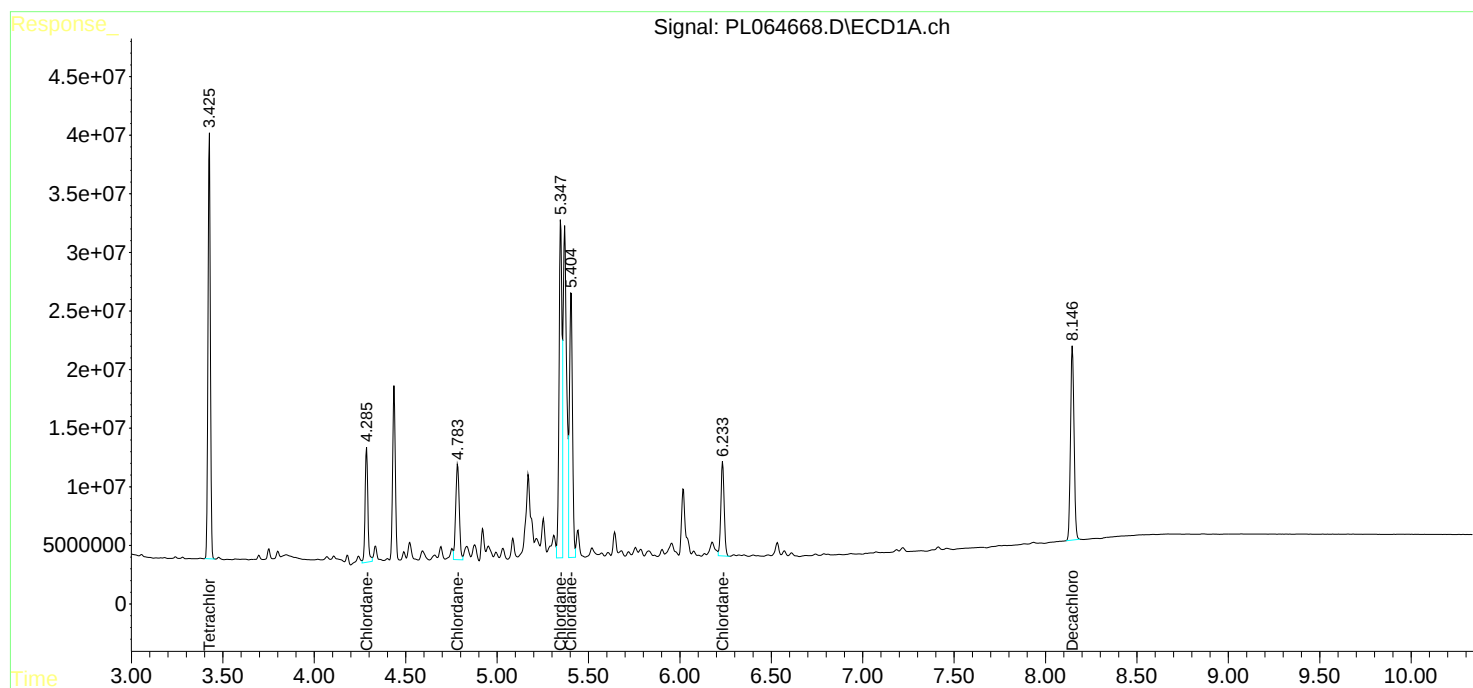


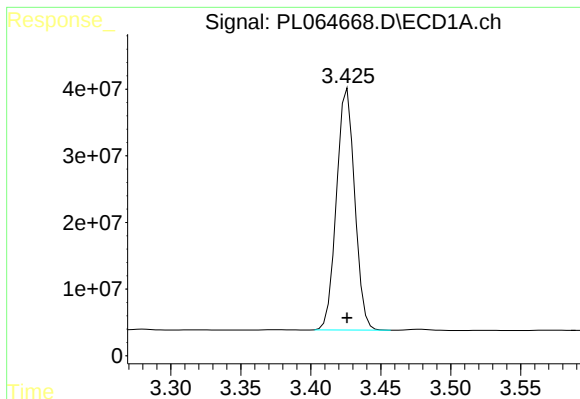

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 327894166
Conc: 104.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

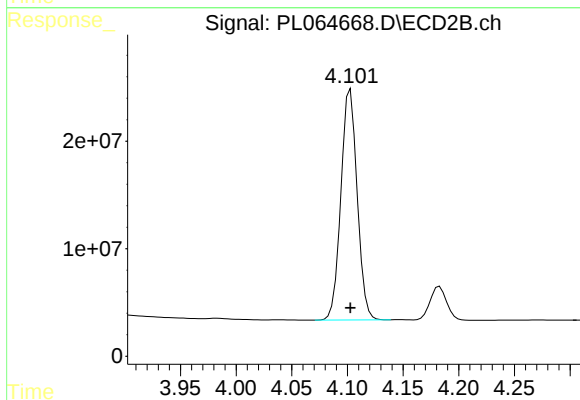


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: 0.000 min
Response: 218059339
Conc: 99.59 ng/ml

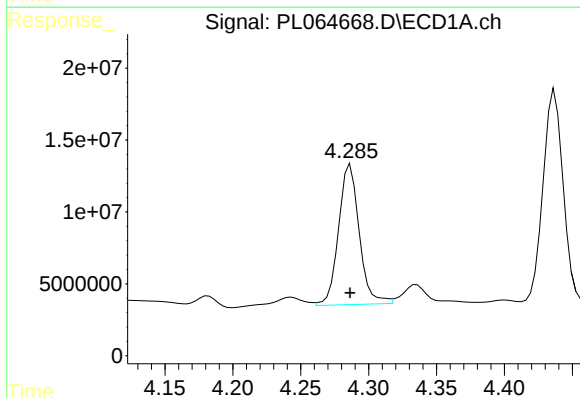


#23 Chlordane-1

R.T.: 4.287 min
Delta R.T.: 0.000 min
Response: 103204985
Conc: 1023.34 ng/ml

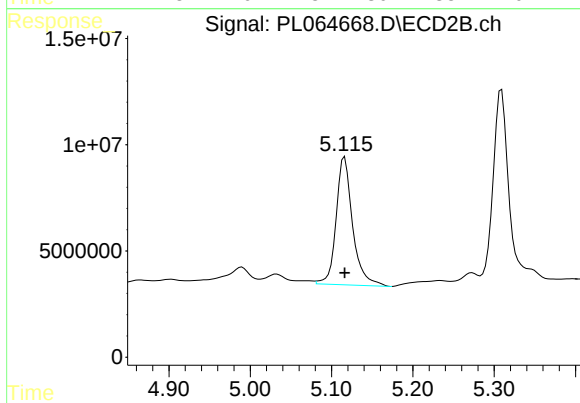

#23 Chlordane-1


R.T.: 5.116 min
Delta R.T.: 0.000 min
Response: 84872420
Conc: 995.14 ng/ml

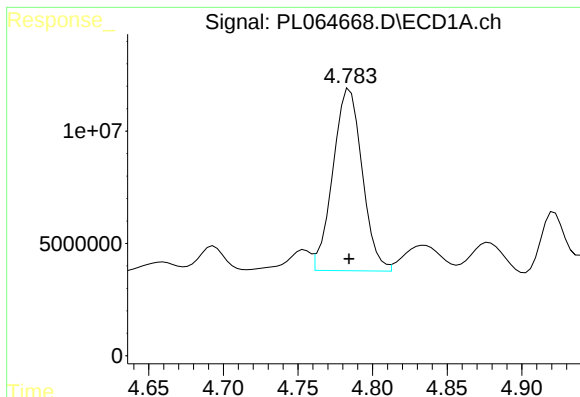

#24 Chlordane-2


R.T.: 4.785 min
Delta R.T.: 0.000 min
Response: 111056011
Conc: 951.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

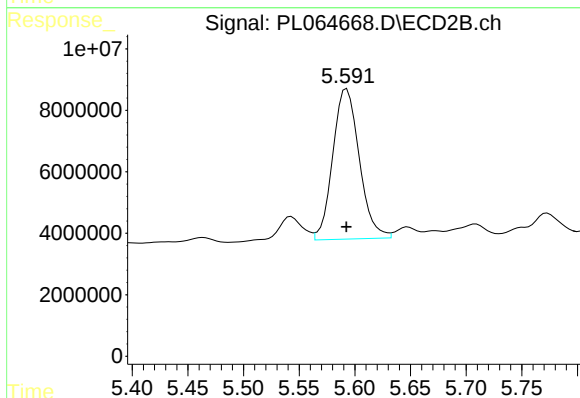


#24 Chlordane-2

R.T.: 5.593 min
Delta R.T.: 0.000 min
Response: 81133343
Conc: 963.84 ng/ml

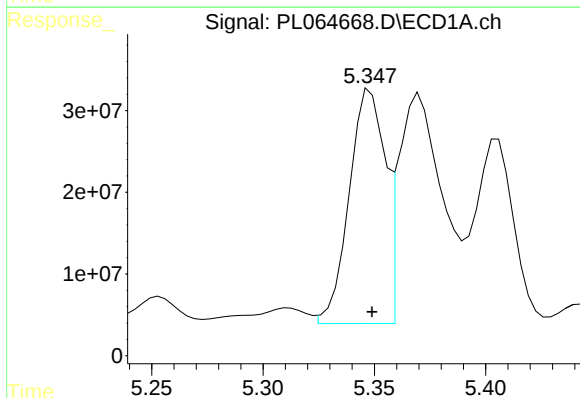


#25 Chlordane-3

R.T.: 5.348 min
Delta R.T.: 0.000 min
Response: 319748056
Conc: 1003.33 ng/ml

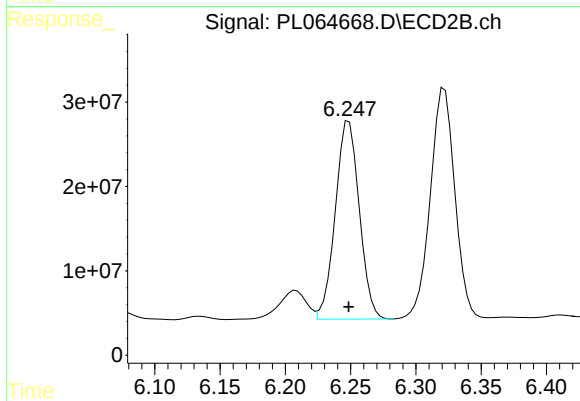

#25 Chlordane-3


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 300221100
Conc: 1021.67 ng/ml

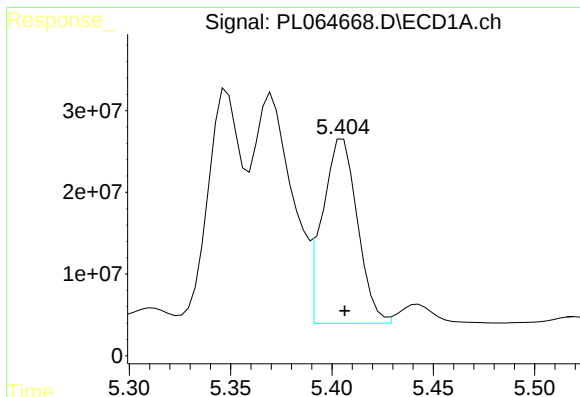

#26 Chlordane-4


R.T.: 5.405 min
Delta R.T.: 0.000 min
Response: 271491735
Conc: 1037.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

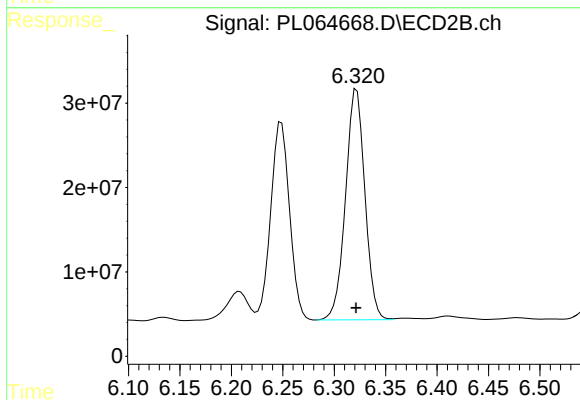


#26 Chlordane-4

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 358523629
Conc: 1007.28 ng/ml

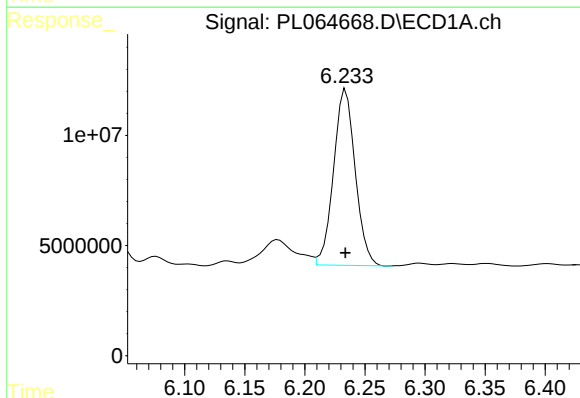


#27 Chlordane-5

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 100261599
Conc: 1018.49 ng/ml

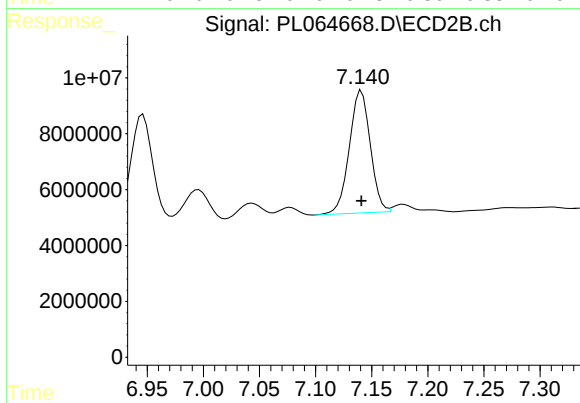

#27 Chlordane-5


R.T.: 7.141 min
Delta R.T.: 0.000 min
Response: 56887834
Conc: 1009.24 ng/ml

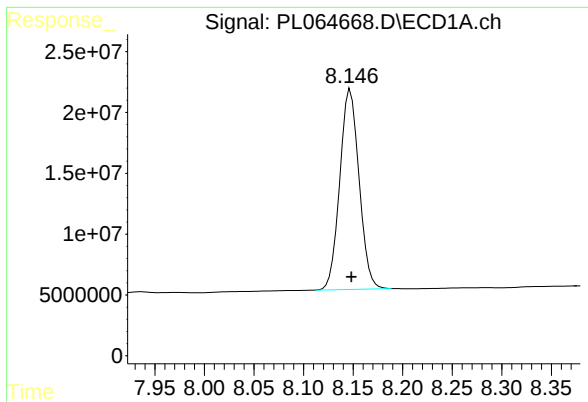

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 223099777
Conc: 96.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

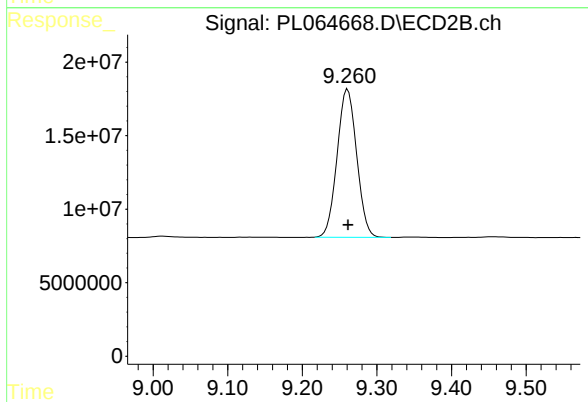

#28 Decachlorobiphenyl

R.T.: 9.261 min
Delta R.T.: 0.000 min
Response: 183863893
Conc: 95.96 ng/ml