

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
 Data File : PL064679.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2021 21:21
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL020821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 05:12:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	4.102	161.4E6	113.0E6	57.363	52.318
28)	SA Decachlor...	8.147	9.260	116.4E6	95765880	51.759	50.420
Target Compounds							
23)	Chlordane-1	4.286	5.116	55496576	43571751	488.196	496.103
24)	Chlordane-2	4.784	5.592	58637412	44080342	473.912	505.542
25)	Chlordane-3	5.347	6.248	160.9E6	151.3E6	489.670	494.838
26)	Chlordane-4	5.404	6.321	134.2E6	182.8E6	487.702	493.316
27)	Chlordane-5	6.233	7.141	50250055	26888374	496.647	476.458



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020821\
Data File : PL064679.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2021 21:21
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
ICVPL020821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 05:12:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

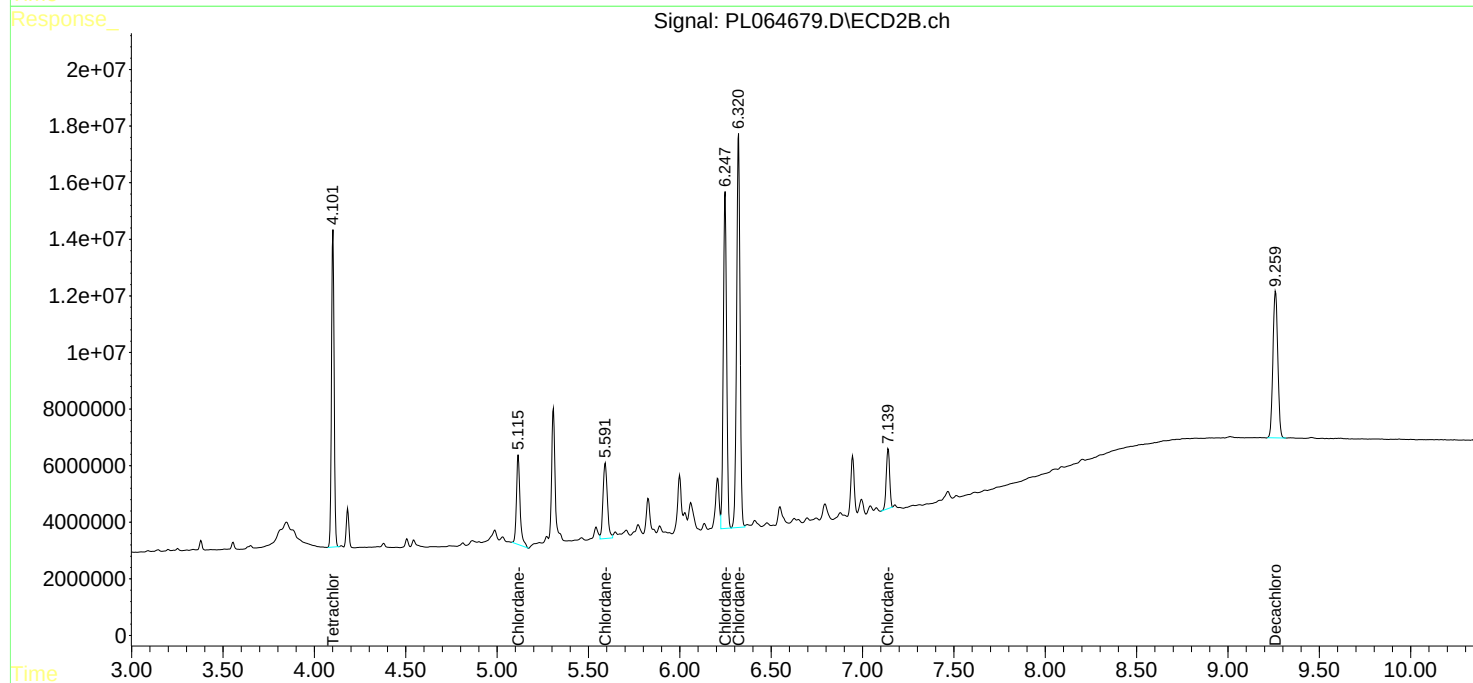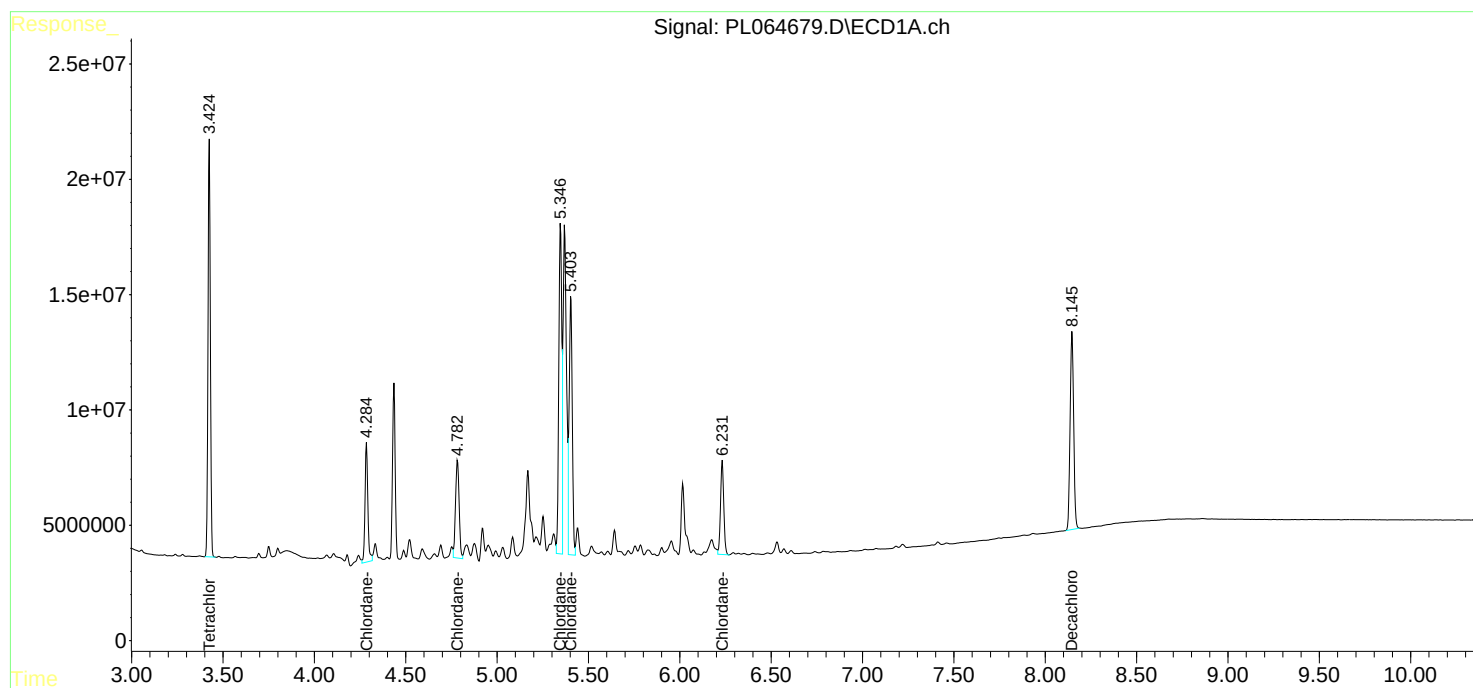


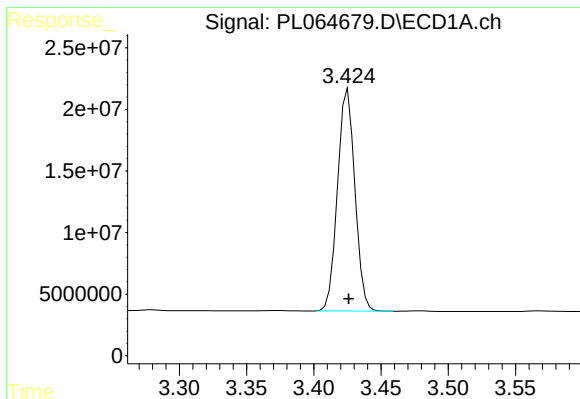

#1 Tetrachloro-m-xylene


R.T.: 3.425 min
Delta R.T.: 0.000 min
Response: 161390996
Conc: 57.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020821

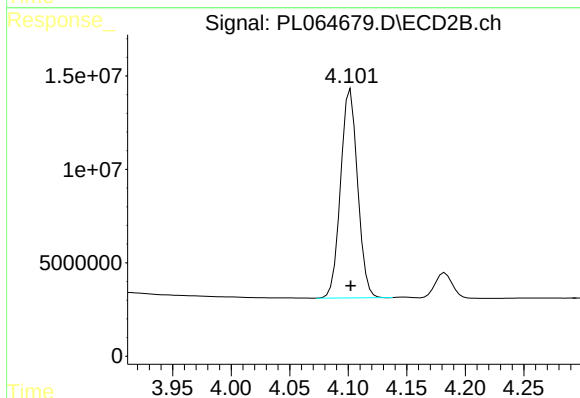


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 113017228
Conc: 52.32 ng/ml

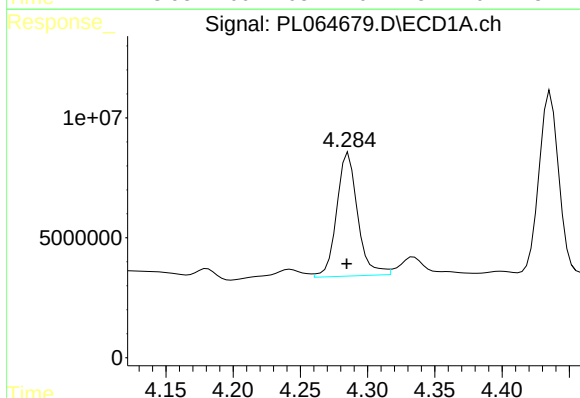


#23 Chlordane-1

R.T.: 4.286 min
Delta R.T.: 0.001 min
Response: 55496576
Conc: 488.20 ng/ml

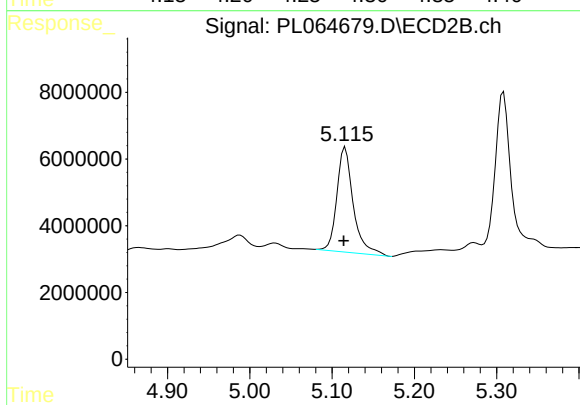

#23 Chlordane-1


R.T.: 5.116 min
Delta R.T.: 0.002 min
Response: 43571751
Conc: 496.10 ng/ml

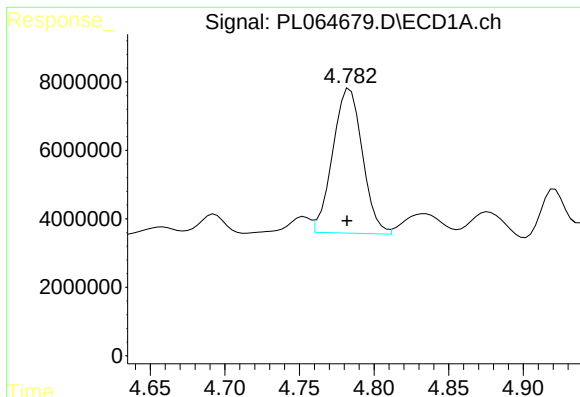

#24 Chlordane-2


R.T.: 4.784 min
Delta R.T.: 0.002 min
Response: 58637412
Conc: 473.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020821

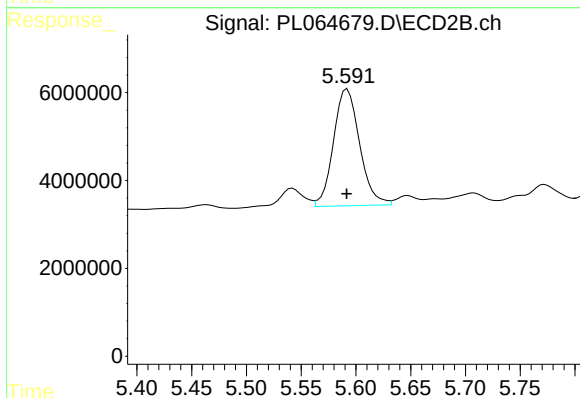


#24 Chlordane-2

R.T.: 5.592 min
Delta R.T.: 0.000 min
Response: 44080342
Conc: 505.54 ng/ml

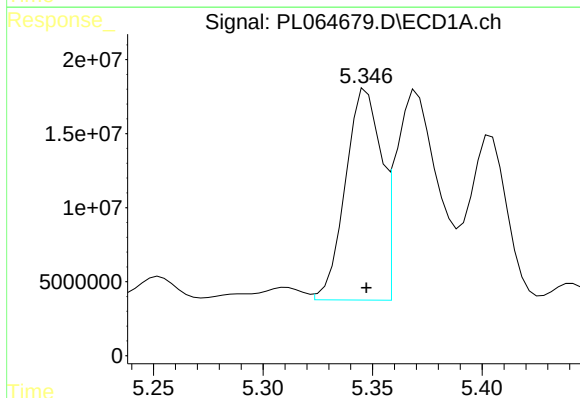


#25 Chlordane-3

R.T.: 5.347 min
Delta R.T.: 0.000 min
Response: 160912743
Conc: 489.67 ng/ml

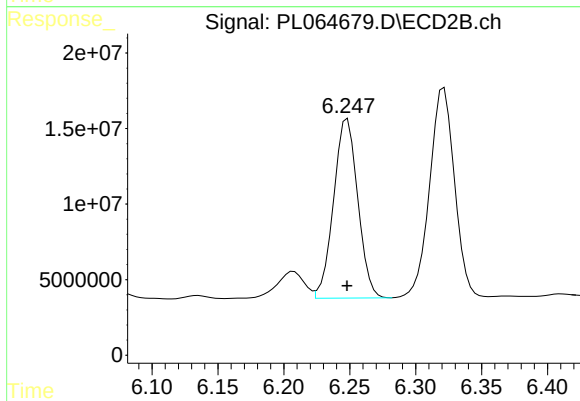

#25 Chlordane-3


R.T.: 6.248 min
Delta R.T.: 0.000 min
Response: 151300935
Conc: 494.84 ng/ml

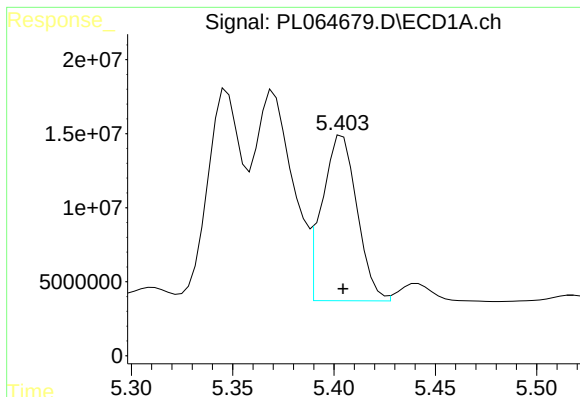

#26 Chlordane-4


R.T.: 5.404 min
Delta R.T.: 0.000 min
Response: 134189016
Conc: 487.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020821

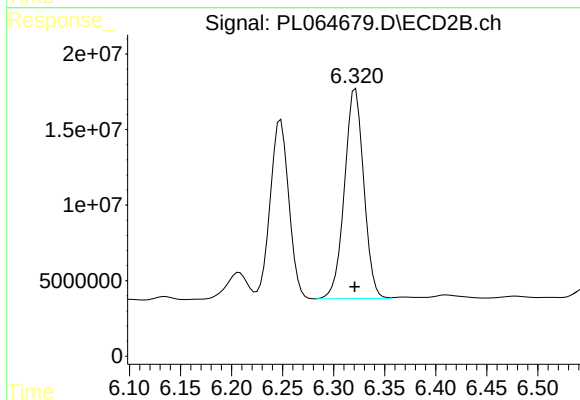


#26 Chlordane-4

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 182762551
Conc: 493.32 ng/ml

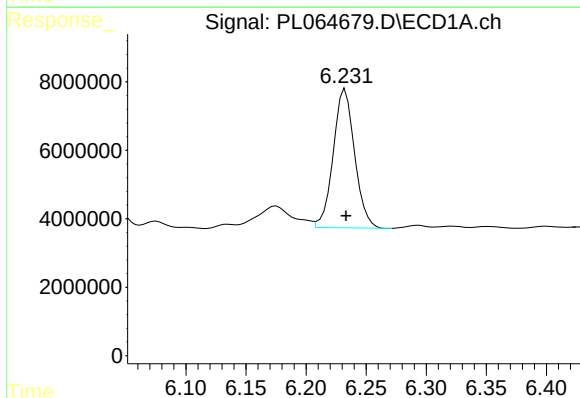


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 50250055
Conc: 496.65 ng/ml

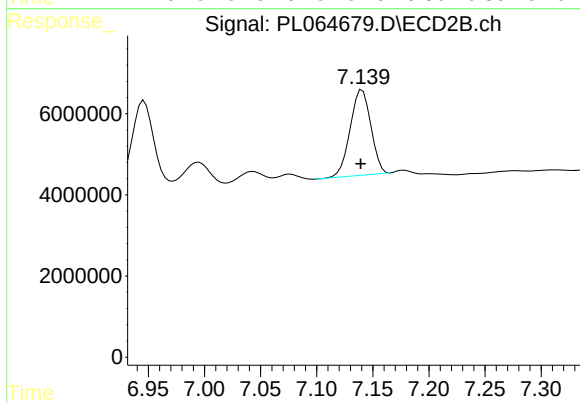

#27 Chlordane-5


R.T.: 7.141 min
Delta R.T.: 0.001 min
Response: 26888374
Conc: 476.46 ng/ml

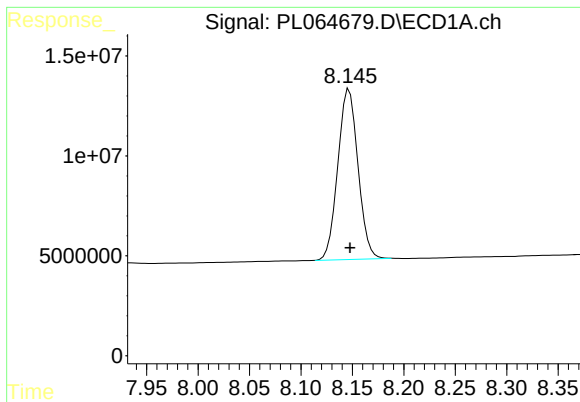

#28 Decachlorobiphenyl

R.T.: 8.147 min
Delta R.T.: 0.000 min
Response: 116395381
Conc: 51.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL020821

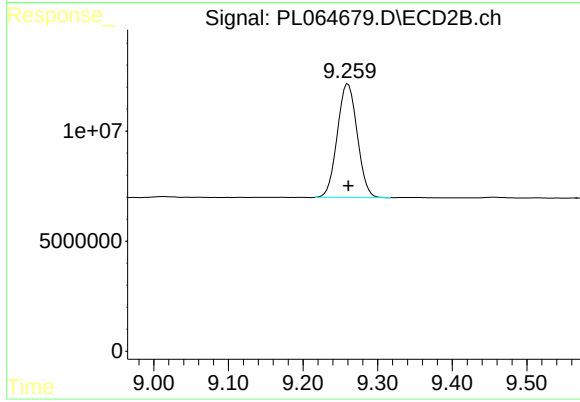

#28 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: 0.000 min
Response: 95765880
Conc: 50.42 ng/ml