

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020822\
 Data File : PL072518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2022 11:18
 Operator : AR\AJ
 Sample : N1397-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 KTS1-MH-01-0-15

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/09/2022
 Supervised By :Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 08 13:34:58 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.557	5.492	7545566	25486968	15.671	14.755
2) SA Decachlor...	10.318	11.385	9705554	21091351	12.820	13.300m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020822\
Data File : PL072518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2022 11:18
Operator : AR\AJ
Sample : N1397-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
KTS1-MH-01-0-15


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/09/2022
Supervised By : Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 08 13:34:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

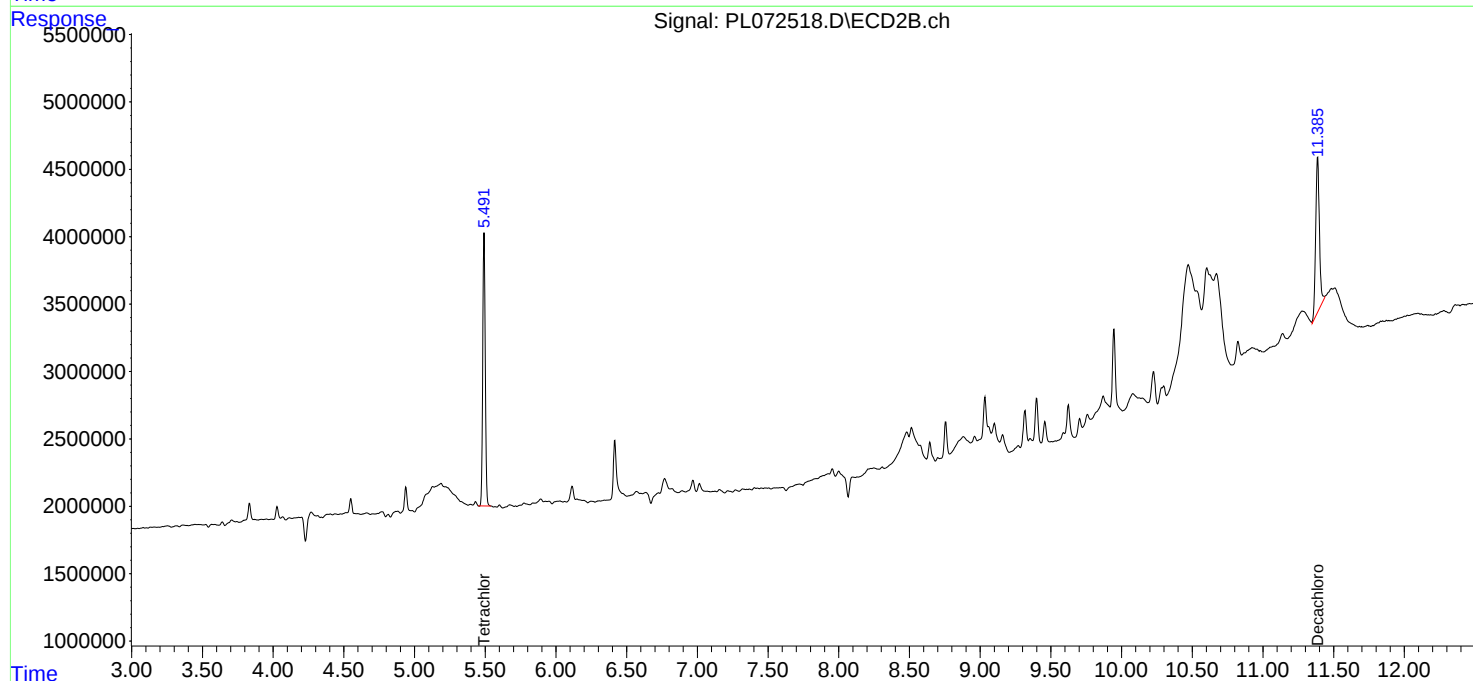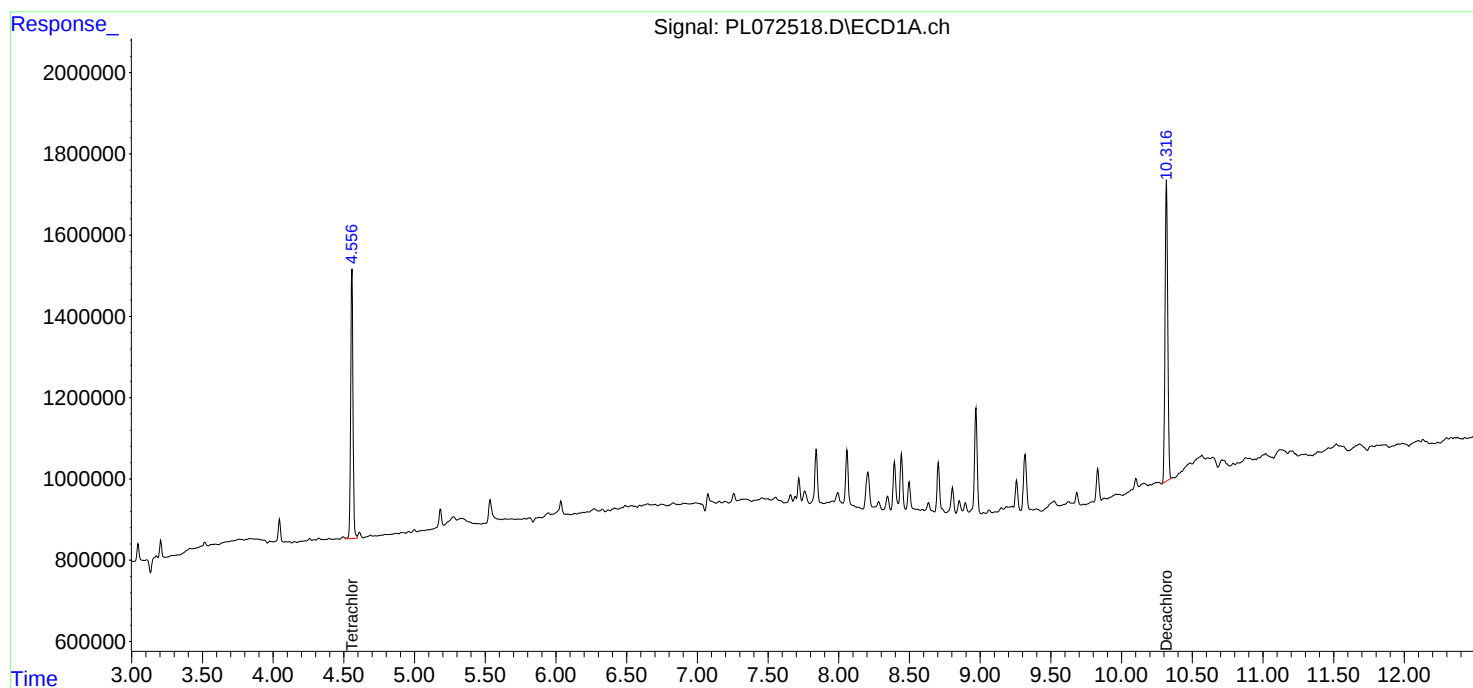

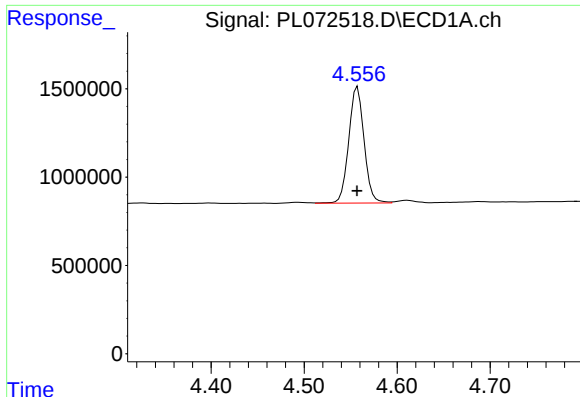


#1 Tetrachloro-m-xylene

R.T.: 4.557 min
Delta R.T.: 0.000 min
Response: 7545566
Conc: 15.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
KTS1-MH-01-0-15


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/09/2022
Supervised By :Ankita Jodhani 02/09/2022

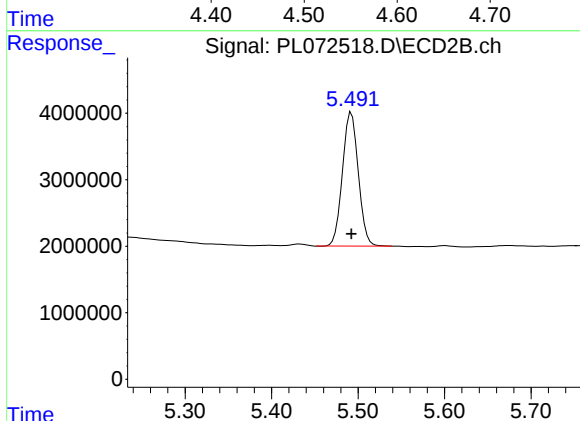


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 25486968
Conc: 14.75 ng/ml

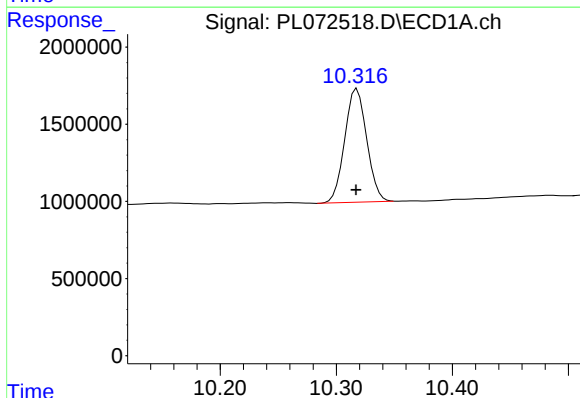

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.000 min
Response: 9705554
Conc: 12.82 ng/ml

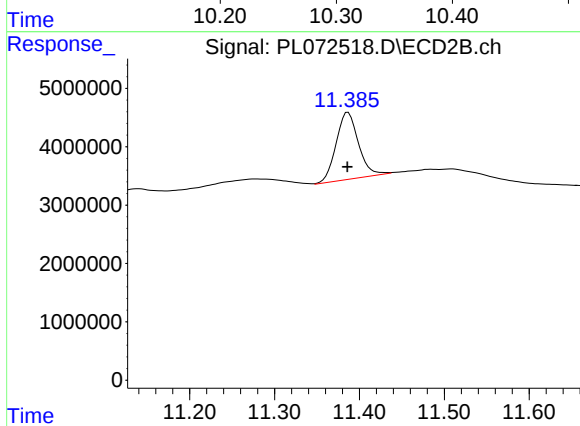

#28 Decachlorobiphenyl

R.T.: 11.385 min
Delta R.T.: 0.000 min
Response: 21091351
Conc: 13.30 ng/ml m