

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020822\
 Data File : PL072527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2022 14:29
 Operator : AR\AJ
 Sample : N1417-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PIT-11-DEWATERING

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/09/2022
 Supervised By : Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 07:50:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.558	5.491	9907648	32411504	20.576	18.763m
28) SA Decachlor...	10.318	11.384	14750126	29864579	19.484	18.833m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020822\
Data File : PL072527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2022 14:29
Operator : AR\AJ
Sample : N1417-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PIT-11-DEWATERING


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/09/2022
Supervised By : Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 07:50:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

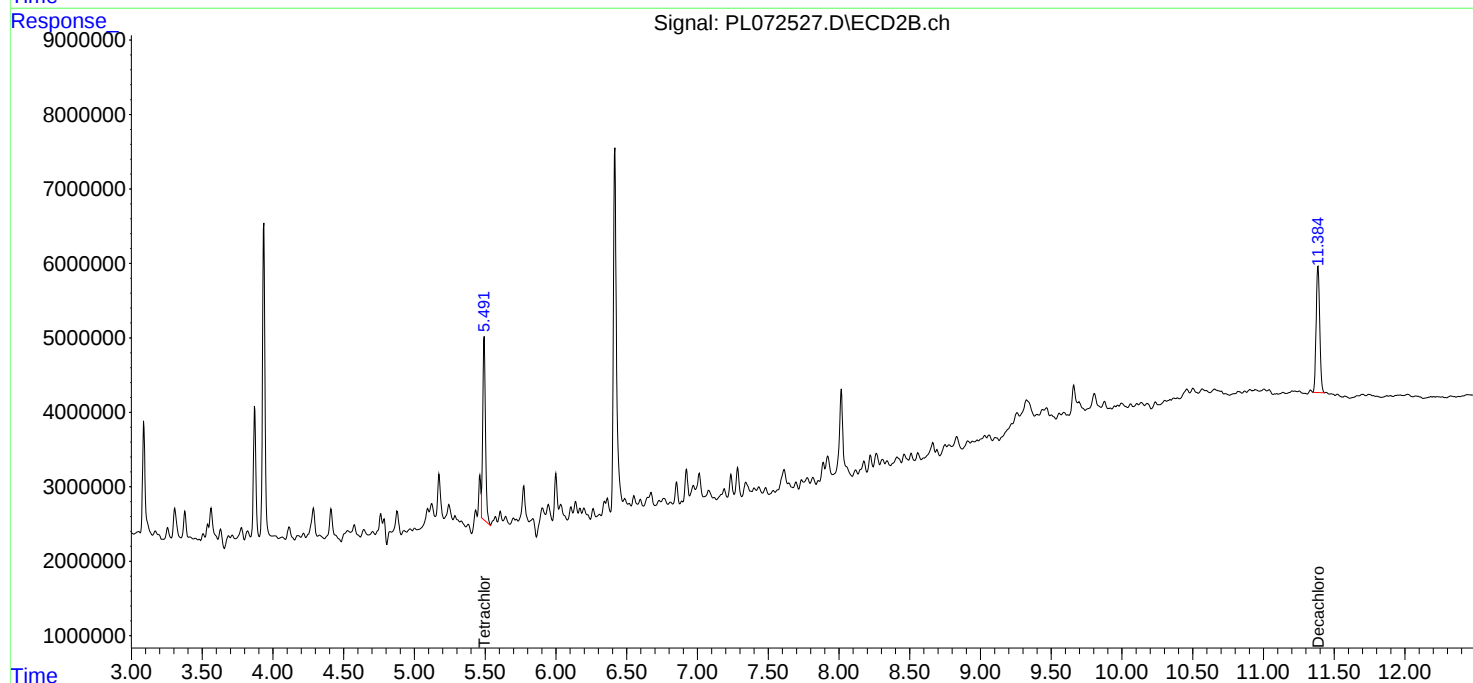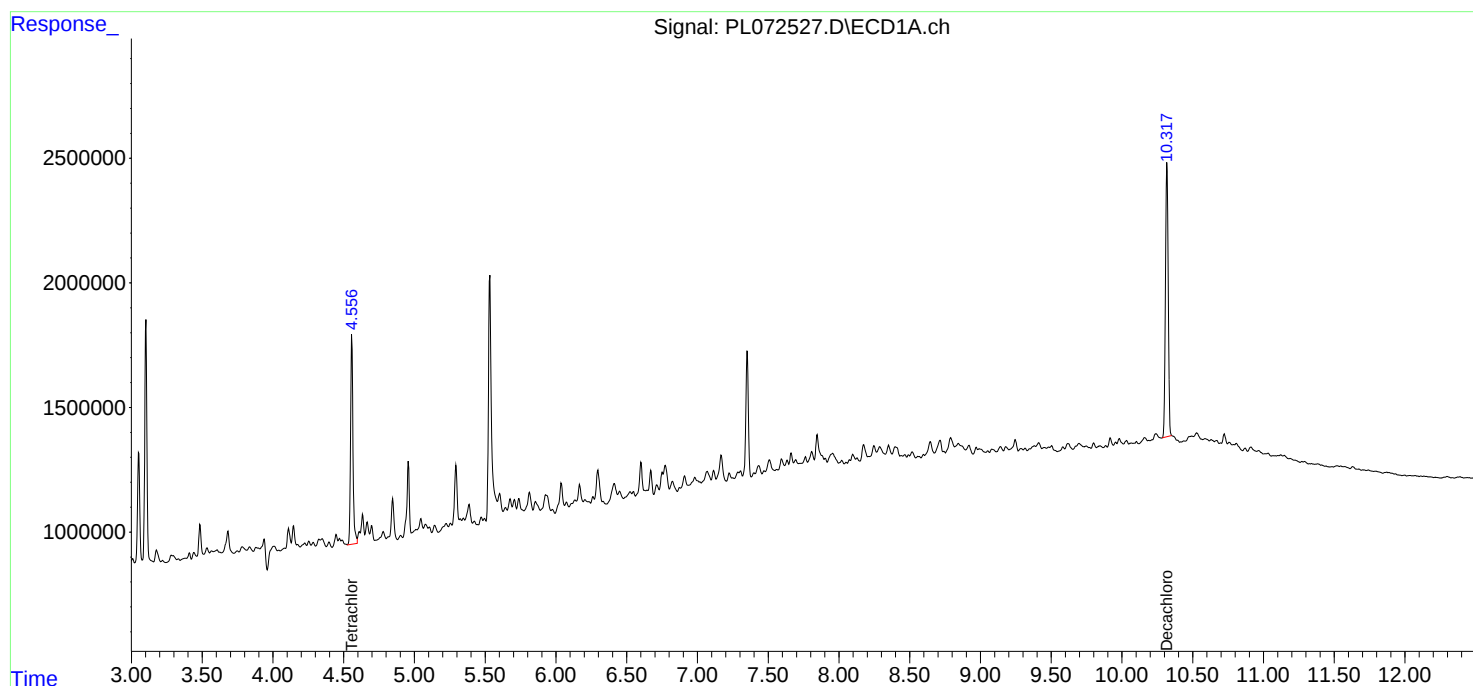

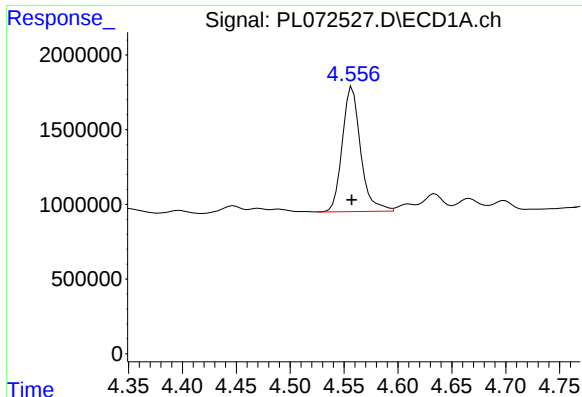


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: 0.000 min
Response: 9907648
Conc: 20.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PIT-11-DEWATERING


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/09/2022
Supervised By :Ankita Jodhani 02/09/2022

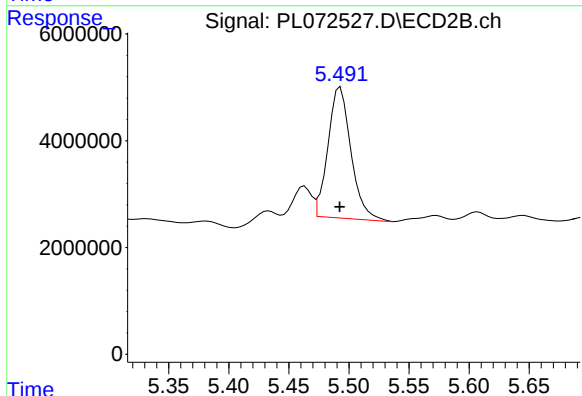


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 32411504
Conc: 18.76 ng/ml m

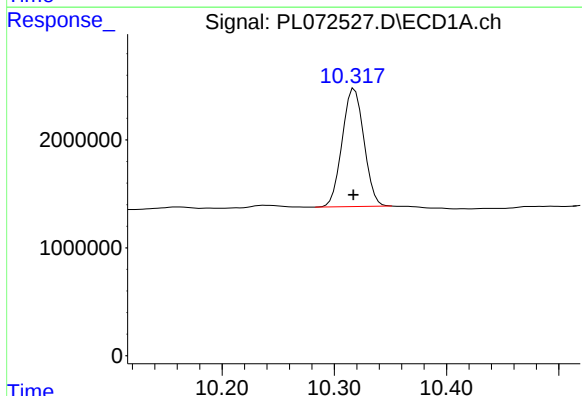

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.000 min
Response: 14750126
Conc: 19.48 ng/ml

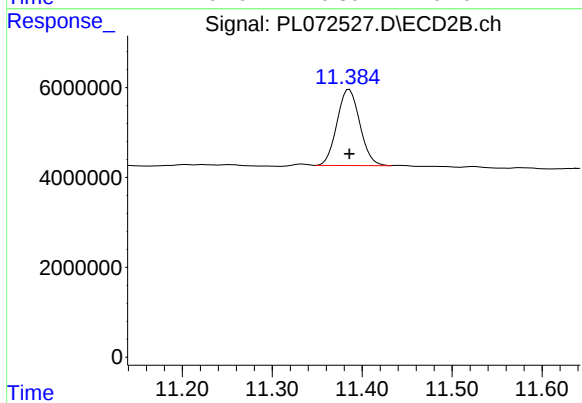

#28 Decachlorobiphenyl

R.T.: 11.384 min
Delta R.T.: -0.002 min
Response: 29864579
Conc: 18.83 ng/ml m