

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020822\
 Data File : PL072550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2022 22:05
 Operator : AR\AJ
 Sample : N1426-04
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 POST-EX-04-0207

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/09/2022
 Supervised By : Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 05:54:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 08 05:14:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.556	5.493	9148778	31372860	19.000m	18.162
2) SA Decachlor...	10.318	11.387	13641751	30501442	18.020	19.234

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020822\
Data File : PL072550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2022 22:05
Operator : AR\AJ
Sample : N1426-04
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
POST-EX-04-0207


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/09/2022
Supervised By : Ankita Jodhani 02/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 05:54:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020722.M
Quant Title : GC Extractables
QLast Update : Tue Feb 08 05:14:10 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

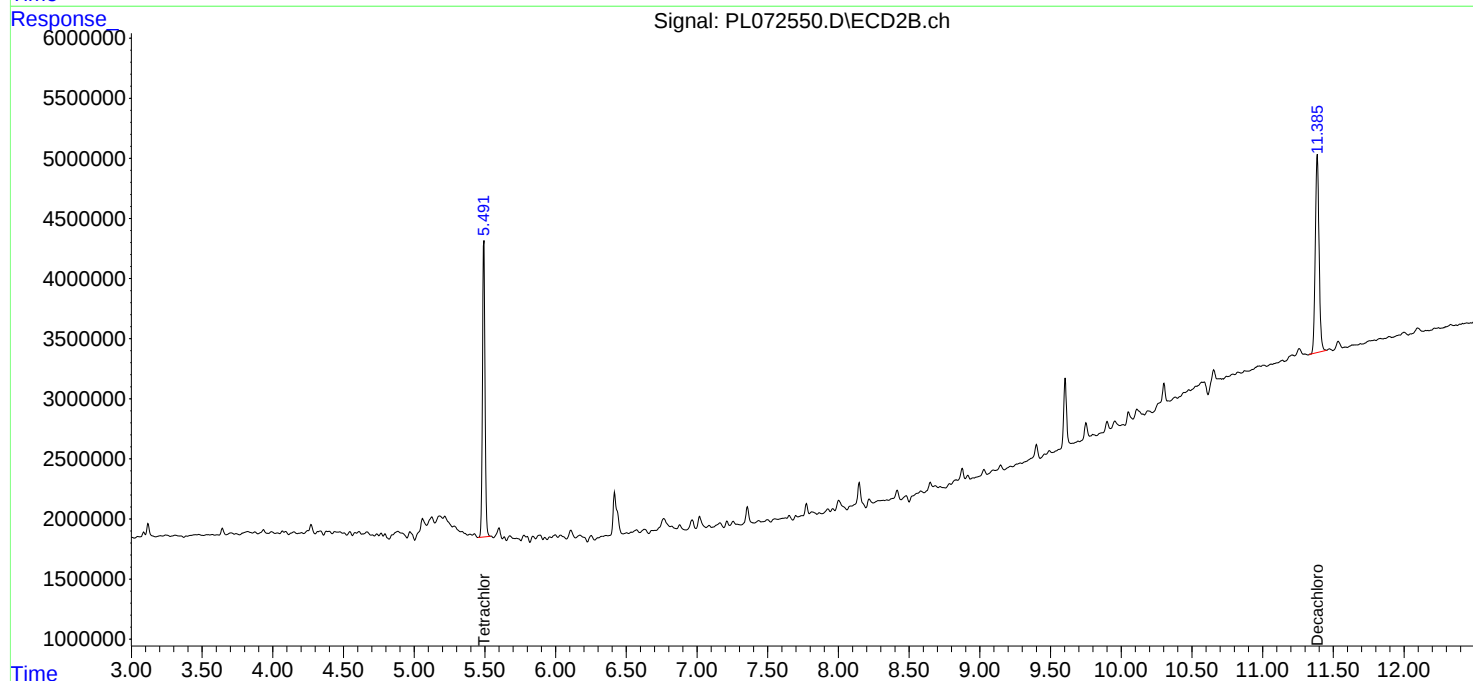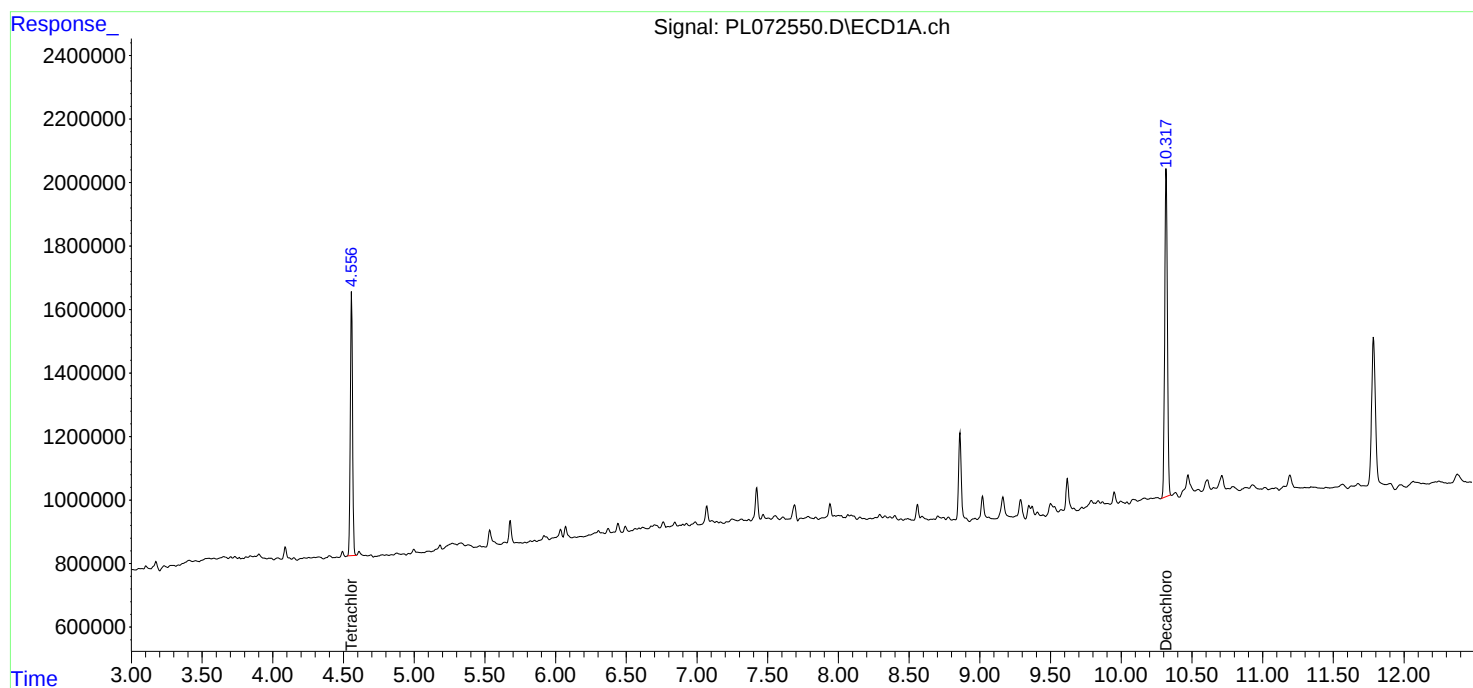

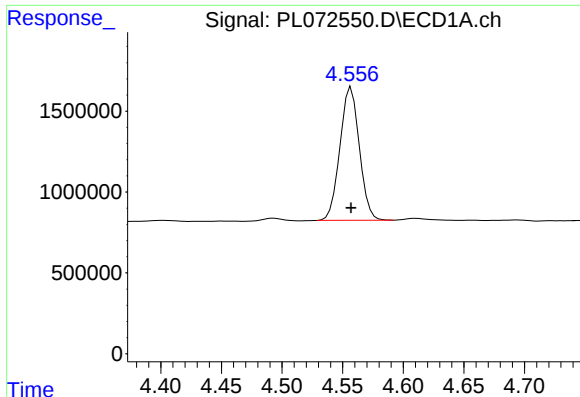


#1 Tetrachloro-m-xylene

R.T.: 4.556 min
Delta R.T.: -0.001 min
Response: 9148778
Conc: 19.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
POST-EX-04-0207


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/09/2022
Supervised By :Ankita Jodhani 02/09/2022

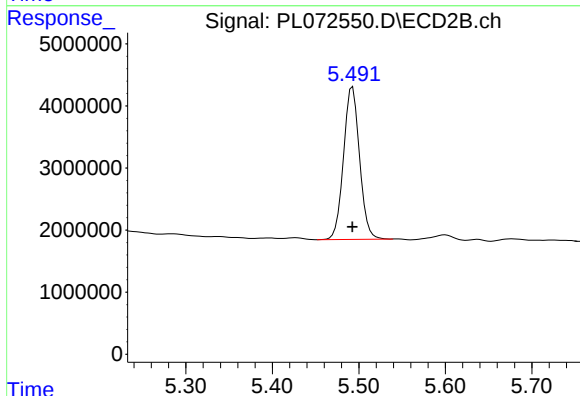


#1 Tetrachloro-m-xylene

R.T.: 5.493 min
Delta R.T.: 0.000 min
Response: 31372860
Conc: 18.16 ng/ml

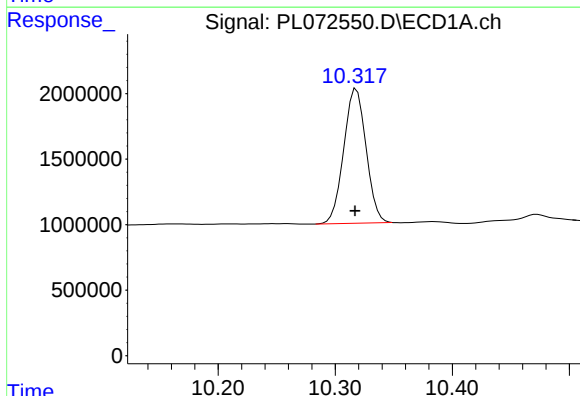

#28 Decachlorobiphenyl

R.T.: 10.318 min
Delta R.T.: 0.001 min
Response: 13641751
Conc: 18.02 ng/ml

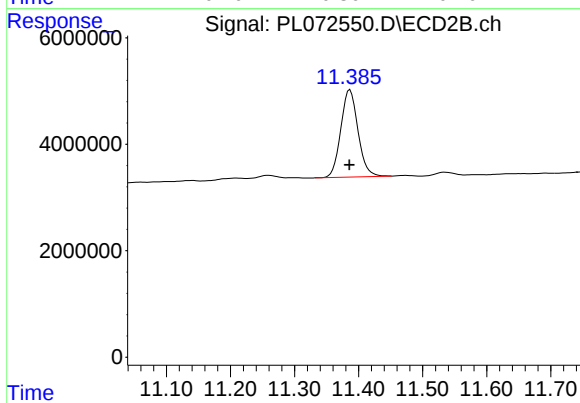

#28 Decachlorobiphenyl

R.T.: 11.387 min
Delta R.T.: 0.000 min
Response: 30501442
Conc: 19.23 ng/ml