

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020823\
 Data File : PL080807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2023 12:16
 Operator : AR\AJ
 Sample : 01378-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-WATER-QT1-2023-02

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/09/2023
 Supervised By :Ankita Jodhani 02/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:26:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020723CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 08 05:59:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.356	2.686	38840531	37966256	18.464	17.713
27)	SA Decachlor...	8.792	7.833	66145039	79634411	37.486m	35.650
Target Compounds							
2)	A alpha-BHC	3.805	3.186	2988488	2694606	0.995	0.916
3)	MA gamma-BHC...	4.132	3.513	2621365	2330674	0.905	0.785m
4)	MA Heptachlor	4.716	3.856	3109200	2832442	1.066	0.940
5)	MB Aldrin	5.055	4.134	2483182	2572502	0.977	0.965
6)	B beta-BHC	4.330	3.811	1155961	1475955	0.827	1.094 #
7)	B delta-BHC	4.571	4.040	3015148	2301762	1.217m	0.835 #
8)	B Heptachlo...	5.478	4.637	2428898	2535907	1.078m	0.970
9)	A Endosulfan I	5.859	5.007	2706048	2298867	1.181m	0.956
10)	B trans-Chl...	5.734	4.888	2659402	2575473	1.162	1.018
11)	B cis-Chlor...	5.811	4.952	2971306	2617582	1.269m	1.006
12)	B 4,4'-DDE	5.991	5.144	2165450	1944066	0.999	0.860
13)	MA Dieldrin	6.134	5.272	2423659	2387569	1.009	0.915
14)	MA Endrin	6.361	5.546	2246445	1952189	1.034	0.867
15)	B Endosulfa...	6.580	5.841	2329228	2171409	1.091m	0.999
16)	A 4,4'-DDD	6.503	5.698	1615175	1485097	0.905m	0.816m
17)	MA 4,4'-DDT	6.817	5.950	2132189	1743391	1.085	0.844
18)	B Endrin al...	6.710	6.021	2048840	1866106	1.193	1.019
19)	B Endosulfa...	6.944	6.244	2264814	2268729	1.106	1.038
20)	A Methoxychlor	7.296	6.528	1344707	1246643	1.254	1.078
21)	B Endrin ke...	7.424	6.748	2342425	2389398	1.073	0.991

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020823\
Data File : PL080807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2023 12:16
Operator : AR\AJ
Sample : 01378-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:26:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020723CLP.M
Quant Title : GC Extractables
QLast Update : Wed Feb 08 05:59:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

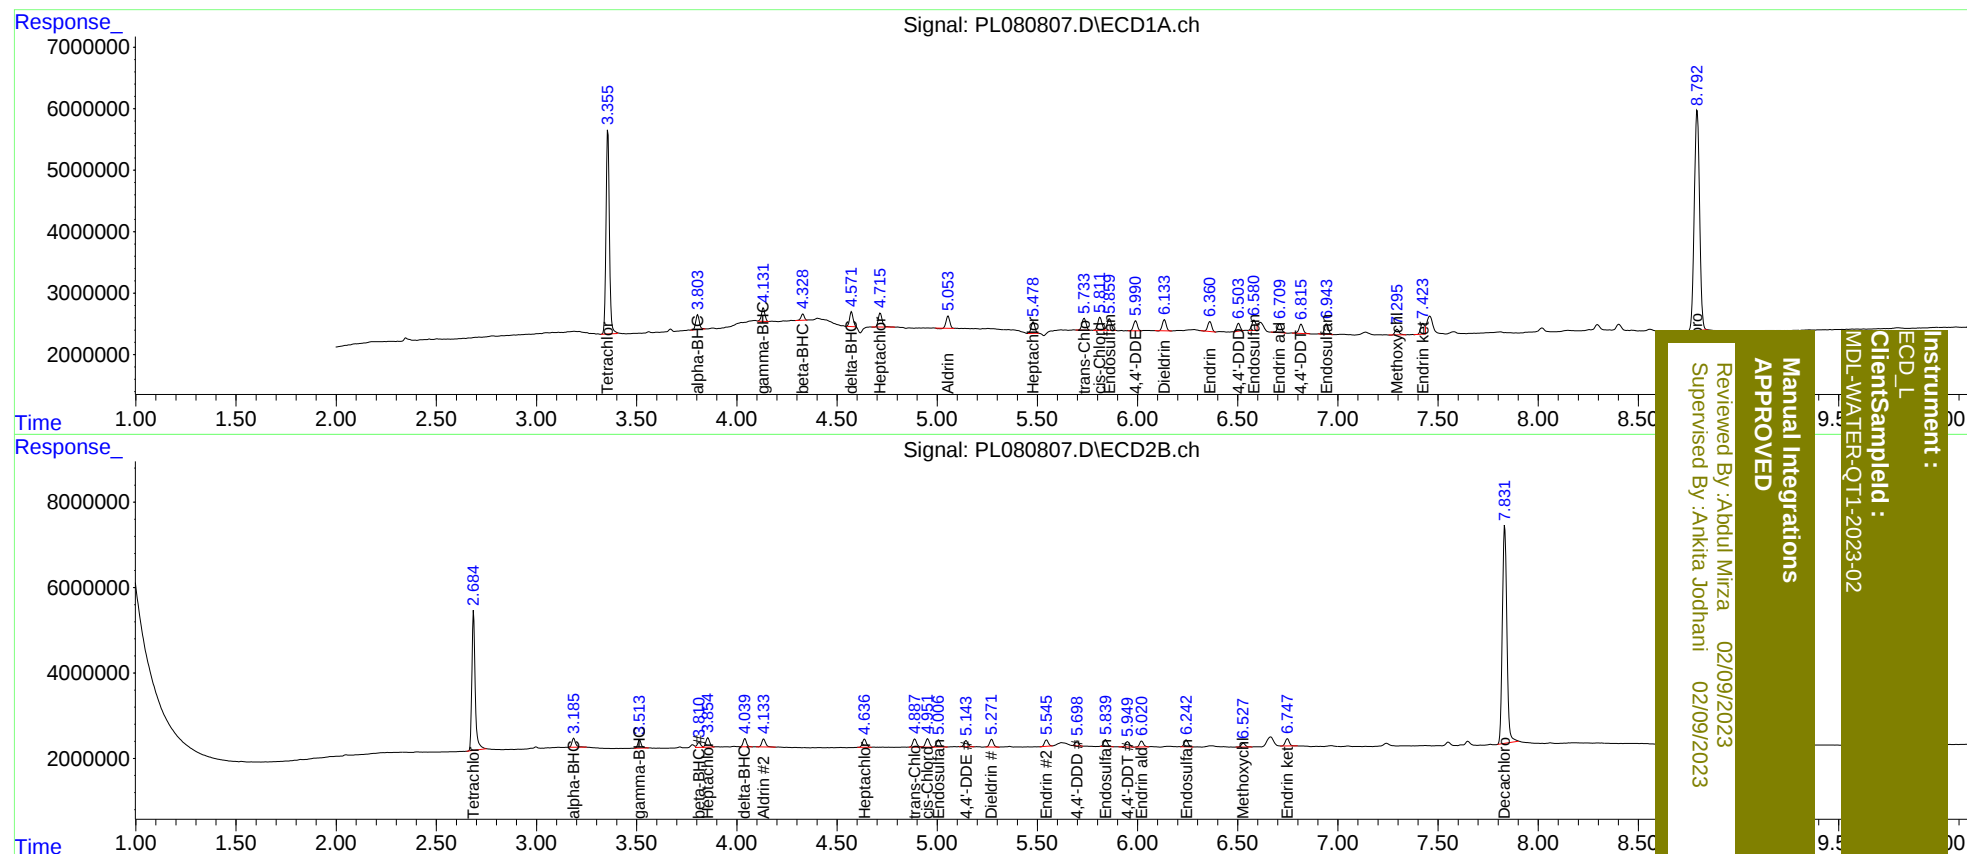

Reviewed By: Abdul Miza 02/09/2023
Supervised By: Ankita Jodhani 02/09/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sample :
MDL-WATER-QT1-2023-02