

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020823\
 Data File : PL080821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2023 16:30
 Operator : AR\AJ
 Sample : 01422-03MSD
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0B45MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/09/2023
 Supervised By : Ankita Jodhani 02/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:30:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020723CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 08 05:59:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.350	2.688	34058042	34520206	16.190	16.106
27)	SA Decachlor...	8.786	7.832	50238058	62260726	28.471	27.872
Target Compounds							
2)	A alpha-BHC	3.799	3.189	154.9E6	150.5E6	51.572	51.150
3)	MA gamma-BHC...	4.127	3.517	145.4E6	145.3E6	50.200	48.943
4)	MA Heptachlor	4.711	3.857	140.3E6	143.1E6	48.093	47.468
5)	MB Aldrin	5.049	4.136	133.0E6	136.2E6	52.348	51.074
6)	B beta-BHC	4.323	3.813	65246435	62308826	46.706	46.180
7)	B delta-BHC	4.565	4.042	127.4E6	124.3E6	51.425m	45.083
8)	B Heptachlo...	5.472	4.638	119.6E6	127.0E6	53.054m	48.570
9)	A Endosulfan I	5.854	5.007	111.1E6	117.0E6	48.492m	48.676
10)	B trans-Chl...	5.728	4.889	117.9E6	126.8E6	51.499	50.146
11)	B cis-Chlor...	5.806	4.953	118.8E6	128.2E6	50.759m	49.295
12)	B 4,4'-DDE	5.985	5.145	218.9E6	230.5E6	101.021	102.029
13)	MA Dieldrin	6.129	5.272	248.5E6	268.4E6	103.441	102.866
14)	MA Endrin	6.356	5.546	217.1E6	238.8E6	99.887	106.067
15)	B Endosulfa...	6.575	5.840	207.4E6	223.6E6	97.142	102.848
16)	A 4,4'-DDD	6.499	5.699	178.9E6	180.3E6	100.263	99.068
17)	MA 4,4'-DDT	6.812	5.951	190.3E6	207.2E6	96.806	100.347
18)	B Endrin al...	6.705	6.021	149.5E6	158.3E6	87.104	86.396
19)	B Endosulfa...	6.938	6.243	195.5E6	211.7E6	95.455	96.836
20)	A Methoxychlor	7.290	6.528	511.1E6	546.3E6	476.634	472.547
21)	B Endrin ke...	7.418	6.748	217.1E6	251.4E6	99.477	104.218

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020823\
Data File : PL080821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2023 16:30
Operator : AR\AJ
Sample : 01422-03MSD
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:30:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020723CLP.M
Quant Title : GC Extractables
QLast Update : Wed Feb 08 05:59:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

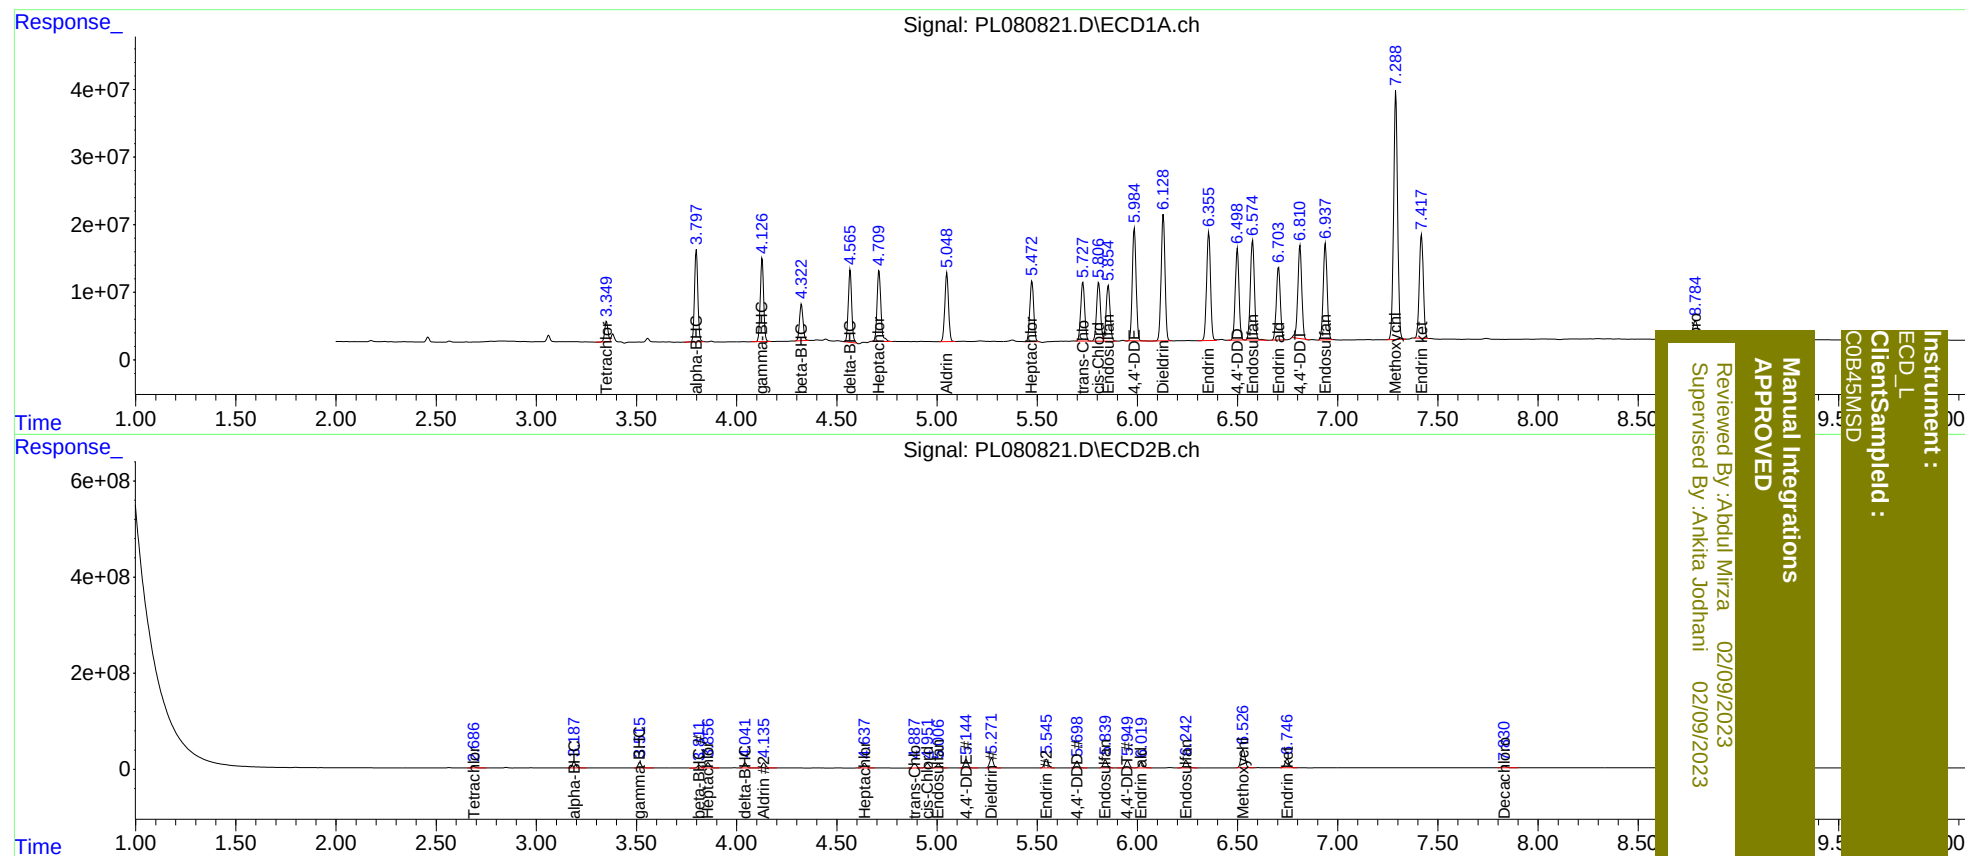

Reviewed By: Abdul Mirza 02/09/2023
Supervised By: Ankita Jodhani 02/09/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
COB45MSD