

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020823\
 Data File : PL080820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Feb 2023 16:16
 Operator : AR\AJ
 Sample : 01422-02MS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C0B45MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/09/2023
 Supervised By :Ankita Jodhani 02/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 09 00:30:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020723CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 08 05:59:16 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.351	2.688	34710735	35061531	16.500	16.358
27)	SA Decachlor...	8.786	7.832	50988508	63549332	28.897	28.449
Target Compounds							
2)	A alpha-BHC	3.800	3.188	158.5E6	153.3E6	52.765	52.115
3)	MA gamma-BHC...	4.128	3.517	149.1E6	148.3E6	51.491	49.961
4)	MA Heptachlor	4.711	3.857	144.0E6	146.7E6	49.351	48.677
5)	MB Aldrin	5.050	4.136	136.5E6	139.5E6	53.695	52.320
6)	B beta-BHC	4.324	3.813	65981452	64157399	47.232	47.550
7)	B delta-BHC	4.565	4.042	129.3E6	127.4E6	52.193m	46.205
8)	B Heptachlo...	5.473	4.638	122.3E6	130.1E6	54.279m	49.765
9)	A Endosulfan I	5.854	5.007	110.6E6	120.1E6	48.260m	49.953
10)	B trans-Chl...	5.729	4.889	120.9E6	130.3E6	52.827	51.518
11)	B cis-Chlor...	5.806	4.953	119.7E6	131.8E6	51.128m	50.671
12)	B 4,4'-DDE	5.986	5.146	227.0E6	237.0E6	104.735	104.894
13)	MA Dieldrin	6.130	5.273	255.5E6	276.1E6	106.381	105.822
14)	MA Endrin	6.357	5.547	223.8E6	244.6E6	102.960	108.642
15)	B Endosulfa...	6.576	5.841	212.1E6	229.0E6	99.361	105.322
16)	A 4,4'-DDD	6.500	5.700	183.9E6	185.5E6	103.077	101.931
17)	MA 4,4'-DDT	6.813	5.951	197.8E6	212.4E6	100.588	102.868
18)	B Endrin al...	6.705	6.021	153.2E6	161.6E6	89.255	88.206
19)	B Endosulfa...	6.939	6.244	200.9E6	216.7E6	98.115	99.113
20)	A Methoxychlor	7.291	6.529	526.2E6	559.3E6	490.757	483.815
21)	B Endrin ke...	7.418	6.749	223.2E6	257.6E6	102.242	106.794

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020823\
Data File : PL080820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Feb 2023 16:16
Operator : AR\AJ
Sample : 01422-02MS
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 09 00:30:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020723CLP.M
Quant Title : GC Extractables
QLast Update : Wed Feb 08 05:59:16 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

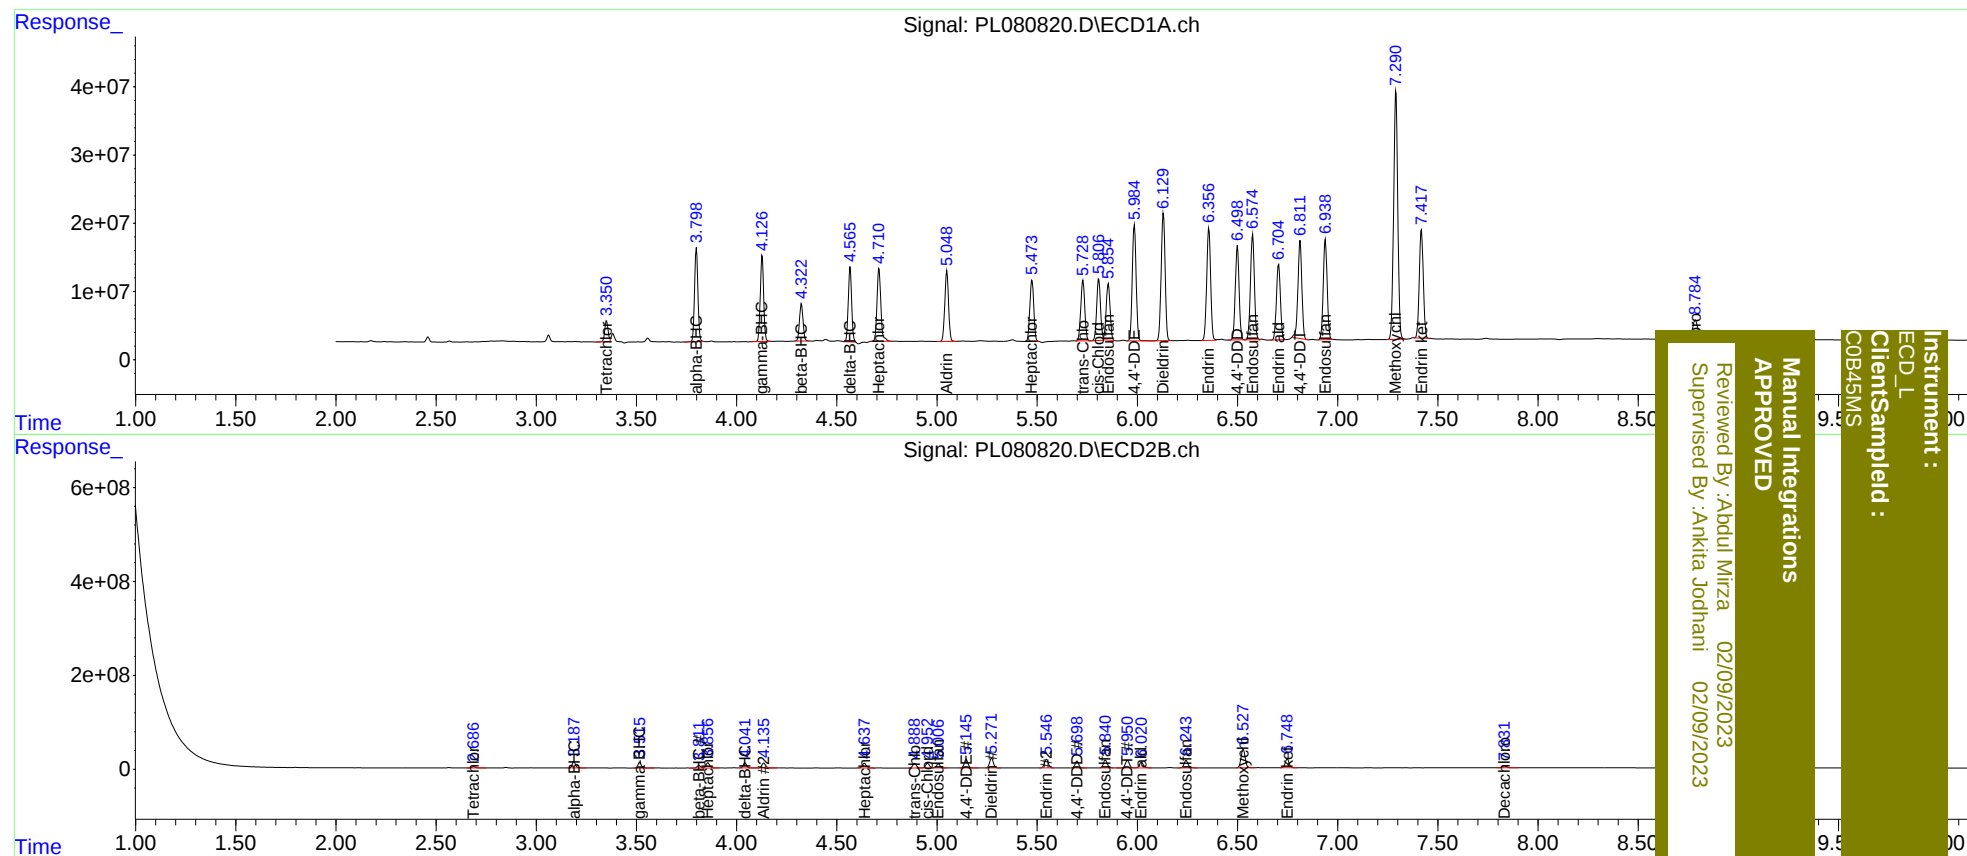

Reviewed By: Abdul Mirza 02/09/2023
Supervised By: Ankita Jodhani 02/09/2023

Manual Integrations
APPROVED

Instrument :
ECD_L
Client Sampled :
COB45MS