

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
 Data File : PL064710.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Feb 2021 18:15
 Operator : AR\AJ
 Sample : PB134518BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB134518BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 10 02:10:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.426	4.101	60035762	48609003	21.338	22.502
28)	SA Decachlor...	8.148	9.260	55722348	41421563	24.779	21.808
Target Compounds							
6)	B beta-BHC	0.000	4.977	0	5214220	N.D.	0.262 #
23)	Chlordane-1	4.313f	0.000	1101558	0	9.690	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020921\
Data File : PL064710.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Feb 2021 18:15
Operator : AR\AJ
Sample : PB134518BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB134518BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 10 02:10:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

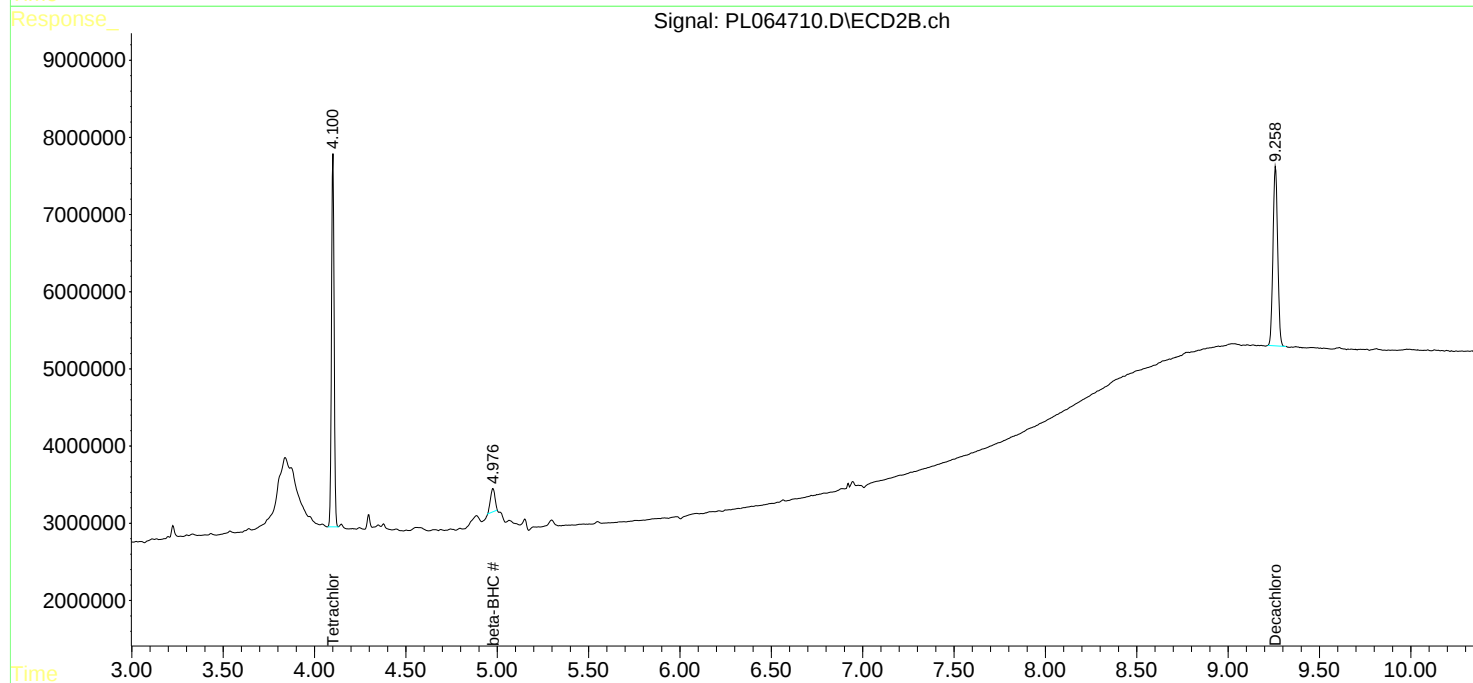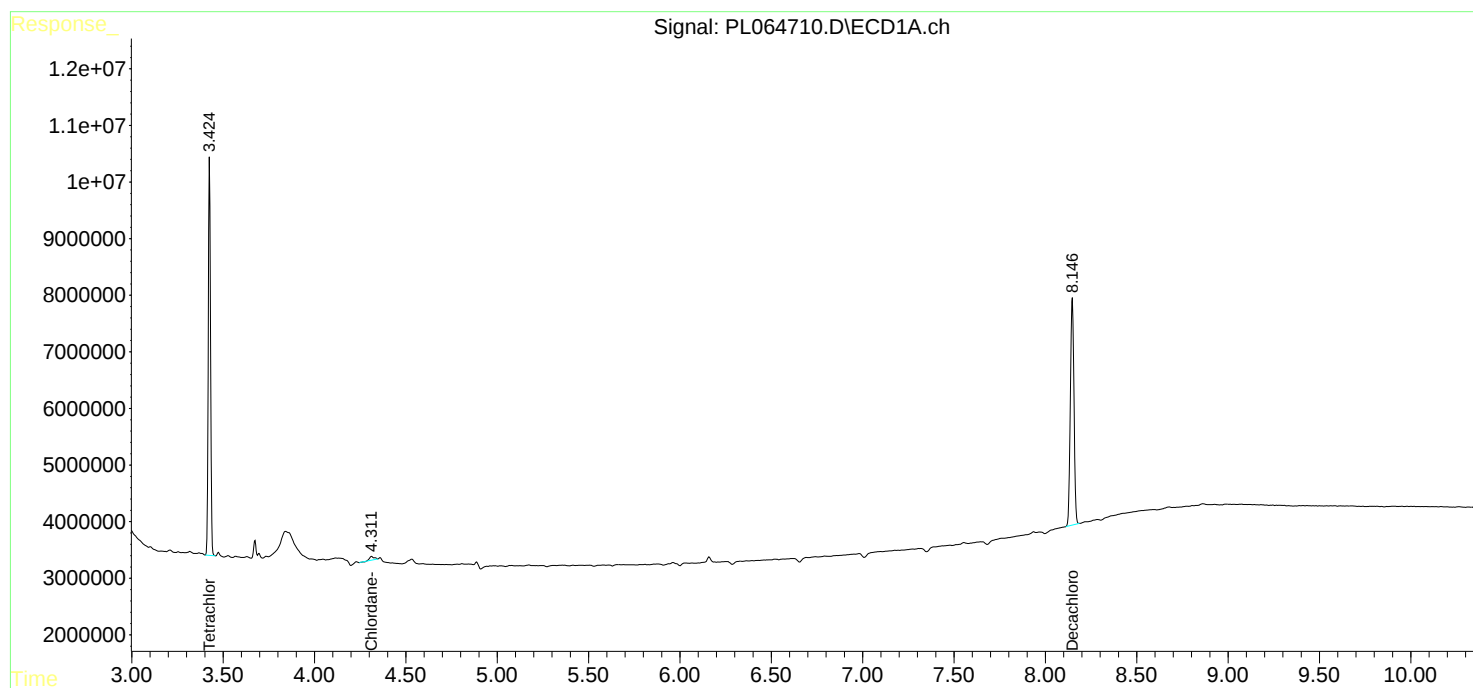


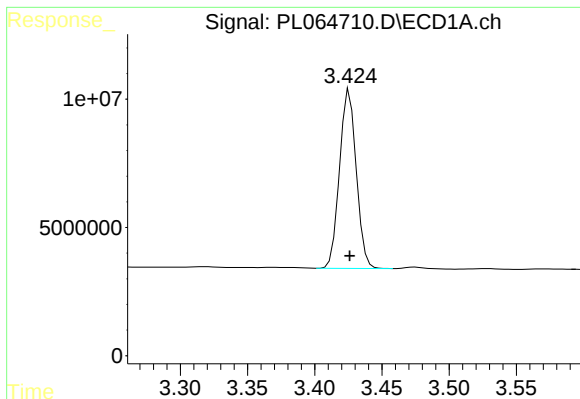

#1 Tetrachloro-m-xylene


R.T.: 3.426 min
Delta R.T.: 0.000 min
Response: 60035762
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134518BL

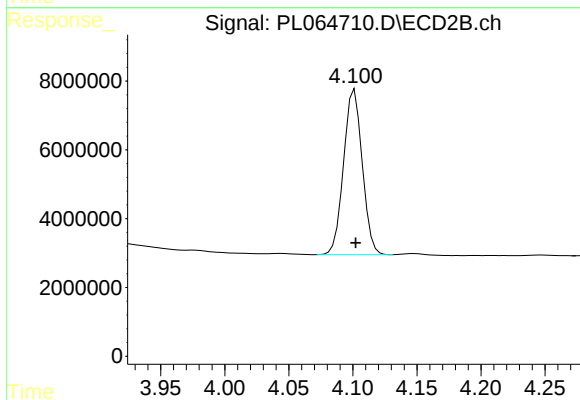


#1 Tetrachloro-m-xylene

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 48609003
Conc: 22.50 ng/ml

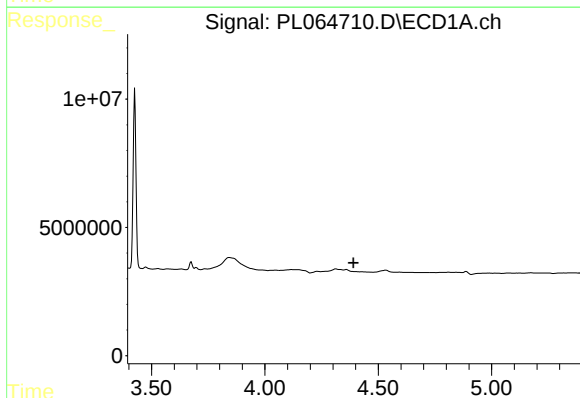


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

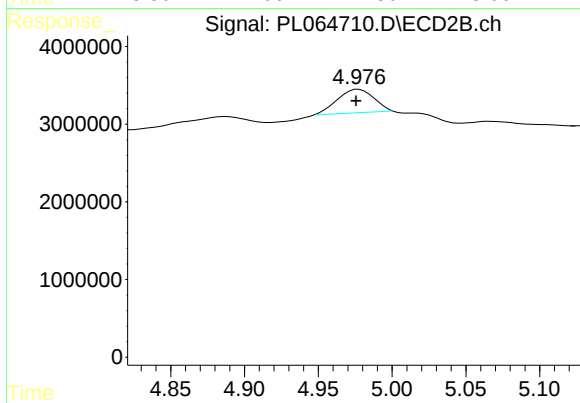

#6 beta-BHC


R.T.: 4.977 min
Delta R.T.: 0.002 min
Response: 5214220
Conc: 0.26 ng/ml

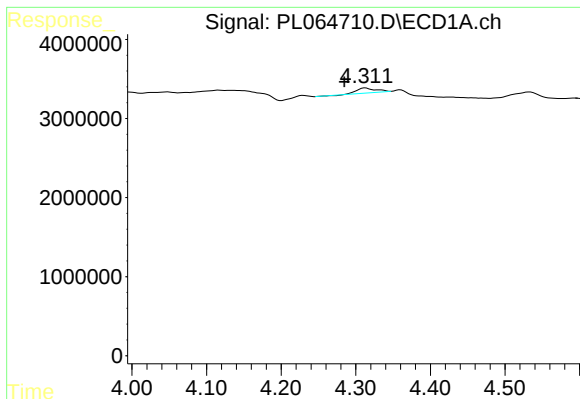

#23 Chlordane-1


R.T.: 4.313 min
Delta R.T.: 0.028 min
Response: 1101558
Conc: 9.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134518BL

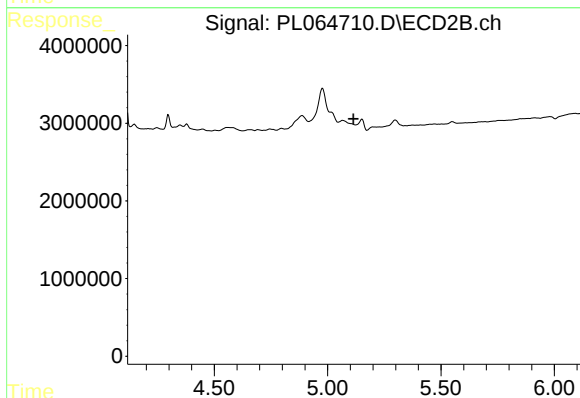


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

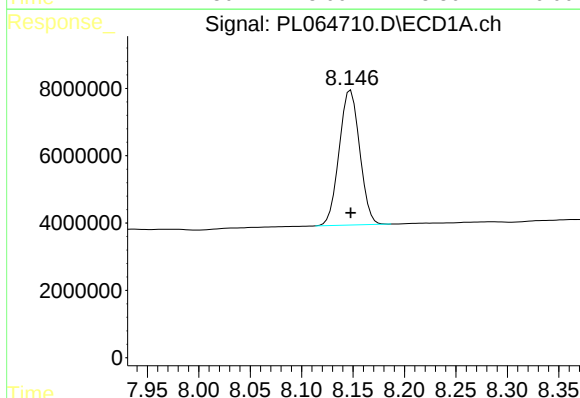

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 55722348
Conc: 24.78 ng/ml

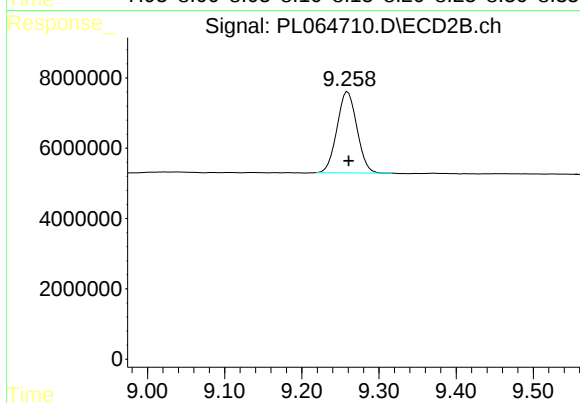

#28 Decachlorobiphenyl

R.T.: 9.260 min
Delta R.T.: -0.001 min
Response: 41421563
Conc: 21.81 ng/ml